


Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD062218\
Data File : VD058291.D
Acq On : 22 Jun 2018 11:57
Operator : VA/AP
Sample : BFB
Misc : 5.00µl/5ml/MSVOA D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D061918S.M
Title : SW846 8260
Last Update : Wed Jun 20 05:52:56 2018

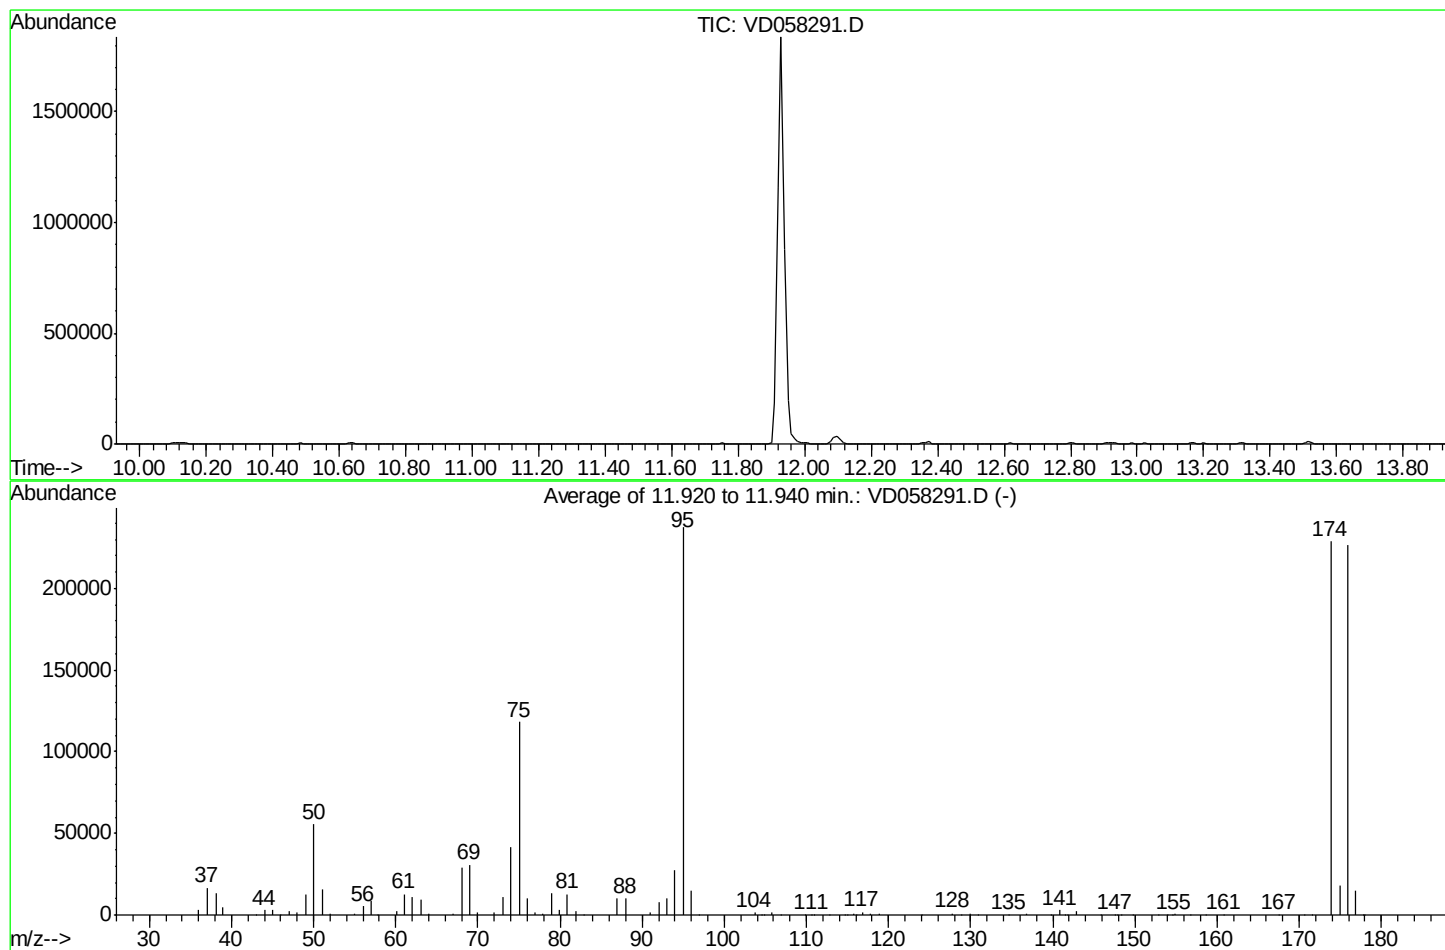

AutoFind: Scans 1188, 1189, 1190; Background Corrected with Scan 1183

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.3	55408	PASS
75	95	30	60	49.8	118349	PASS
95	95	100	100	100.0	237461	PASS
96	95	5	9	6.4	15228	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	96.3	228757	PASS
175	174	5	9	7.7	17689	PASS
176	174	95	101	98.9	226261	PASS
177	176	5	9	6.5	14731	PASS