


Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD062218\
Data File : VD058315.D
Acq On : 23 Jun 2018 00:58
Operator : VA/AP
Sample : BFB
Misc : 5.00µl/5ml/MSVOA D/SOIL
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D061918S.M
Title : SW846 8260
Last Update : Wed Jun 20 05:52:56 2018

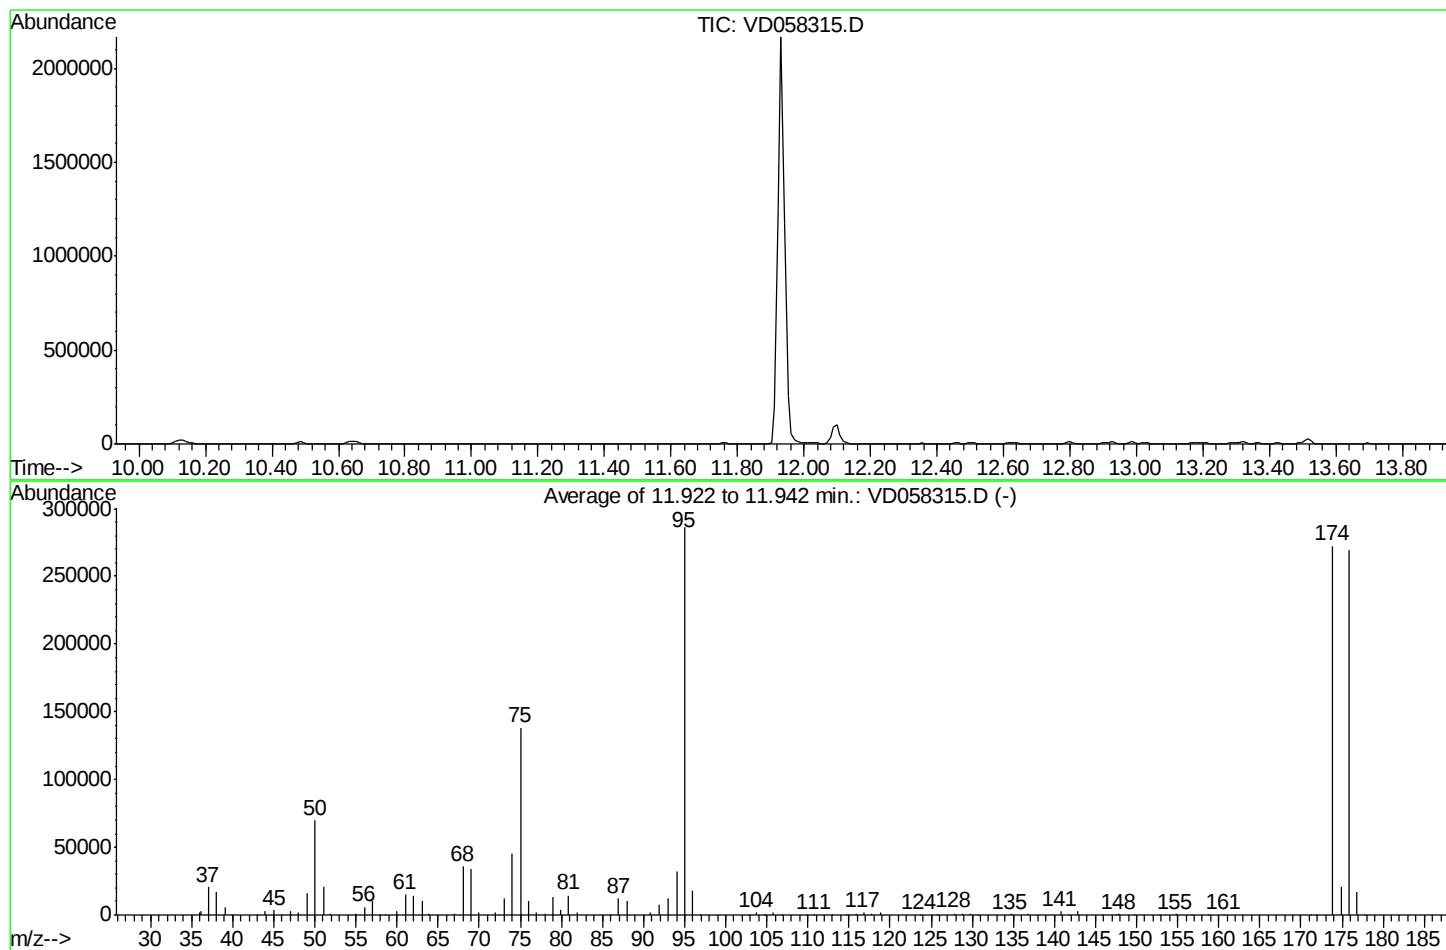

AutoFind: Scans 1188, 1189, 1190; Background Corrected with Scan 1183

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.4	69693	PASS
75	95	30	60	48.3	138256	PASS
95	95	100	100	100.0	286144	PASS
96	95	5	9	6.4	18299	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	95.2	272341	PASS
175	174	5	9	7.6	20581	PASS
176	174	95	101	98.8	268992	PASS
177	176	5	9	6.5	17467	PASS