

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD062221\
 Data File : VD069517.D
 Acq On : 22 Jun 2021 15:44
 Operator : VA/SY
 Sample : M2773-03
 Misc : 4.91G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 SB-3

Quant Time: Jun 23 04:28:39 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D062121S.M
 Quant Title : SW846 8260
 QLast Update : Tue Jun 22 04:33:24 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.979	168	414079	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.867	114	835146	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.644	117	872041	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.567	152	371380	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.332	65	315772	61.179	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	122.360%
35) Dibromofluoromethane	7.914	113	306026	54.208	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	108.420%
50) Toluene-d8	10.338	98	1088129	51.386	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	102.780%
62) 4-Bromofluorobenzene	12.626	95	379928	54.575	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	109.140%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD062221\
Data File : VD069517.D
Acq On : 22 Jun 2021 15:44
Operator : VA/SY
Sample : M2773-03
Misc : 4.91G/5.00ml/MSVOA_D/SOIL
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
SB-3

Quant Time: Jun 23 04:28:39 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D062121S.M
Quant Title : SW846 8260
QLast Update : Tue Jun 22 04:33:24 2021
Response via : Initial Calibration




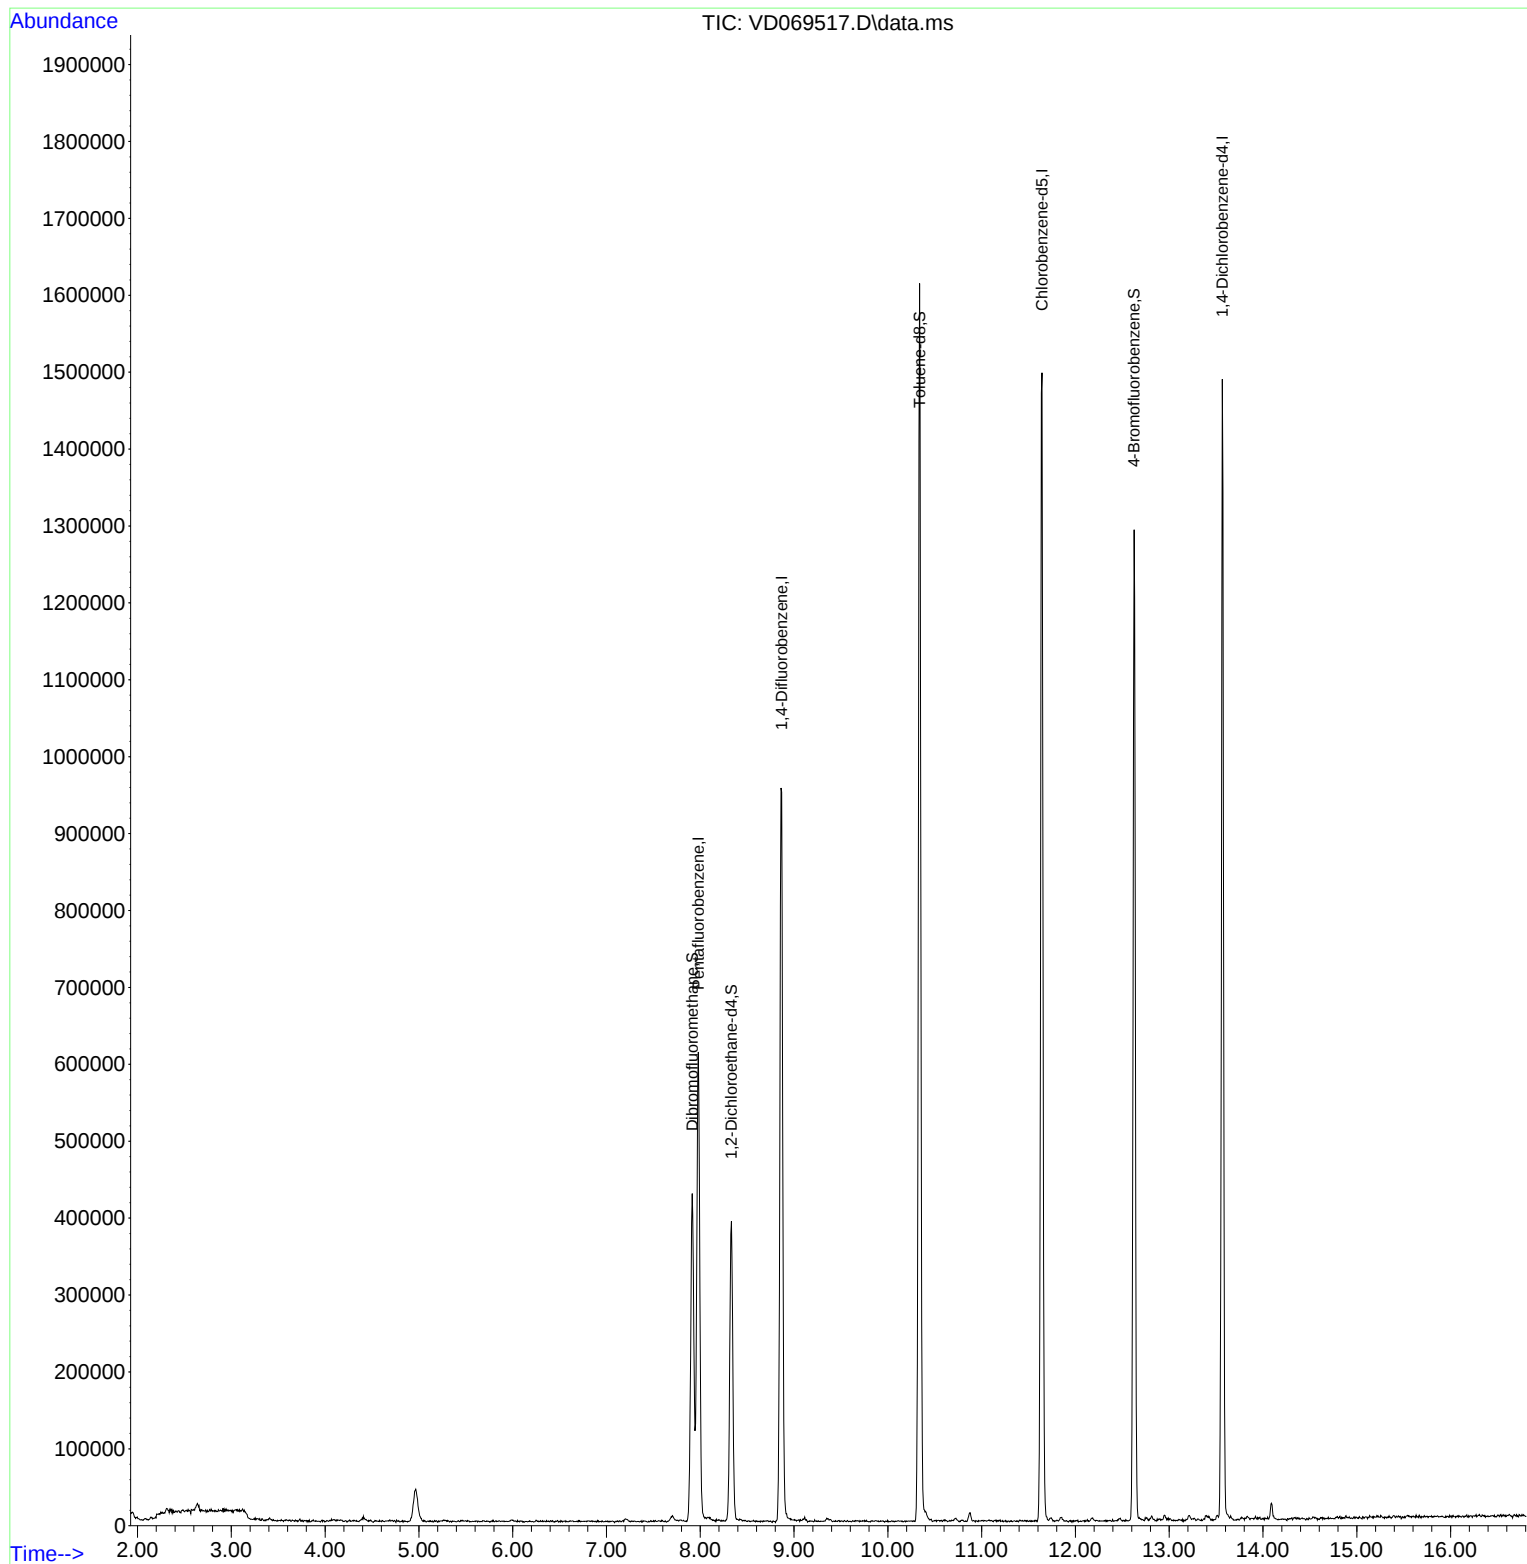


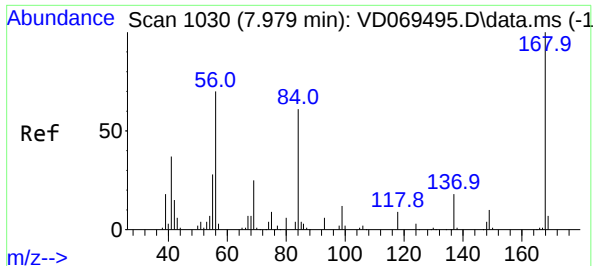

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.979 min Scan# 1030
Delta R.T. 0.000 min
Lab File: VD069517.D
Acq: 22 Jun 2021 15:44




Instrument :
MSVOA_D
ClientSampled :
SB-3


Tgt Ion:168 Resp: 414079
Ion Ratio Lower Upper
168 100
99 64.1 49.3 73.9

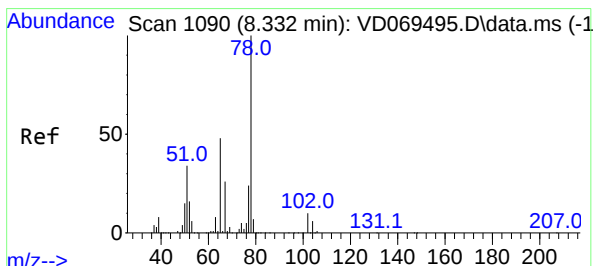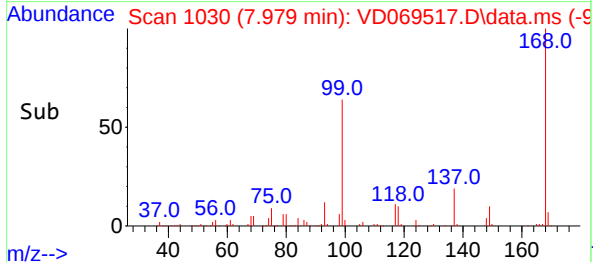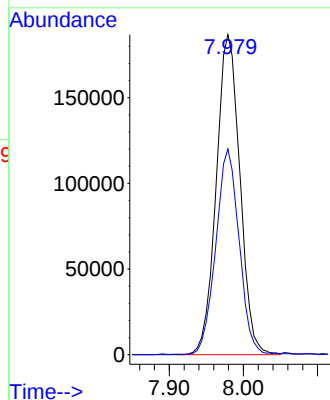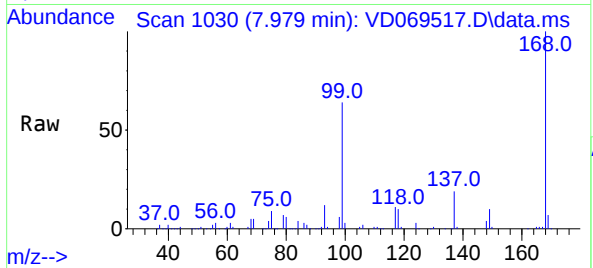

#33
1,2-Dichloroethane-d4
Concen: 61.179 ug/l
RT: 8.332 min Scan# 1090
Delta R.T. -0.000 min
Lab File: VD069517.D
Acq: 22 Jun 2021 15:44

Tgt Ion: 65 Resp: 315772
Ion Ratio Lower Upper
65 100
67 52.6 0.0 105.6

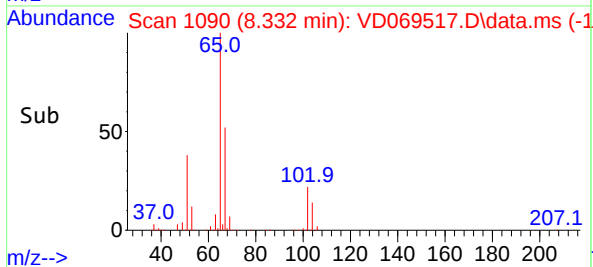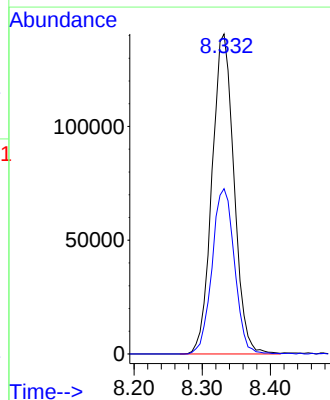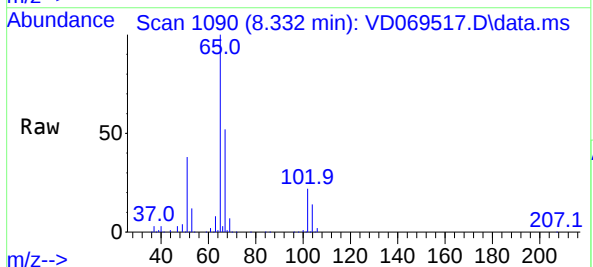




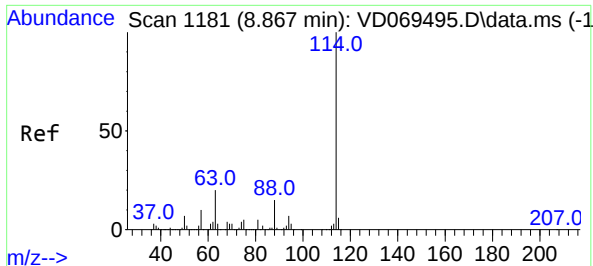


#34

1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.867 min Scan# 1181
Delta R.T. 0.000 min
Lab File: VD069517.D
Acq: 22 Jun 2021 15:44

Instrument :
MSVOA_D
ClientSampled :
SB-3




Tgt Ion:114 Resp: 835146
Ion Ratio Lower Upper
114 100
63 20.4 0.0 39.6
88 15.7 0.0 29.8

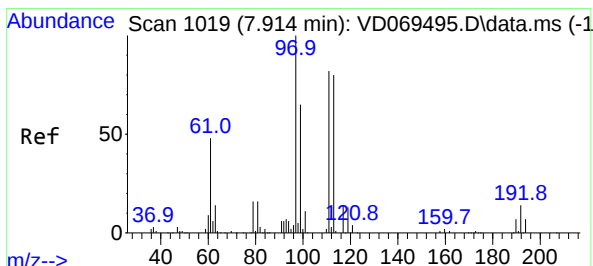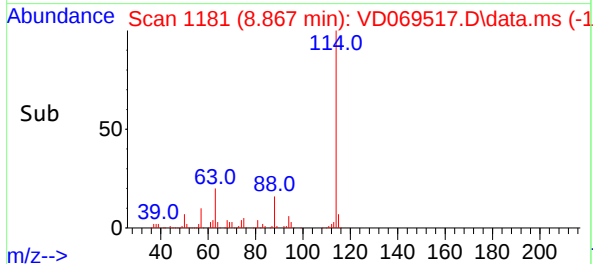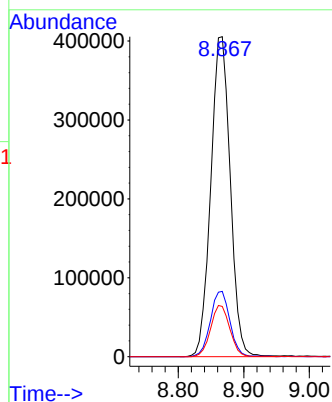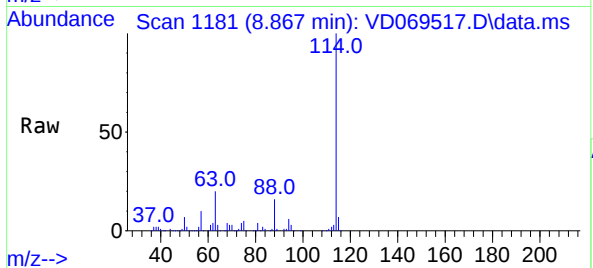


#35

Dibromofluoromethane
Concen: 54.208 ug/l
RT: 7.914 min Scan# 1019
Delta R.T. -0.000 min
Lab File: VD069517.D
Acq: 22 Jun 2021 15:44

Tgt Ion:113 Resp: 306026
Ion Ratio Lower Upper
113 100
111 103.2 81.8 122.8
192 16.3 13.8 20.6


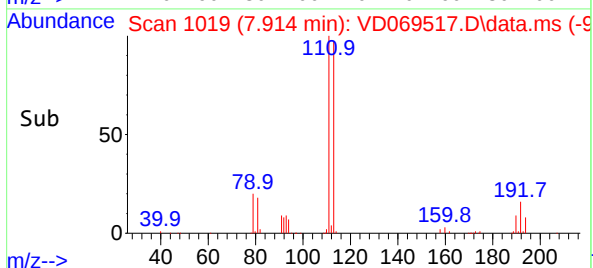
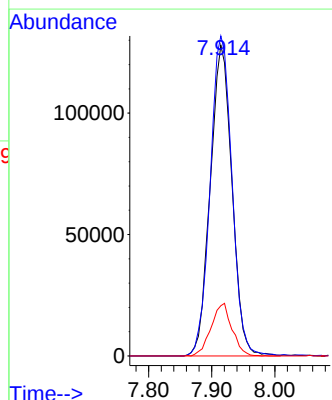
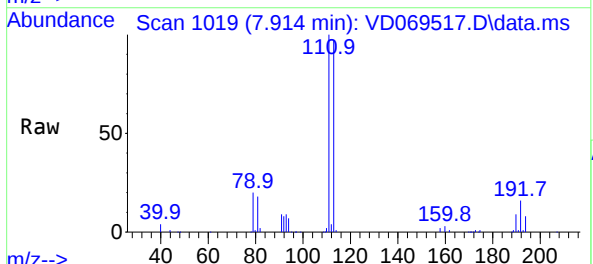


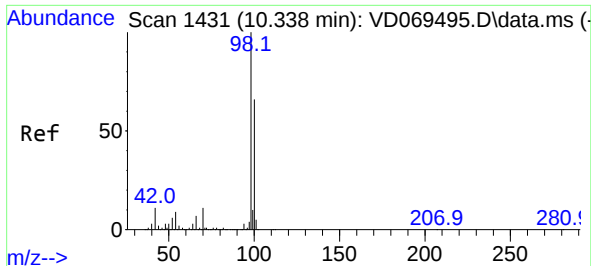

#50
Toluene-d8
Concen: 51.386 ug/l
RT: 10.338 min Scan# 1431
Delta R.T. -0.000 min
Lab File: VD069517.D
Acq: 22 Jun 2021 15:44




Instrument :
MSVOA_D
ClientSampleId :
SB-3


Tgt Ion: 98 Resp: 1088129
Ion Ratio Lower Upper
98 100
100 64.4 52.3 78.5

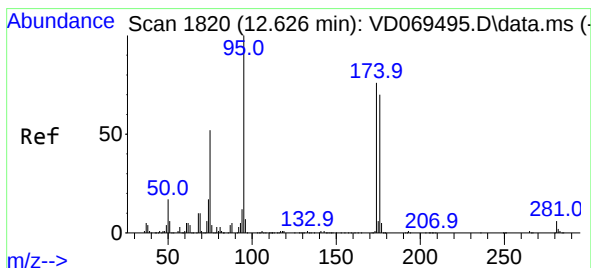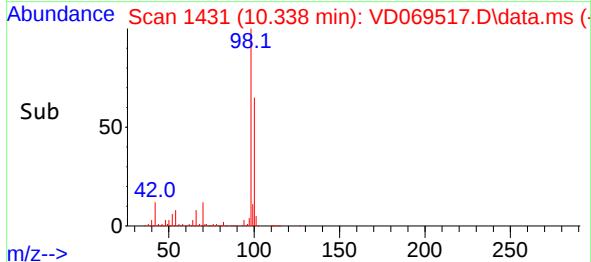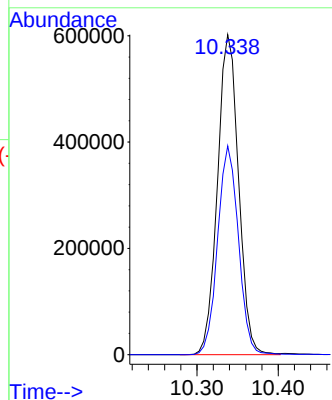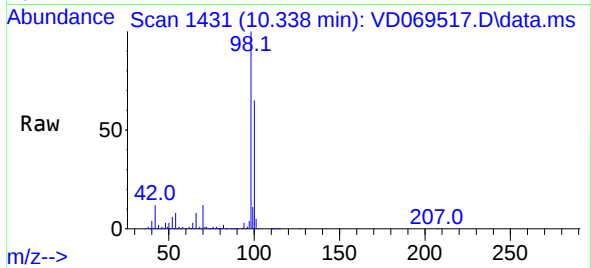

#62
4-Bromofluorobenzene
Concen: 54.575 ug/l
RT: 12.626 min Scan# 1820
Delta R.T. -0.000 min
Lab File: VD069517.D
Acq: 22 Jun 2021 15:44


Tgt Ion: 95 Resp: 379928
Ion Ratio Lower Upper
95 100
174 74.7 0.0 148.0
176 72.4 0.0 139.8

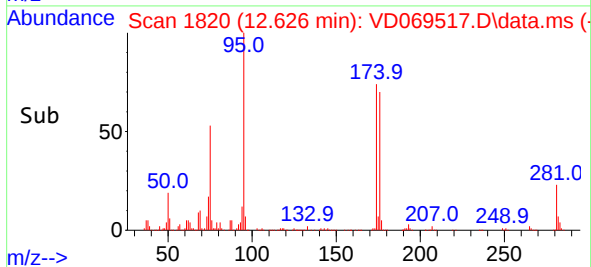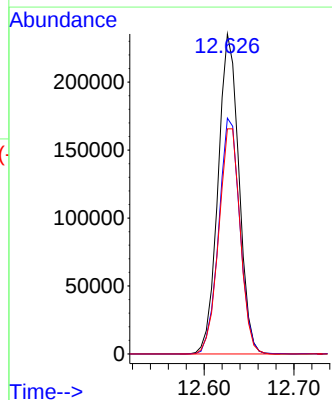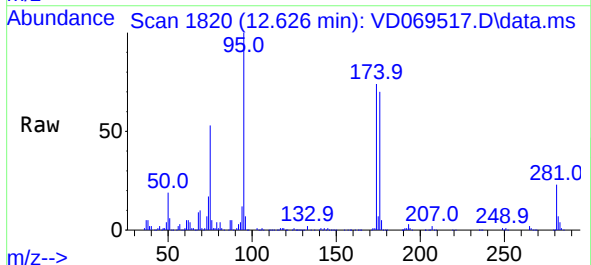



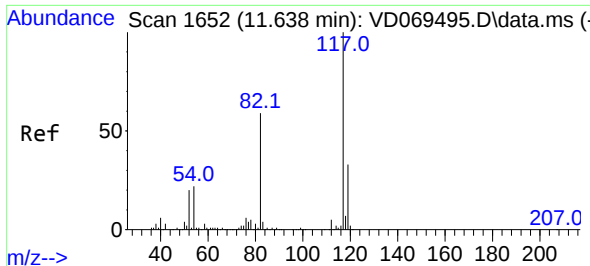


#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.644 min Scan# 1653
Delta R.T. 0.006 min
Lab File: VD069517.D
Acq: 22 Jun 2021 15:44

Instrument :
MSVOA_D
ClientSampleId :
SB-3

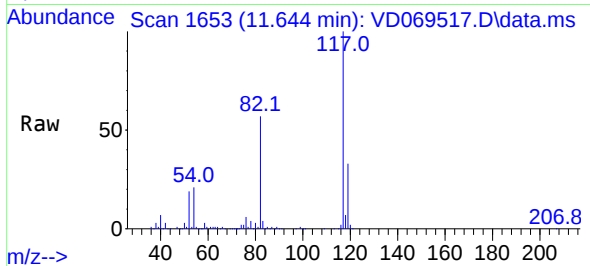

Tgt Ion:117 Resp: 872041
Ion Ratio Lower Upper
117 100
82 57.3 46.8 70.2
119 33.5 26.2 39.2

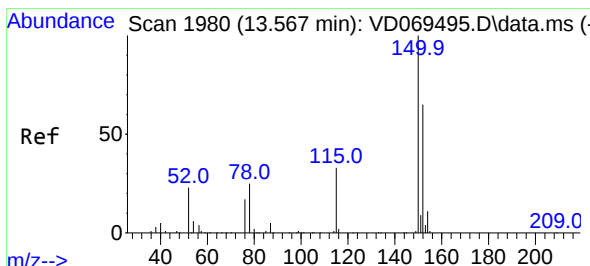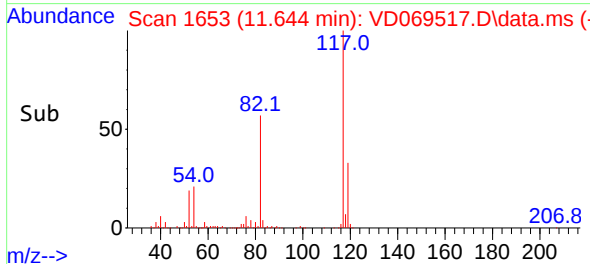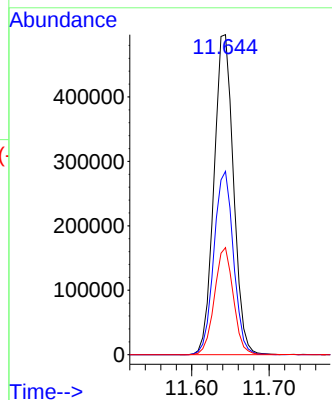

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.567 min Scan# 1980
Delta R.T. -0.000 min
Lab File: VD069517.D
Acq: 22 Jun 2021 15:44

Tgt Ion:152 Resp: 371380
Ion Ratio Lower Upper
152 100
115 62.3 31.7 95.1
150 157.5 0.0 350.8

