
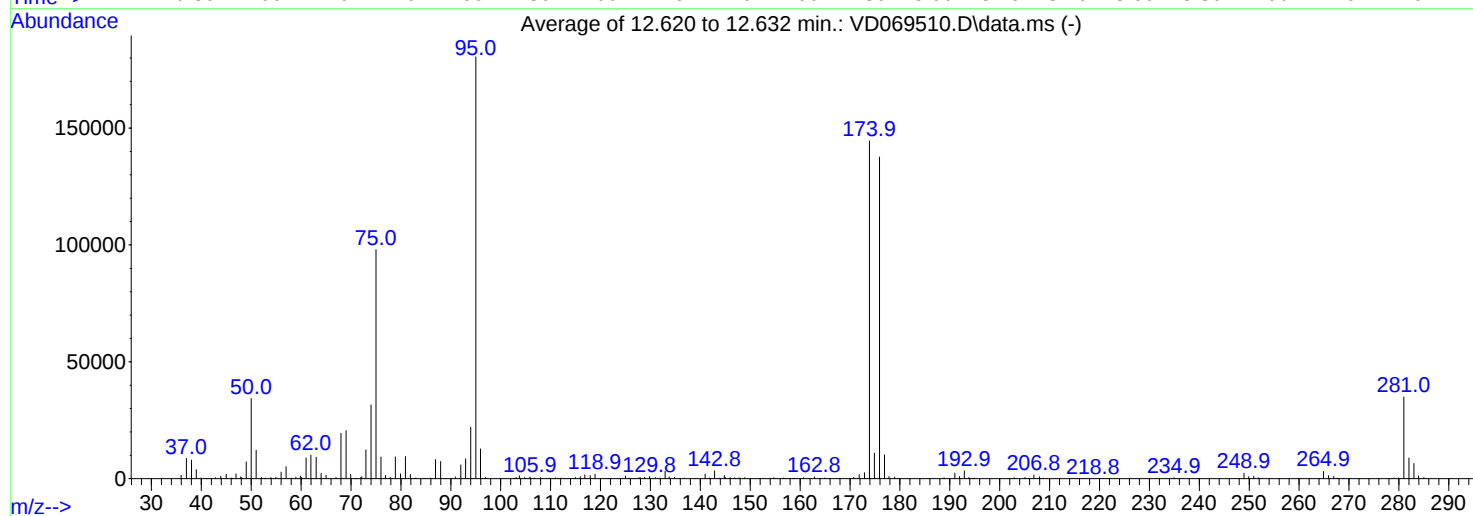


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD062221\
 Data File : VD069510.D
 Acq On : 22 Jun 2021 12:22
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D062121S.M
 Title : SW846 8260
 Last Update : Tue Jun 22 04:33:24 2021

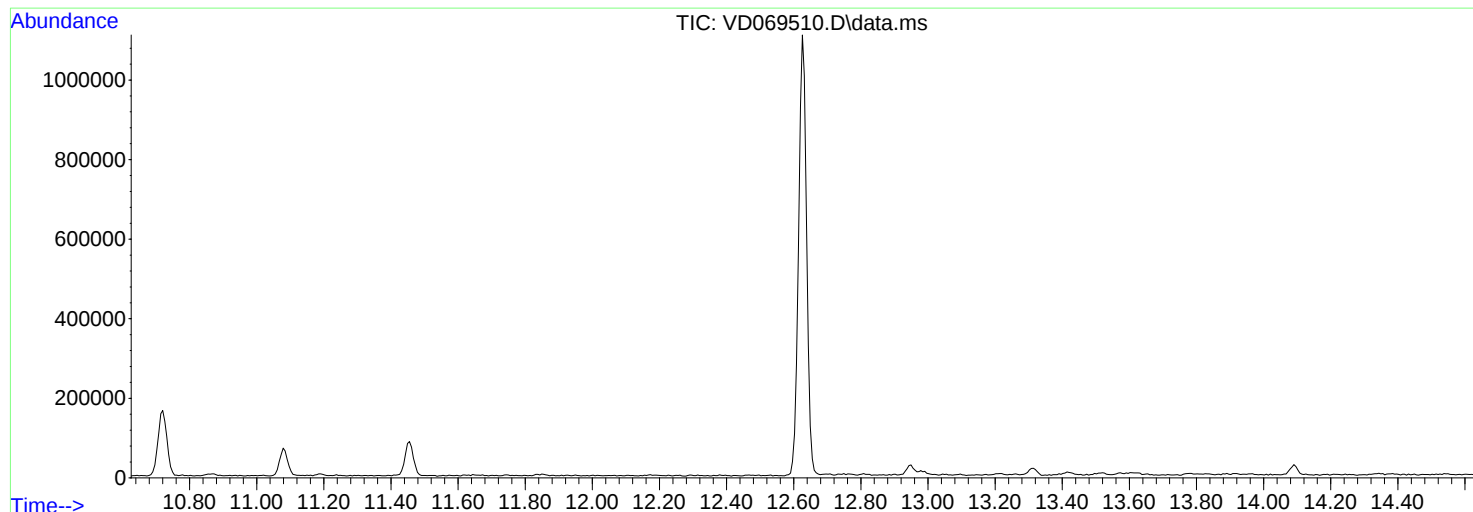

AutoFind: Scans 1819, 1820, 1821; Background Corrected with Scan 1810

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.0	34336	PASS
75	95	30	60	54.3	98011	PASS
95	95	100	100	100.0	180501	PASS
96	95	5	9	7.1	12769	PASS
173	174	0.00	2	1.8	2558	PASS
174	95	50	100	80.1	144565	PASS
175	174	5	9	7.5	10874	PASS
176	174	95	101	95.2	137637	PASS
177	176	5	9	7.4	10234	PASS