

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD062223\
 Data File : VD076530.D
 Acq On : 22 Jun 2023 10:48
 Operator : KP/SY
 Sample : VD0622SBL01
 Misc : 5.00G/5.0ml/MSVOA_D/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 VD0622SBL01

Quant Time: Jun 23 06:34:51 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D061623S.M
 Quant Title : SW846 8260
 QLast Update : Mon Jun 19 04:51:45 2023
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.875	168	123307	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.775	114	224012	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.581	117	203123	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.516	152	91766	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.228	65	66121	53.521	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	= 107.040%	
35) Dibromofluoromethane	7.805	113	68951	51.812	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	= 103.620%	
50) Toluene-d8	10.269	98	243340	48.215	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	= 96.440%	
62) 4-Bromofluorobenzene	12.575	95	77209	47.138	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	= 94.280%	
Target Compounds						
					Qvalue	
16) Acetone	4.016	43	514	1.748	ug/l #	32
20) Methylene Chloride	4.799	84	4110	Below Cal	#	78
25) 2-Butanone	7.052	43	567	1.247	ug/l #	37
28) Bromochloromethane	7.563	49	66	Below Cal	#	1
36) 1,1-Dichloropropene	7.875	75	9452	5.072	ug/l #	48
38) Carbon Tetrachloride	7.875	117	13010	7.811	ug/l #	14
76) 1,2,3-Trichloropropane	12.575	75	40828	44.829	ug/l #	100
81) trans-1,4-Dichloro-2-b...	12.575	75	40828	98.230	ug/l #	17


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD062223\
Data File : VD076530.D
Acq On : 22 Jun 2023 10:48
Operator : KP/SY
Sample : VD0622SBL01
Misc : 5.00G/5.0ml/MSVOA_D/SOIL
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
VD0622SBL01

Quant Time: Jun 23 06:34:51 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D061623S.M
Quant Title : SW846 8260
QLast Update : Mon Jun 19 04:51:45 2023
Response via : Initial Calibration




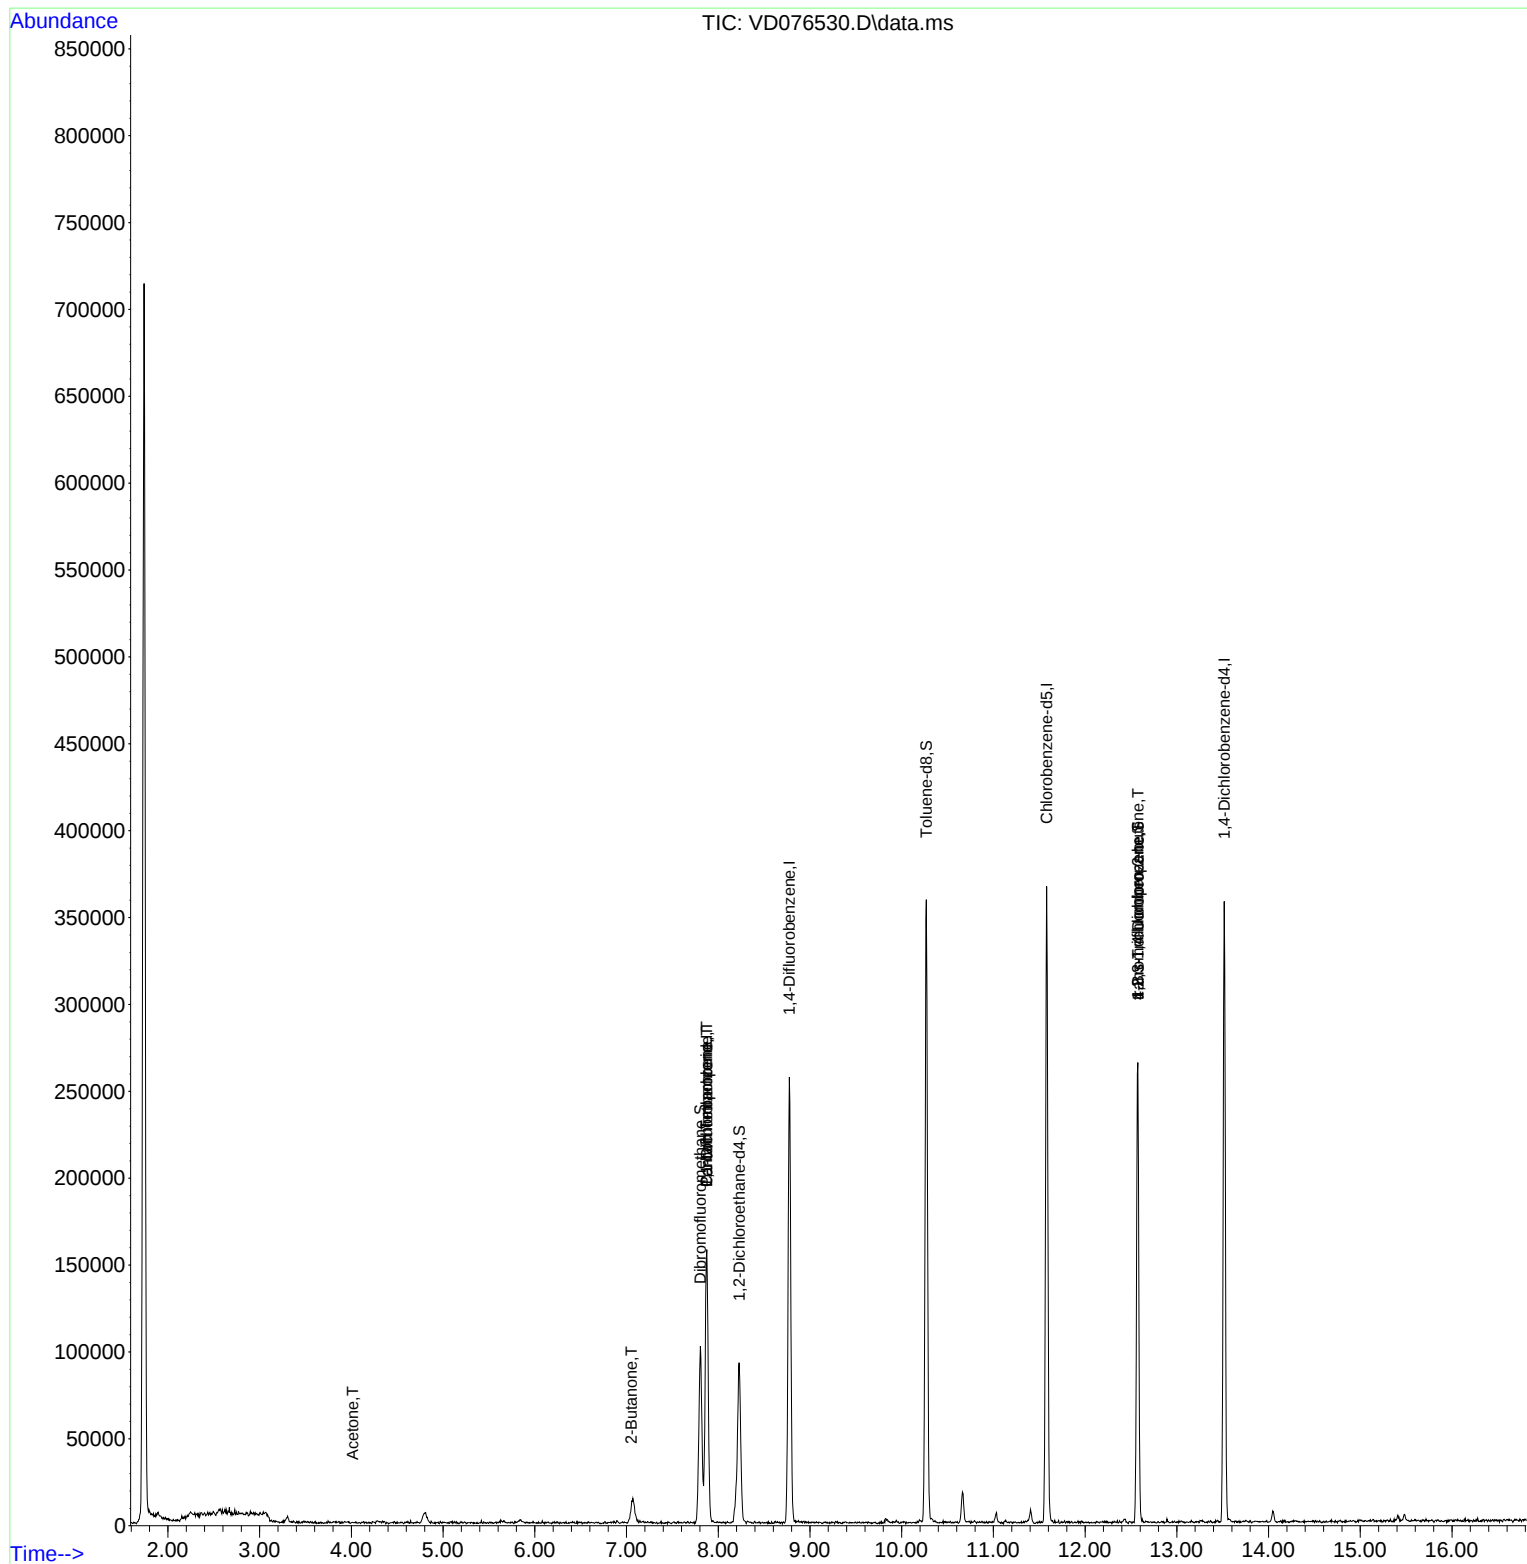


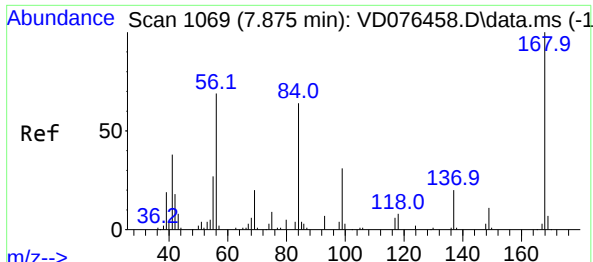

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.875 min Scan# 1069
Delta R.T. 0.000 min
Lab File: VD076530.D
Acq: 22 Jun 2023 10:48




Instrument :
MSVOA_D
ClientSampleId :
VD0622SBL01


Tgt Ion:168 Resp: 123307
Ion Ratio Lower Upper
168 100
99 50.1 36.7 55.1

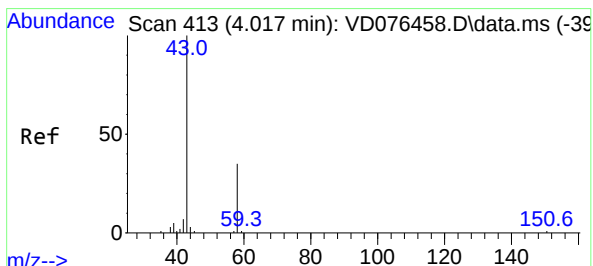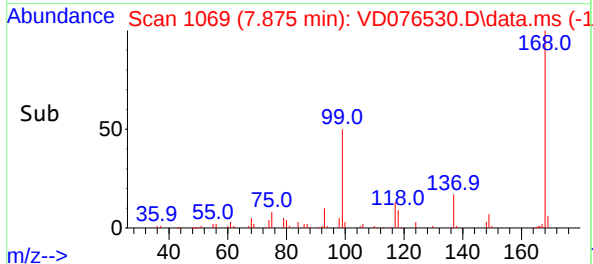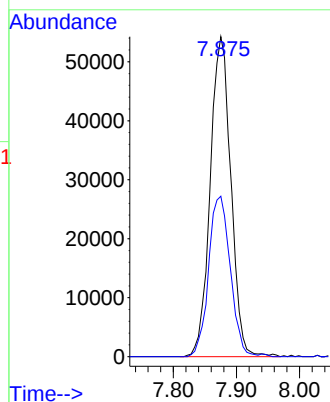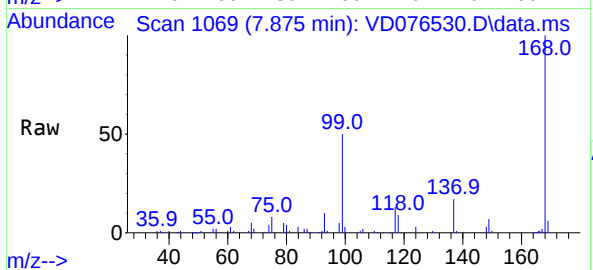

#16
Acetone
Concen: 1.748 ug/l
RT: 4.016 min Scan# 413
Delta R.T. -0.000 min
Lab File: VD076530.D
Acq: 22 Jun 2023 10:48

Tgt Ion: 43 Resp: 514
Ion Ratio Lower Upper
43 100
58 0.0 34.7 52.1#


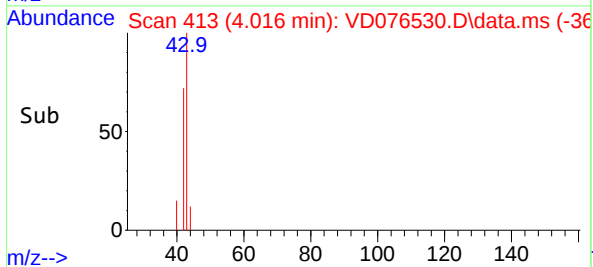
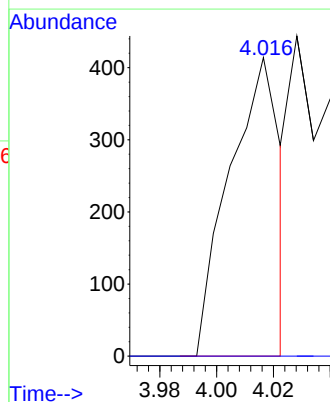
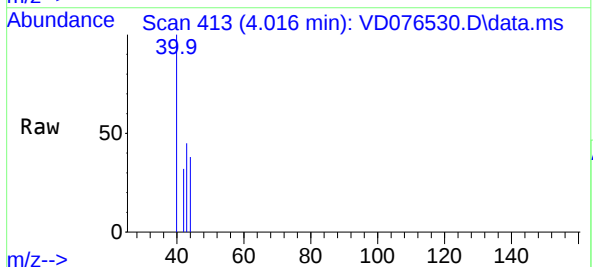


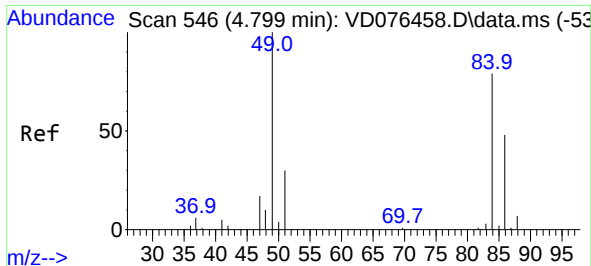

#20
Methylene Chloride
Concen: Below Cal
RT: 4.799 min Scan# 54
Delta R.T. -0.000 min
Lab File: VD076530.D
Acq: 22 Jun 2023 10:48




Instrument :
MSVOA_D
ClientSampleId :
VD0622SBL01


Tgt Ion:	84	Resp:	4110
Ion	Ratio	Lower	Upper
84	100		
49	105.7	71.4	107.2
51	64.4	24.5	36.7#
86	54.0	48.7	73.1

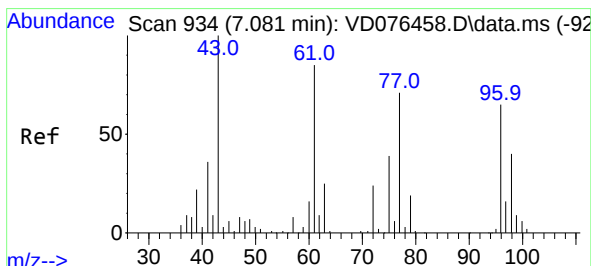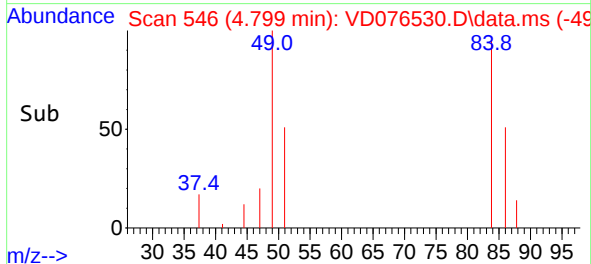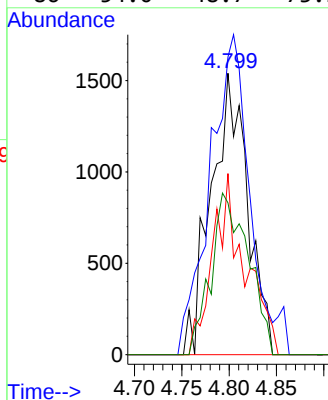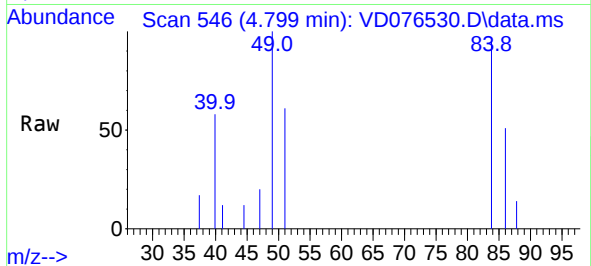

#25
2-Butanone
Concen: 1.247 ug/l
RT: 7.052 min Scan# 929
Delta R.T. -0.029 min
Lab File: VD076530.D
Acq: 22 Jun 2023 10:48

Tgt Ion:	43	Resp:	567
Ion	Ratio	Lower	Upper
43	100		
72	0.0	30.7	46.1#


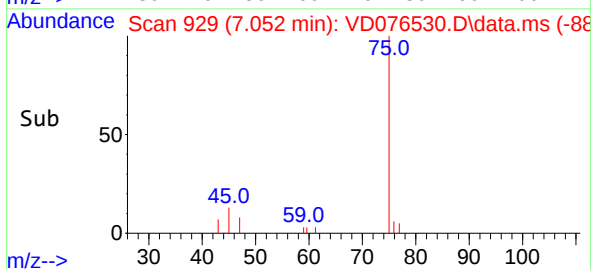
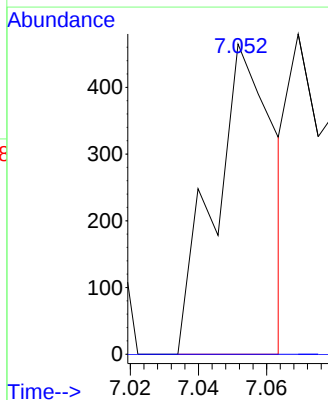
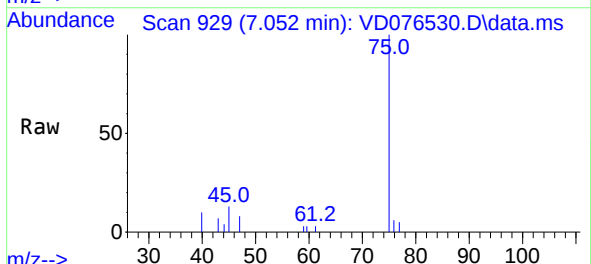


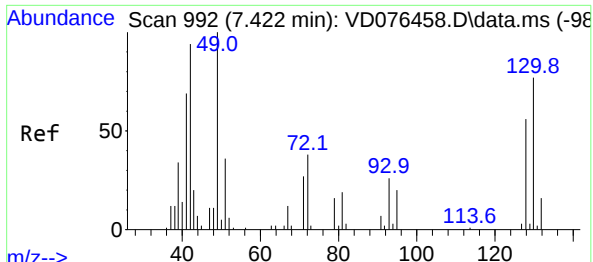

#28
Bromochloromethane
Concen: Below Cal
RT: 7.563 min Scan# 1016
Delta R.T. 0.141 min
Lab File: VD076530.D
Acq: 22 Jun 2023 10:48




Instrument :
MSVOA_D
ClientSampleId :
VD0622SBL01


Tgt Ion: 49 Resp: 66
Ion Ratio Lower Upper
49 100
129 0.0 0.0 6.0
130 0.0 83.2 124.8#

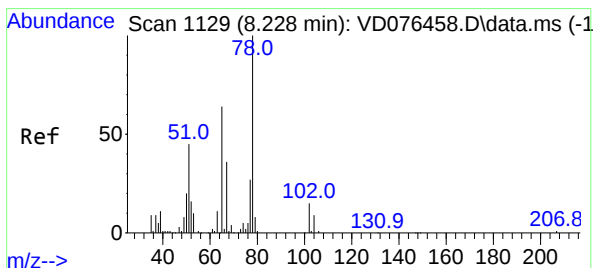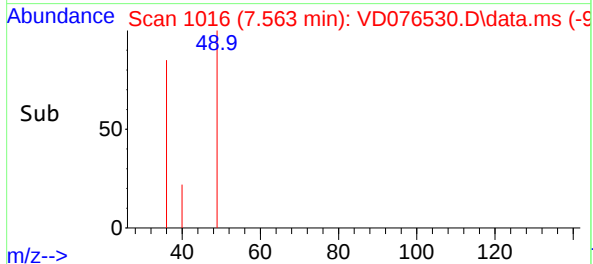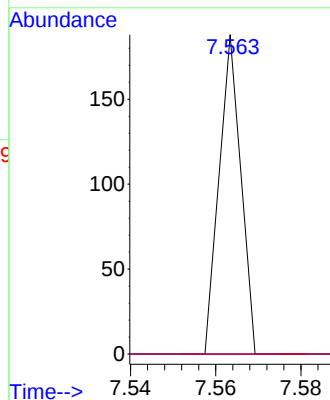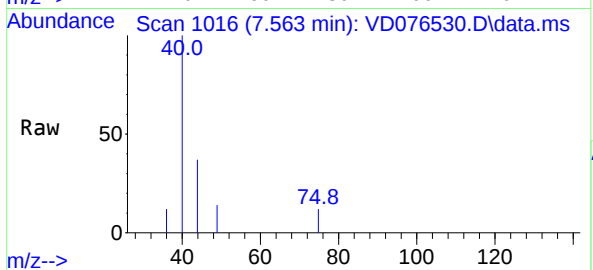

#33
1,2-Dichloroethane-d4
Concen: 53.521 ug/l
RT: 8.228 min Scan# 1129
Delta R.T. -0.000 min
Lab File: VD076530.D
Acq: 22 Jun 2023 10:48

Tgt Ion: 65 Resp: 66121
Ion Ratio Lower Upper
65 100
67 55.1 0.0 115.0

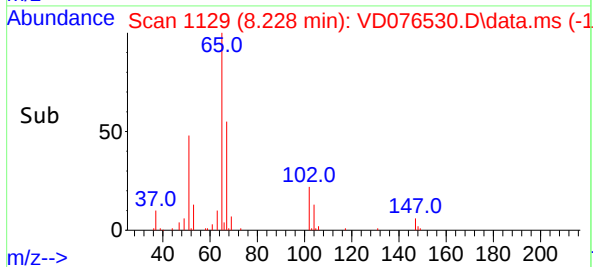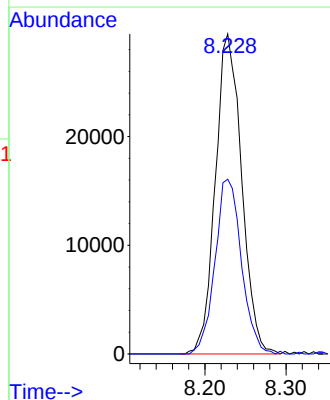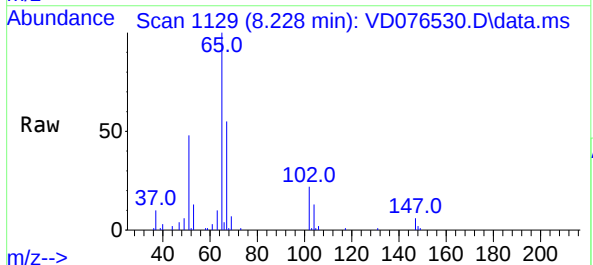

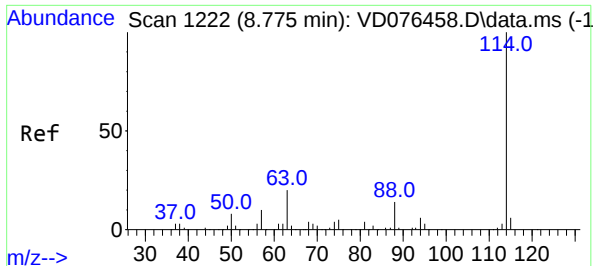

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.775 min Scan# 11

Delta R.T. -0.000 min

Lab File: VD076530.D

Acq: 22 Jun 2023 10:48

Instrument :

MSVOA_D

ClientSampleId :

VD0622SBL01





Tgt Ion:114 Resp: 224012

Ion Ratio Lower Upper

114 100

63 18.4 0.0 33.4

88 13.8 0.0 26.2

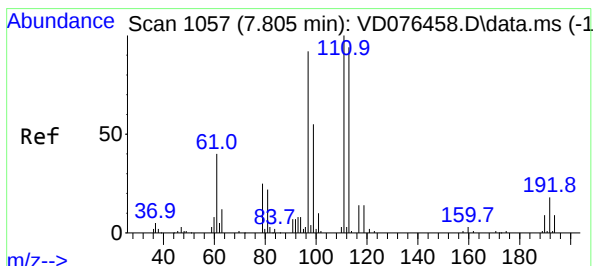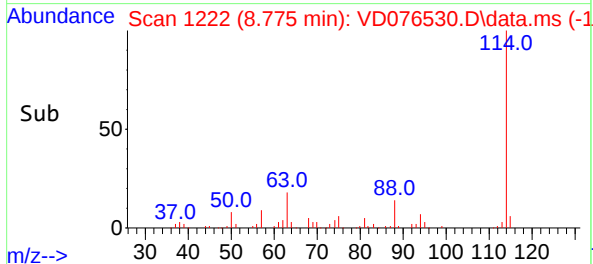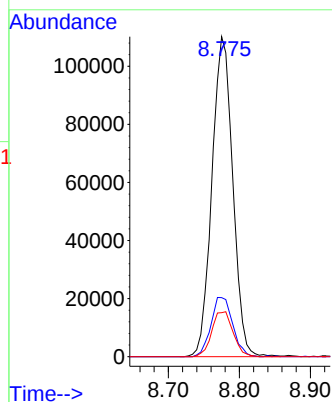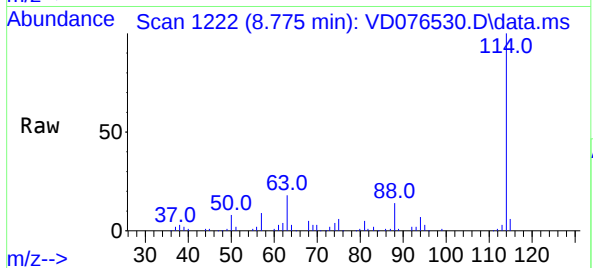

#35

Dibromofluoromethane

Concen: 51.812 ug/l

RT: 7.805 min Scan# 1057

Delta R.T. -0.000 min

Lab File: VD076530.D

Acq: 22 Jun 2023 10:48




Tgt Ion:113 Resp: 68951


Ion Ratio Lower Upper

113 100

111 104.2 84.7 127.1

192 19.8 16.8 25.2


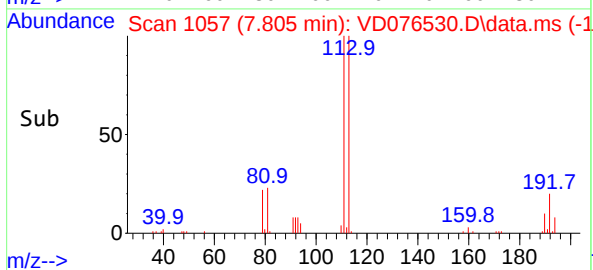
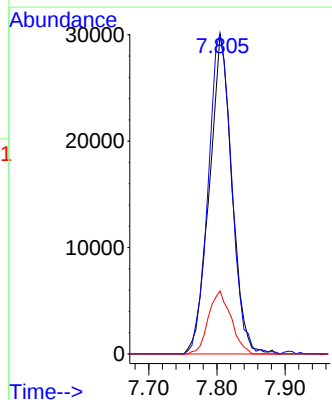
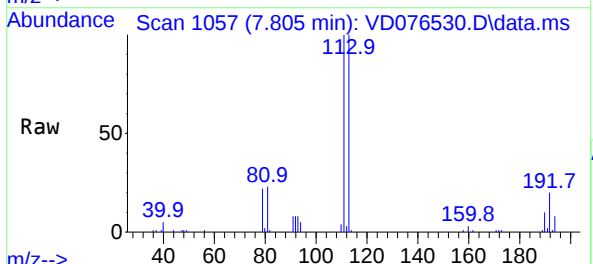


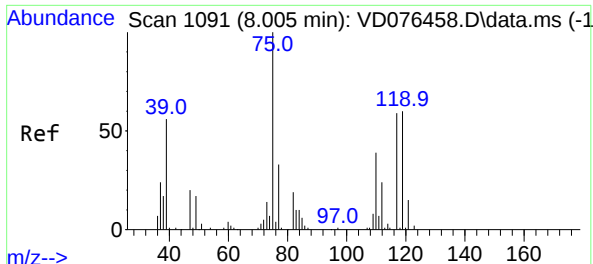

#36
1,1-Dichloropropene
Concen: 5.072 ug/l
RT: 7.875 min Scan# 1069
Delta R.T. -0.129 min
Lab File: VD076530.D
Acq: 22 Jun 2023 10:48




Instrument :
MSVOA_D
ClientSampleId :
VD0622SBL01


Tgt Ion: 75 Resp: 9452
Ion Ratio Lower Upper
75 100
110 9.7 19.9 59.6#
77 0.6 24.7 37.1#

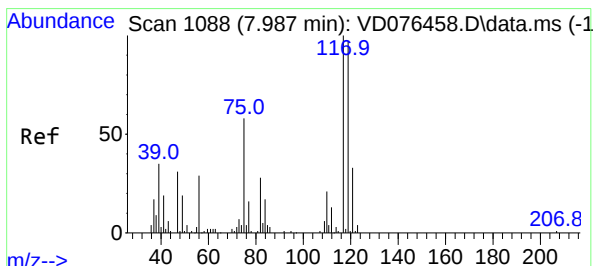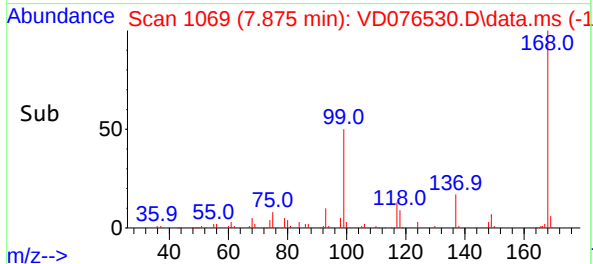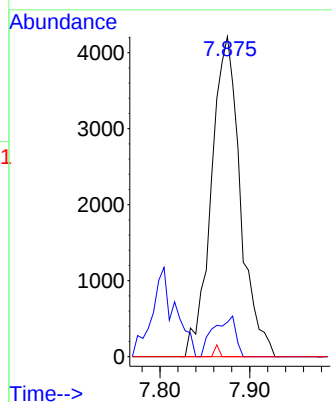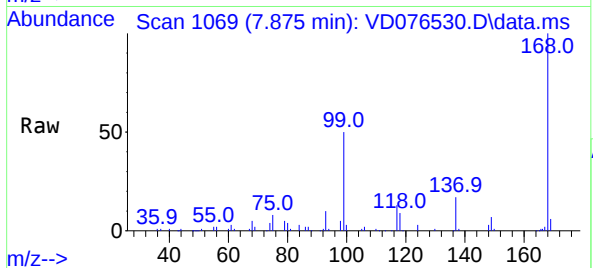

#38
Carbon Tetrachloride
Concen: 7.811 ug/l
RT: 7.875 min Scan# 1069
Delta R.T. -0.112 min
Lab File: VD076530.D
Acq: 22 Jun 2023 10:48

Tgt Ion: 117 Resp: 13010
Ion Ratio Lower Upper
117 100
119 3.9 78.0 117.0#
121 0.0 24.2 36.2#


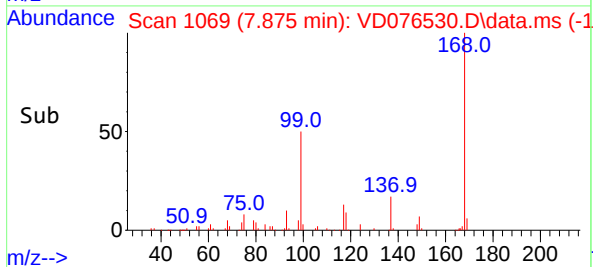
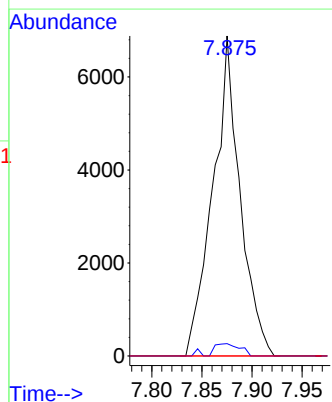
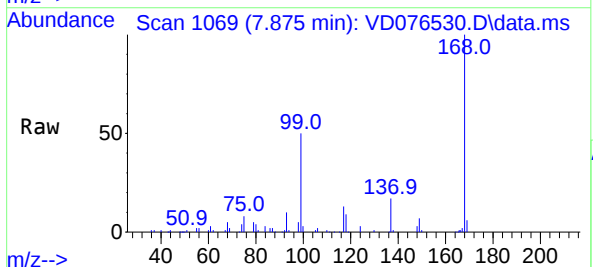


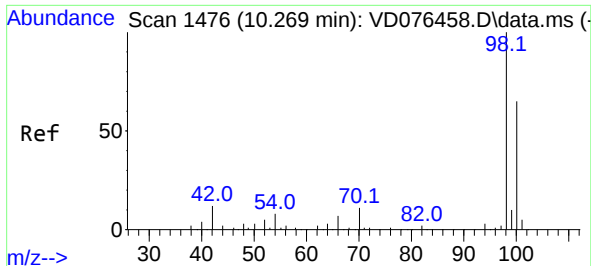

#50
Toluene-d8
Concen: 48.215 ug/l
RT: 10.269 min Scan# 1476
Delta R.T. -0.000 min
Lab File: VD076530.D
Acq: 22 Jun 2023 10:48




Instrument :
MSVOA_D
ClientSampleId :
VD0622SBL01


Tgt Ion: 98 Resp: 243340
Ion Ratio Lower Upper
98 100
100 64.6 50.3 75.5

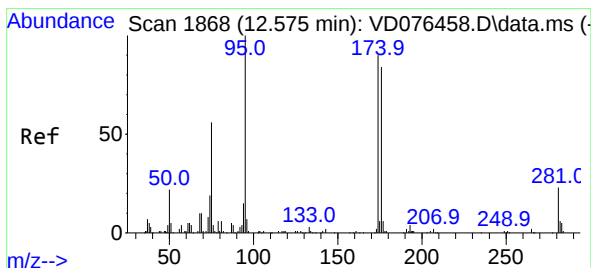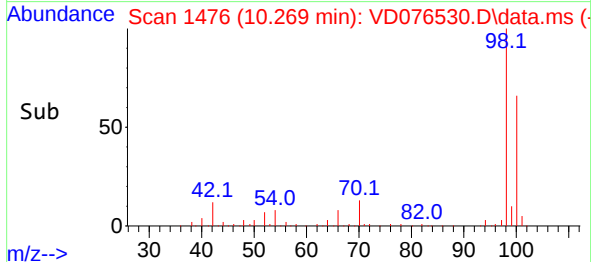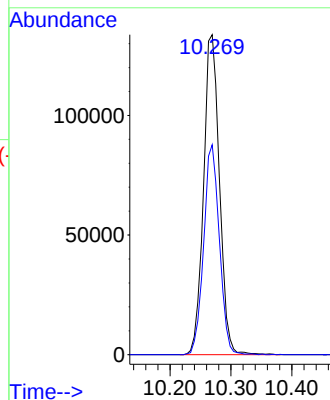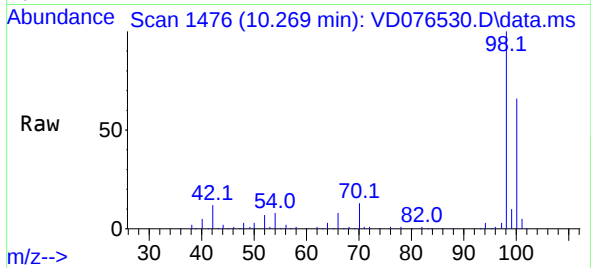

#62
4-Bromofluorobenzene
Concen: 47.138 ug/l
RT: 12.575 min Scan# 1868
Delta R.T. -0.000 min
Lab File: VD076530.D
Acq: 22 Jun 2023 10:48

Tgt Ion: 95 Resp: 77209
Ion Ratio Lower Upper
95 100
174 92.0 0.0 201.8
176 85.7 0.0 191.8


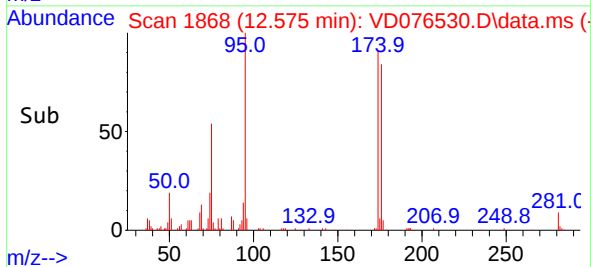
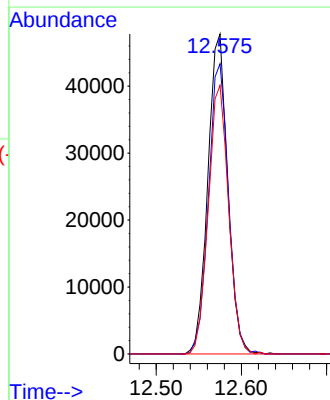
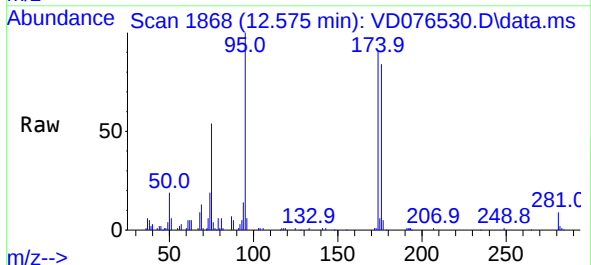


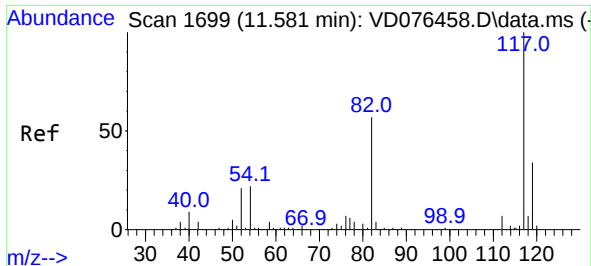

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.581 min Scan# 1699
Delta R.T. -0.000 min
Lab File: VD076530.D
Acq: 22 Jun 2023 10:48




Instrument :
MSVOA_D
ClientSampleId :
VD0622SBL01


Tgt Ion:117 Resp: 203123
Ion Ratio Lower Upper
117 100
82 54.4 38.3 57.5
119 31.9 25.0 37.4

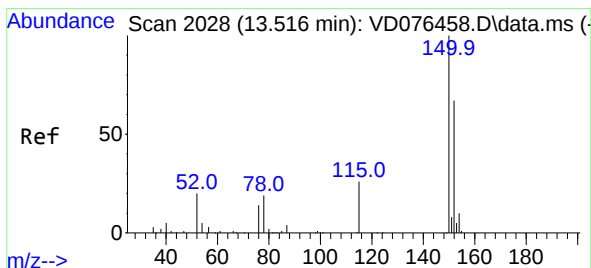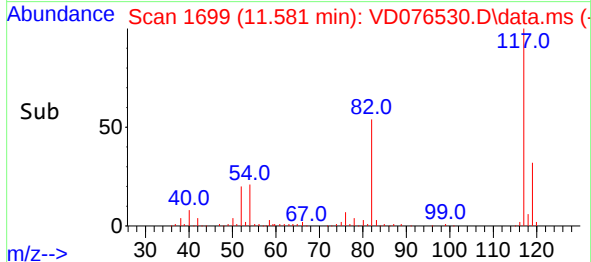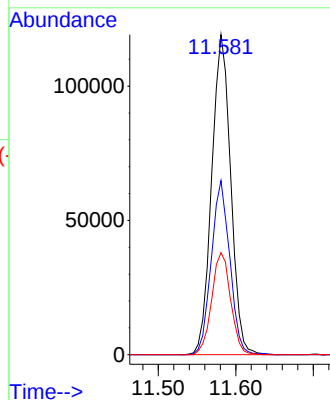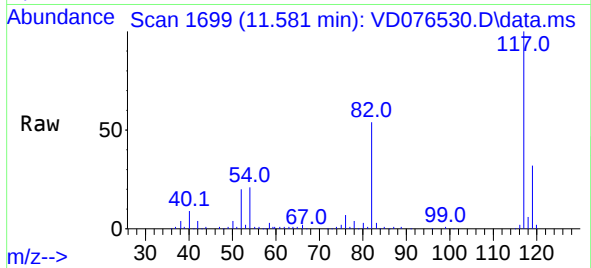

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.516 min Scan# 2028
Delta R.T. -0.000 min
Lab File: VD076530.D
Acq: 22 Jun 2023 10:48

Tgt Ion:152 Resp: 91766
Ion Ratio Lower Upper
152 100
115 57.4 27.1 81.3
150 159.8 0.0 353.6


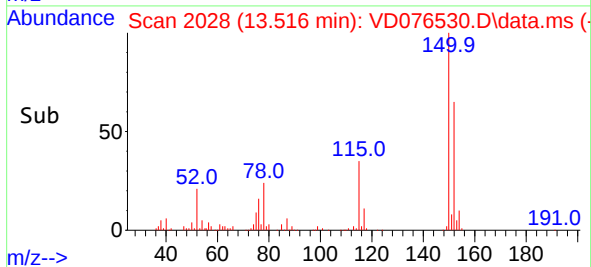
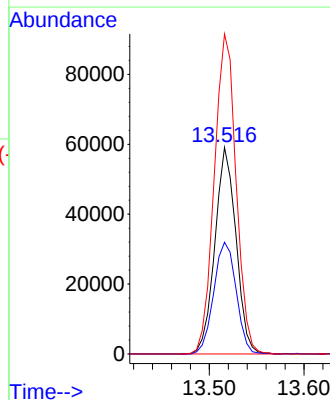
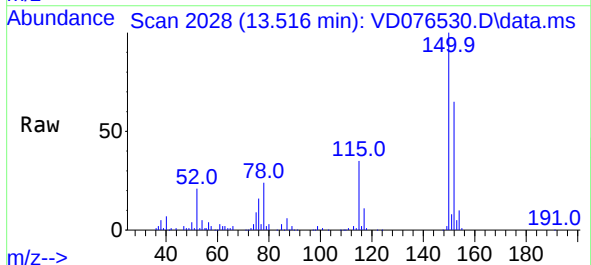


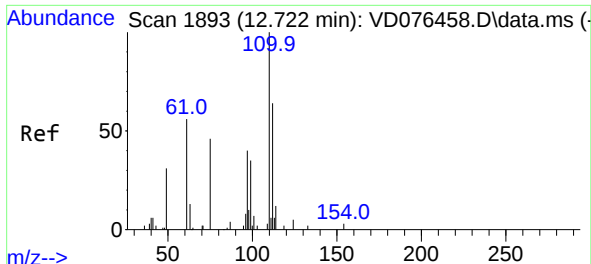

#76
1,2,3-Trichloropropane
Concen: 44.829 ug/l
RT: 12.575 min Scan# 1868
Delta R.T. -0.147 min
Lab File: VD076530.D
Acq: 22 Jun 2023 10:48

Instrument :
MSVOA_D
ClientSampleId :
VD0622SBL01

Tgt Ion: 75 Resp: 40828
Ion Ratio Lower Upper
75 100
77 1.2 0.0 0.0#

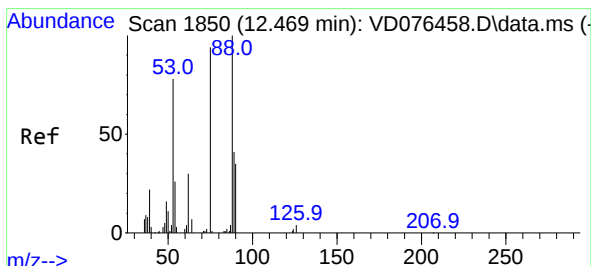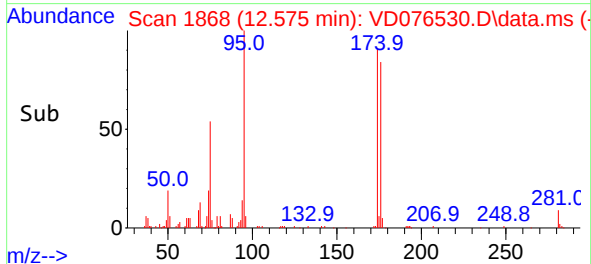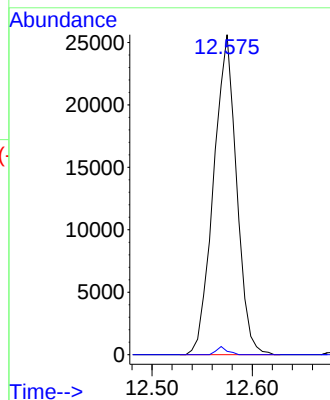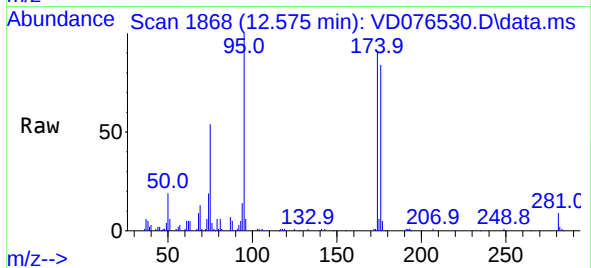

#81
trans-1,4-Dichloro-2-butene
Concen: 98.230 ug/l
RT: 12.575 min Scan# 1868
Delta R.T. 0.106 min
Lab File: VD076530.D
Acq: 22 Jun 2023 10:48

Tgt Ion: 75 Resp: 40828
Ion Ratio Lower Upper
75 100
53 0.0 63.0 94.4#
89 0.0 37.9 56.9#

