

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD062223\
 Data File : VD076533.D
 Acq On : 22 Jun 2023 12:17
 Operator : KP/SY
 Sample : 03289-16RE
 Misc : 5.09G/5.0ml/MSVOA_D/SOIL
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 SB-06-12.0-14.0RE

Quant Time: Jun 22 13:44:51 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D061623S.M
 Quant Title : SW846 8260
 QLast Update : Mon Jun 19 04:51:45 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.875	168	58411	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.775	114	108285	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.581	117	106701	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.516	152	52923	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.228	65	140681	240.386	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	480.780%#
35) Dibromofluoromethane	7.805	113	124265	193.172	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	386.340%#
50) Toluene-d8	10.269	98	452463	185.463	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	370.920%#
62) 4-Bromofluorobenzene	12.575	95	152677	192.831	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	385.660%#


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD062223\
Data File : VD076533.D
Acq On : 22 Jun 2023 12:17
Operator : KP/SY
Sample : 03289-16RE
Misc : 5.09G/5.0ml/MSVOA_D/SOIL
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
SB-06-12.0-14.0RE


Quant Time: Jun 22 13:44:51 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D061623S.M
Quant Title : SW846 8260
QLast Update : Mon Jun 19 04:51:45 2023
Response via : Initial Calibration

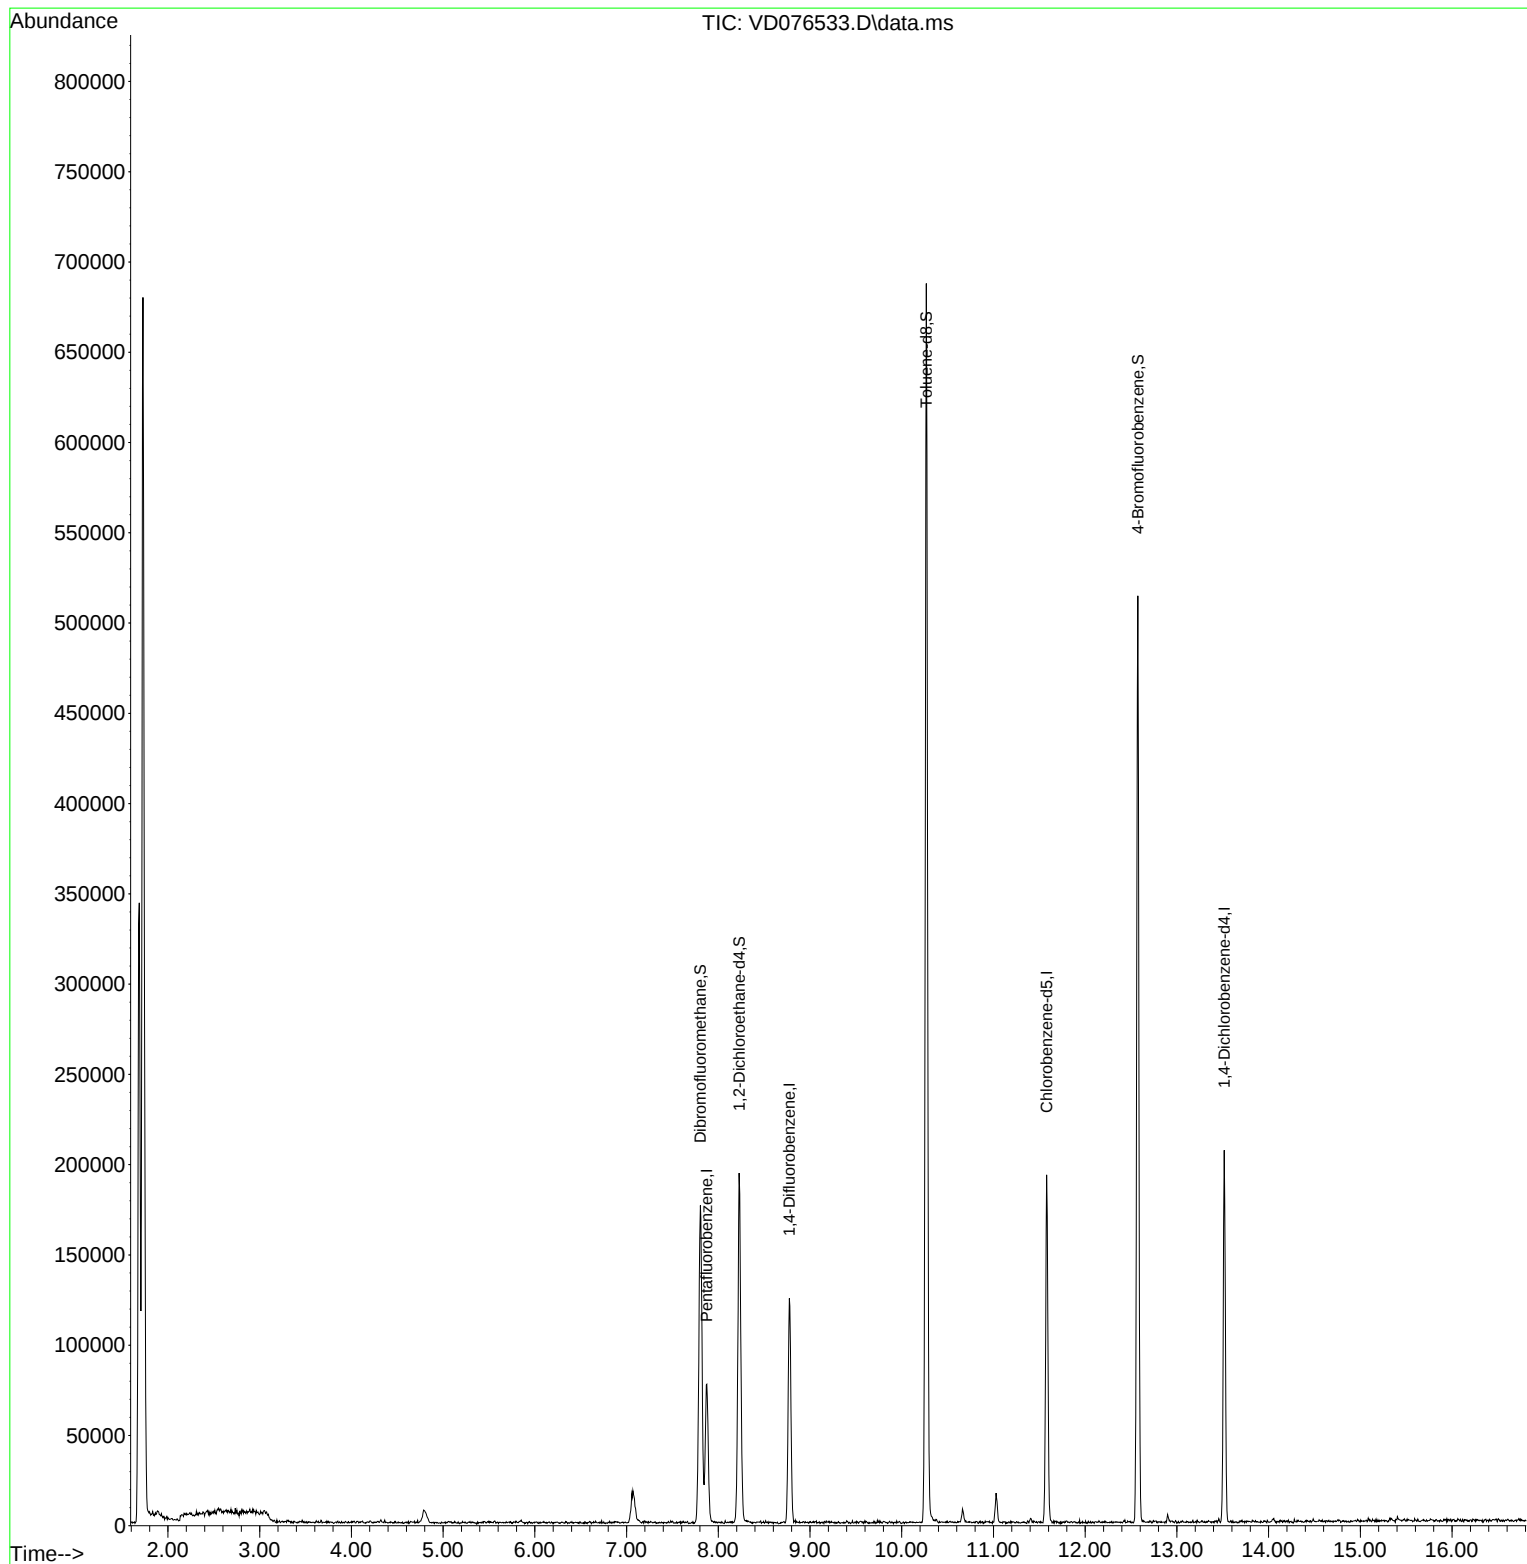



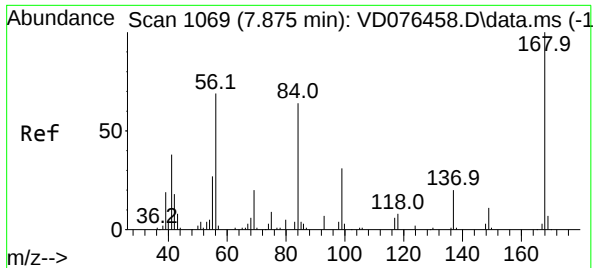


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.875 min Scan# 1069
Delta R.T. 0.000 min
Lab File: VD076533.D
Acq: 22 Jun 2023 12:17

Instrument :
MSVOA_D
ClientSampleId :
SB-06-12.0-14.0RE



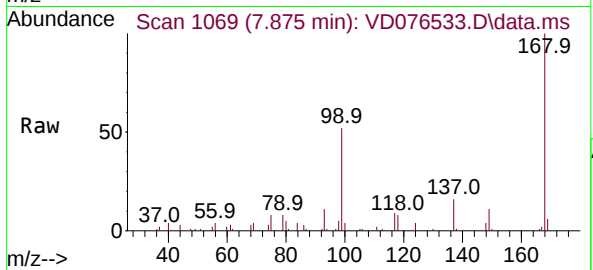



Tgt Ion:168 Resp: 58411
Ion Ratio Lower Upper
168 100
99 51.6 36.7 55.1

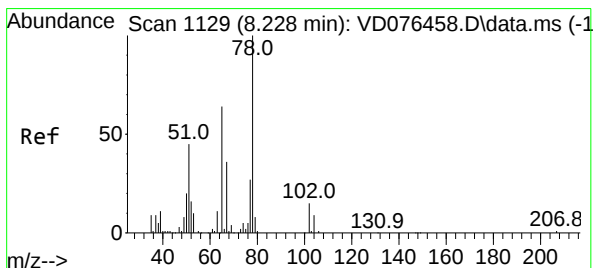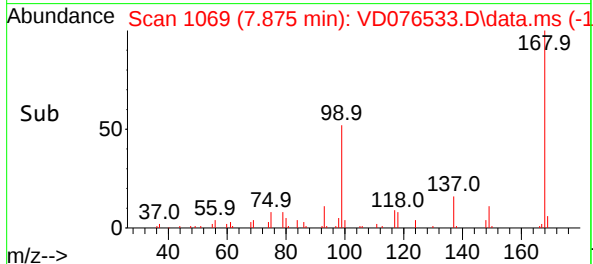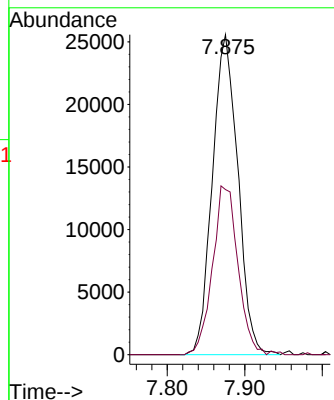

#33
1,2-Dichloroethane-d4
Concen: 240.386 ug/l
RT: 8.228 min Scan# 1129
Delta R.T. -0.000 min
Lab File: VD076533.D
Acq: 22 Jun 2023 12:17

Tgt Ion: 65 Resp: 140681
Ion Ratio Lower Upper
65 100
67 52.4 0.0 115.0

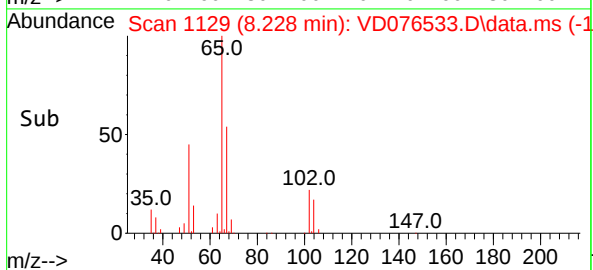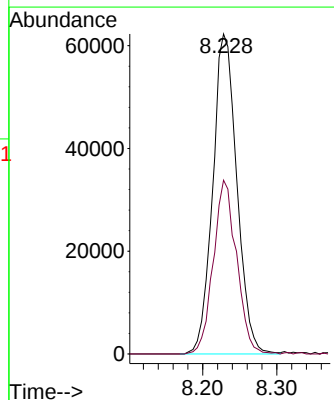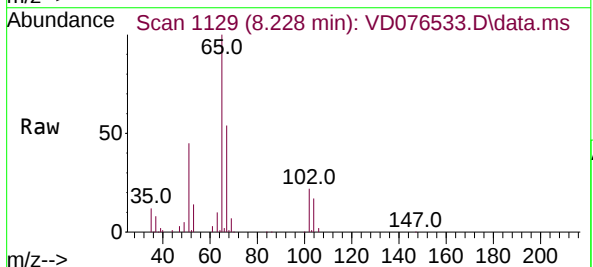

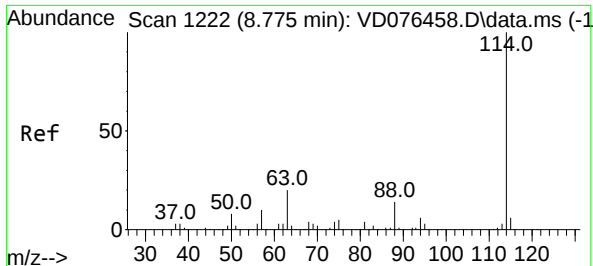

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.775 min Scan# 1

Delta R.T. -0.000 min

Lab File: VD076533.D

Acq: 22 Jun 2023 12:17

Instrument :

MSVOA_D

ClientSampleId :

SB-06-12.0-14.0RE





Tgt Ion:114 Resp: 108285

Ion Ratio Lower Upper

114 100

63 21.2 0.0 33.4

88 16.2 0.0 26.2

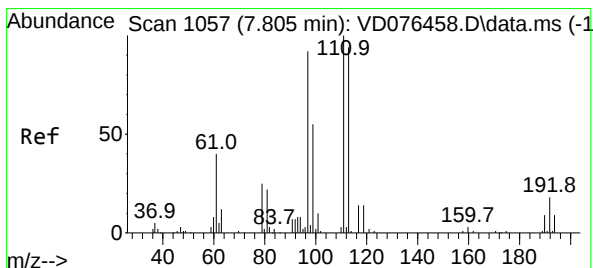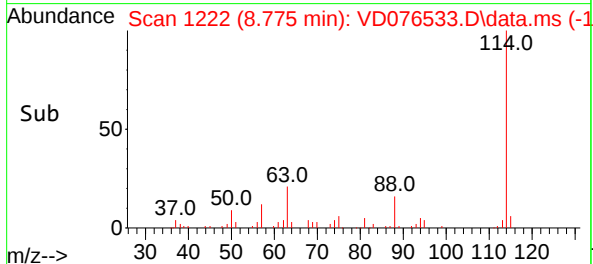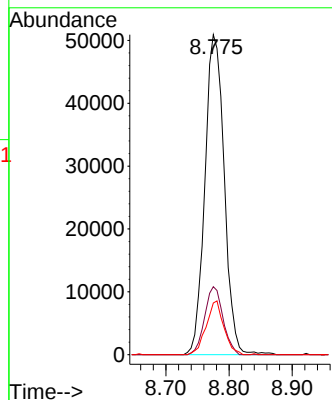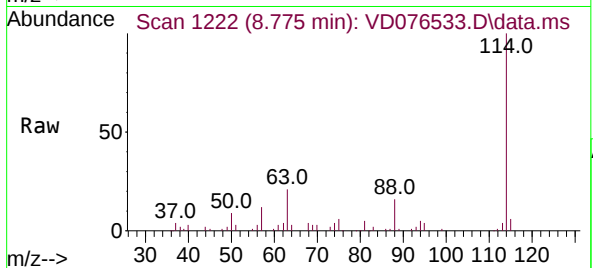

#35

Dibromofluoromethane

Concen: 193.172 ug/l

RT: 7.805 min Scan# 1057

Delta R.T. -0.000 min

Lab File: VD076533.D

Acq: 22 Jun 2023 12:17




Tgt Ion:113 Resp: 124265


Ion Ratio Lower Upper

113 100

111 104.3 84.7 127.1

192 20.8 16.8 25.2

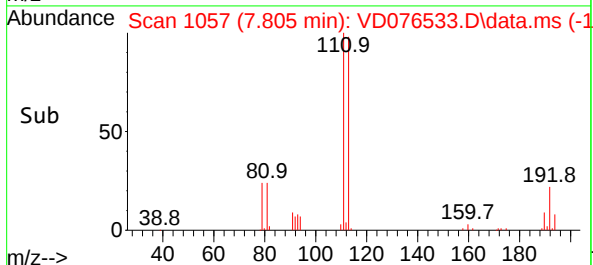
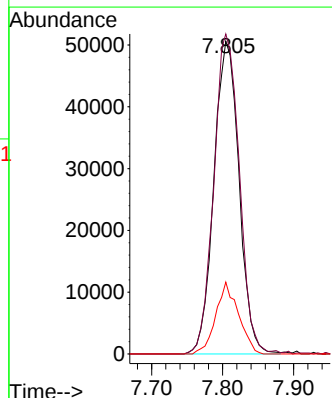
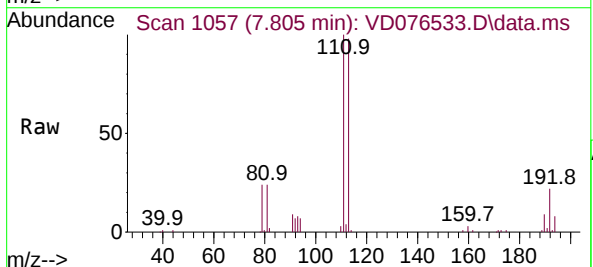


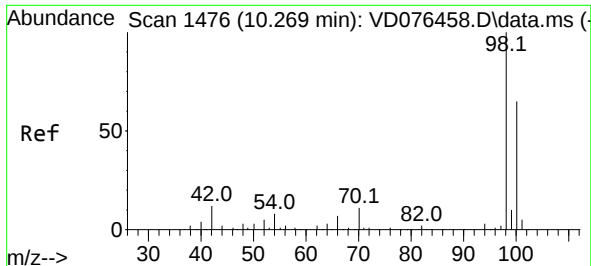

#50
Toluene-d8
Concen: 185.463 ug/l
RT: 10.269 min Scan# 1476
Delta R.T. -0.000 min
Lab File: VD076533.D
Acq: 22 Jun 2023 12:17




Instrument :
MSVOA_D
ClientSampleId :
SB-06-12.0-14.0RE


Tgt Ion: 98 Resp: 452463
Ion Ratio Lower Upper
98 100
100 64.3 50.3 75.5

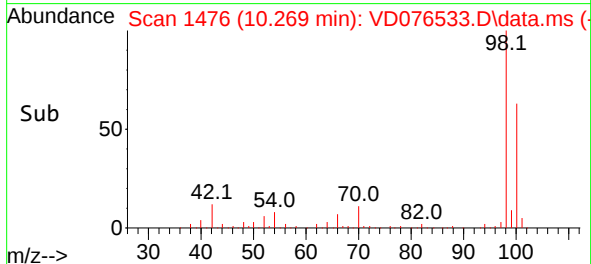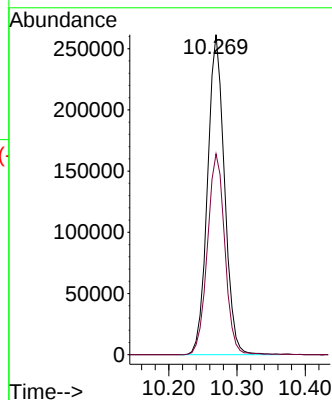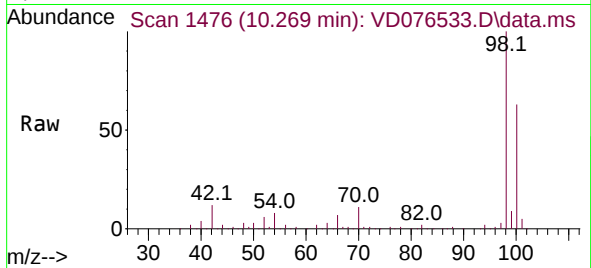

#62
4-Bromofluorobenzene
Concen: 192.831 ug/l
RT: 12.575 min Scan# 1868
Delta R.T. -0.000 min
Lab File: VD076533.D
Acq: 22 Jun 2023 12:17

Tgt Ion: 95 Resp: 152677
Ion Ratio Lower Upper
95 100
174 86.9 0.0 201.8
176 83.8 0.0 191.8


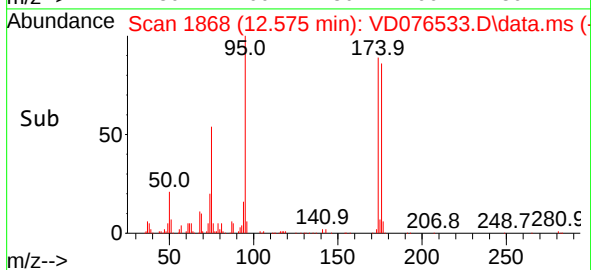
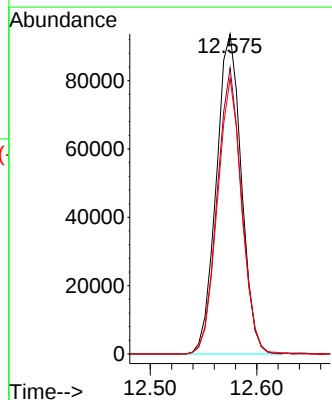
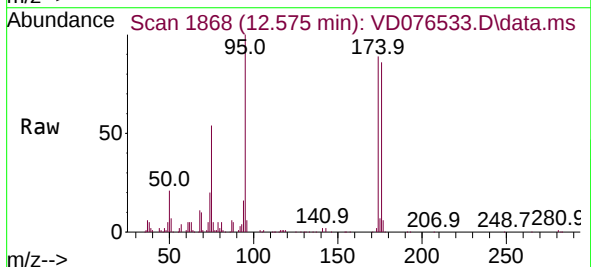


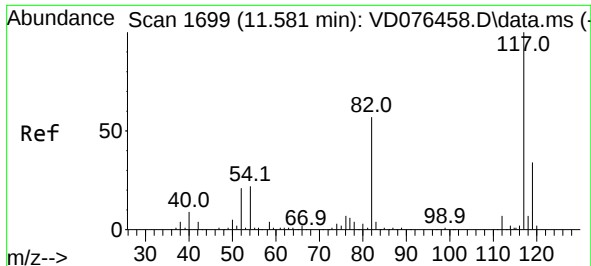

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.581 min Scan# 1
Delta R.T. -0.000 min
Lab File: VD076533.D
Acq: 22 Jun 2023 12:17

Instrument :
MSVOA_D
ClientSampleId :
SB-06-12.0-14.0RE

Tgt Ion:117 Resp: 106701
Ion Ratio Lower Upper
117 100
82 46.9 38.3 57.5
119 31.1 25.0 37.4

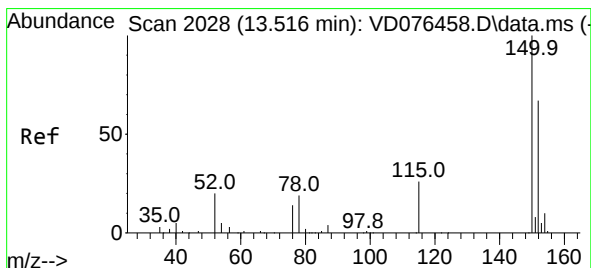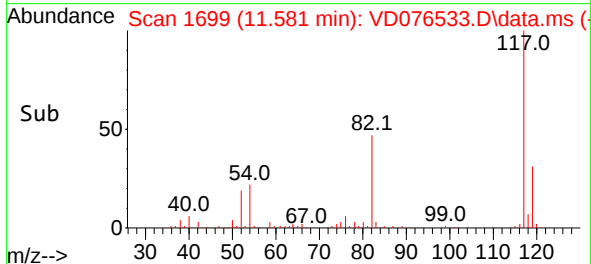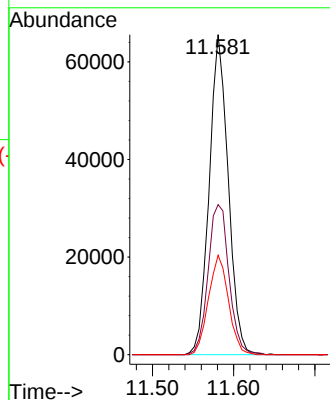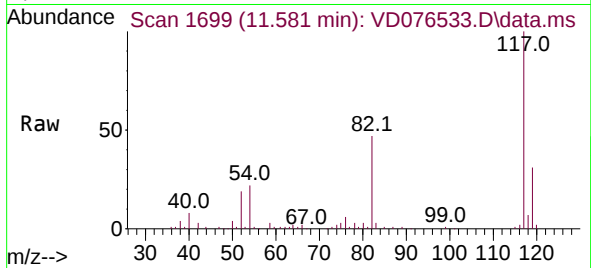

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.516 min Scan# 2028
Delta R.T. -0.000 min
Lab File: VD076533.D
Acq: 22 Jun 2023 12:17

Tgt Ion:152 Resp: 52923
Ion Ratio Lower Upper
152 100
115 55.6 27.1 81.3
150 152.7 0.0 353.6

