

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD062223\
 Data File : VD076534.D
 Acq On : 22 Jun 2023 12:46
 Operator : KP/SY
 Sample : 03355-03RE
 Misc : 5.09G/5.0ml/MSVOA_D/SOIL
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 SB-02-6.5-7.0RE

Quant Time: Jun 23 06:35:36 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D061623S.M
 Quant Title : SW846 8260
 QLast Update : Mon Jun 19 04:51:45 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	0.000	168	0	0.000	ug/l	-7.88
34) 1,4-Difluorobenzene	0.000	114	0	0.000	ug/l	-8.78
63) Chlorobenzene-d5	0.000	117	0	0.000	ug/l	-11.58
72) 1,4-Dichlorobenzene-d4	0.000	152	0	0.000	ug/l	-13.52
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.310	65	62	0.000	ug/l	0.08
Spiked Amount	50.000	Range	50 - 163	Recovery	=	0.000%#
35) Dibromofluoromethane	0.000	113	0	0.000	ug/l	
Spiked Amount	50.000	Range	54 - 147	Recovery	=	0.000%#
50) Toluene-d8	0.000	98	0	0.000	ug/l	
Spiked Amount	50.000	Range	58 - 134	Recovery	=	0.000%#
62) 4-Bromofluorobenzene	0.000	95	0	0.000	ug/l	
Spiked Amount	50.000	Range	30 - 143	Recovery	=	0.000%#


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD062223\
Data File : VD076534.D
Acq On : 22 Jun 2023 12:46
Operator : KP/SY
Sample : 03355-03RE
Misc : 5.09G/5.0ml/MSVOA_D/SOIL
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
SB-02-6.5-7.0RE

Quant Time: Jun 23 06:35:36 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D061623S.M
Quant Title : SW846 8260
QLast Update : Mon Jun 19 04:51:45 2023
Response via : Initial Calibration

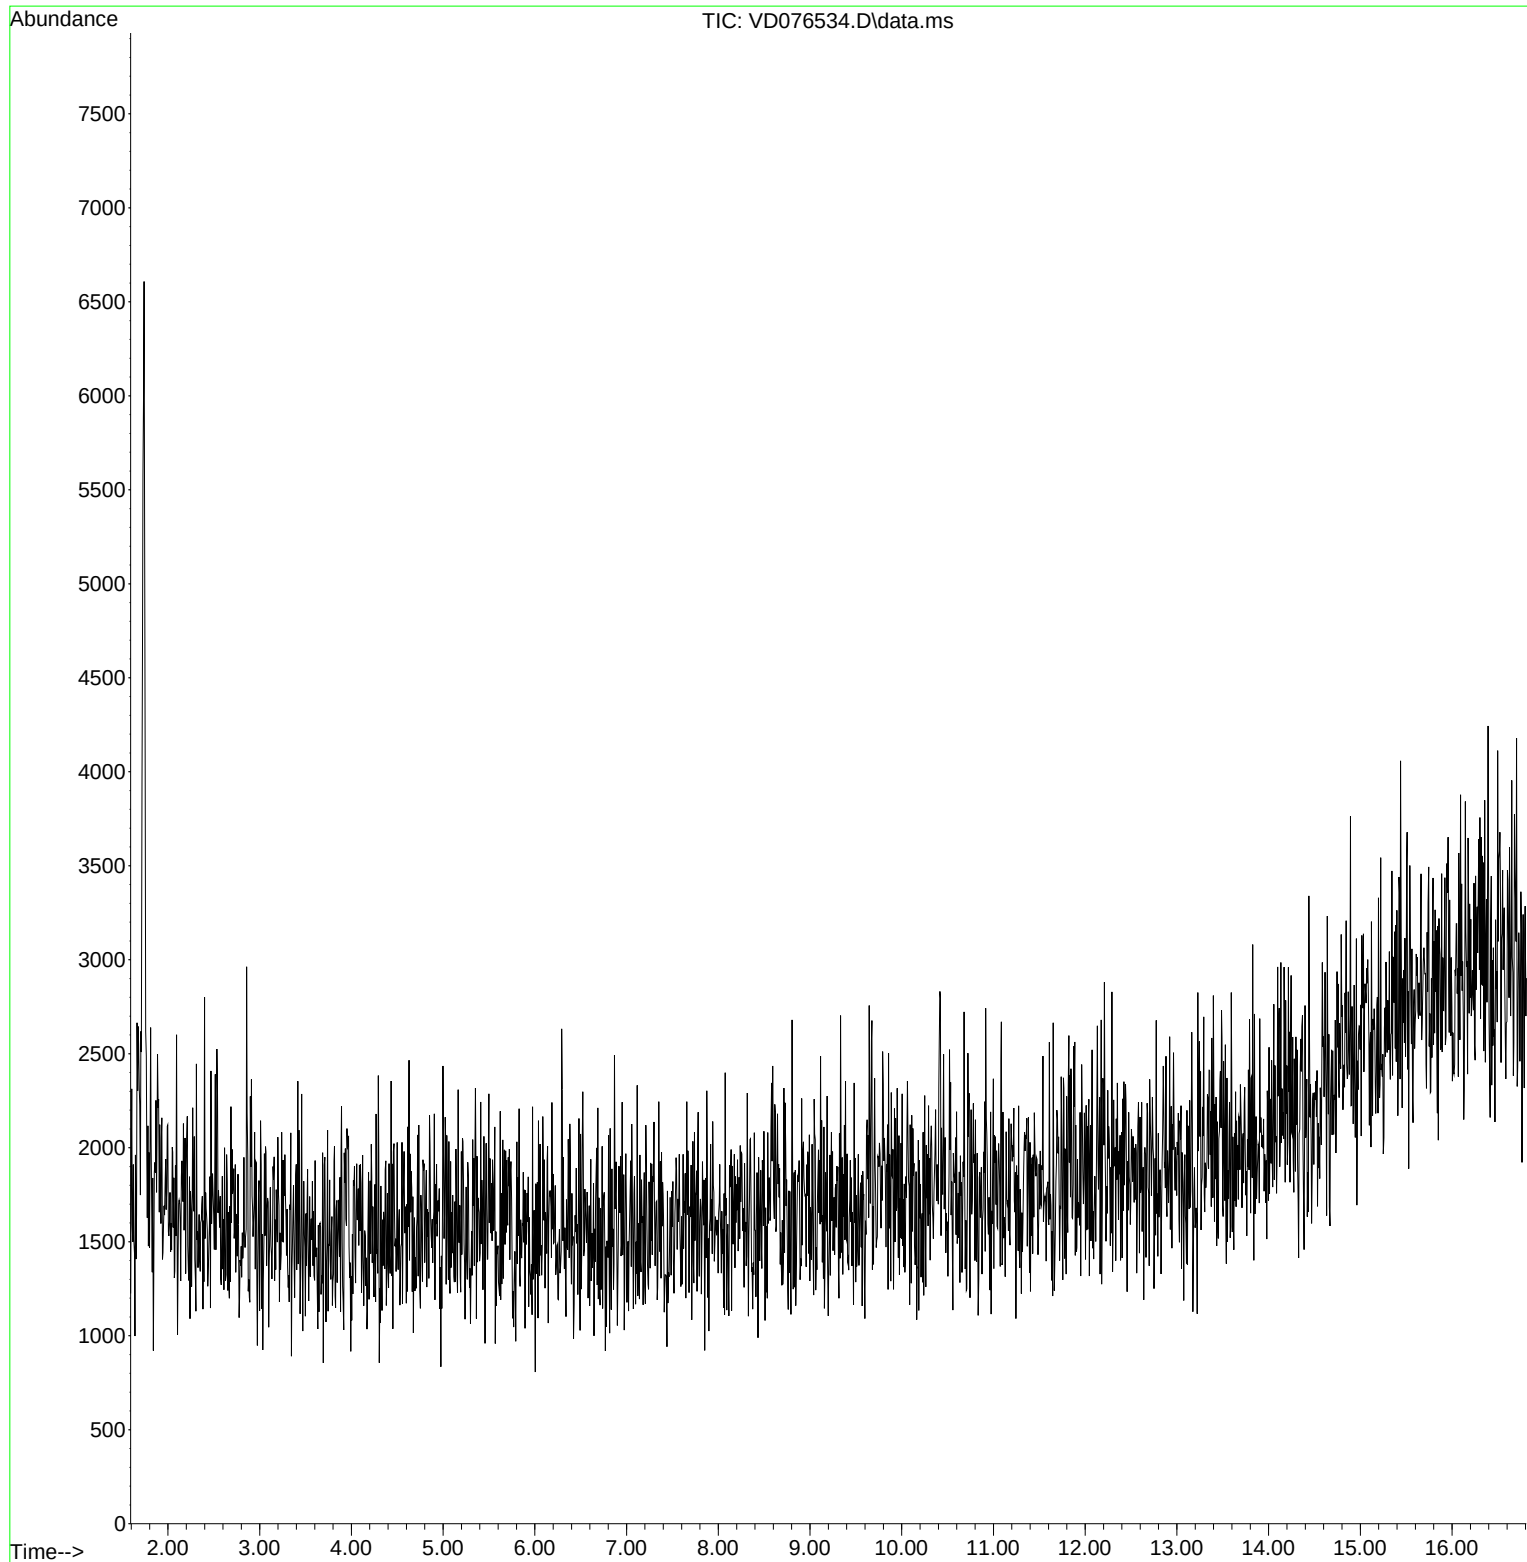


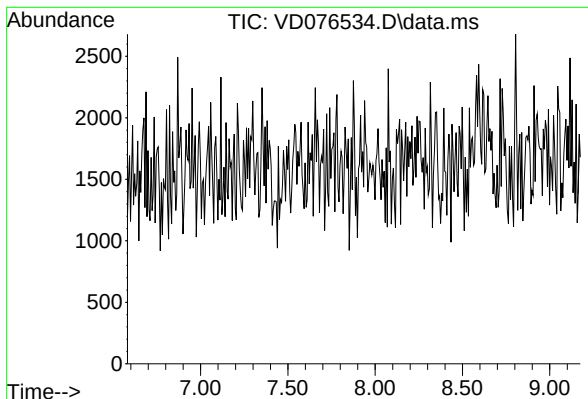


#1
Pentafluorobenzene
Concen: 0.000 ug/l
Expected RT: 7.88 min

Lab File: VD076534.D
Acq: 22 Jun 2023 12:46




Instrument :
MSVOA_D
ClientSampleId :
SB-02-6.5-7.0RE


Tgt Ion: 168
Sig Exp Ratio
168 100
99 45.9

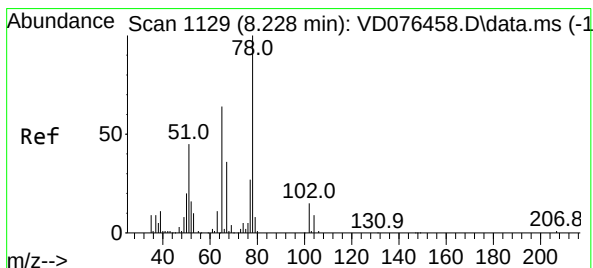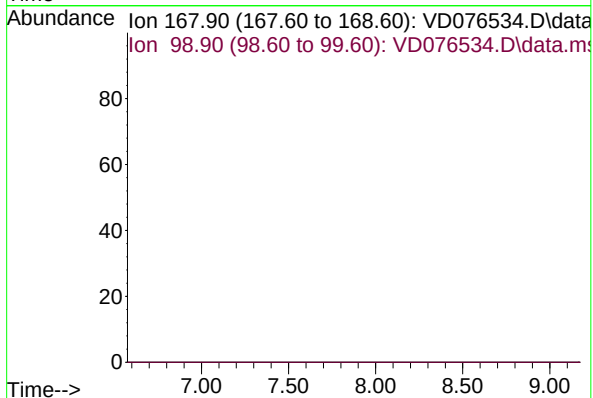

#33
1,2-Dichloroethane-d4
Concen: 0.000 ug/l
RT: 8.310 min Scan# 1143
Delta R.T. 0.082 min
Lab File: VD076534.D
Acq: 22 Jun 2023 12:46

Tgt Ion: 65 Resp: 62
Ion Ratio Lower Upper
65 100
67 0.0 0.0 115.0

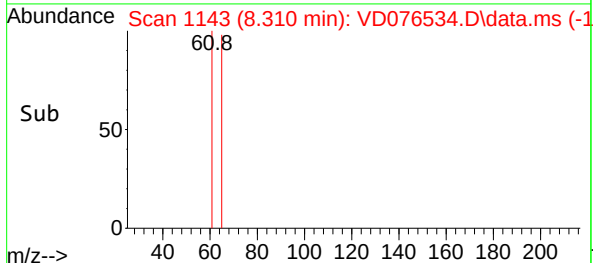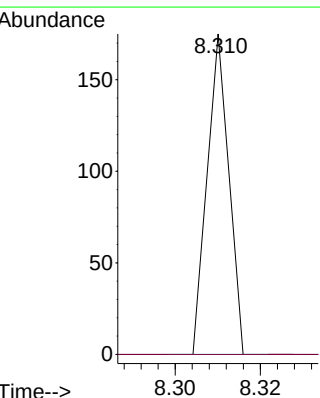
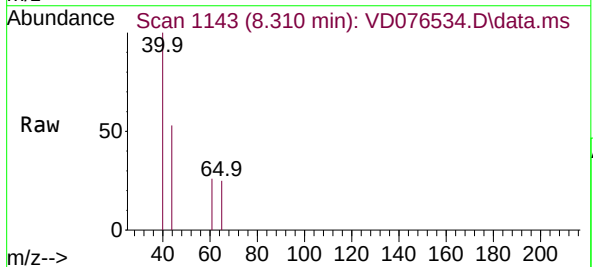


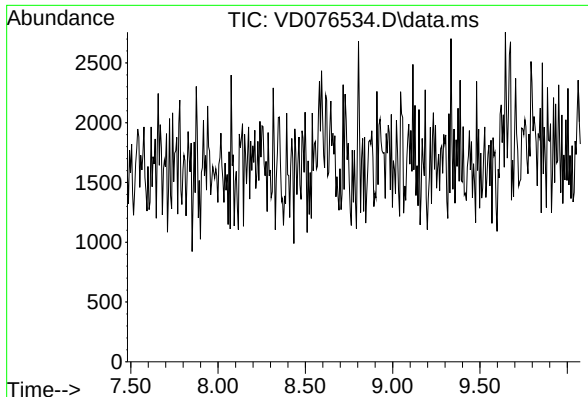

#34
 1,4-Difluorobenzene
 Concen: 0.000 ug/l
 Expected RT: 8.78 min
 Lab File: VD076534.D
 Acq: 22 Jun 2023 12:46


Instrument :
 MSVOA_D
 ClientSampleId :
 SB-02-6.5-7.0RE


Tgt Ion: 114
 Sig Exp Ratio
 114 100
 63 16.7
 88 13.1

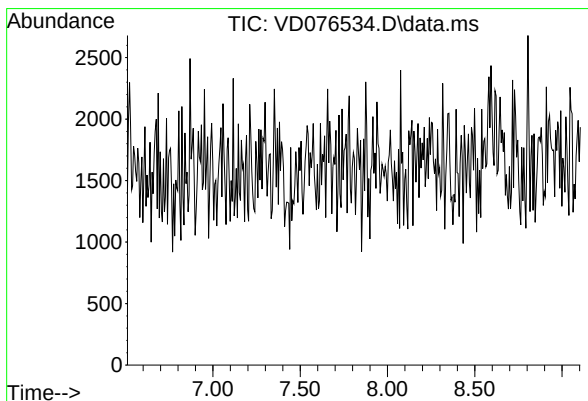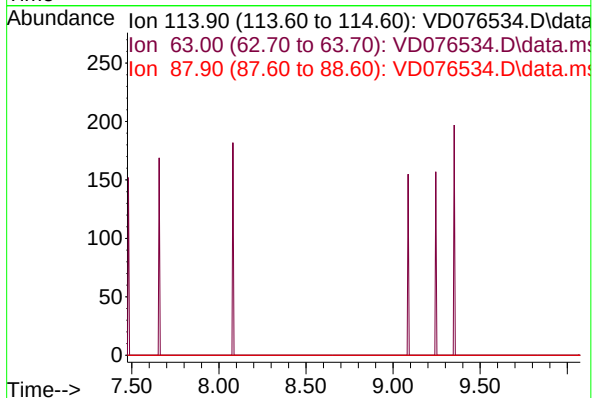

#35
 Dibromofluoromethane
 Concen: 0.000 ug/l
 Expected RT: 7.80 min
 Lab File: VD076534.D
 Acq: 22 Jun 2023 12:46

Tgt Ion: 113
 Sig Exp Ratio
 113 100
 111 105.9
 192 21.0


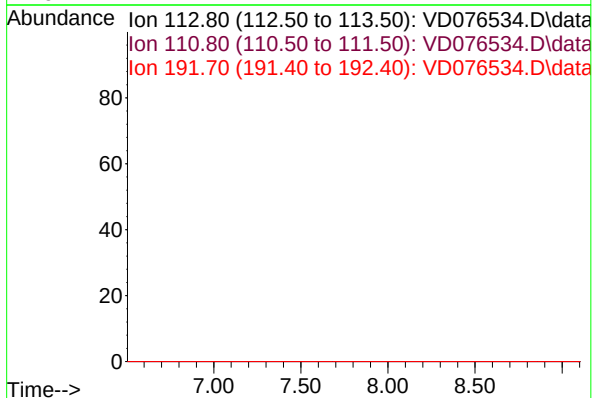


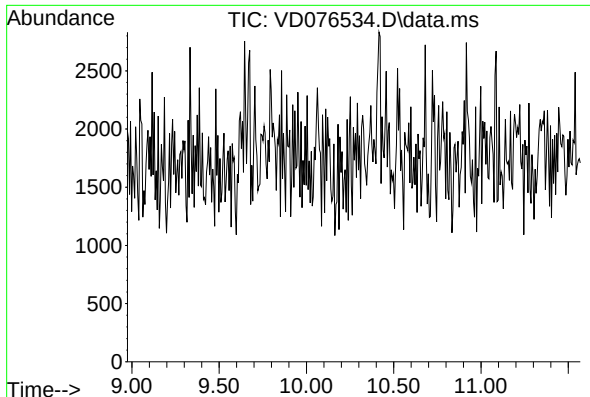

#50
Toluene-d8
Concen: 0.000 ug/l
Expected RT: 10.27 min
Lab File: VD076534.D
Acq: 22 Jun 2023 12:46


Instrument :
MSVOA_D
ClientSampleId :
SB-02-6.5-7.0RE


Tgt Ion: 98
Sig Exp Ratio
98 100
100 62.9

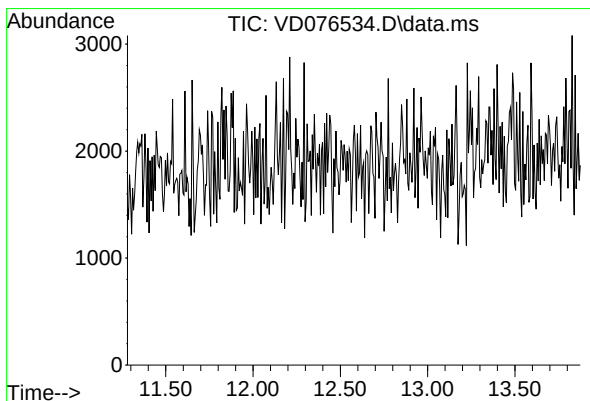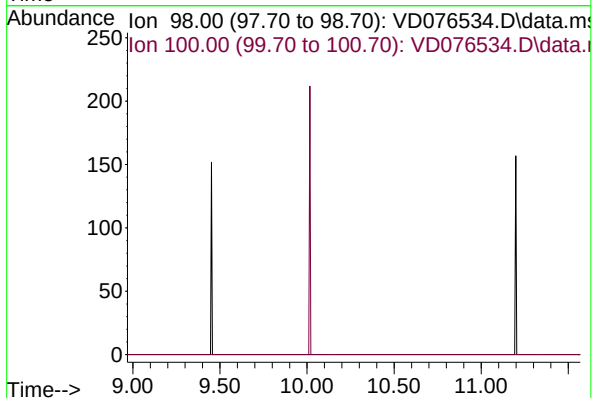

#62
4-Bromofluorobenzene
Concen: 0.000 ug/l
Expected RT: 12.57 min
Lab File: VD076534.D
Acq: 22 Jun 2023 12:46

Tgt Ion: 95
Sig Exp Ratio
95 100
174 100.9
176 95.9

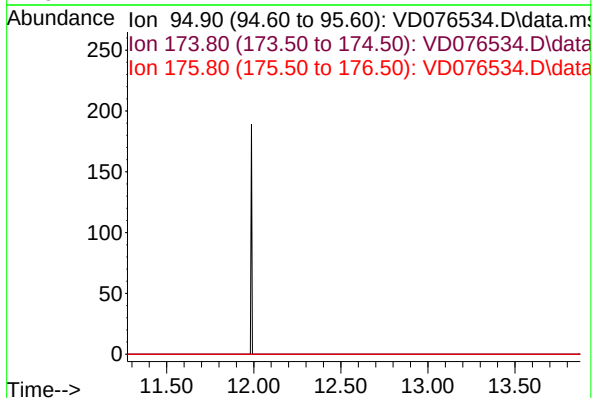


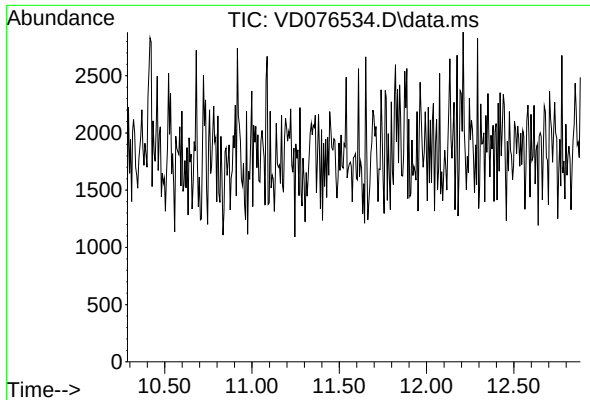


#63
 Chlorobenzene-d5
 Concen: 0.000 ug/l
 Expected RT: 11.58 min
 Lab File: VD076534.D
 Acq: 22 Jun 2023 12:46

Instrument :
 MSVOA_D
 ClientSampleId :
 SB-02-6.5-7.0RE

Tgt Ion: 117

Sig	Exp Ratio
117	100
82	47.9
119	31.2

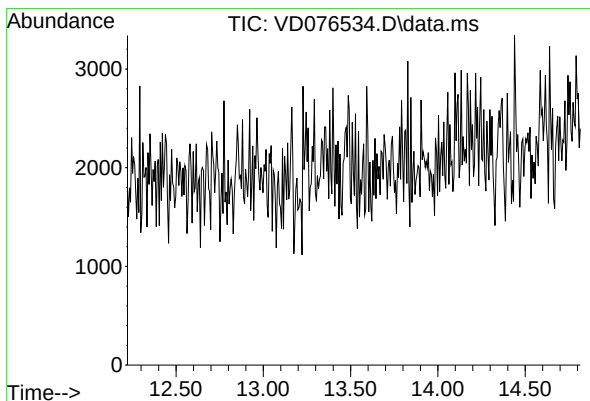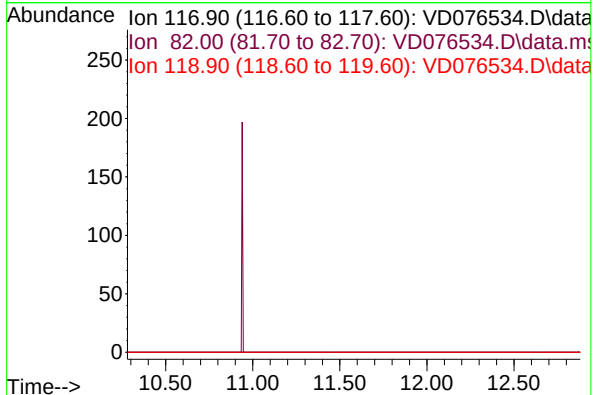

#72
 1,4-Dichlorobenzene-d4
 Concen: 0.000 ug/l
 Expected RT: 13.52 min
 Lab File: VD076534.D
 Acq: 22 Jun 2023 12:46

Tgt Ion: 152

Sig	Exp Ratio
152	100
115	54.2
150	176.8

