

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD062223\
 Data File : VD076539.D
 Acq On : 22 Jun 2023 15:14
 Operator : KP/SY
 Sample : 03360-01
 Misc : 11.47G/5.0ml/MSVOA_D/SOIL
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 CE-91-062023

Quant Time: Jun 23 06:36:27 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D061623S.M
 Quant Title : SW846 8260
 QLast Update : Mon Jun 19 04:51:45 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.875	168	153223	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	8.775	114	268927	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.581	117	238224	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.516	152	98734	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.228	65	102702	66.900	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	133.800%
35) Dibromofluoromethane	7.804	113	104447	65.377	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	130.760%
50) Toluene-d8	10.269	98	390206	64.402	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	128.800%
62) 4-Bromofluorobenzene	12.575	95	110041	55.962	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	111.920%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD062223\
Data File : VD076539.D
Acq On : 22 Jun 2023 15:14
Operator : KP/SY
Sample : 03360-01
Misc : 11.47G/5.0ml/MSVOA_D/SOIL
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
CE-91-062023


Quant Time: Jun 23 06:36:27 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D061623S.M
Quant Title : SW846 8260
QLast Update : Mon Jun 19 04:51:45 2023
Response via : Initial Calibration

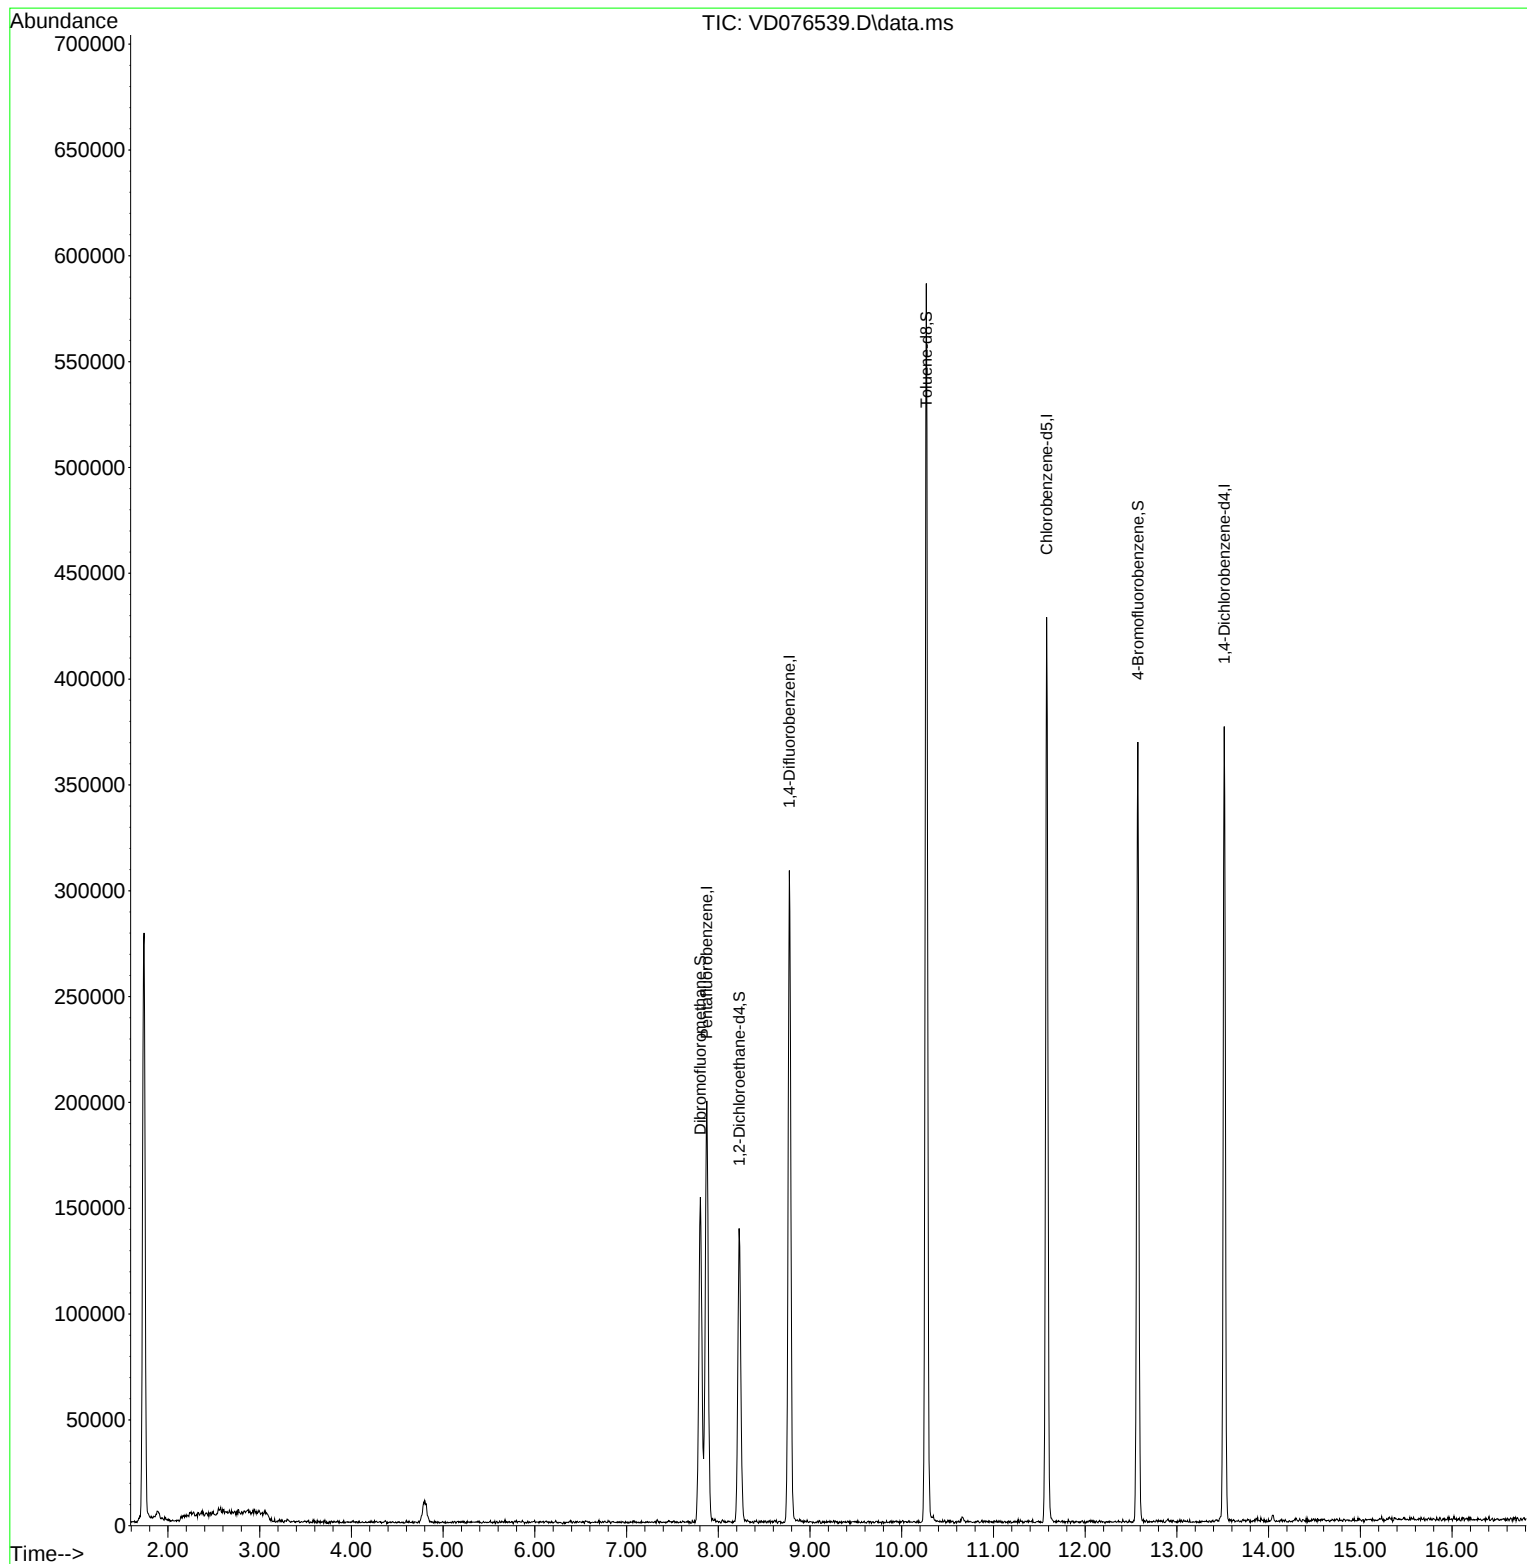



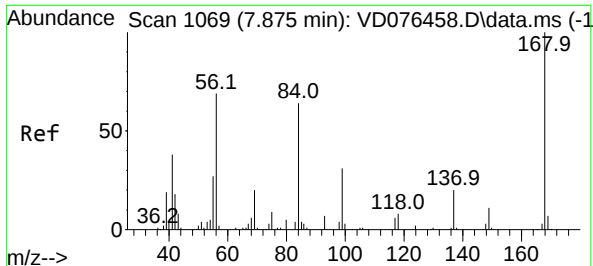


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.875 min Scan# 1069
Delta R.T. 0.000 min
Lab File: VD076539.D
Acq: 22 Jun 2023 15:14

Instrument :
MSVOA_D
ClientSampleId :
CE-91-062023



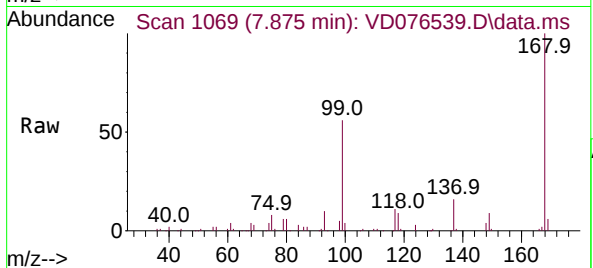



Tgt Ion:168 Resp: 153223
Ion Ratio Lower Upper
168 100
99 55.6 36.7 55.1#

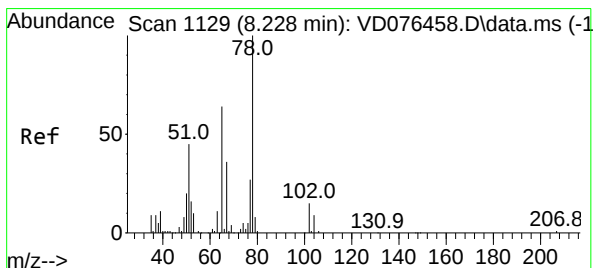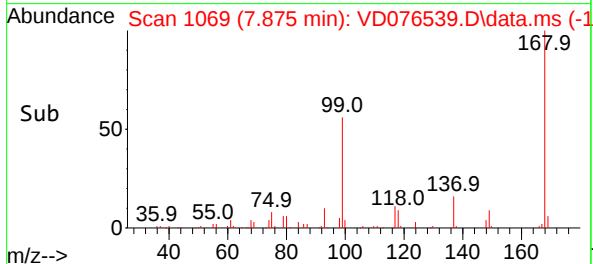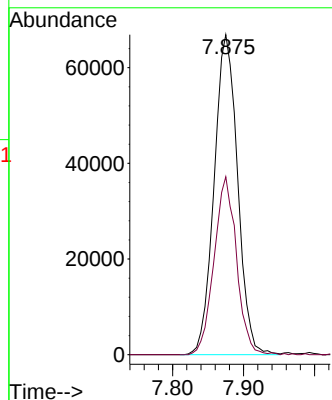

#33
1,2-Dichloroethane-d4
Concen: 66.900 ug/l
RT: 8.228 min Scan# 1129
Delta R.T. -0.000 min
Lab File: VD076539.D
Acq: 22 Jun 2023 15:14

Tgt Ion: 65 Resp: 102702
Ion Ratio Lower Upper
65 100
67 54.5 0.0 115.0

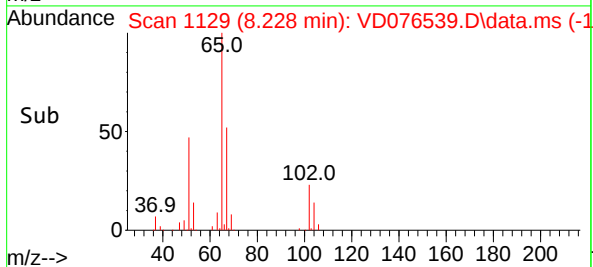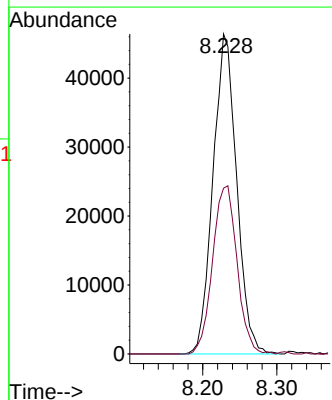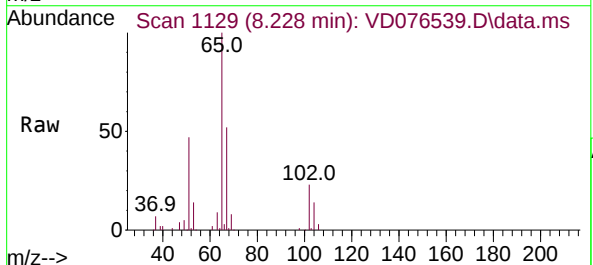

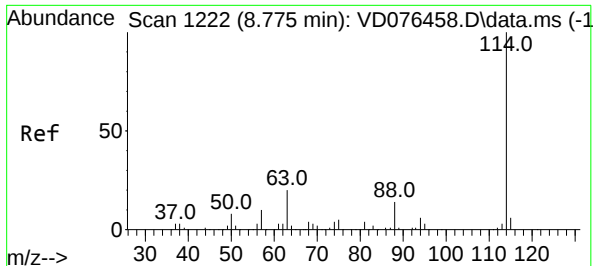

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.775 min Scan# 11

Delta R.T. -0.000 min

Lab File: VD076539.D

Acq: 22 Jun 2023 15:14

Instrument :

MSVOA_D

ClientSampleId :

CE-91-062023





Tgt Ion:114 Resp: 268927

Ion Ratio Lower Upper

114 100

63 18.6 0.0 33.4

88 13.3 0.0 26.2

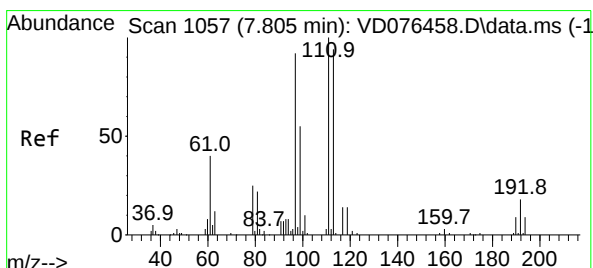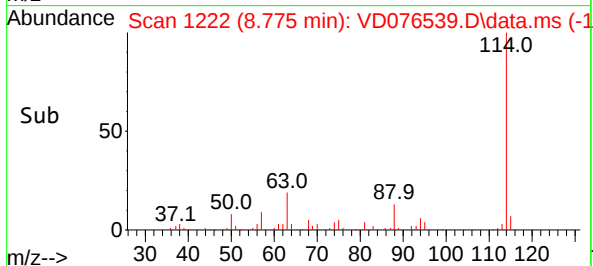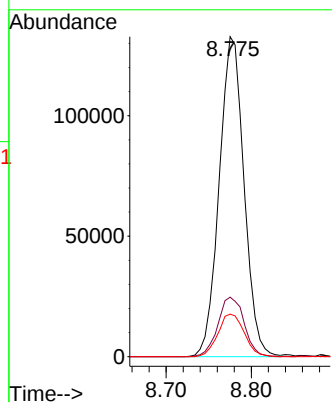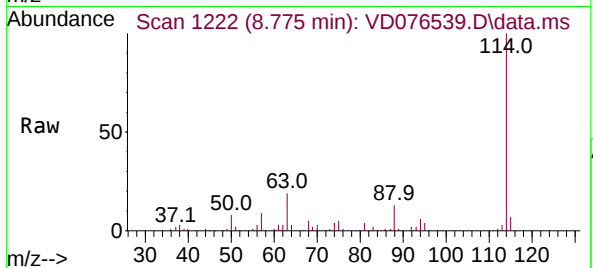

#35

Dibromofluoromethane

Concen: 65.377 ug/l

RT: 7.804 min Scan# 1057

Delta R.T. -0.000 min

Lab File: VD076539.D

Acq: 22 Jun 2023 15:14




Tgt Ion:113 Resp: 104447


Ion Ratio Lower Upper

113 100

111 103.1 84.7 127.1

192 20.2 16.8 25.2

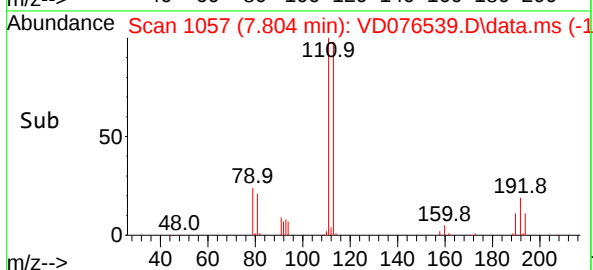
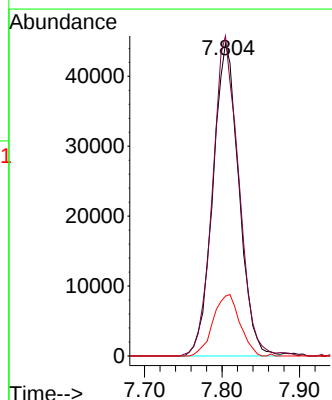
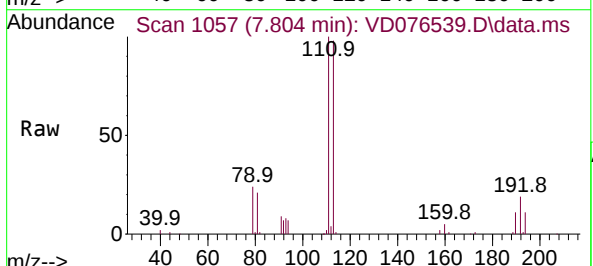


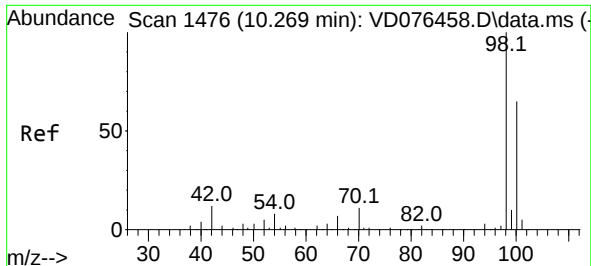

#50
Toluene-d8
Concen: 64.402 ug/l
RT: 10.269 min Scan# 1476
Delta R.T. -0.000 min
Lab File: VD076539.D
Acq: 22 Jun 2023 15:14




Instrument :
MSVOA_D
ClientSampleId :
CE-91-062023


Tgt Ion: 98 Resp: 390206
Ion Ratio Lower Upper
98 100
100 64.4 50.3 75.5

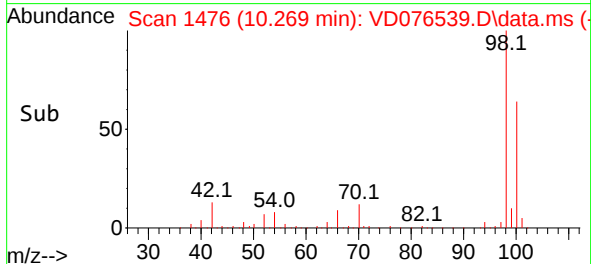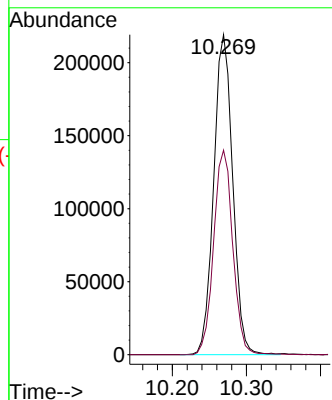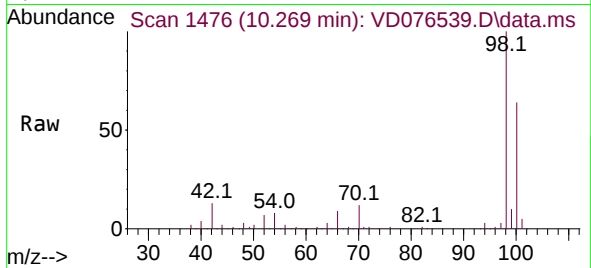

#62
4-Bromofluorobenzene
Concen: 55.962 ug/l
RT: 12.575 min Scan# 1868
Delta R.T. -0.000 min
Lab File: VD076539.D
Acq: 22 Jun 2023 15:14

Tgt Ion: 95 Resp: 110041
Ion Ratio Lower Upper
95 100
174 88.8 0.0 201.8
176 86.6 0.0 191.8


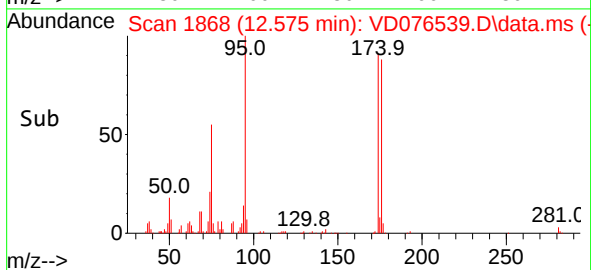
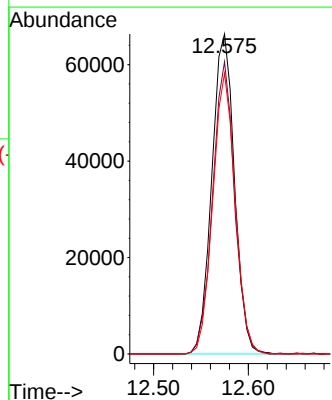
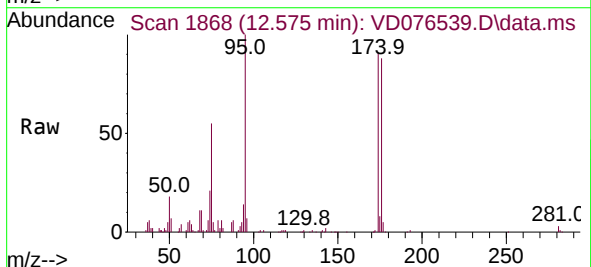


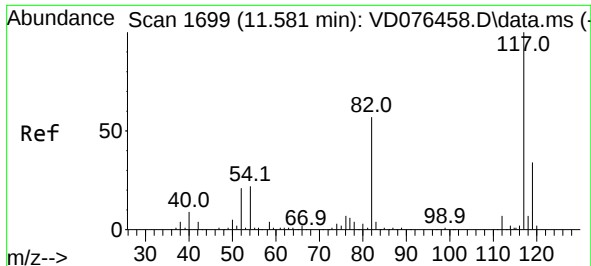

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.581 min Scan# 1
Delta R.T. -0.000 min
Lab File: VD076539.D
Acq: 22 Jun 2023 15:14

Instrument :
MSVOA_D
ClientSampleId :
CE-91-062023

Tgt Ion:117 Resp: 238224
Ion Ratio Lower Upper
117 100
82 52.7 38.3 57.5
119 29.5 25.0 37.4

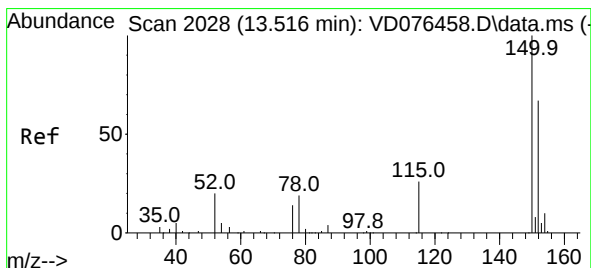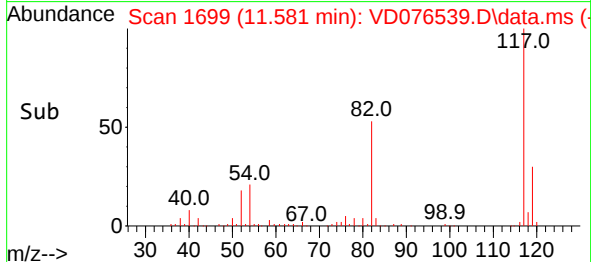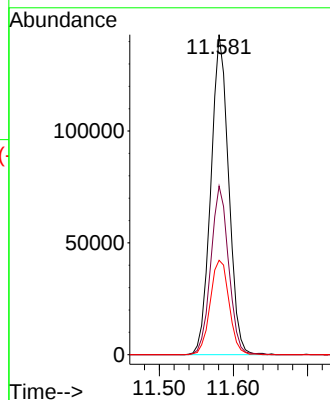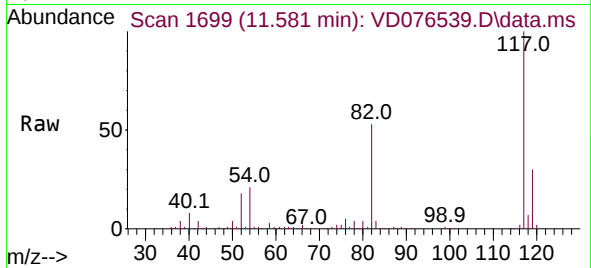

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.516 min Scan# 2028
Delta R.T. -0.000 min
Lab File: VD076539.D
Acq: 22 Jun 2023 15:14

Tgt Ion:152 Resp: 98734
Ion Ratio Lower Upper
152 100
115 56.3 27.1 81.3
150 157.1 0.0 353.6

