
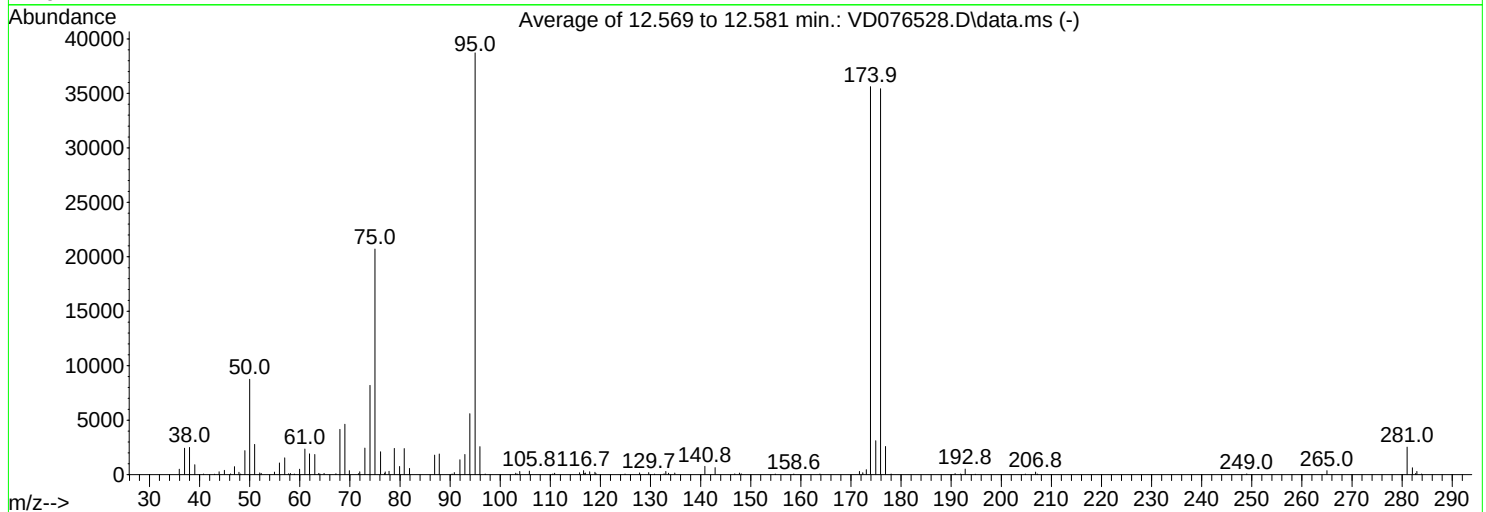


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD062223\
Data File : VD076528.D
Acq On : 22 Jun 2023 09:07
Operator : KP/SY
Sample : BFB
Misc : 5.00G/5.0ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D061623S.M
Title : SW846 8260
Last Update : Mon Jun 19 04:51:45 2023

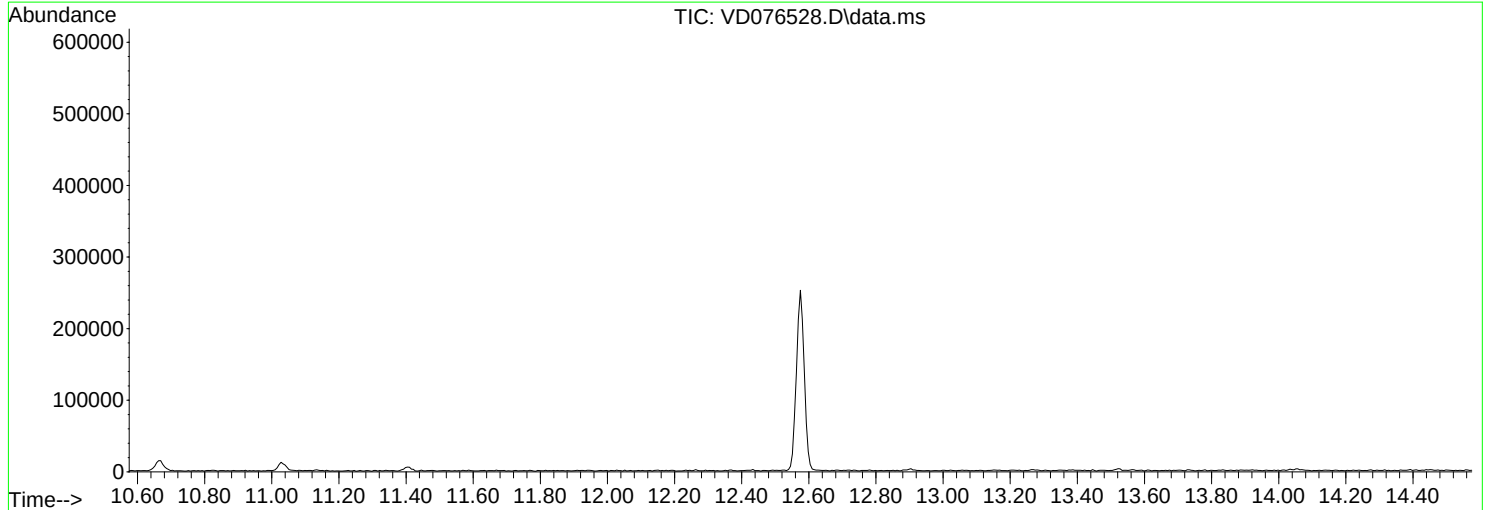

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1860

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	22.6	8762	PASS
75	95	30	60	53.5	20707	PASS
95	95	100	100	100.0	38725	PASS
96	95	5	9	6.6	2573	PASS
173	174	0.00	2	1.3	453	PASS
174	95	50	100	92.0	35619	PASS
175	174	5	9	8.8	3118	PASS
176	174	95	101	99.5	35432	PASS
177	176	5	9	7.3	2590	PASS