


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD062318\
Data File : VD058338.D
Acq On : 23 Jun 2018 13:28
Operator : VA/AP
Sample : BFB
Misc : 5.00µl/5ml/MSVOA D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D061918S.M
Title : SW846 8260
Last Update : Wed Jun 20 05:52:56 2018

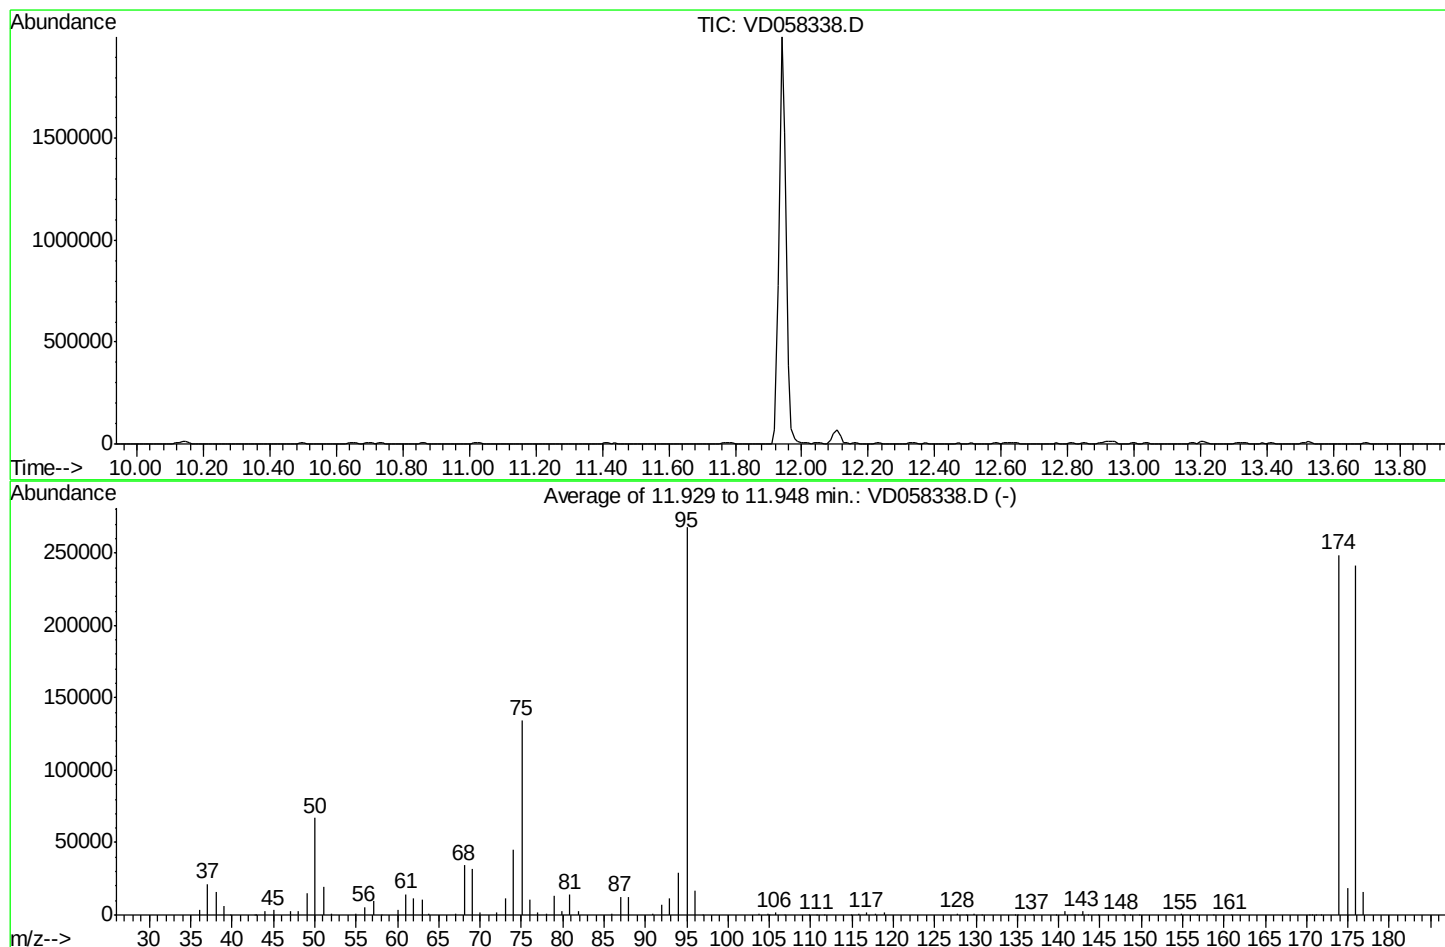

AutoFind: Scans 1189, 1190, 1191; Background Corrected with Scan 1184

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	25.0	67066	PASS
75	95	30	60	50.1	134189	PASS
95	95	100	100	100.0	267818	PASS
96	95	5	9	6.2	16600	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	92.8	248568	PASS
175	174	5	9	7.5	18675	PASS
176	174	95	101	97.2	241520	PASS
177	176	5	9	6.8	16321	PASS