
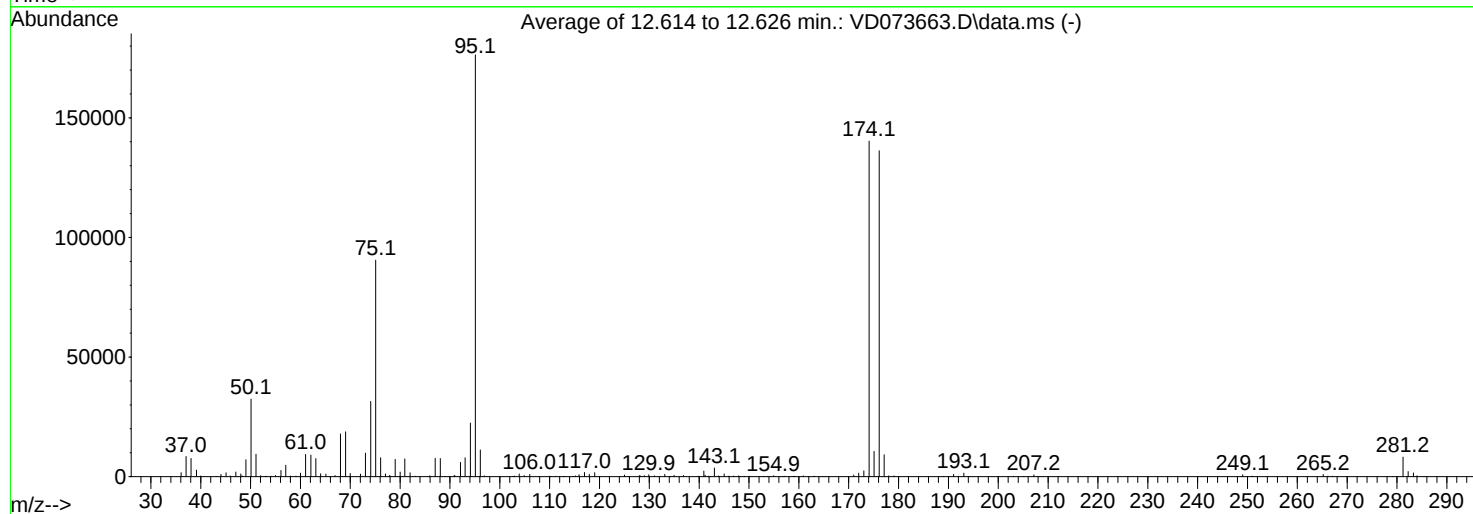


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD062322\
 Data File : VD073663.D
 Acq On : 23 Jun 2022 10:11
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D062322S.M
 Title : SW846 8260
 Last Update : Fri Jun 24 07:36:47 2022

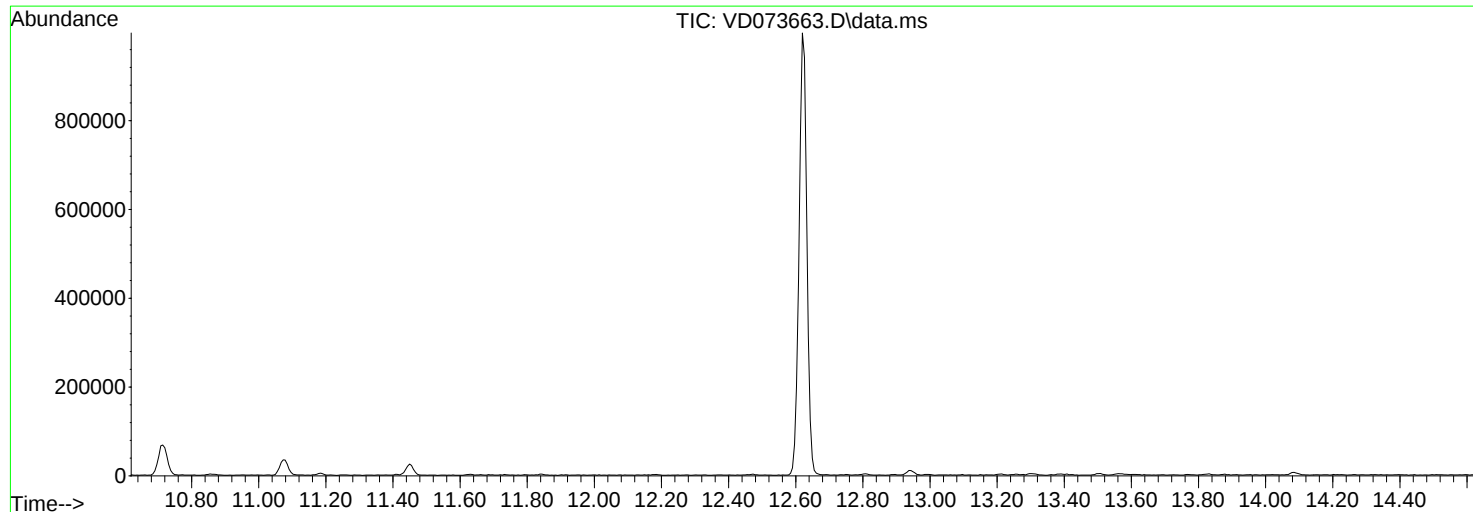

AutoFind: Scans 1818, 1819, 1820; Background Corrected with Scan 1810

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.4	32421	PASS
75	95	30	60	51.3	90528	PASS
95	95	100	100	100.0	176341	PASS
96	95	5	9	6.3	11167	PASS
173	174	0.00	2	1.7	2446	PASS
174	95	50	100	79.5	140259	PASS
175	174	5	9	7.5	10580	PASS
176	174	95	101	97.1	136251	PASS
177	176	5	9	6.7	9196	PASS