


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD062418\  
 Data File : VD058362.D  
 Acq On : 24 Jun 2018 9:30  
 Operator : VA/AP  
 Sample : BFB  
 Misc : 5.00g/5ml/MSVOA D/SOIL  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_D  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_D\METHOD\82D061918S.M  
 Title : SW846 8260  
 Last Update : Wed Jun 20 05:52:56 2018

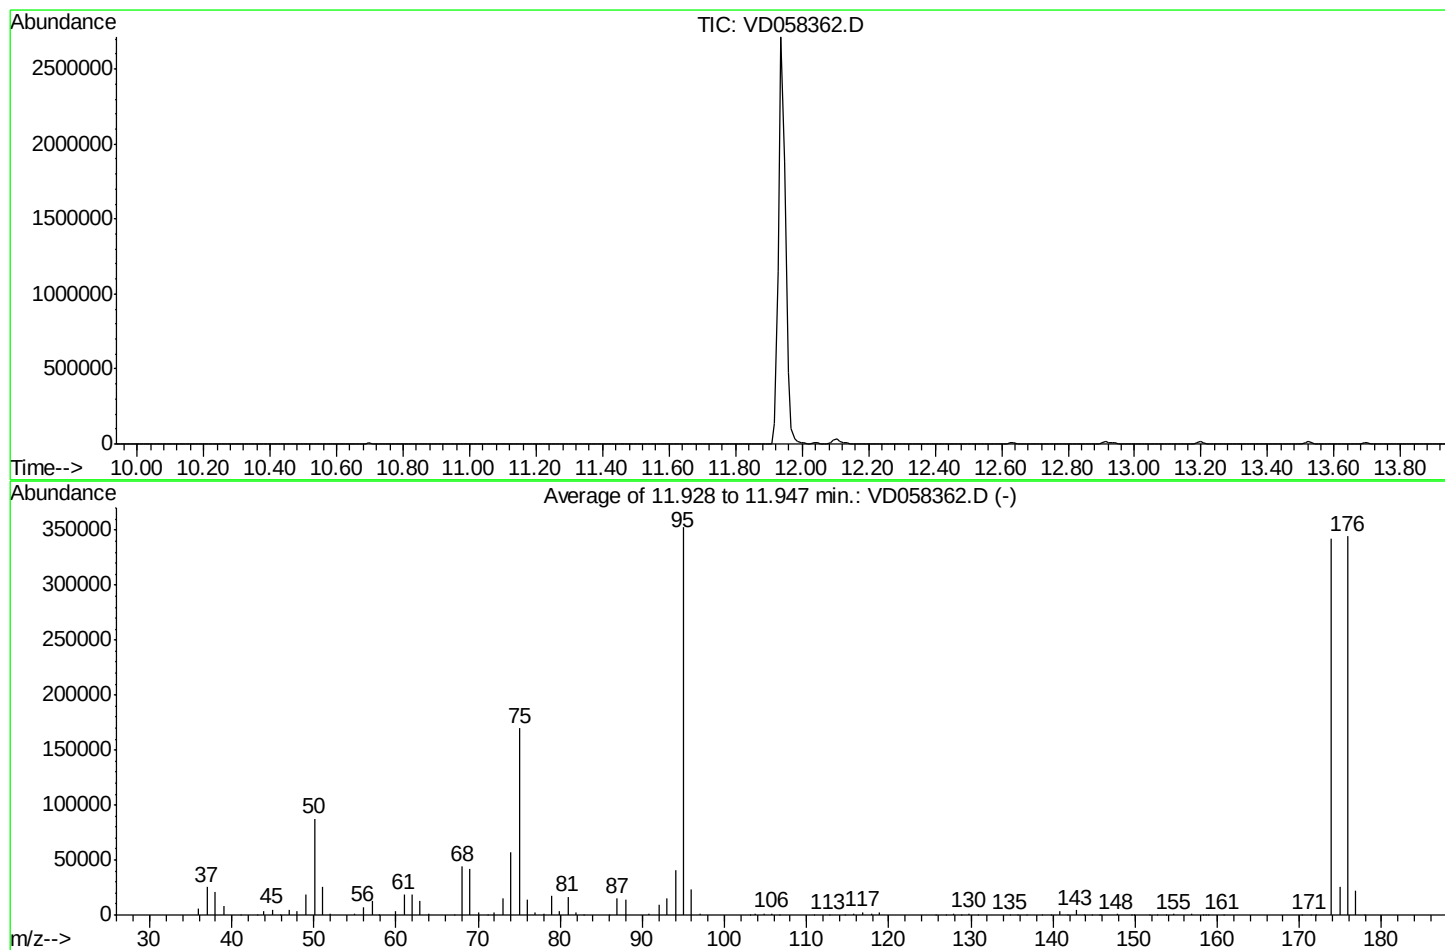

AutoFind: Scans 1189, 1190, 1191; Background Corrected with Scan 1184

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 24.9      | 87640   | PASS             |
| 75          | 95           | 30           | 60           | 48.1      | 169469  | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 352618  | PASS             |
| 96          | 95           | 5            | 9            | 6.5       | 22866   | PASS             |
| 173         | 174          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 174         | 95           | 50           | 100          | 97.1      | 342528  | PASS             |
| 175         | 174          | 5            | 9            | 7.6       | 26148   | PASS             |
| 176         | 174          | 95           | 101          | 100.5     | 344128  | PASS             |
| 177         | 176          | 5            | 9            | 6.3       | 21685   | PASS             |