


Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD062419\
Data File : VD062854.D
Acq On : 24 Jun 2019 22:26
Operator : VA/AP
Sample : BFB
Misc : 5.00µl/5ml/MSVOA D/SOIL
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D061919S.M
Title : SW846 8260
Last Update : Thu Jun 20 01:50:56 2019

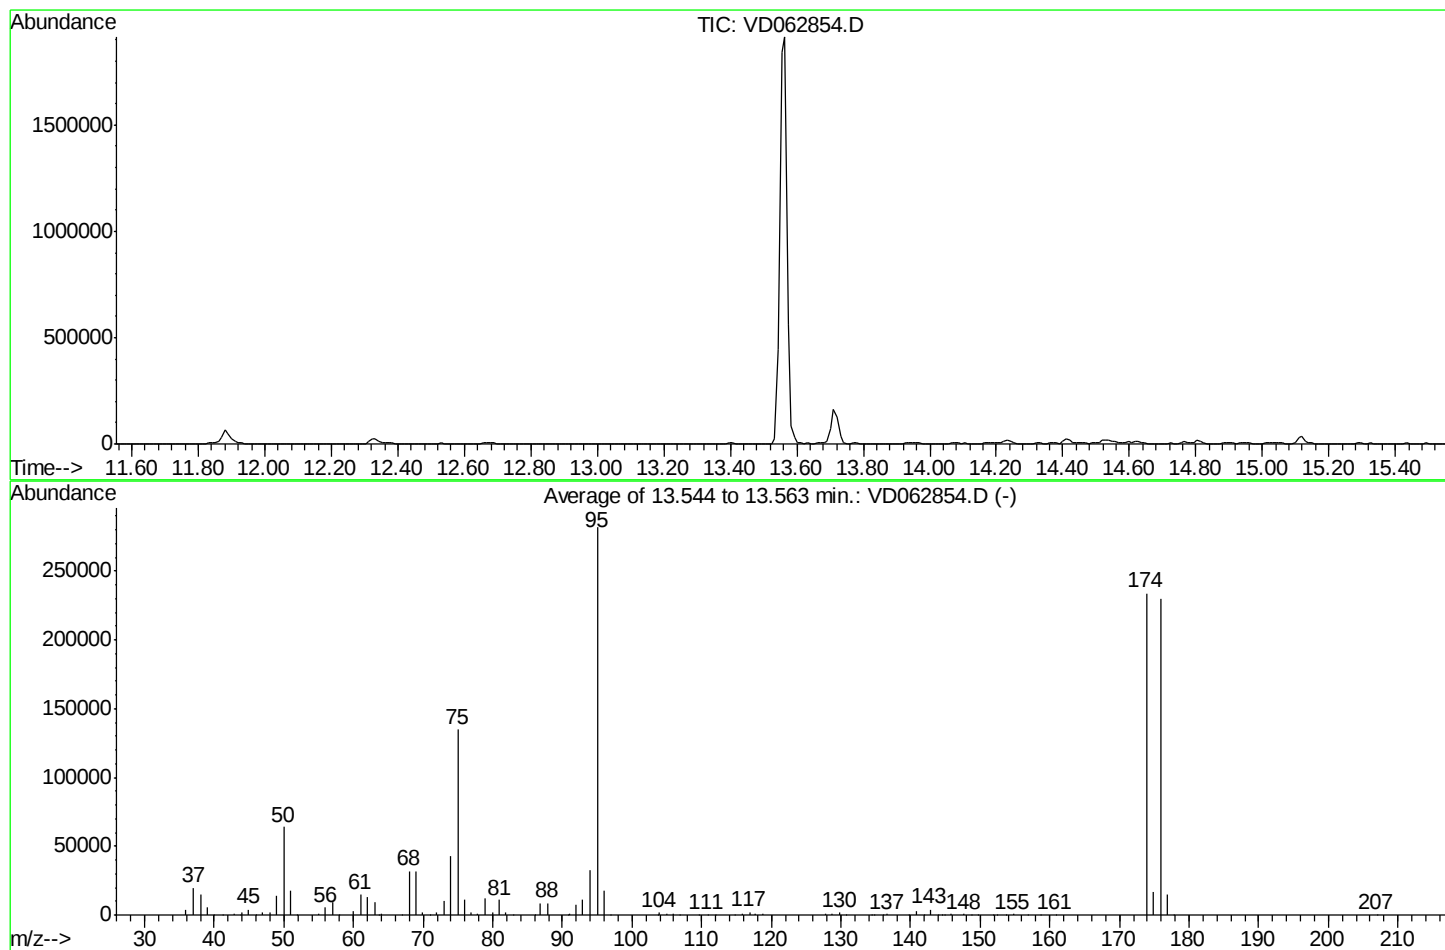

AutoFind: Scans 1231, 1232, 1233; Background Corrected with Scan 1226

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.7	64030	PASS
75	95	30	60	47.8	134760	PASS
95	95	100	100	100.0	281738	PASS
96	95	5	9	6.4	18101	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	83.0	233816	PASS
175	174	5	9	7.2	16813	PASS
176	174	95	101	98.3	229872	PASS
177	176	5	9	6.6	15117	PASS