


Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD062518\
 Data File : VD059394.D
 Acq On : 25 Jun 2018 10:52
 Operator : VA/AP
 Sample : BFB
 Misc : 5.00µl/5ml/MSVOA D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D062518S.M
 Title : SW846 8260
 Last Update : Mon Jun 25 07:29:35 2018

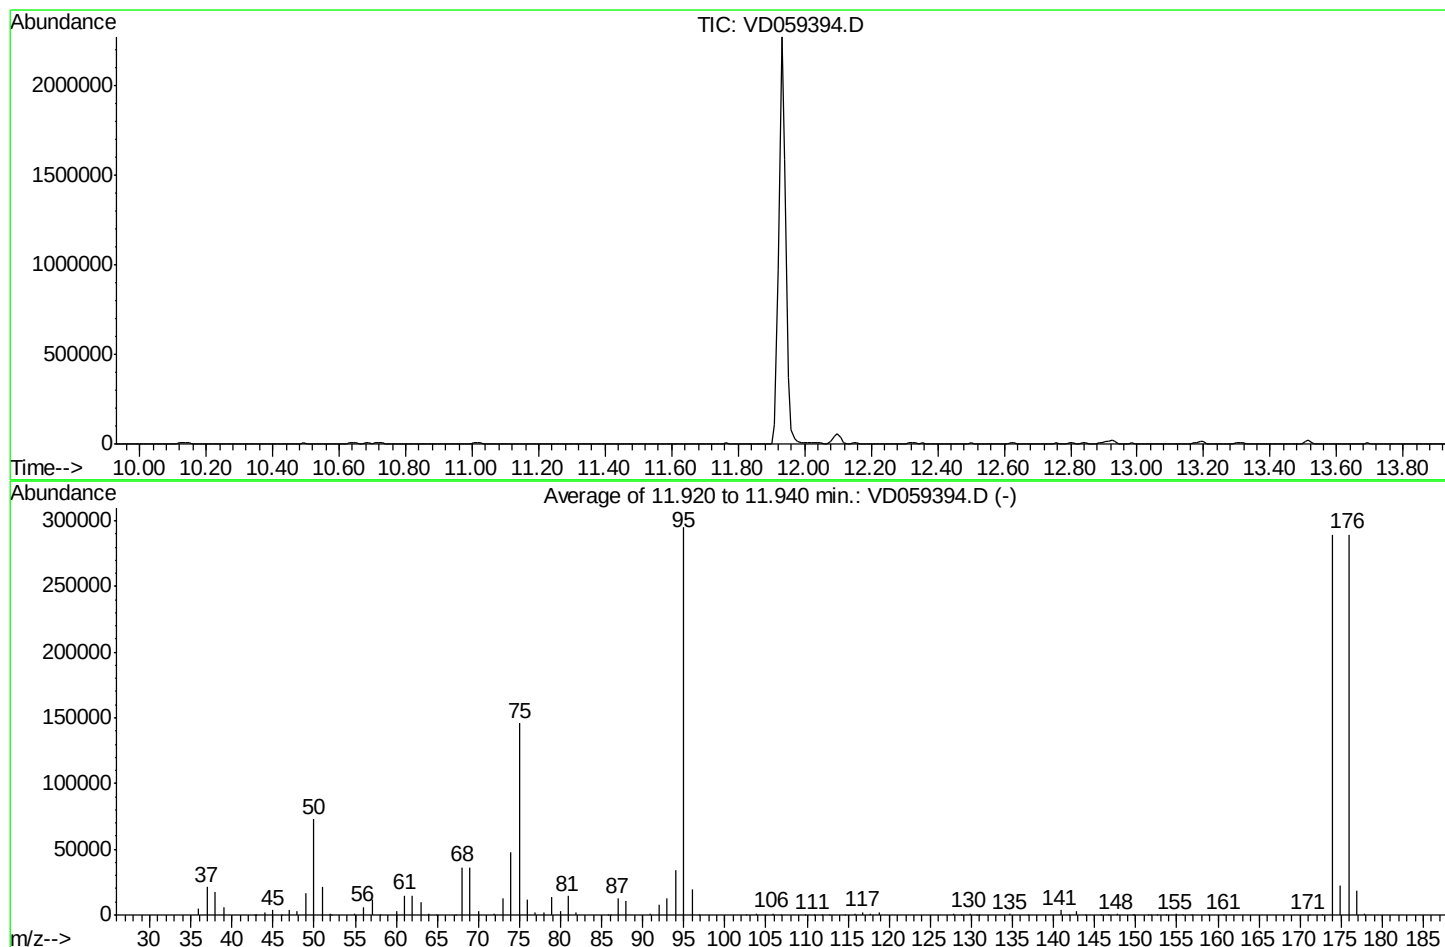

AutoFind: Scans 1188, 1189, 1190; Background Corrected with Scan 1183

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.6	72698	PASS
75	95	30	60	49.5	146026	PASS
95	95	100	100	100.0	294933	PASS
96	95	5	9	6.6	19587	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	98.1	289472	PASS
175	174	5	9	7.8	22698	PASS
176	174	95	101	100.0	289490	PASS
177	176	5	9	6.5	18876	PASS