

Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD062519\
 Data File : VD062874.D
 Acq On : 25 Jun 2019 12:58
 Operator : VA/AP
 Sample : K3164-09
 Misc : 4.51g/5ml/MSVOA D/SOIL
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BAT-B08

Quant Time: Jun 26 05:33:47 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D061919S.M
 Quant Title : SW846 8260
 QLast Update : Thu Jun 20 01:50:56 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.05	168	690352	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.23	114	1077012	50.00	ug/l	0.00
63) Chlorobenzene-d5	12.37	117	895050	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	14.53	152	396741	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	7.46	65	444322	59.21	ug/l	0.00
Spiked Amount			Recovery	=	118.42%	
35) Dibromofluoromethane	6.93	113	476296	52.45	ug/l	0.00
Spiked Amount			Recovery	=	104.90%	
50) Toluene-d8	10.41	98	964186	48.78	ug/l	0.00
Spiked Amount			Recovery	=	97.56%	
62) 4-Bromofluorobenzene	13.56	95	387424	43.11	ug/l	0.00
Spiked Amount			Recovery	=	86.22%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
11) Tert butyl alcohol	4.10	59	1057	3.093	ug/l #	77
13) Acrolein	3.03	56	438	1.255	ug/l #	62
16) Acetone	3.23	43	124913	77.251	ug/l	99
18) Methyl Acetate	3.64	43	16112	7.113	ug/l #	90
20) Methylene Chloride	3.82	84	19130	3.343	ug/l #	88
36) 1,1-Dichloropropene	7.05	75	58563	5.744	ug/l #	57
38) Carbon Tetrachloride	7.05	117	71972	4.694	ug/l #	16
44) Trichloroethene	8.55	130	17541	2.186	ug/l	61
58) 2-Chloroethyl Vinyl ether	9.86	63	3943	1.521	ug/l #	47
59) 2-Hexanone	11.49	43	4842	1.794	ug/l #	31
67) Ethyl Benzene	12.53	91	56490	1.894	ug/l	96
68) m/p-Xylenes	12.67	106	81926	7.887	ug/l	91
69) o-Xylene	13.05	106	33538	3.532	ug/l	98
81) trans-1,4-Dichloro-2-buten	13.56	75	182846	152.325	ug/l #	2


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA D\DATA\VD062519\
Data File : VD062874.D
Acq On : 25 Jun 2019 12:58
Operator : VA/AP
Sample : K3164-09
Misc : 4.51g/5ml/MSVOA D/SOIL
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BAT-B08

Quant Time: Jun 26 05:33:47 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_D\METHOD\82D061919S.M
Quant Title : SW846 8260
QLast Update : Thu Jun 20 01:50:56 2019
Response via : Initial Calibration

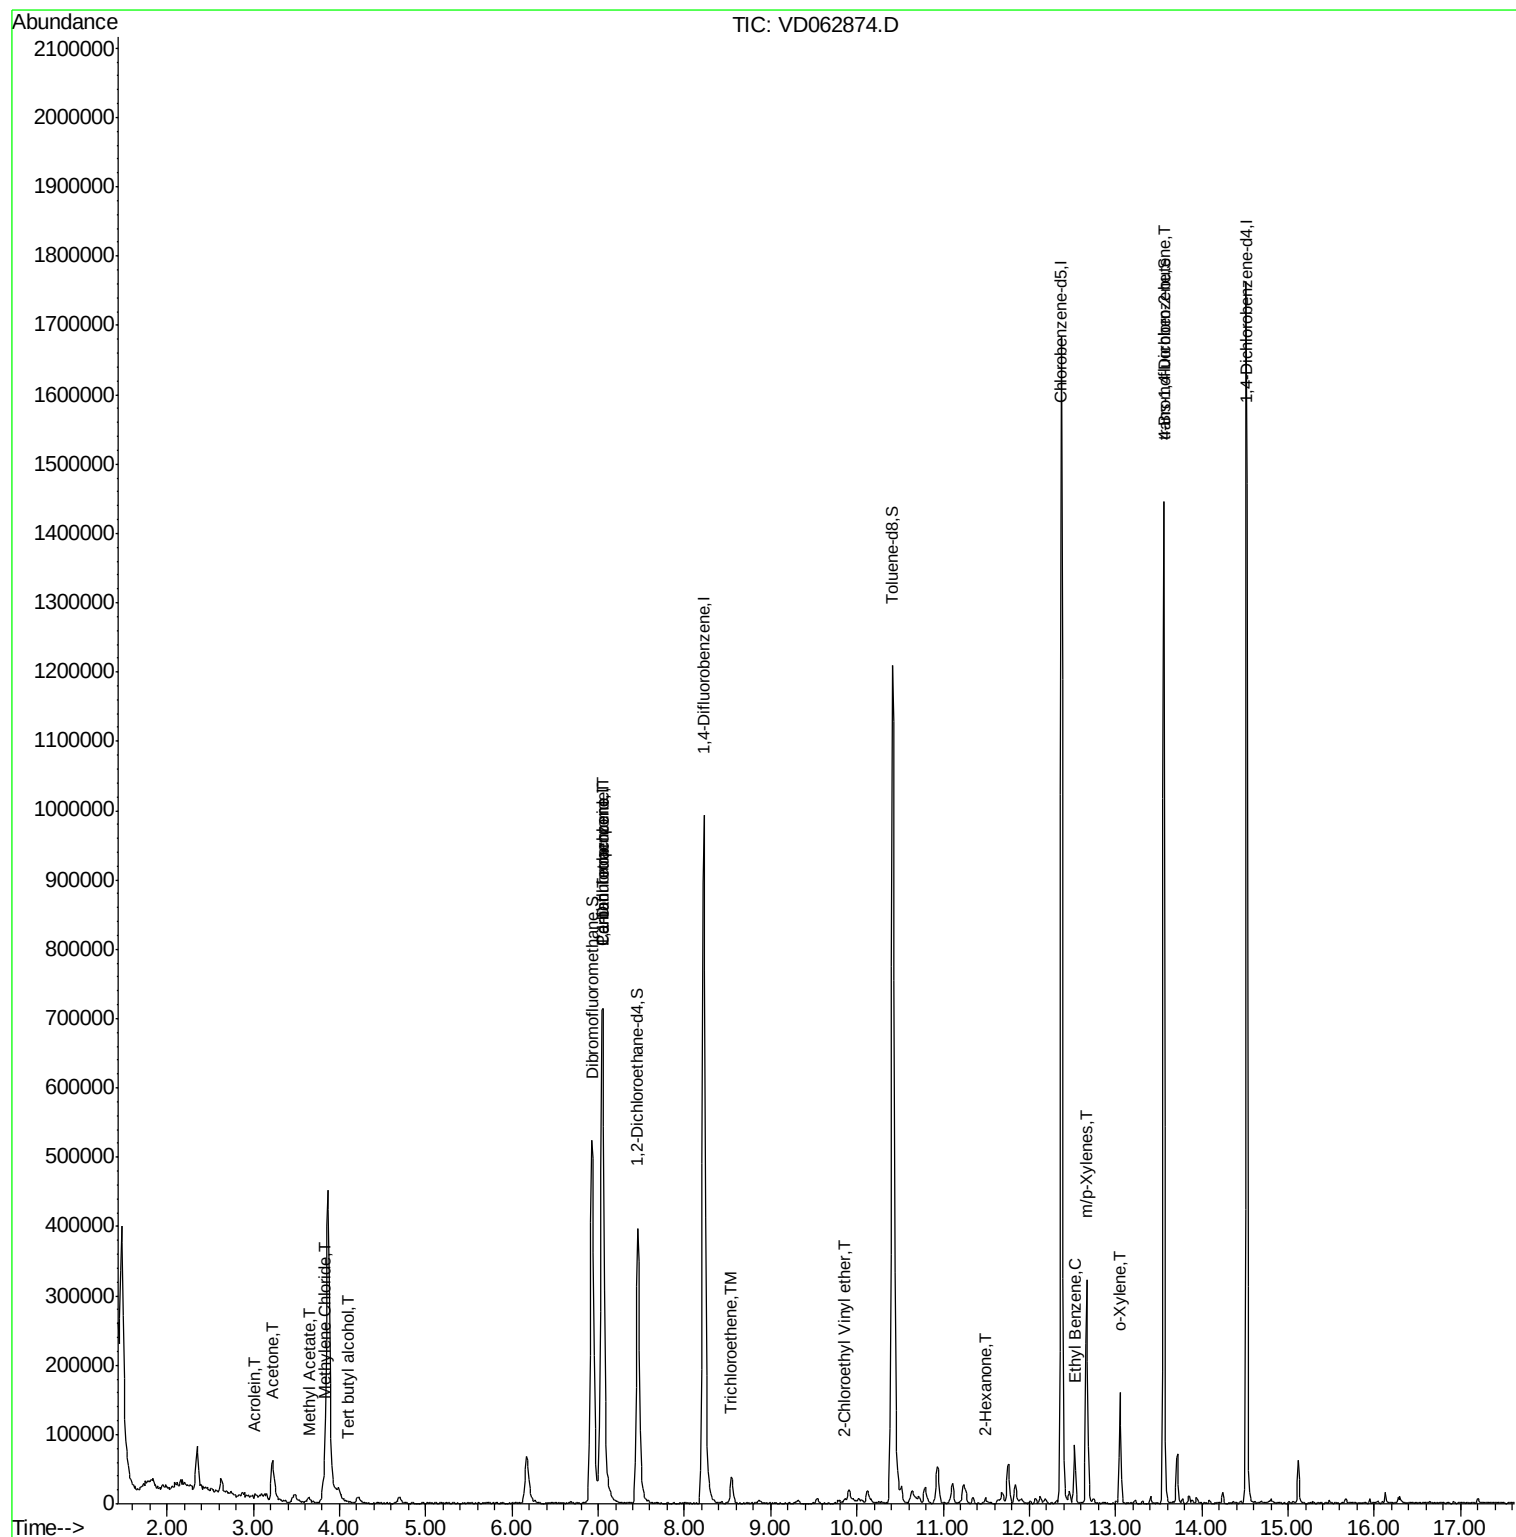

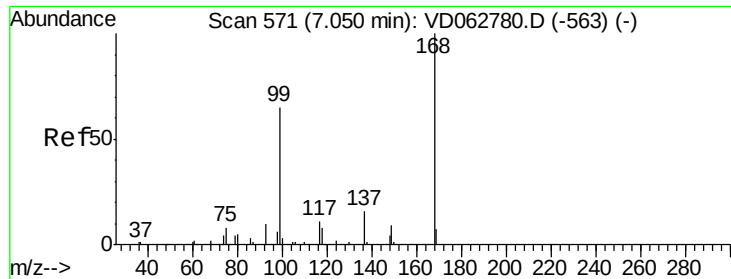

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.05 min Scan# 572

Delta R.T. 0.01 min

Lab File: VD062874.D

Acq: 25 Jun 2019 12:58

Instrument :

MSVOA_D

ClientSampleId :


BAT-B08

Tot Ion:168 Resp: 690352

Ion Ratio Lower Upper

168 100

99 59.9 53.0 79.6

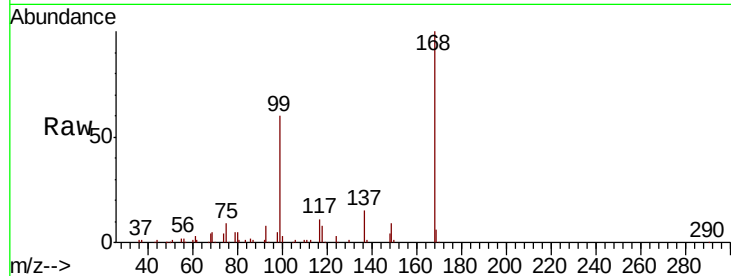

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.95 (98.65 to 99.65): VDC

7.05

250000

200000



150000

100000

50000

0

Time-->

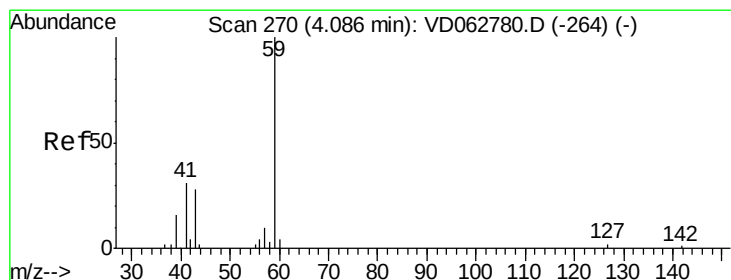

#11

Tert butyl alcohol

Concen: 3.093 ug/l

RT: 4.10 min Scan# 272

Delta R.T. 0.01 min

Lab File: VD062874.D


Acq: 25 Jun 2019 12:58

Tgt Ion: 59 Resp: 1057

Ion Ratio Lower Upper

59 100

57 0.0 6.6 10.0#



Abundance Ion 58.95 (58.65 to 59.65): VDC

Ion 56.95 (56.65 to 57.65): VDC

800


600


400

200

0

Time-->





#13

Acrolein

Concen: 1.255 ug/l

RT: 3.03 min Scan# 163

Delta R.T. -0.00 min

Lab File: VD062874.D

Acq: 25 Jun 2019 12:58

Instrument :

MSVOA_D

ClientSampleId :


BAT-B08

Tot Ion: 56 Resp: 438

Ion Ratio Lower Upper




56 100

55 100.0 55.4 83.0#

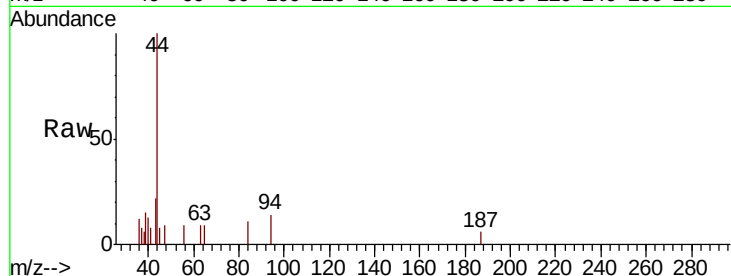

Abundance Ion 55.95 (55.65 to 56.65): VDC

Ion 55.00 (54.70 to 55.70): VDC

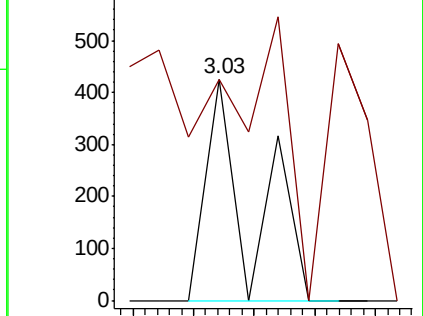

#16

Acetone

Concen: 77.251 ug/l

RT: 3.23 min Scan# 183

Delta R.T. -0.00 min

Lab File: VD062874.D


Acq: 25 Jun 2019 12:58

Tgt Ion: 43 Resp: 124913

Ion Ratio Lower Upper



43 100


58 14.3 11.9 17.9



Abundance Ion 42.95 (42.65 to 43.65): VDC

Ion 57.95 (57.65 to 58.65): VDC




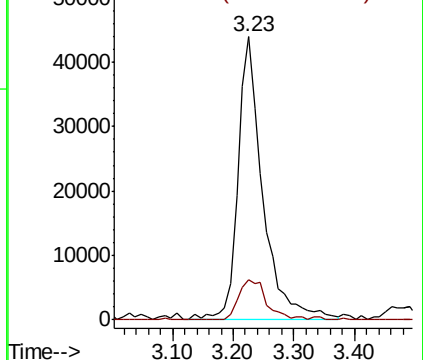


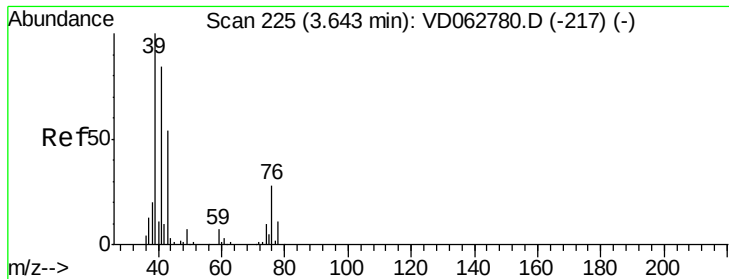

#18
Methvl Acetate
Concen: 7.113 ug/l
RT: 3.64 min Scan# 225
Delta R.T. -0.00 min
Lab File: VD062874.D
Acq: 25 Jun 2019 12:58




Instrument :
MSVOA_D
ClientSampleId :
BAT-B08


Tot Ion: 43 Resp: 16112
Ion Ratio Lower Upper
43 100
74 14.3 15.2 22.8#

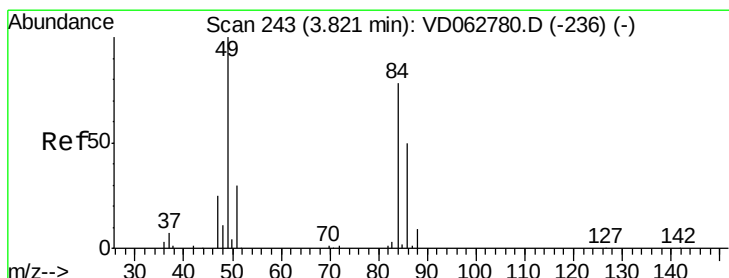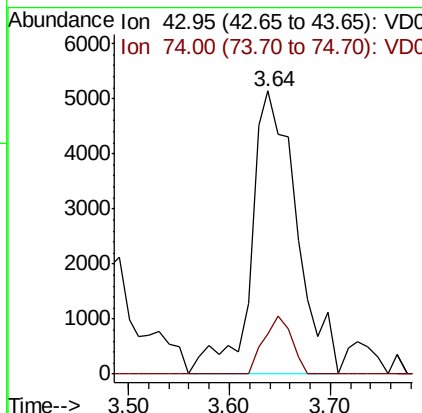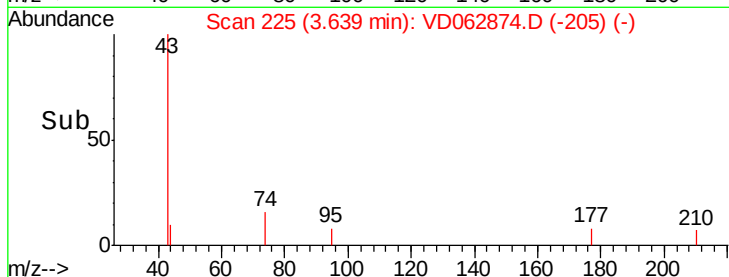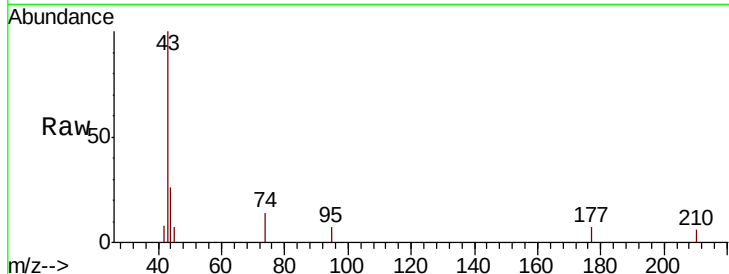

#20
Methylene Chloride
Concen: 3.343 ug/l
RT: 3.82 min Scan# 243
Delta R.T. -0.00 min
Lab File: VD062874.D
Acq: 25 Jun 2019 12:58

Tgt Ion: 84 Resp: 19130
Ion Ratio Lower Upper
84 100
49 122.5 102.9 154.3
51 43.7 31.2 46.8
86 43.0 51.4 77.2#


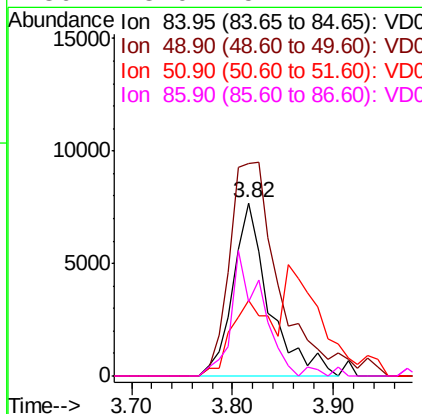
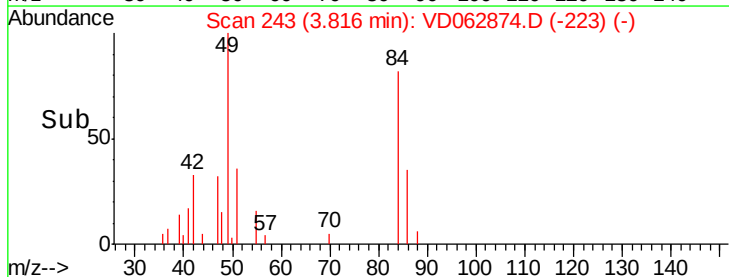
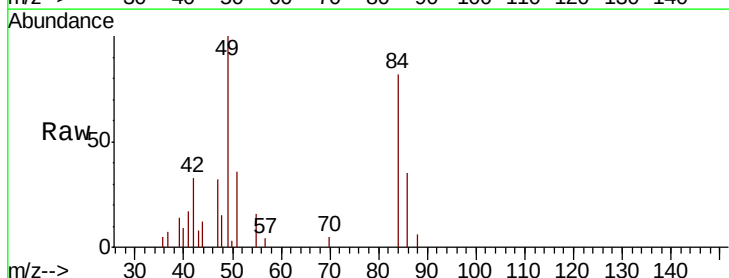


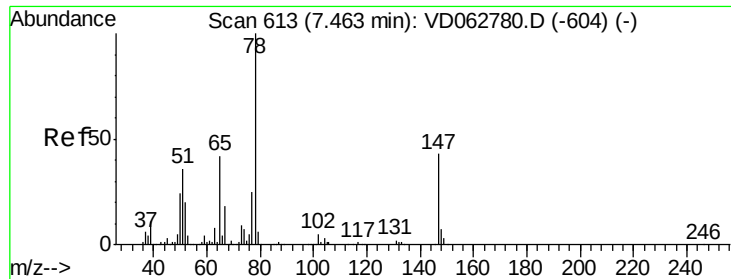

#33
 1,2-Dichloroethane-d4
 Concen: 59.211 ug/l
 RT: 7.46 min Scan# 613
 Delta R.T. -0.00 min
 Lab File: VD062874.D
 Acq: 25 Jun 2019 12:58




Instrument :
 MSVOA_D
 ClientSampleId :
 BAT-B08


Tot Ion: 65 Resp: 444322
 Ion Ratio Lower Upper
 65 100
 67 42.4 0.0 87.4

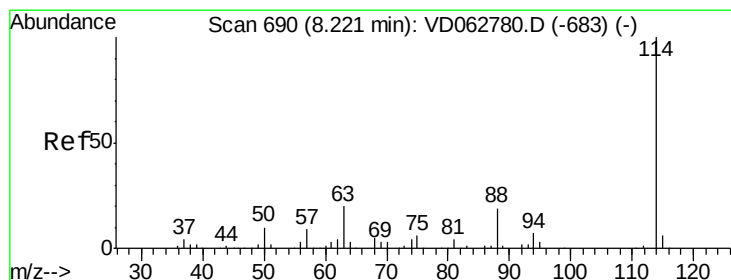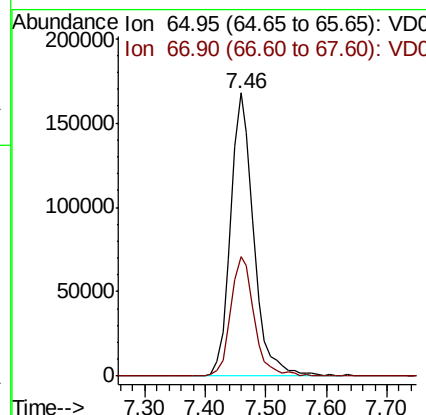

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.23 min Scan# 691
 Delta R.T. 0.01 min
 Lab File: VD062874.D
 Acq: 25 Jun 2019 12:58

Tgt Ion: 114 Resp: 1077012
 Ion Ratio Lower Upper
 114 100
 63 18.4 0.0 40.0
 88 17.2 0.0 38.8



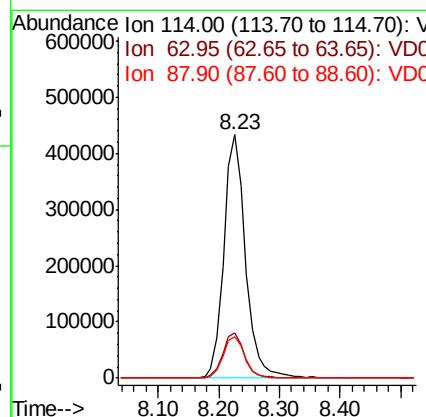





#35
 Dibromofluoromethane
 Concen: 52.448 ug/l
 RT: 6.93 min Scan# 559
 Delta R.T. -0.00 min
 Lab File: VD062874.D
 Acq: 25 Jun 2019 12:58




Instrument :
 MSVOA_D
 ClientSampleId :
 BAT-B08


Tot Ion	Ratio	Lower	Upper
113	100		
111	106.6	81.2	121.8
192	14.5	12.9	19.3

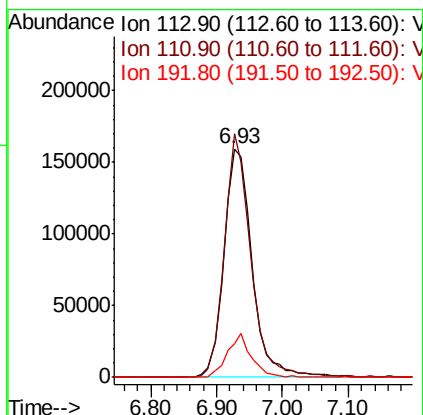

#36
 1,1-Dichloropropene
 Concen: 5.744 ug/l
 RT: 7.05 min Scan# 572
 Delta R.T. -0.09 min
 Lab File: VD062874.D
 Acq: 25 Jun 2019 12:58

Tgt Ion	Ratio	Lower	Upper
75	100		
110	11.8	15.0	45.1#
77	0.0	22.2	33.2#



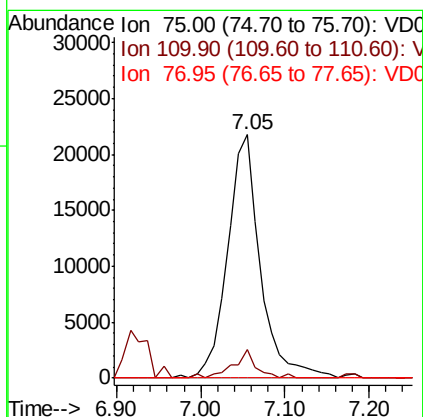



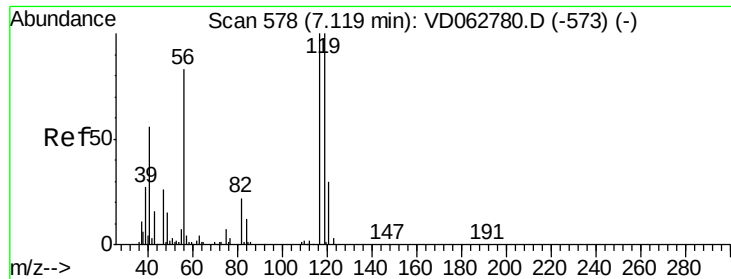

#38
Carbon Tetrachloride
Concen: 4.694 ug/l
RT: 7.05 min Scan# 572
Delta R.T. -0.06 min
Lab File: VD062874.D
Acq: 25 Jun 2019 12:58




Instrument :
MSVOA_D
ClientSampleId :
BAT-B08


Tot Ion:117 Resp: 71972
Ion Ratio Lower Upper
117 100
119 3.6 75.4 113.2#
121 0.0 22.3 33.5#

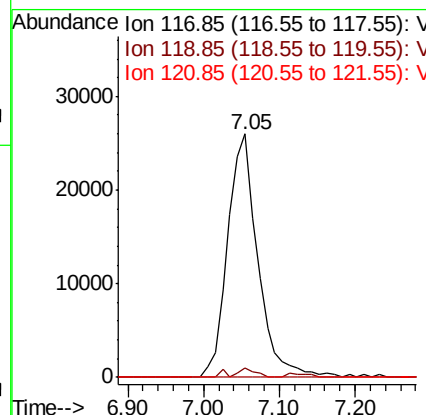

#44
Trichloroethene
Concen: 2.186 ug/l
RT: 8.55 min Scan# 724
Delta R.T. 0.01 min
Lab File: VD062874.D
Acq: 25 Jun 2019 12:58

Tgt Ion:130 Resp: 17541
Ion Ratio Lower Upper
130 100
95 61.9 0.0 201.6



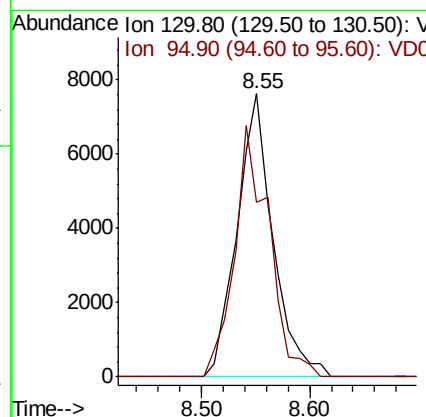



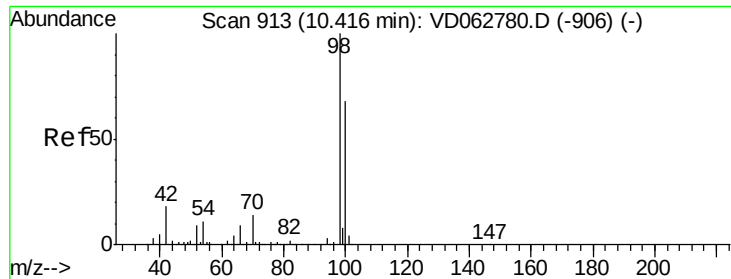

#50
Toluene-d8
Concen: 48.782 ug/l
RT: 10.41 min Scan# 913
Delta R.T. -0.00 min
Lab File: VD062874.D
Acq: 25 Jun 2019 12:58




Instrument :
MSVOA_D
ClientSampleId :
BAT-B08


Tot Ion: 98 Resp: 964186
Ion Ratio Lower Upper
98 100
100 66.6 54.7 82.1

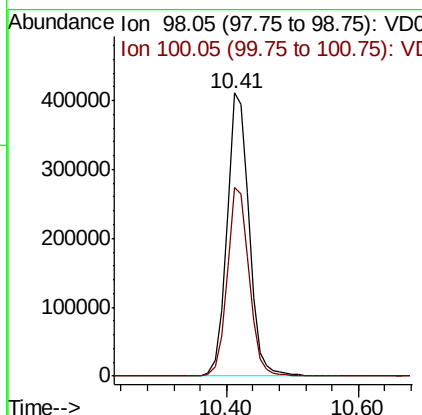

#58
2-Chloroethyl Vinyl ether
Concen: 1.521 ug/l
RT: 9.86 min Scan# 857
Delta R.T. -0.00 min
Lab File: VD062874.D
Acq: 25 Jun 2019 12:58

Tgt Ion: 63 Resp: 3943
Ion Ratio Lower Upper
63 100
106 0.0 22.1 33.1#


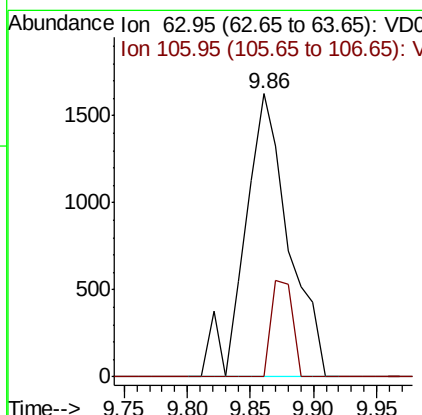




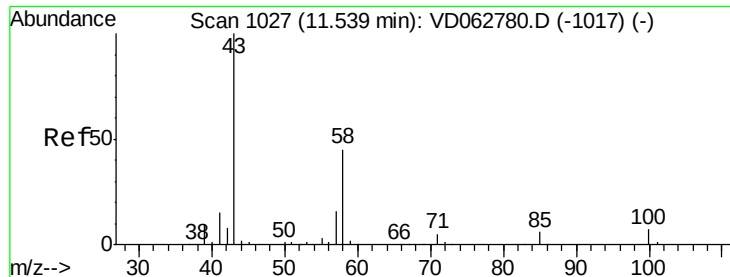

#59
2-Hexanone
Concen: 1.794 ug/l
RT: 11.49 min Scan# 1023
Delta R.T. -0.04 min
Lab File: VD062874.D
Acq: 25 Jun 2019 12:58




Instrument :
MSVOA_D
ClientSampleId :
BAT-B08


Tot Ion: 43 Resp: 4842
Ion Ratio Lower Upper
43 100
58 0.0 22.4 67.2#

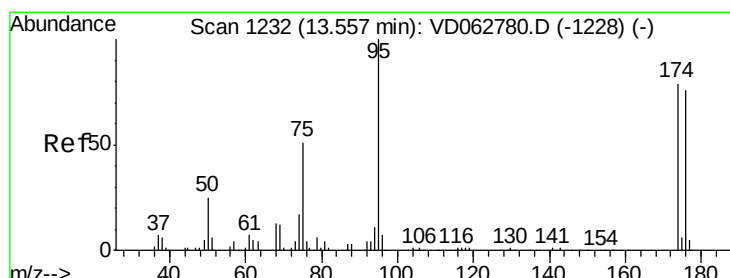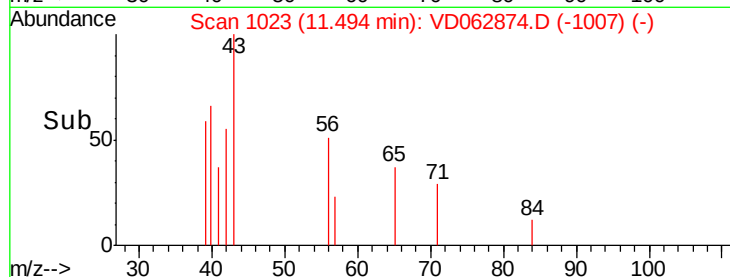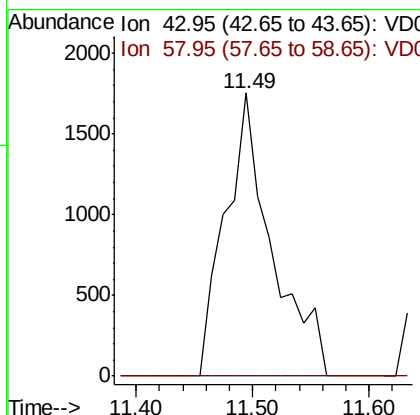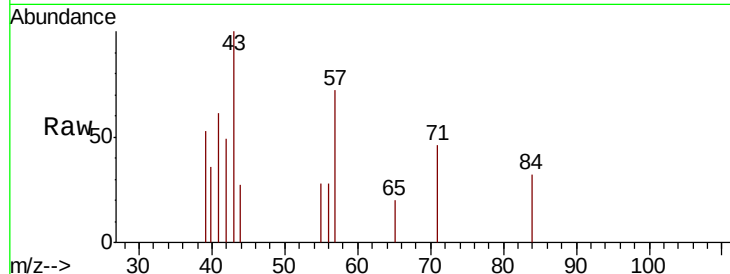

#62
4-Bromofluorobenzene
Concen: 43.108 ug/l
RT: 13.56 min Scan# 1233
Delta R.T. 0.01 min
Lab File: VD062874.D
Acq: 25 Jun 2019 12:58

Tgt Ion: 95 Resp: 387424
Ion Ratio Lower Upper
95 100
174 92.4 0.0 158.0
176 96.3 0.0 151.6

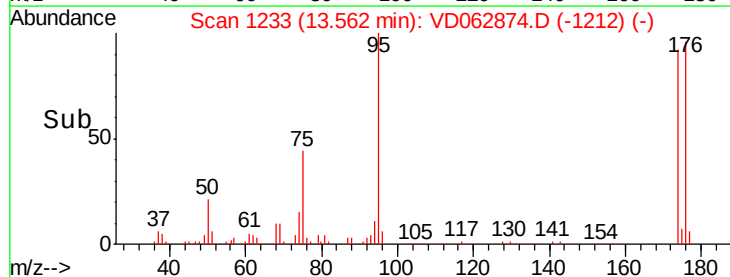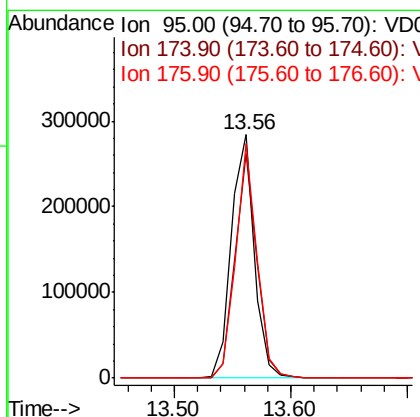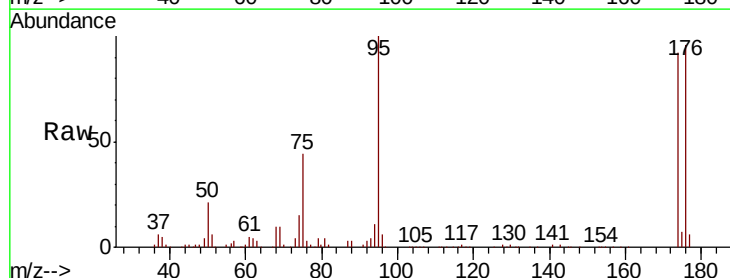







#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 12.37 min Scan# 1112
Delta R.T. -0.00 min
Lab File: VD062874.D
Acq: 25 Jun 2019 12:58

Instrument :
MSVOA_D
ClientSampleId :
BAT-B08

Tot Ion:117 Resp: 895050
Ion Ratio Lower Upper
117 100
82 52.9 40.4 60.6
119 31.7 25.2 37.8

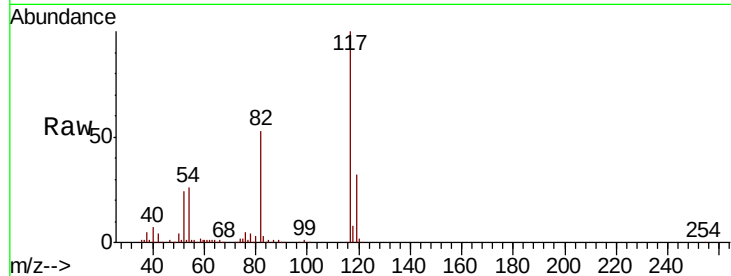


Abundance Ion 116.95 (116.65 to 117.65): V
Ion 82.05 (81.75 to 82.75): V
Ion 118.95 (118.65 to 119.65): V


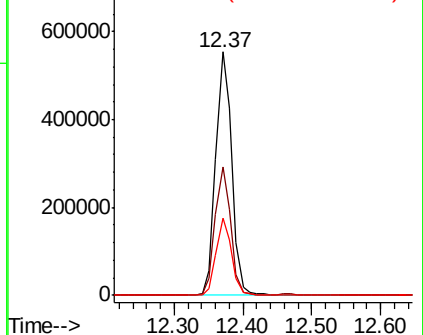



#67
Ethyl Benzene
Concen: 1.894 ug/l
RT: 12.53 min Scan# 1128
Delta R.T. -0.00 min
Lab File: VD062874.D
Acq: 25 Jun 2019 12:58

Tgt Ion: 91 Resp: 56490
Ion Ratio Lower Upper
91 100
106 26.8 23.1 34.7



Abundance Ion 91.00 (90.70 to 91.70): V
Ion 106.05 (105.75 to 106.75): V




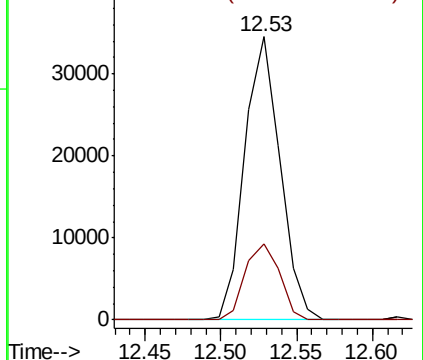


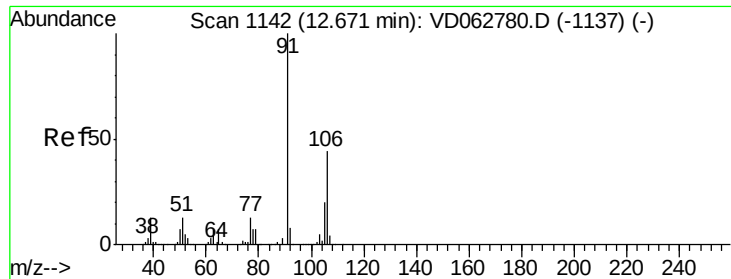

#68
m/p-Xylenes
Concen: 7.887 ug/l
RT: 12.67 min Scan# 1142
Delta R.T. -0.00 min
Lab File: VD062874.D
Acq: 25 Jun 2019 12:58




Instrument :
MSVOA_D
ClientSampleId :
BAT-B08


Tot Ion:106 Resp: 81926
Ion Ratio Lower Upper
106 100
91 243.0 183.0 274.6

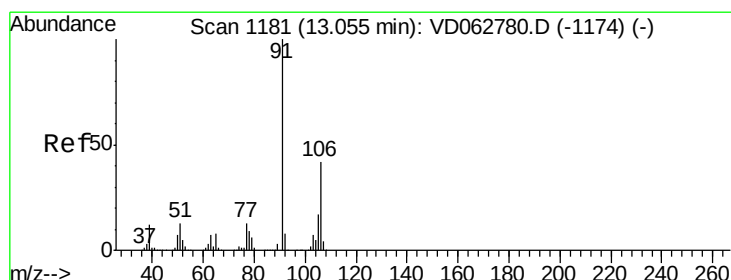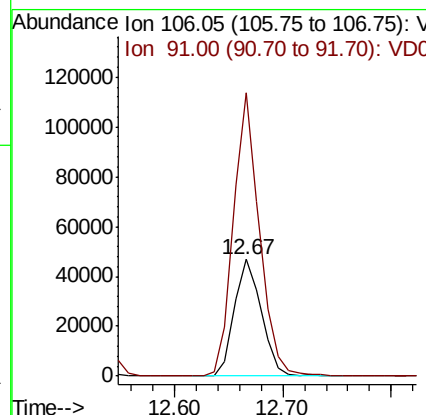

#69
o-Xylene
Concen: 3.532 ug/l
RT: 13.05 min Scan# 1181
Delta R.T. -0.00 min
Lab File: VD062874.D
Acq: 25 Jun 2019 12:58

Tgt Ion:106 Resp: 33538
Ion Ratio Lower Upper
106 100
91 232.4 117.9 353.6

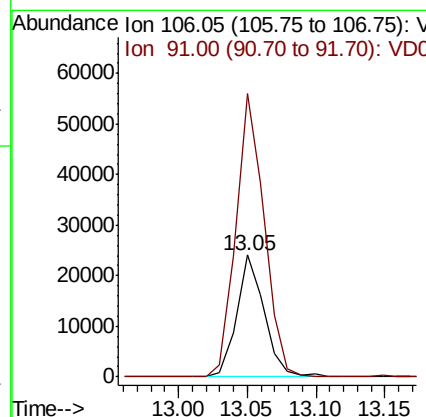


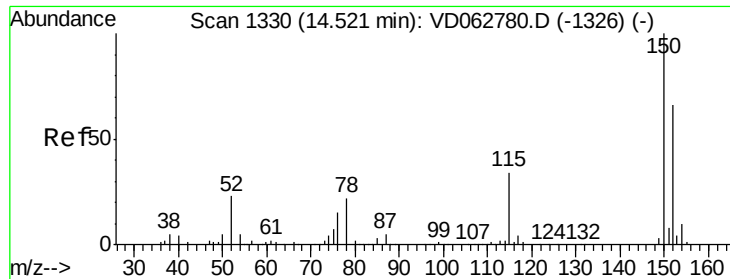




#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 14.53 min Scan# 1331
 Delta R.T. 0.01 min
 Lab File: VD062874.D
 Acq: 25 Jun 2019 12:58

Instrument :
 MSVOA_D
 ClientSampleId :
 BAT-B08

Tot Ion:152 Resp: 396741
 Ion Ratio Lower Upper
 152 100
 115 50.4 29.2 87.6
 150 150.0 0.0 305.8

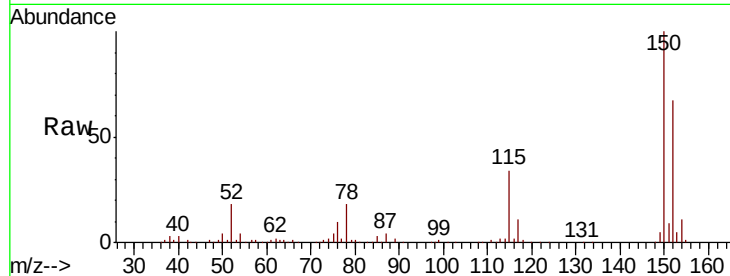


Abundance Ion 151.90 (151.60 to 152.60): V
 Ion 115.00 (114.70 to 115.70): V
 Ion 149.90 (149.60 to 150.60): V

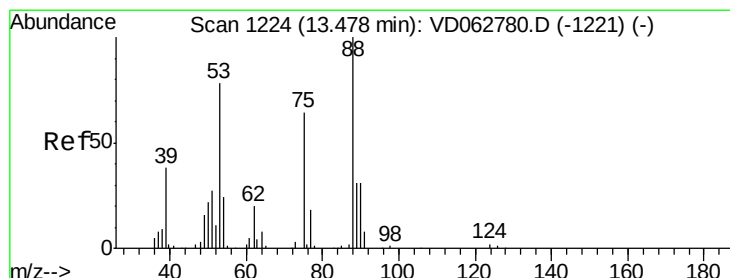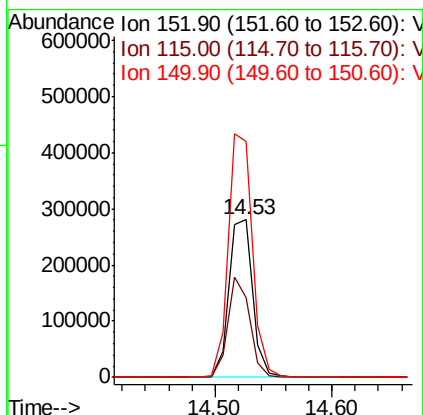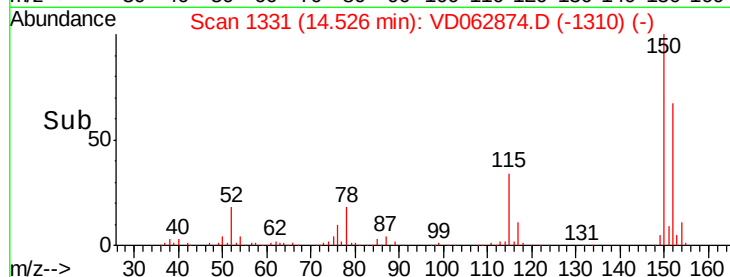

#81
 trans-1,4-Dichloro-2-butene
 Concen: 152.325 ug/l
 RT: 13.56 min Scan# 1233
 Delta R.T. 0.08 min
 Lab File: VD062874.D
 Acq: 25 Jun 2019 12:58

Tgt Ion: 75 Resp: 182846
 Ion Ratio Lower Upper
 75 100
 53 0.0 97.8 146.8#
 89 0.0 39.4 59.2#

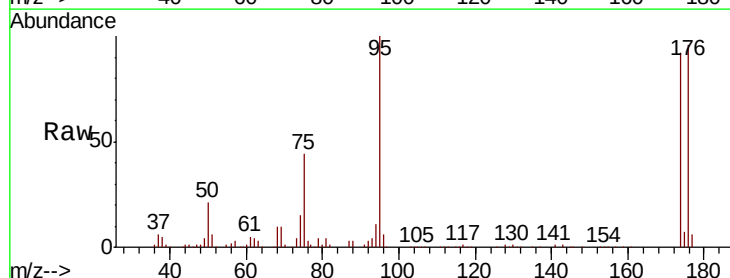

Abundance Ion 75.00 (74.70 to 75.70): VDC
 Ion 53.00 (52.70 to 53.70): VDC
 Ion 89.00 (88.70 to 89.70): VDC

