


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA D\DATA\VD062519\  
Data File : VD062891.D  
Acq On : 25 Jun 2019 21:36  
Operator : VA/AP  
Sample : BFB  
Misc : 5.00µl/5ml/MSVOA D/SOIL  
ALS Vial : 25 Sample Multiplier: 1

Instrument :  
MSVOA\_D  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\V0ASRV\HPCHEM1\MSVOA\_D\METHOD\82D061919S.M  
Title : SW846 8260  
Last Update : Thu Jun 20 01:50:56 2019

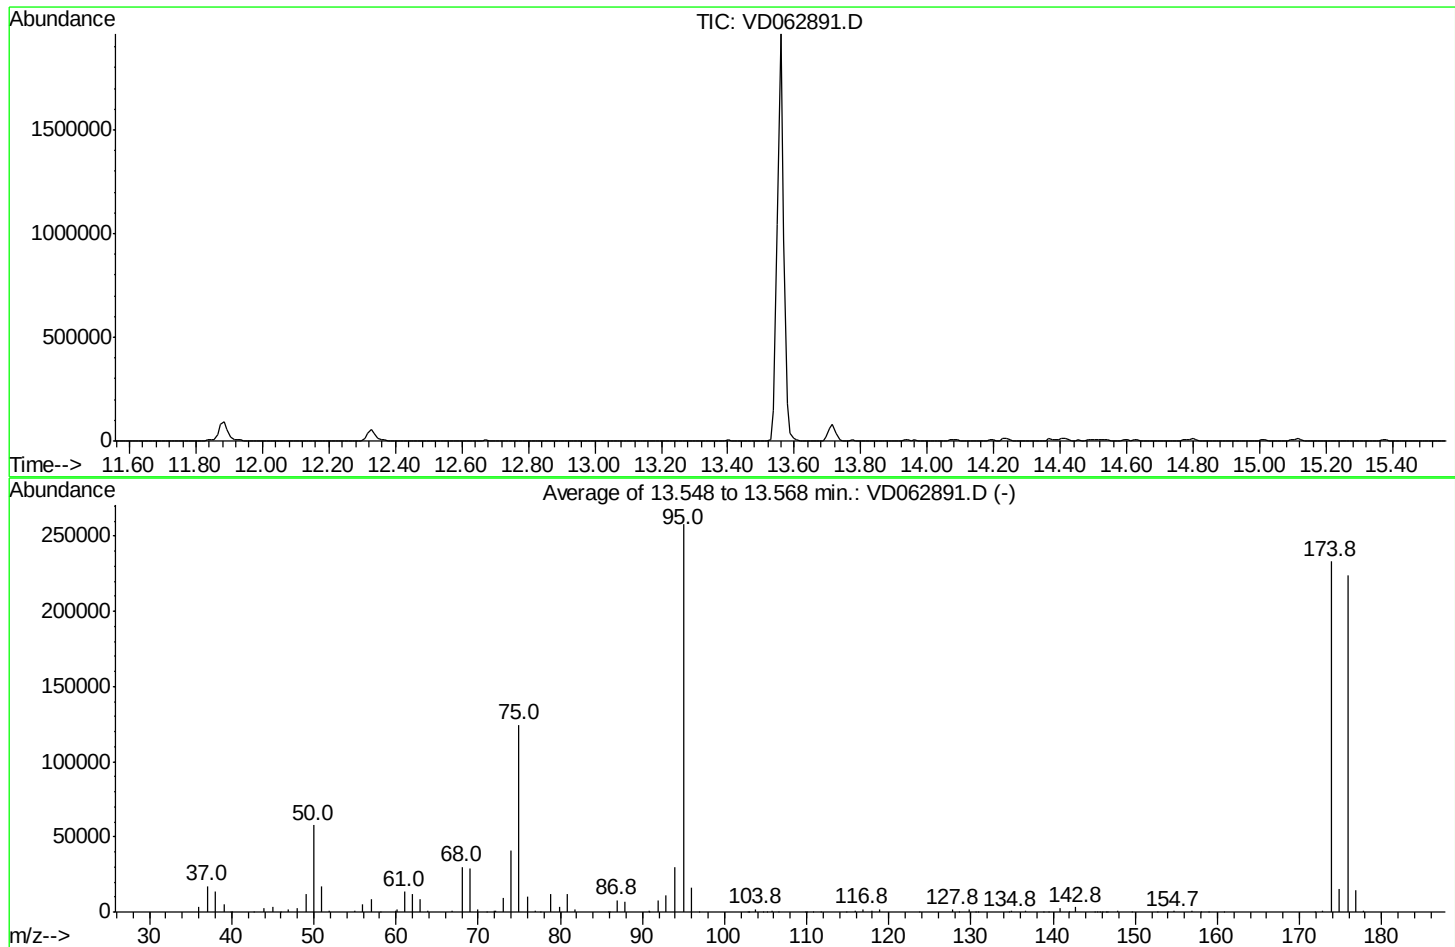

AutoFind: Scans 1231, 1232, 1233; Background Corrected with Scan 1226

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 22.4      | 57845   | PASS             |
| 75          | 95           | 30           | 60           | 48.2      | 124317  | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 257856  | PASS             |
| 96          | 95           | 5            | 9            | 6.4       | 16491   | PASS             |
| 173         | 174          | 0.00         | 2            | 0.3       | 690     | PASS             |
| 174         | 95           | 50           | 100          | 90.3      | 232938  | PASS             |
| 175         | 174          | 5            | 9            | 6.6       | 15480   | PASS             |
| 176         | 174          | 95           | 101          | 96.0      | 223704  | PASS             |
| 177         | 176          | 5            | 9            | 6.3       | 14090   | PASS             |