
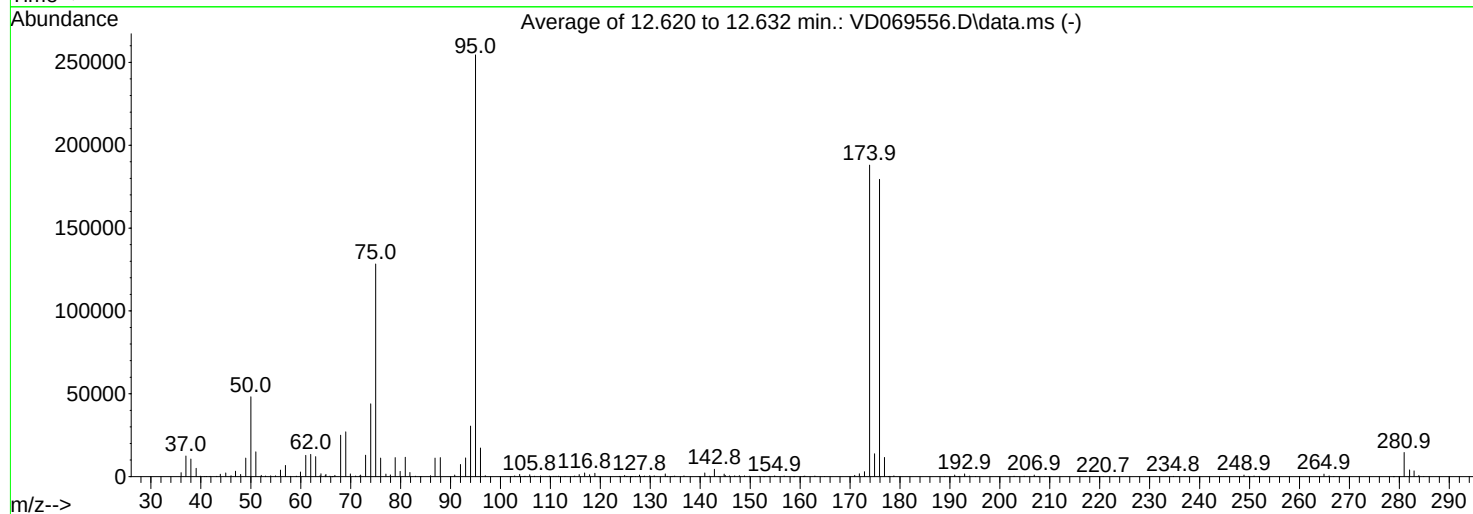


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_D\Data\VD062521\  
Data File : VD069556.D  
Acq On : 25 Jun 2021 09:54  
Operator : VA/SY  
Sample : BFB  
Misc : 5.00G/5.00ml/MSVOA\_D/SOIL  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_D  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_D\Method\82D062121S.M  
Title : SW846 8260  
Last Update : Tue Jun 22 04:33:24 2021

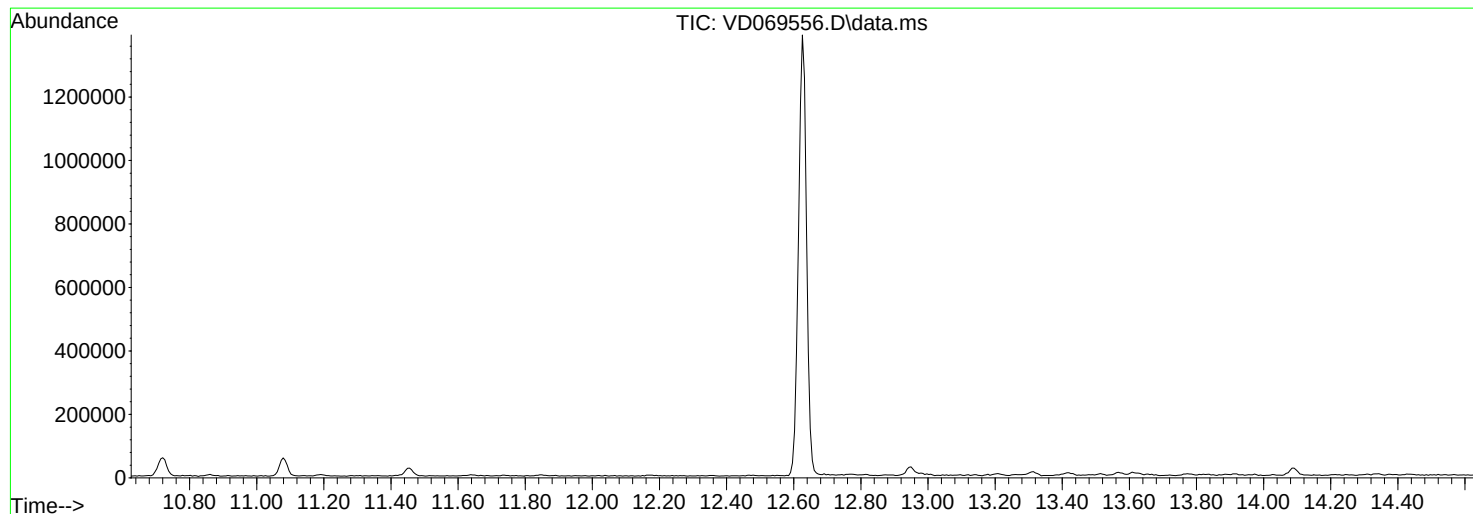

AutoFind: Scans 1819, 1820, 1821; Background Corrected with Scan 1810

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 50             | 95              | 15              | 40              | 18.9         | 48237      | PASS                |
| 75             | 95              | 30              | 60              | 50.4         | 128309     | PASS                |
| 95             | 95              | 100             | 100             | 100.0        | 254549     | PASS                |
| 96             | 95              | 5               | 9               | 6.8          | 17282      | PASS                |
| 173            | 174             | 0.00            | 2               | 1.6          | 2983       | PASS                |
| 174            | 95              | 50              | 100             | 73.9         | 187989     | PASS                |
| 175            | 174             | 5               | 9               | 7.4          | 13866      | PASS                |
| 176            | 174             | 95              | 101             | 95.4         | 179371     | PASS                |
| 177            | 176             | 5               | 9               | 6.5          | 11573      | PASS                |