

Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD062619\
 Data File : VD062921.D
 Acq On : 26 Jun 2019 16:53
 Operator : VA/AP
 Sample : K3526-07
 Misc : 5.06g/5ml/MSVOA D/SOIL
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 SB-04-9.5-10.0

Quant Time: Jun 27 09:28:07 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D061919S.M
 Quant Title : SW846 8260
 QLast Update : Thu Jun 20 01:50:56 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.05	168	770726	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.22	114	1029521	50.00	ug/l	0.00
63) Chlorobenzene-d5	12.36	117	868984	50.00	ug/l	-0.01
72) 1,4-Dichlorobenzene-d4	14.52	152	491159	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	7.45	65	413573	49.37	ug/l	-0.01
Spiked Amount	50.000		Recovery	=	98.74%	
35) Dibromofluoromethane	6.93	113	449489	51.78	ug/l	0.00
Spiked Amount	50.000		Recovery	=	103.56%	
50) Toluene-d8	10.41	98	965399	51.10	ug/l	0.00
Spiked Amount	50.000		Recovery	=	102.20%	
62) 4-Bromofluorobenzene	13.55	95	404690	47.11	ug/l	0.00
Spiked Amount	50.000		Recovery	=	94.22%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA D\DATA\VD062619\
Data File : VD062921.D
Acq On : 26 Jun 2019 16:53
Operator : VA/AP
Sample : K3526-07
Misc : 5.06g/5ml/MSVOA D/SOIL
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
SB-04-9.5-10.0

Quant Time: Jun 27 09:28:07 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_D\METHOD\82D061919S.M
Quant Title : SW846 8260
QLast Update : Thu Jun 20 01:50:56 2019
Response via : Initial Calibration

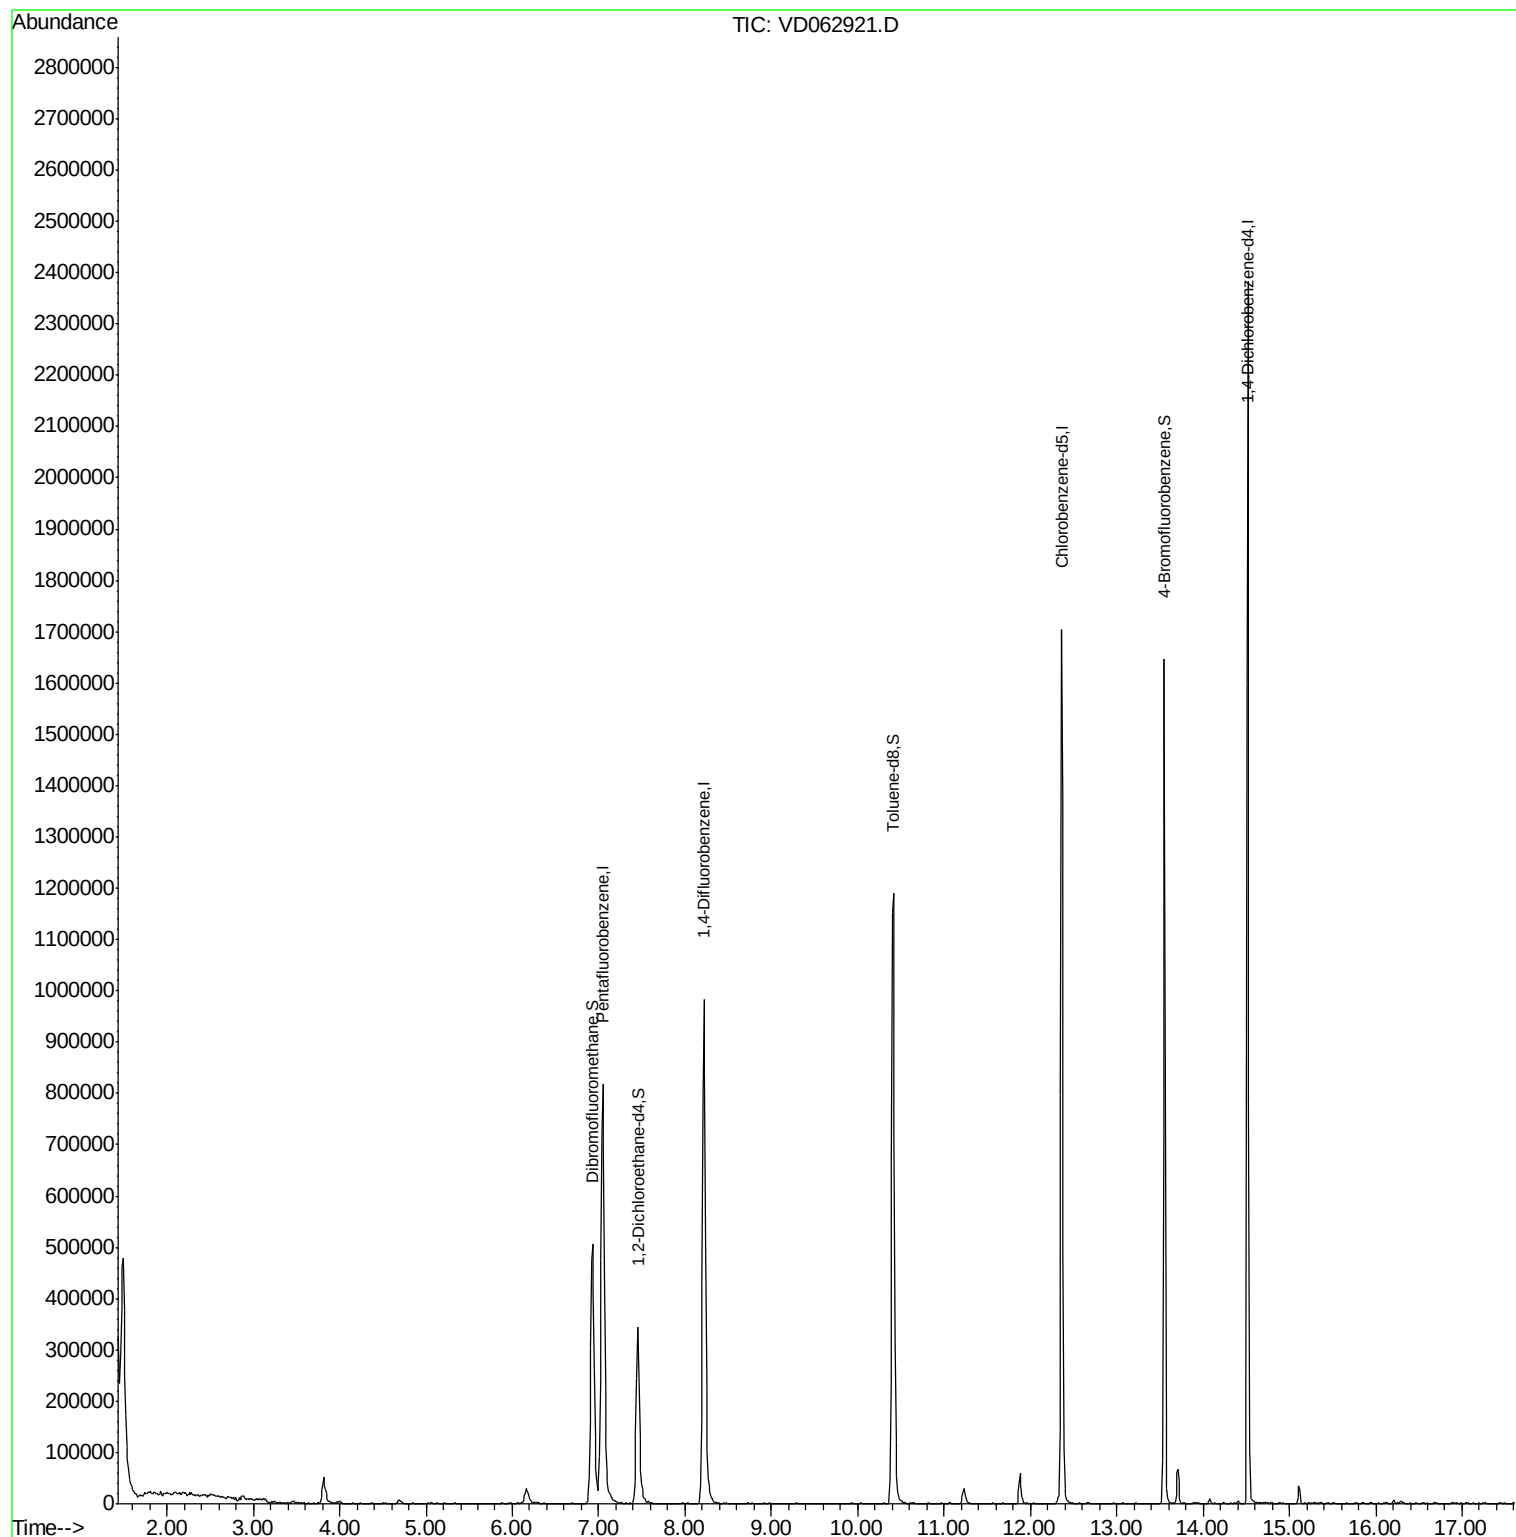

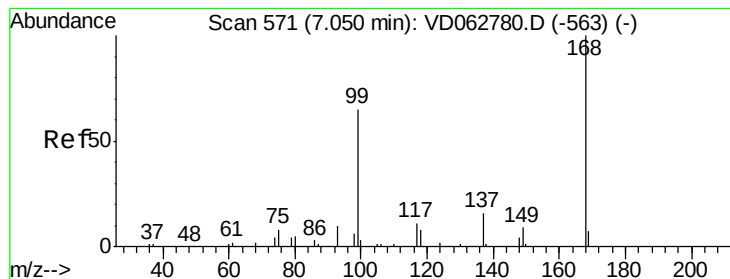

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.05 min Scan# 571

Delta R.T. -0.00 min

Lab File: VD062921.D

Acq: 26 Jun 2019 16:53

Instrument :

MSVOA_D

ClientSampleId :


SB-04-9.5-10.0

Tot Ion:168 Resp: 770726

Ion Ratio Lower Upper




168 100

99 64.8 53.0 79.6

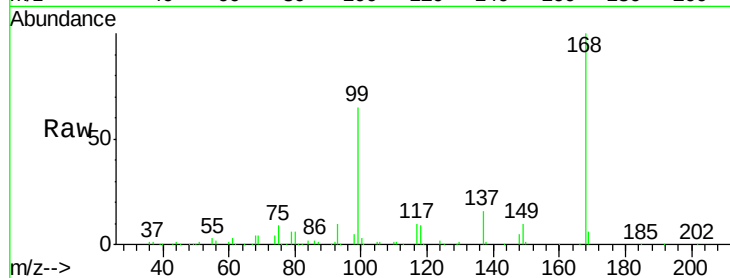

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.95 (98.65 to 99.65): VDC

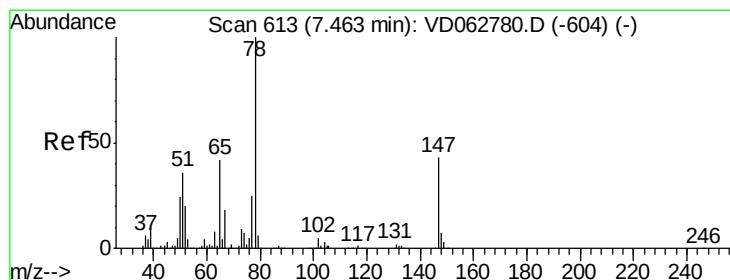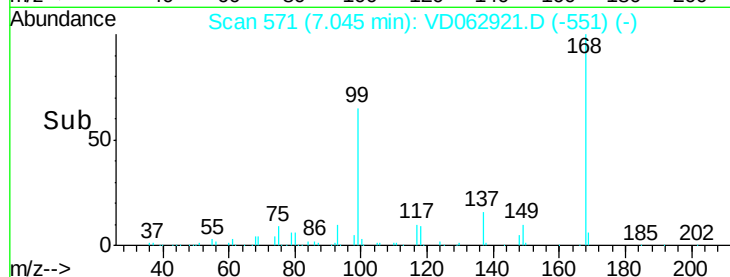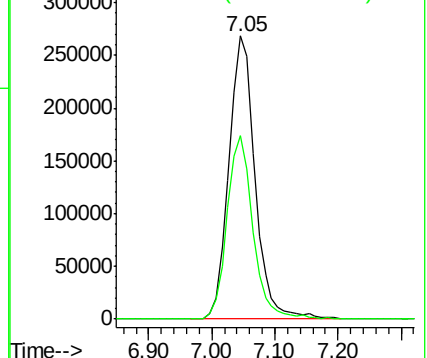

#33

1,2-Dichloroethane-d4

Concen: 49.366 ug/l

RT: 7.45 min Scan# 612

Delta R.T. -0.01 min

Lab File: VD062921.D


Acq: 26 Jun 2019 16:53

Tgt Ion: 65 Resp: 413573

Ion Ratio Lower Upper



65 100


67 40.4 0.0 87.4

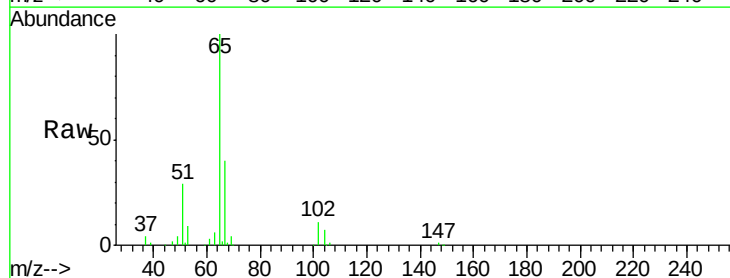

Abundance Ion 64.95 (64.65 to 65.65): VDC

Ion 66.90 (66.60 to 67.60): VDC

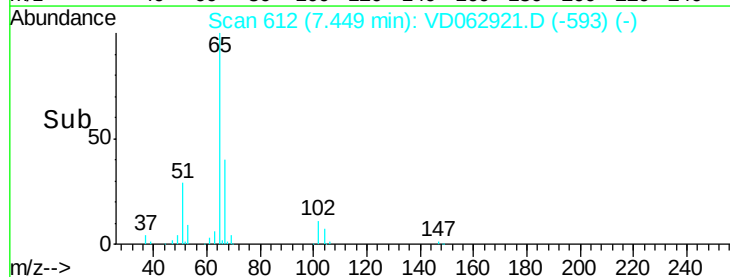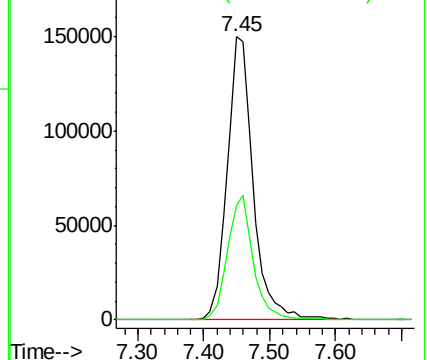


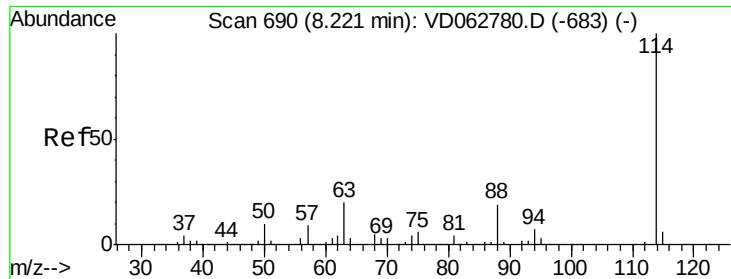




#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.22 min Scan# 690
 Delta R.T. -0.00 min
 Lab File: VD062921.D
 Acq: 26 Jun 2019 16:53

Instrument :
 MSVOA_D
 ClientSampleId :
 SB-04-9.5-10.0

Tot Ion:114 Resp: 1029521
 Ion Ratio Lower Upper
 114 100
 63 19.7 0.0 40.0
 88 18.8 0.0 38.8

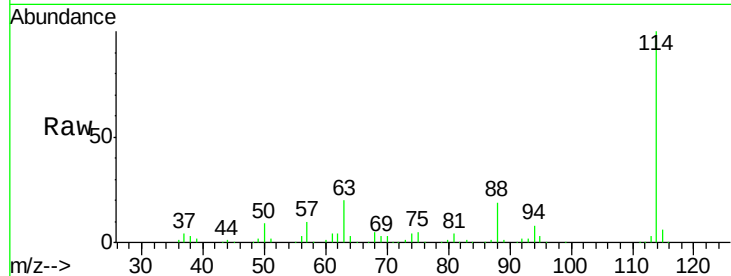


Abundance Ion 114.00 (113.70 to 114.70): V
 Ion 62.95 (62.65 to 63.65): V
 Ion 87.90 (87.60 to 88.60): V

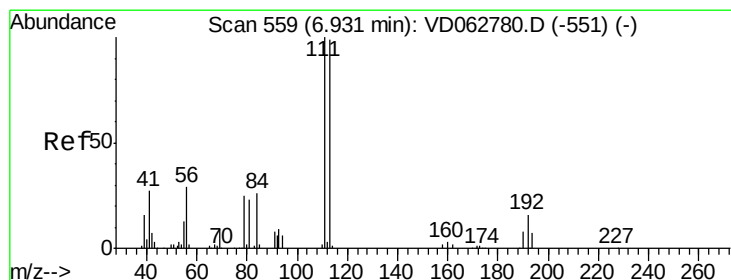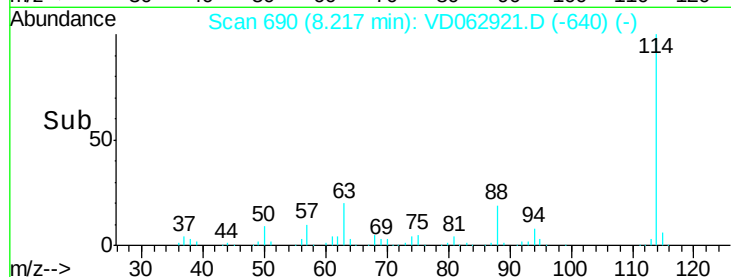
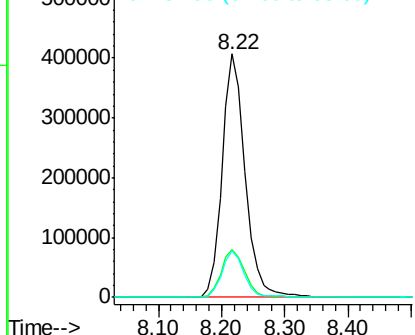



#35
 Dibromofluoromethane
 Concen: 51.779 ug/l
 RT: 6.93 min Scan# 559
 Delta R.T. -0.00 min
 Lab File: VD062921.D
 Acq: 26 Jun 2019 16:53

Tgt Ion:113 Resp: 449489
 Ion Ratio Lower Upper
 113 100
 111 110.0 81.2 121.8
 192 19.4 12.9 19.3#

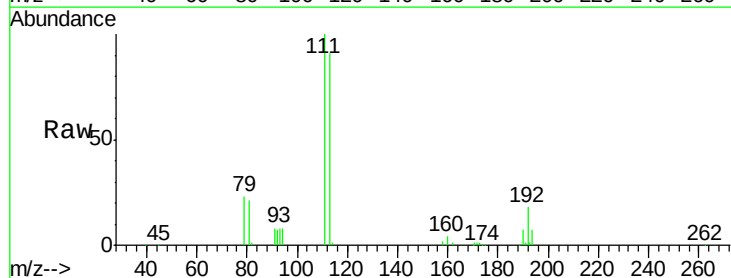

Abundance Ion 112.90 (112.60 to 113.60): V
 Ion 110.90 (110.60 to 111.60): V
 Ion 191.80 (191.50 to 192.50): V



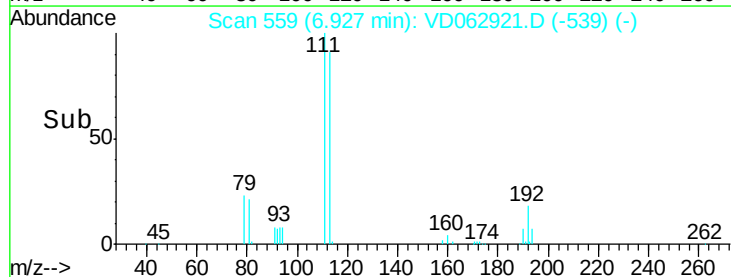
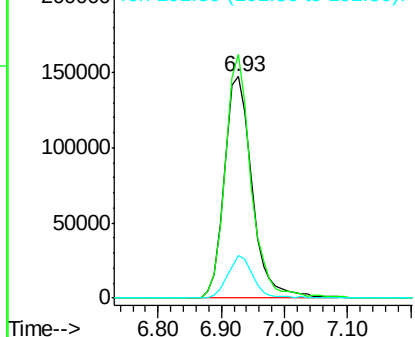


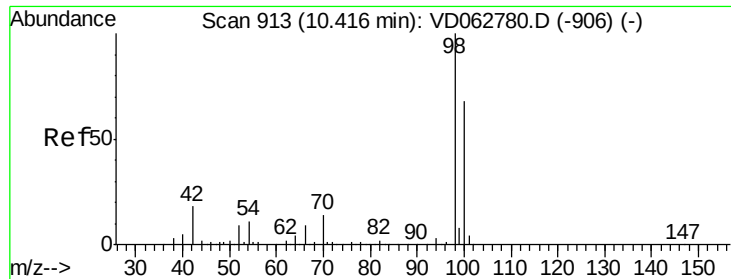

#50
Toluene-d8
Concen: 51.097 ug/l
RT: 10.41 min Scan# 913
Delta R.T. -0.00 min
Lab File: VD062921.D
Acq: 26 Jun 2019 16:53




Instrument :
MSVOA_D
ClientSampleId :
SB-04-9.5-10.0


Tot Ion: 98 Resp: 965399
Ion Ratio Lower Upper
98 100
100 69.2 54.7 82.1

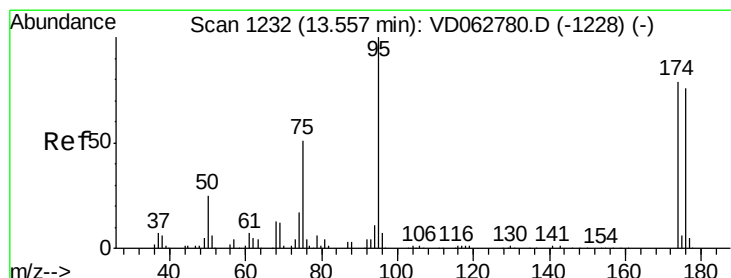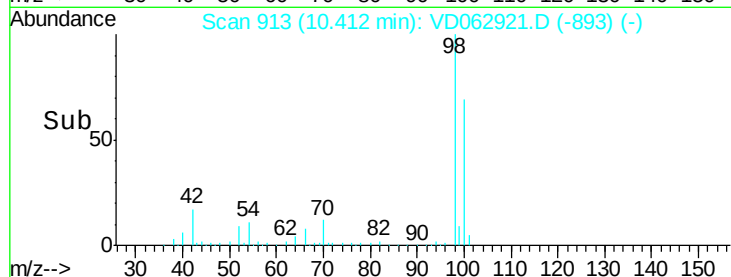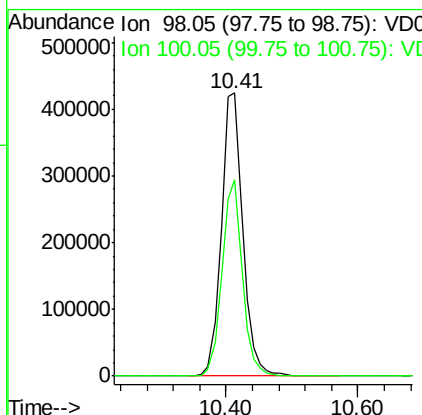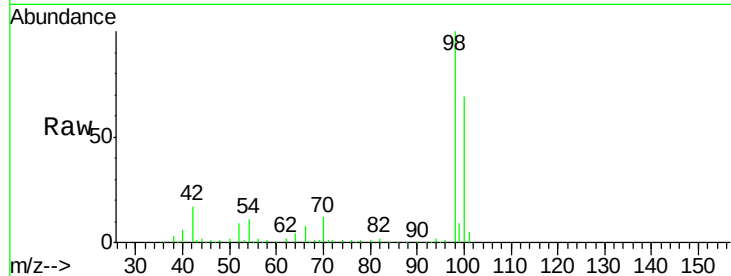

#62
4-Bromofluorobenzene
Concen: 47.106 ug/l
RT: 13.55 min Scan# 1232
Delta R.T. -0.00 min
Lab File: VD062921.D
Acq: 26 Jun 2019 16:53

Tgt Ion: 95 Resp: 404690
Ion Ratio Lower Upper
95 100
174 88.8 0.0 158.0
176 80.6 0.0 151.6


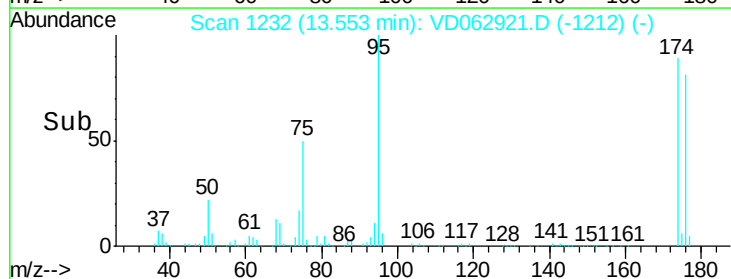
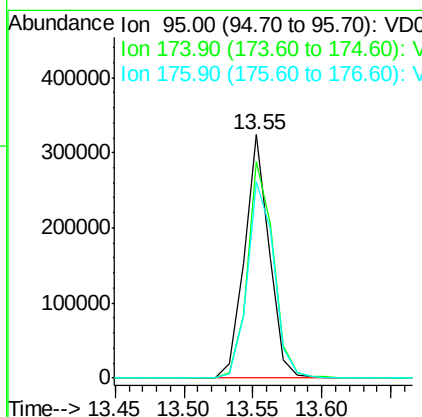
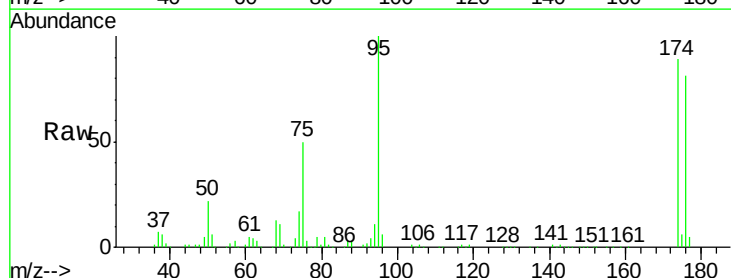


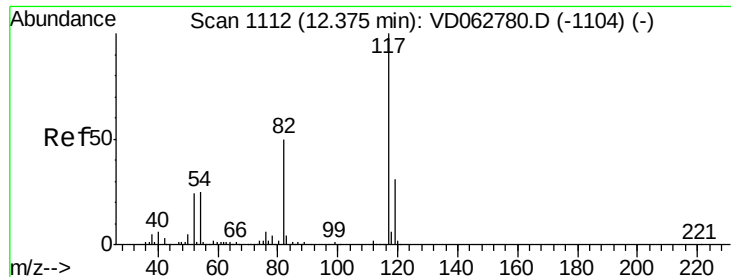

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 12.36 min Scan# 1111
Delta R.T. -0.01 min
Lab File: VD062921.D
Acq: 26 Jun 2019 16:53

Instrument :
MSVOA_D
ClientSampleId :
SB-04-9.5-10.0

Tot Ion:117 Resp: 868984
Ion Ratio Lower Upper
117 100
82 57.7 40.4 60.6
119 32.6 25.2 37.8

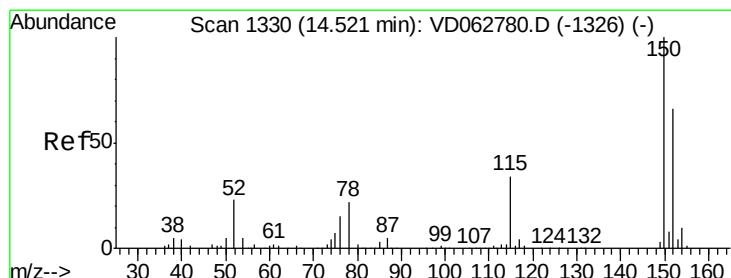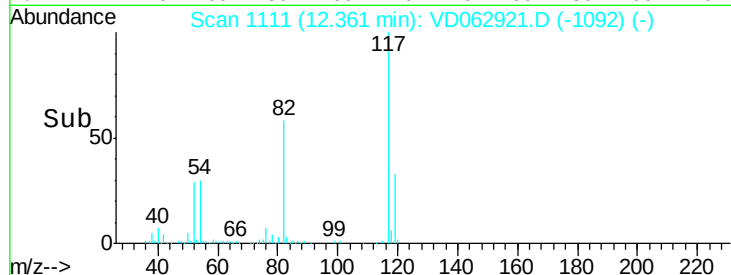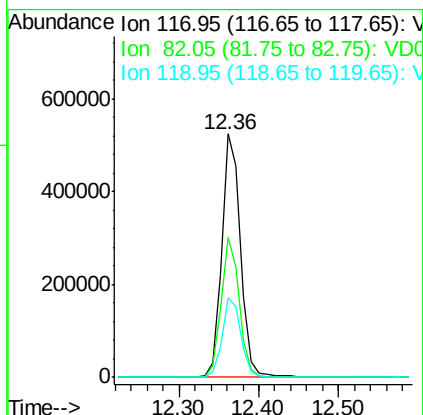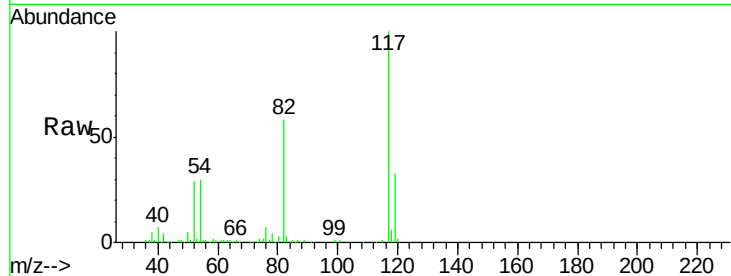

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 14.52 min Scan# 1330
Delta R.T. -0.00 min
Lab File: VD062921.D
Acq: 26 Jun 2019 16:53

Tgt Ion:152 Resp: 491159
Ion Ratio Lower Upper
152 100
115 58.3 29.2 87.6
150 154.9 0.0 305.8

