


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD062718\  
 Data File : VD059437.D  
 Acq On : 27 Jun 2018 10:31  
 Operator : VA/AP  
 Sample : BFB  
 Misc : 5.00µ/5ml/MSVOA D/SOIL  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_D  
 ClientSampled :  
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_D\METHOD\82D062518S.M  
 Title : SW846 8260  
 Last Update : Mon Jun 25 07:29:35 2018

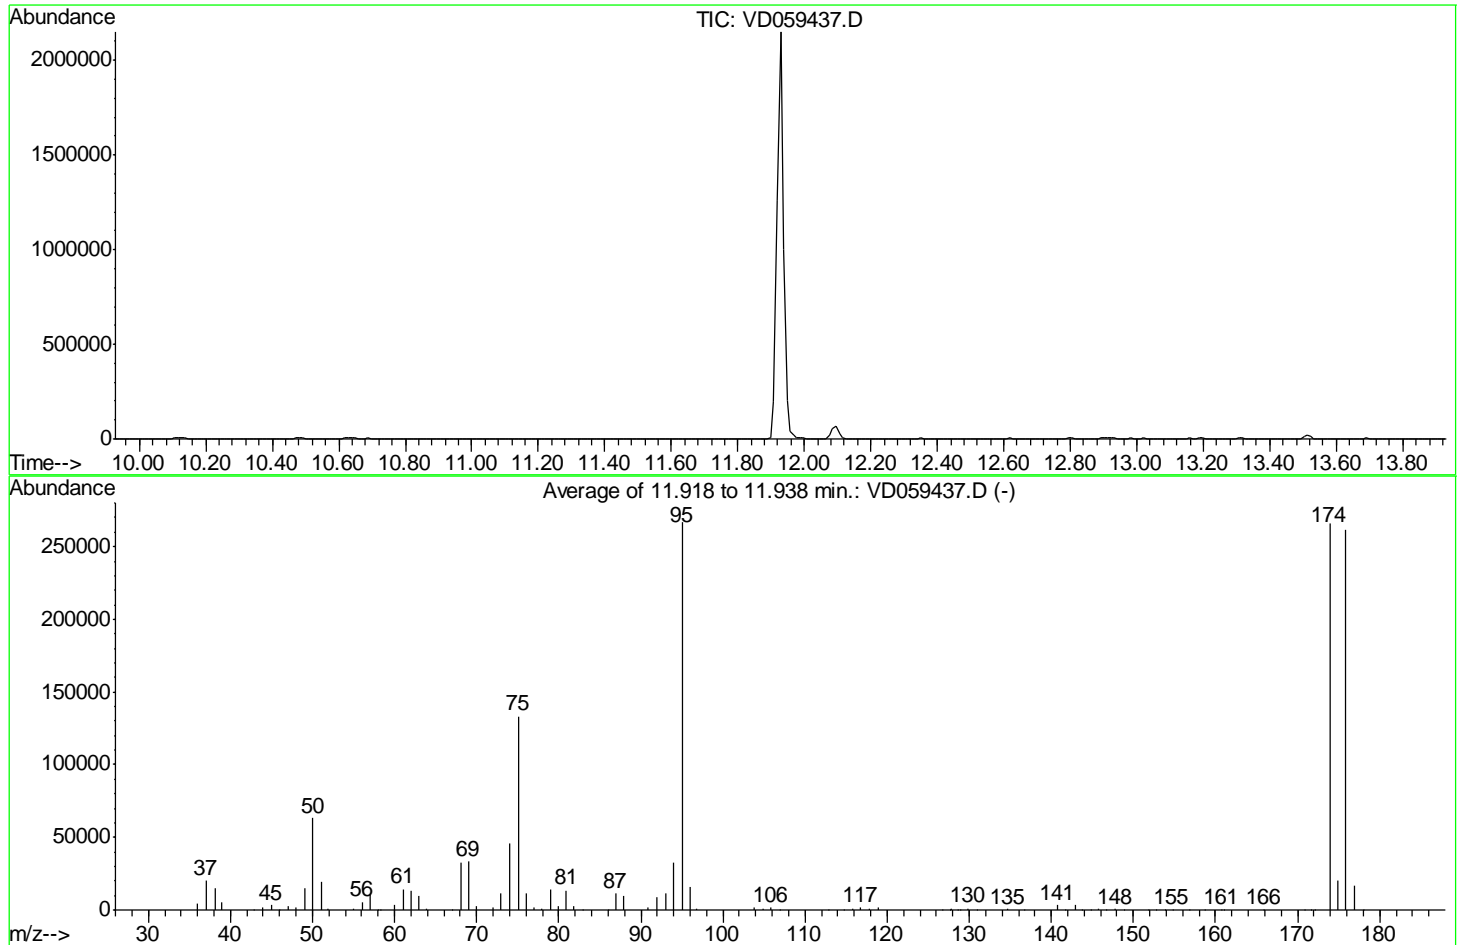

AutoFind: Scans 1188, 1189, 1190; Background Corrected with Scan 1183

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.7	63112	PASS
75	95	30	60	49.9	133045	PASS
95	95	100	100	100.0	266752	PASS
96	95	5	9	6.1	16317	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	99.6	265792	PASS
175	174	5	9	7.6	20235	PASS
176	174	95	101	98.3	261226	PASS
177	176	5	9	6.3	16574	PASS