

Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD062719\
 Data File : VD062940.D
 Acq On : 27 Jun 2019 19:11
 Operator : VA/AP
 Sample : K3552-04
 Misc : 5.00g/5ml/MSVOA D/SOIL
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 M-2A

Integration Parameters: RTEINT.P

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D061919S.M

Title : SW846 8260

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.705	25	28	29	rBV	7309	9456	1.79%	0.295%
2	1.745	29	32	33	rBV	6099	10690	2.03%	0.334%
3	1.833	39	41	42	rBV2	7971	9149	1.73%	0.286%
4	1.971	54	55	56	rBV2	5917	5334	1.01%	0.167%
5	2.089	62	67	69	rBV2	8255	21960	4.16%	0.686%
6	2.266	82	85	87	rVV3	5970	12006	2.28%	0.375%
7	2.316	87	90	91	rVB2	9021	9848	1.87%	0.307%
8	2.729	129	132	134	rVB2	3379	5439	1.03%	0.170%
9	2.847	142	144	147	rBV	4054	7606	1.44%	0.237%
10	3.024	161	162	165	rVB2	4881	5621	1.07%	0.175%
11	3.162	173	176	178	rVV	4751	8141	1.54%	0.254%
12	3.211	180	181	187	rVB2	6445	12136	2.30%	0.379%
13	3.448	200	205	212	rVB2	3969	12429	2.36%	0.388%
14	3.782	238	239	244	rBV3	4234	9194	1.74%	0.287%
15	3.960	253	257	263	rBV2	8468	19536	3.70%	0.610%
16	6.135	471	478	489	rBV2	83952	288735	54.73%	9.015%
17	6.893	549	555	561	rBV2	85527	241303	45.74%	7.534%
18	7.021	563	568	573	rVB2	59258	159429	30.22%	4.978%
19	7.425	603	609	616	rBV	98057	269291	51.05%	8.408%
20	8.193	681	687	695	rBV	118730	293594	55.65%	9.166%
21	10.280	895	899	902	rBB	2431	5439	1.03%	0.170%
22	10.388	905	910	917	rVV	132365	290118	54.99%	9.058%
23	11.215	989	994	1000	rBV2	14328	39050	7.40%	1.219%
24	11.865	1056	1060	1064	rBV2	25814	48537	9.20%	1.515%
25	12.347	1105	1109	1119	rVB	266158	468402	88.79%	14.624%
26	13.548	1227	1231	1238	rBV	273091	401295	76.07%	12.529%
27	13.696	1242	1246	1251	rVV	7024	11635	2.21%	0.363%
28	14.503	1325	1328	1332	rBV	387482	527553	100.00%	16.471%


Sum of corrected areas: 3202926

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA D\DATA\VD062719\
Data File : VD062940.D
Acq On : 27 Jun 2019 19:11
Operator : VA/AP
Sample : K3552-04
Misc : 5.00µl/5ml/MSVOA D/SOIL
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
M-2A

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_D\METHOD\82D061919S.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

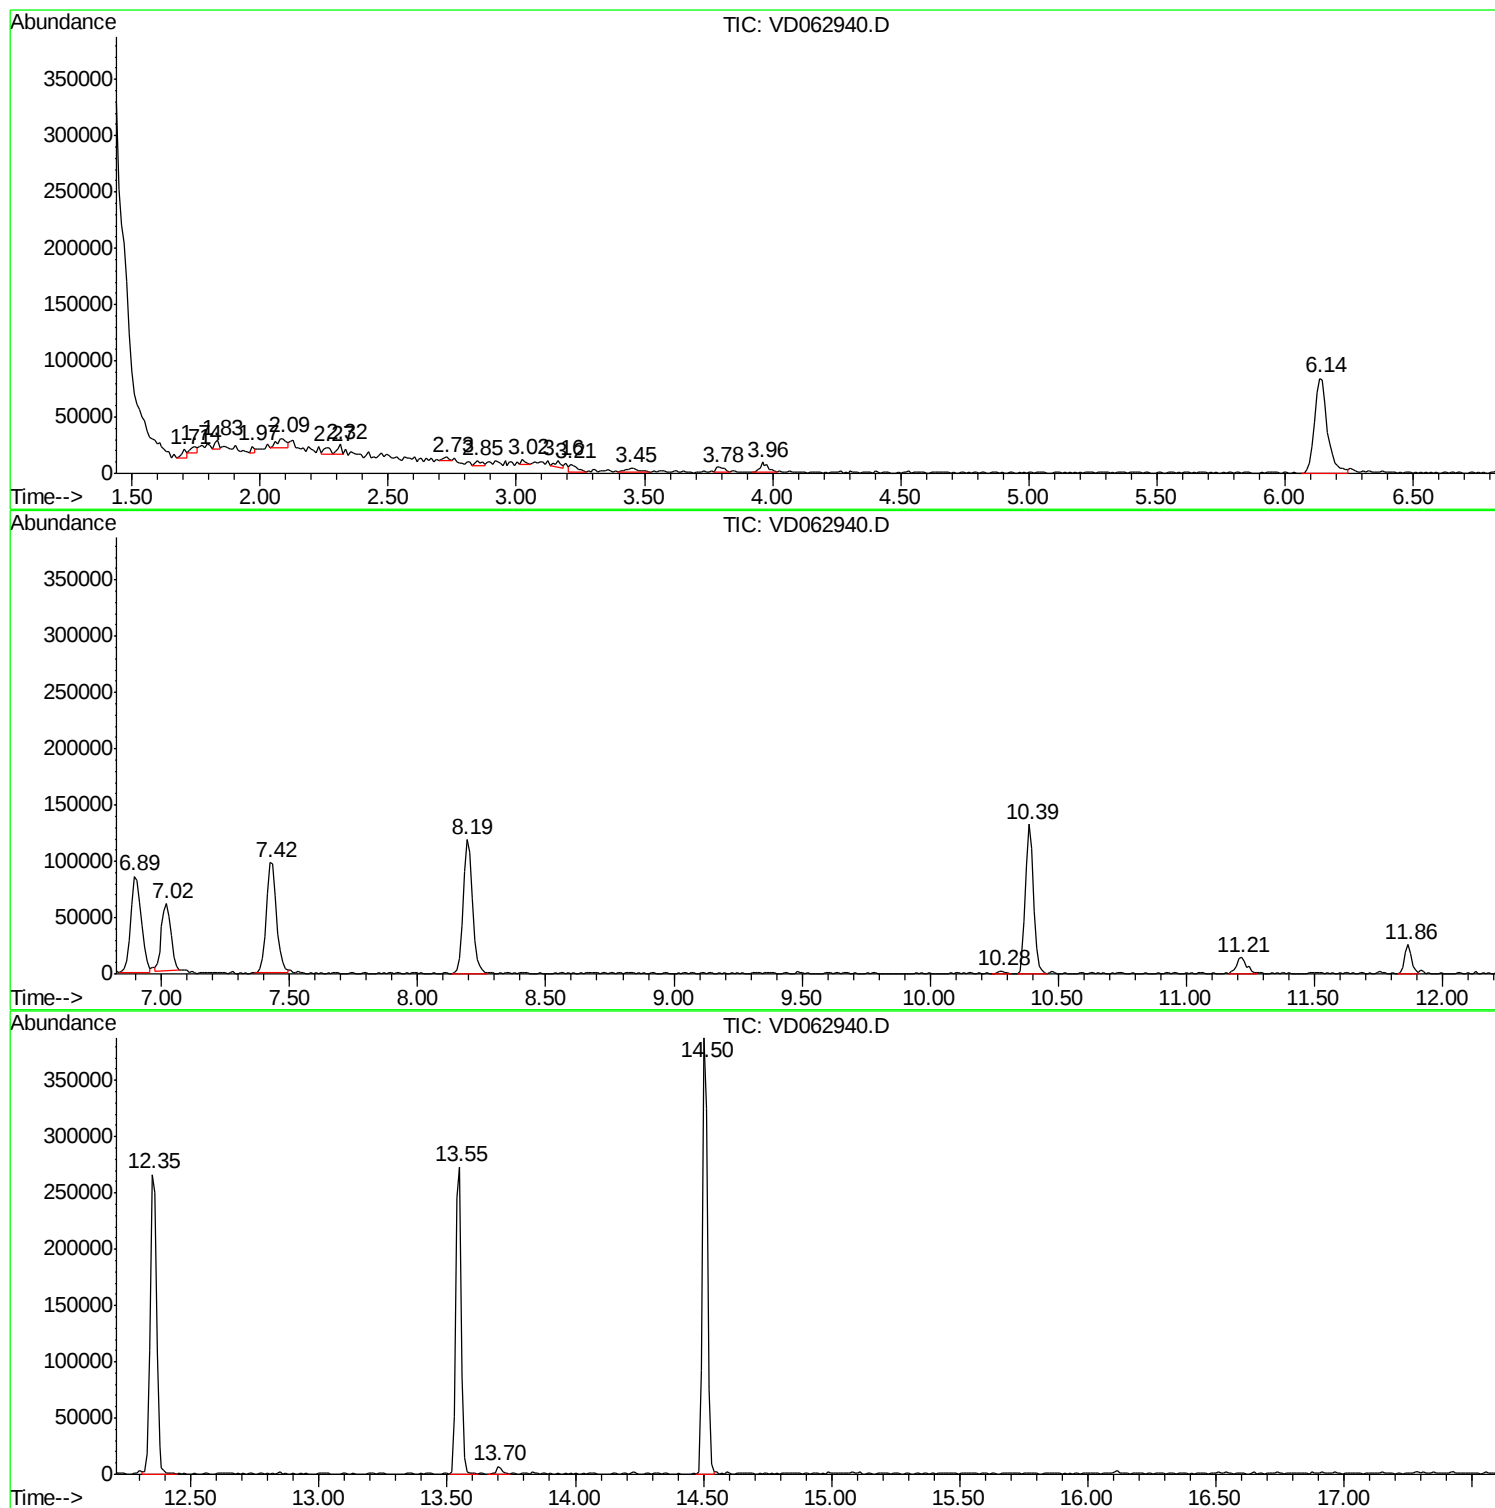

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA D\DATA\VD062719\
Data File : VD062940.D
Acq On : 27 Jun 2019 19:11
Operator : VA/AP
Sample : K3552-04
Misc : 5.00µl/5ml/MSVOA D/SOIL
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
M-2A










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_D\METHOD\82D061919S.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 4 unknown11.86 Concentration Rank 4

R.T.	EstConc	Area	Relative to ISTD	R.T.
11.86	5.18 ug/l	48537	Chlorobenzene-d5	12.36

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	1,2,4-Triazole, 3,5-dithioxo-	133	C2H3N3S2	005650-03-3	27
2		5-Methyl-7-amino-s-triazolo(1,5-...	149	C6H7N5	033376-96-4	25
3		Tricyclo[4.3.1.1(3,8)]undecane, ...	184	C11H17Cl	027011-46-7	17
4		6-Methylthieno[2,3-b]pyridine	149	C8H7NS	001759-30-4	16
5		1,3-Dioxolane, 2-phenyl-	150	C9H10O2	000936-51-6	9

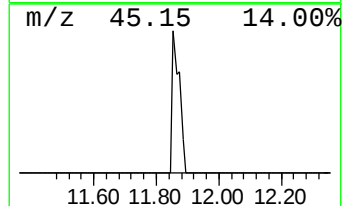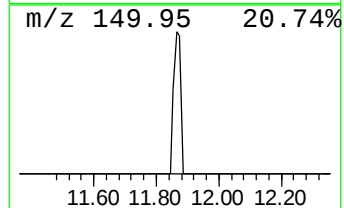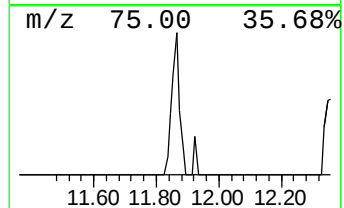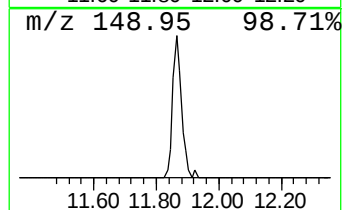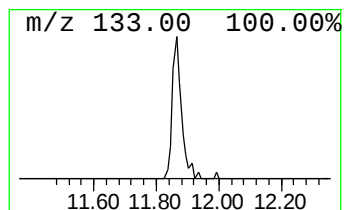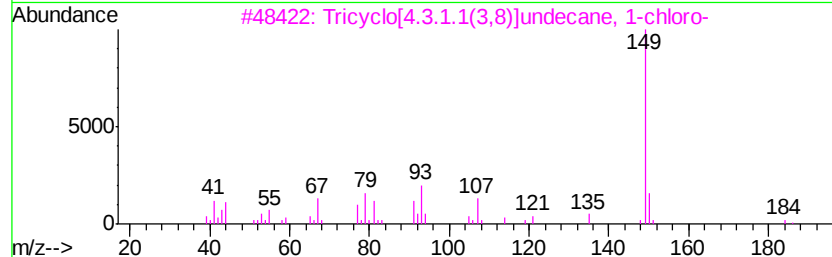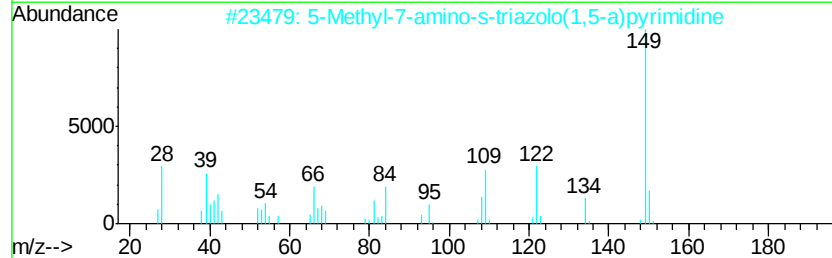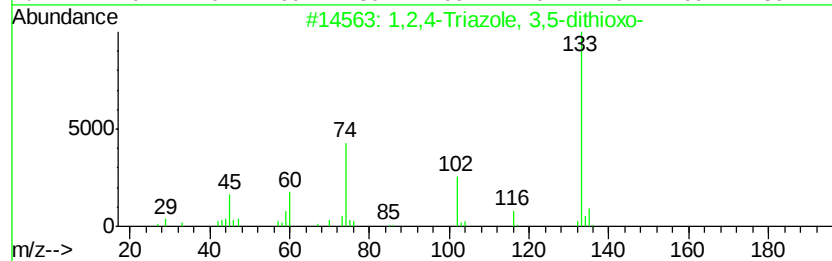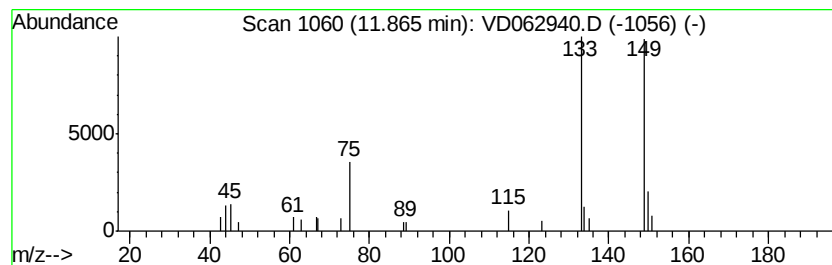

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_D\DATA\VD062719\
Data File : VD062940.D
Acq On : 27 Jun 2019 19:11
Operator : VA/AP
Sample : K3552-04
Misc : 5.00g/5ml/MSVOA_D/SOIL
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
M-2A

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_D\METHOD\82D061919S.M
Quant Title : SW846 8260

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown11.86	11.86	5.2	ug/l	48537	3	12.36	468402	50.0