


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD062719\  
 Data File : VD062923.D  
 Acq On : 27 Jun 2019 10:19  
 Operator : VA/AP  
 Sample : BFB  
 Misc : 5.00µ/5ml/MSVOA D/SOIL  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 MSVOA\_D  
 ClientSampleId :  
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_D\METHOD\82D061919S.M  
 Title : SW846 8260  
 Last Update : Thu Jun 20 01:50:56 2019

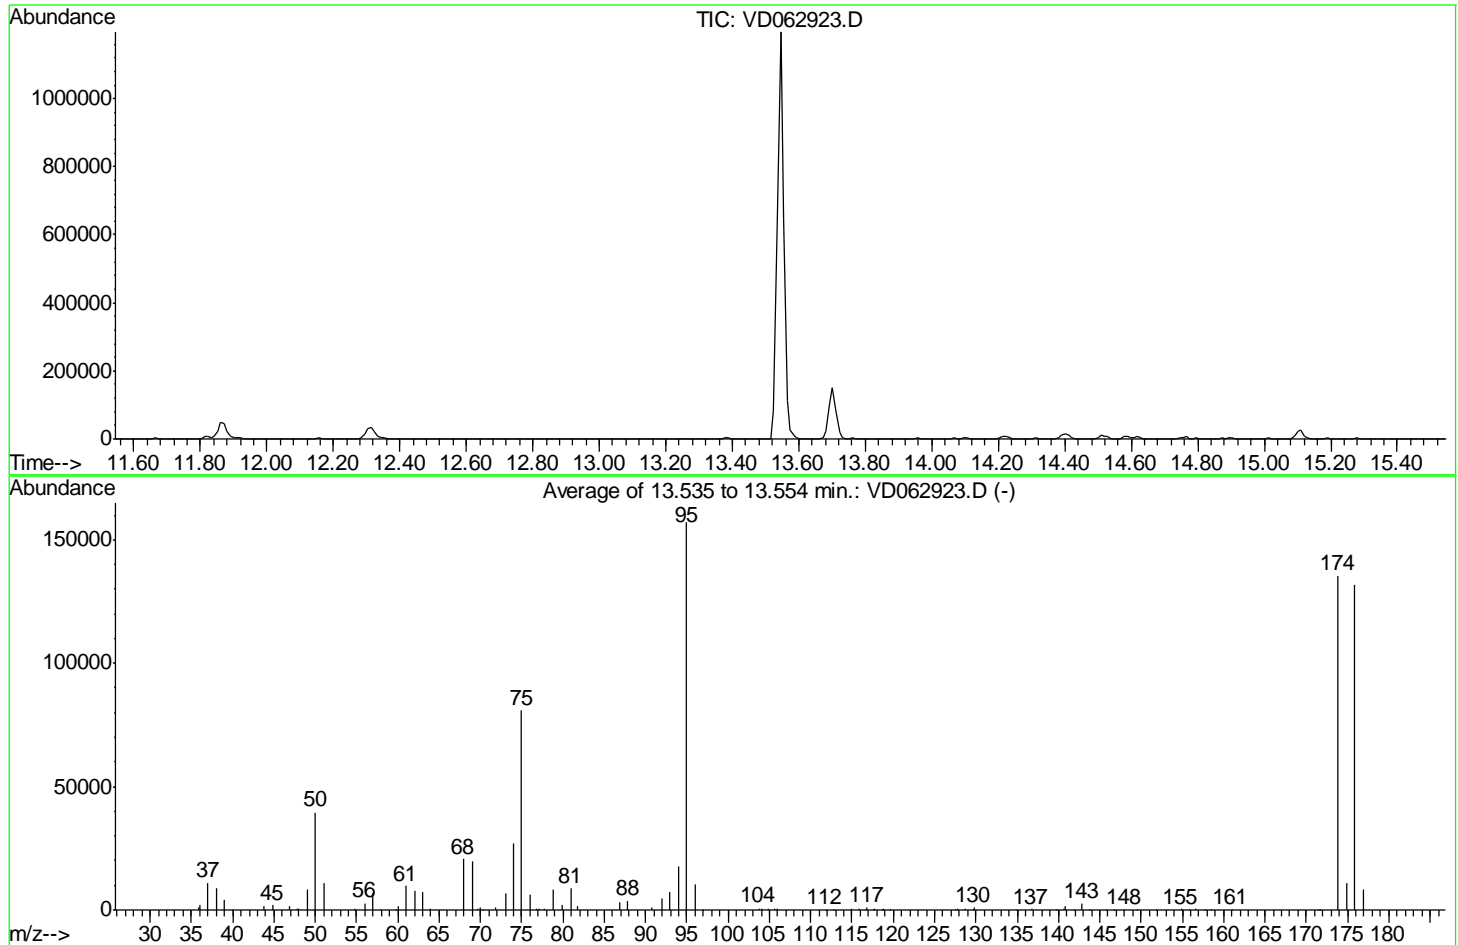

AutoFind: Scans 1230, 1231, 1232; Background Corrected with Scan 1225

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	25.2	39610	PASS
75	95	30	60	51.5	80850	PASS
95	95	100	100	100.0	157064	PASS
96	95	5	9	6.7	10463	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	86.3	135592	PASS
175	174	5	9	7.9	10693	PASS
176	174	95	101	97.2	131768	PASS
177	176	5	9	6.2	8141	PASS