


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD062719\
Data File : VD062947.D
Acq On : 27 Jun 2019 22:50
Operator : VA/AP
Sample : BFB
Misc : 5.00µl/5ml/MSVOA D/SOIL
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D061919S.M
Title : SW846 8260
Last Update : Thu Jun 20 01:50:56 2019

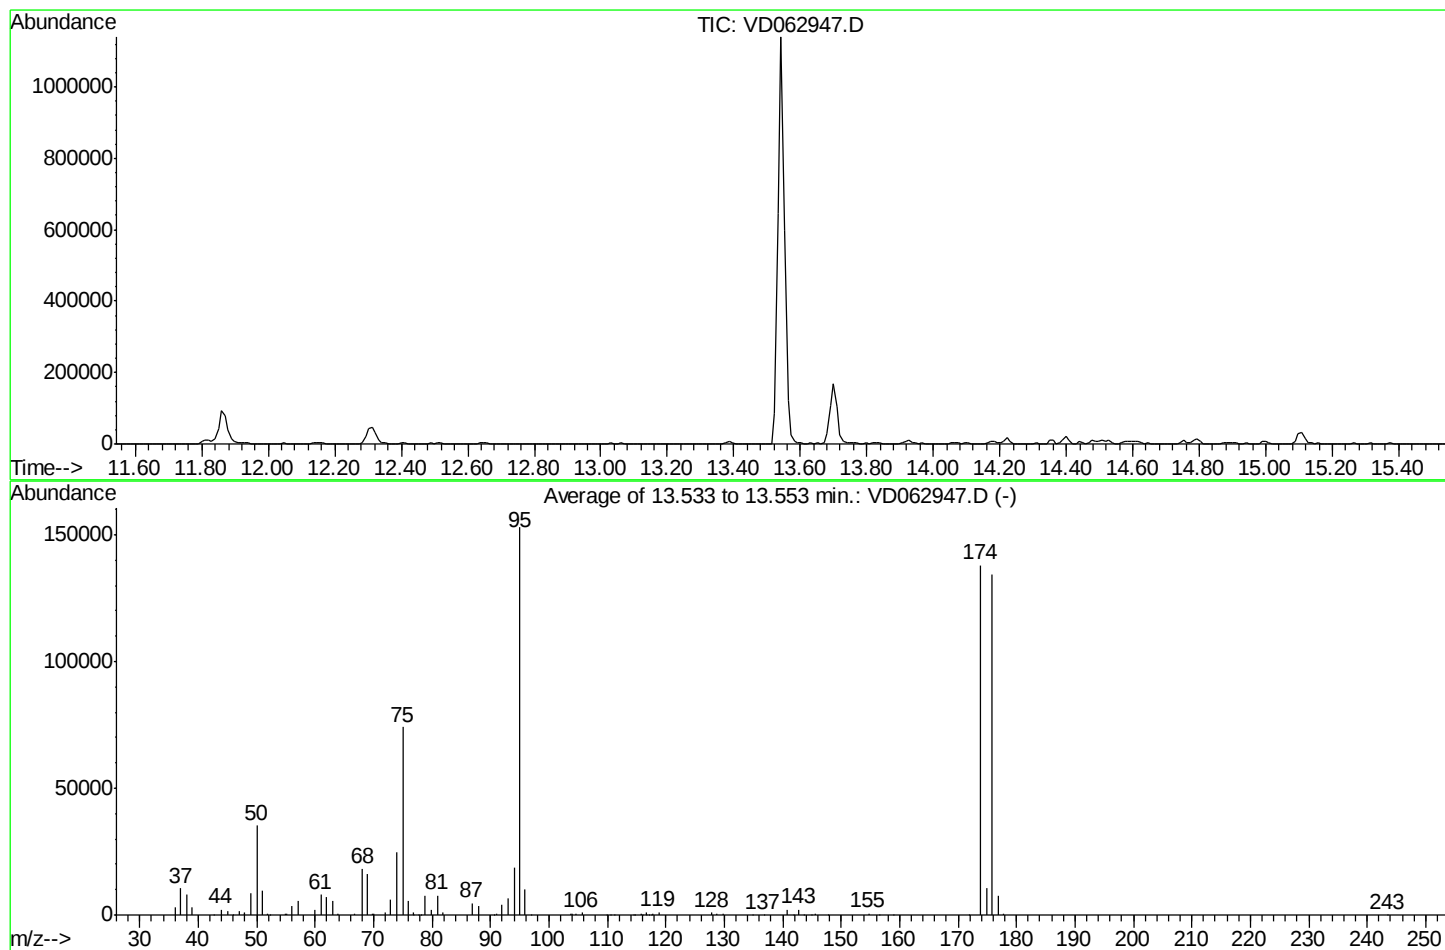

AutoFind: Scans 1230, 1231, 1232; Background Corrected with Scan 1225

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.0	35184	PASS
75	95	30	60	48.4	74122	PASS
95	95	100	100	100.0	152989	PASS
96	95	5	9	6.5	9959	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	90.3	138093	PASS
175	174	5	9	7.6	10557	PASS
176	174	95	101	97.2	134274	PASS
177	176	5	9	5.7	7656	PASS