



Dichlorodifluoromethane

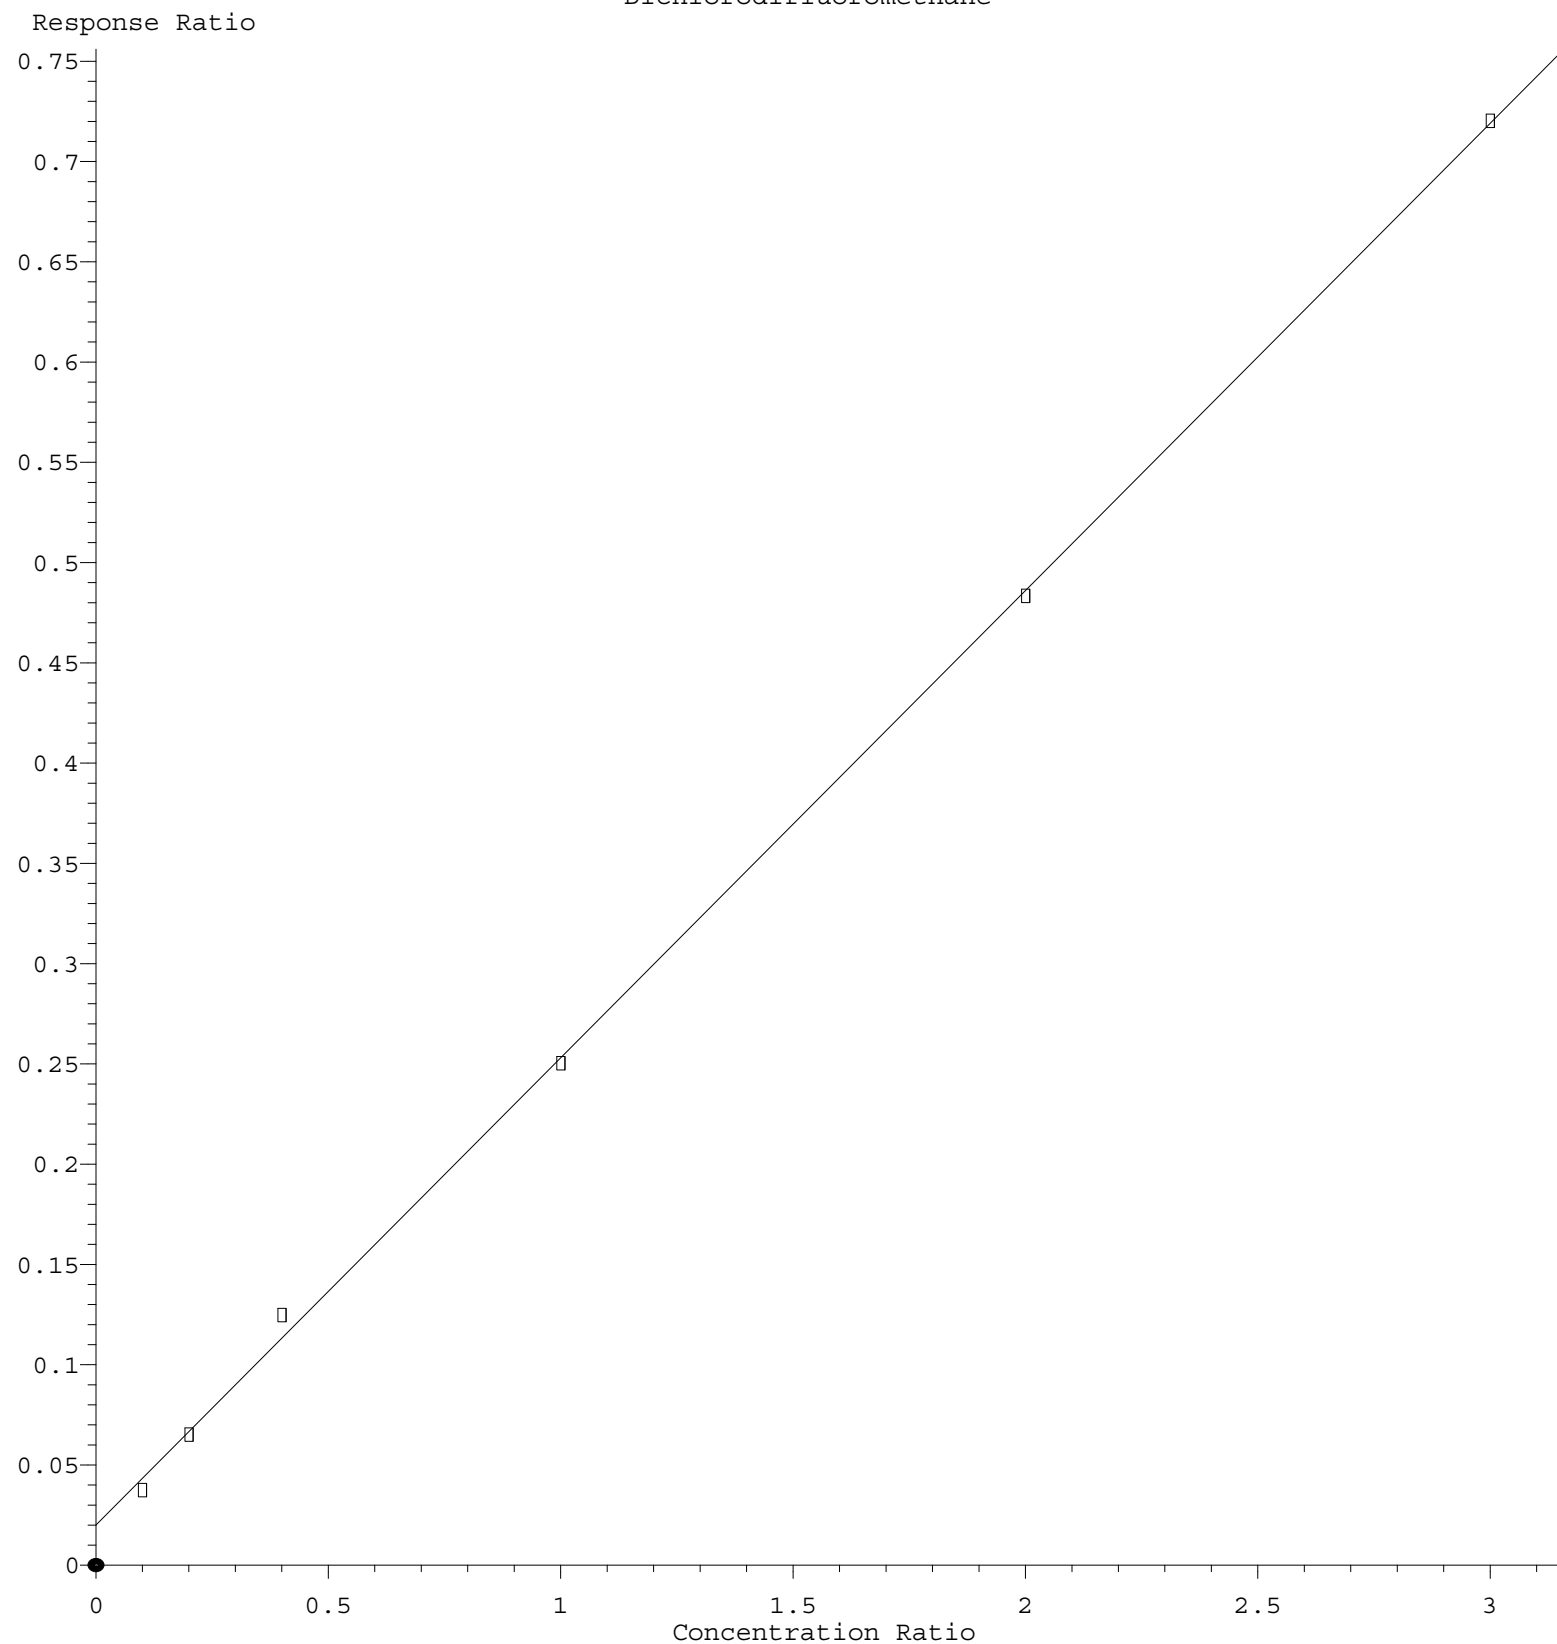

Response = 2.329e-001 * Amt + 2.011e-002
 Coef of Det (r^2) = 0.999493 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D062722S.M
 Calibration Table Last Updated: Mon Jun 27 16:20:04 2022


Vinyl Chloride

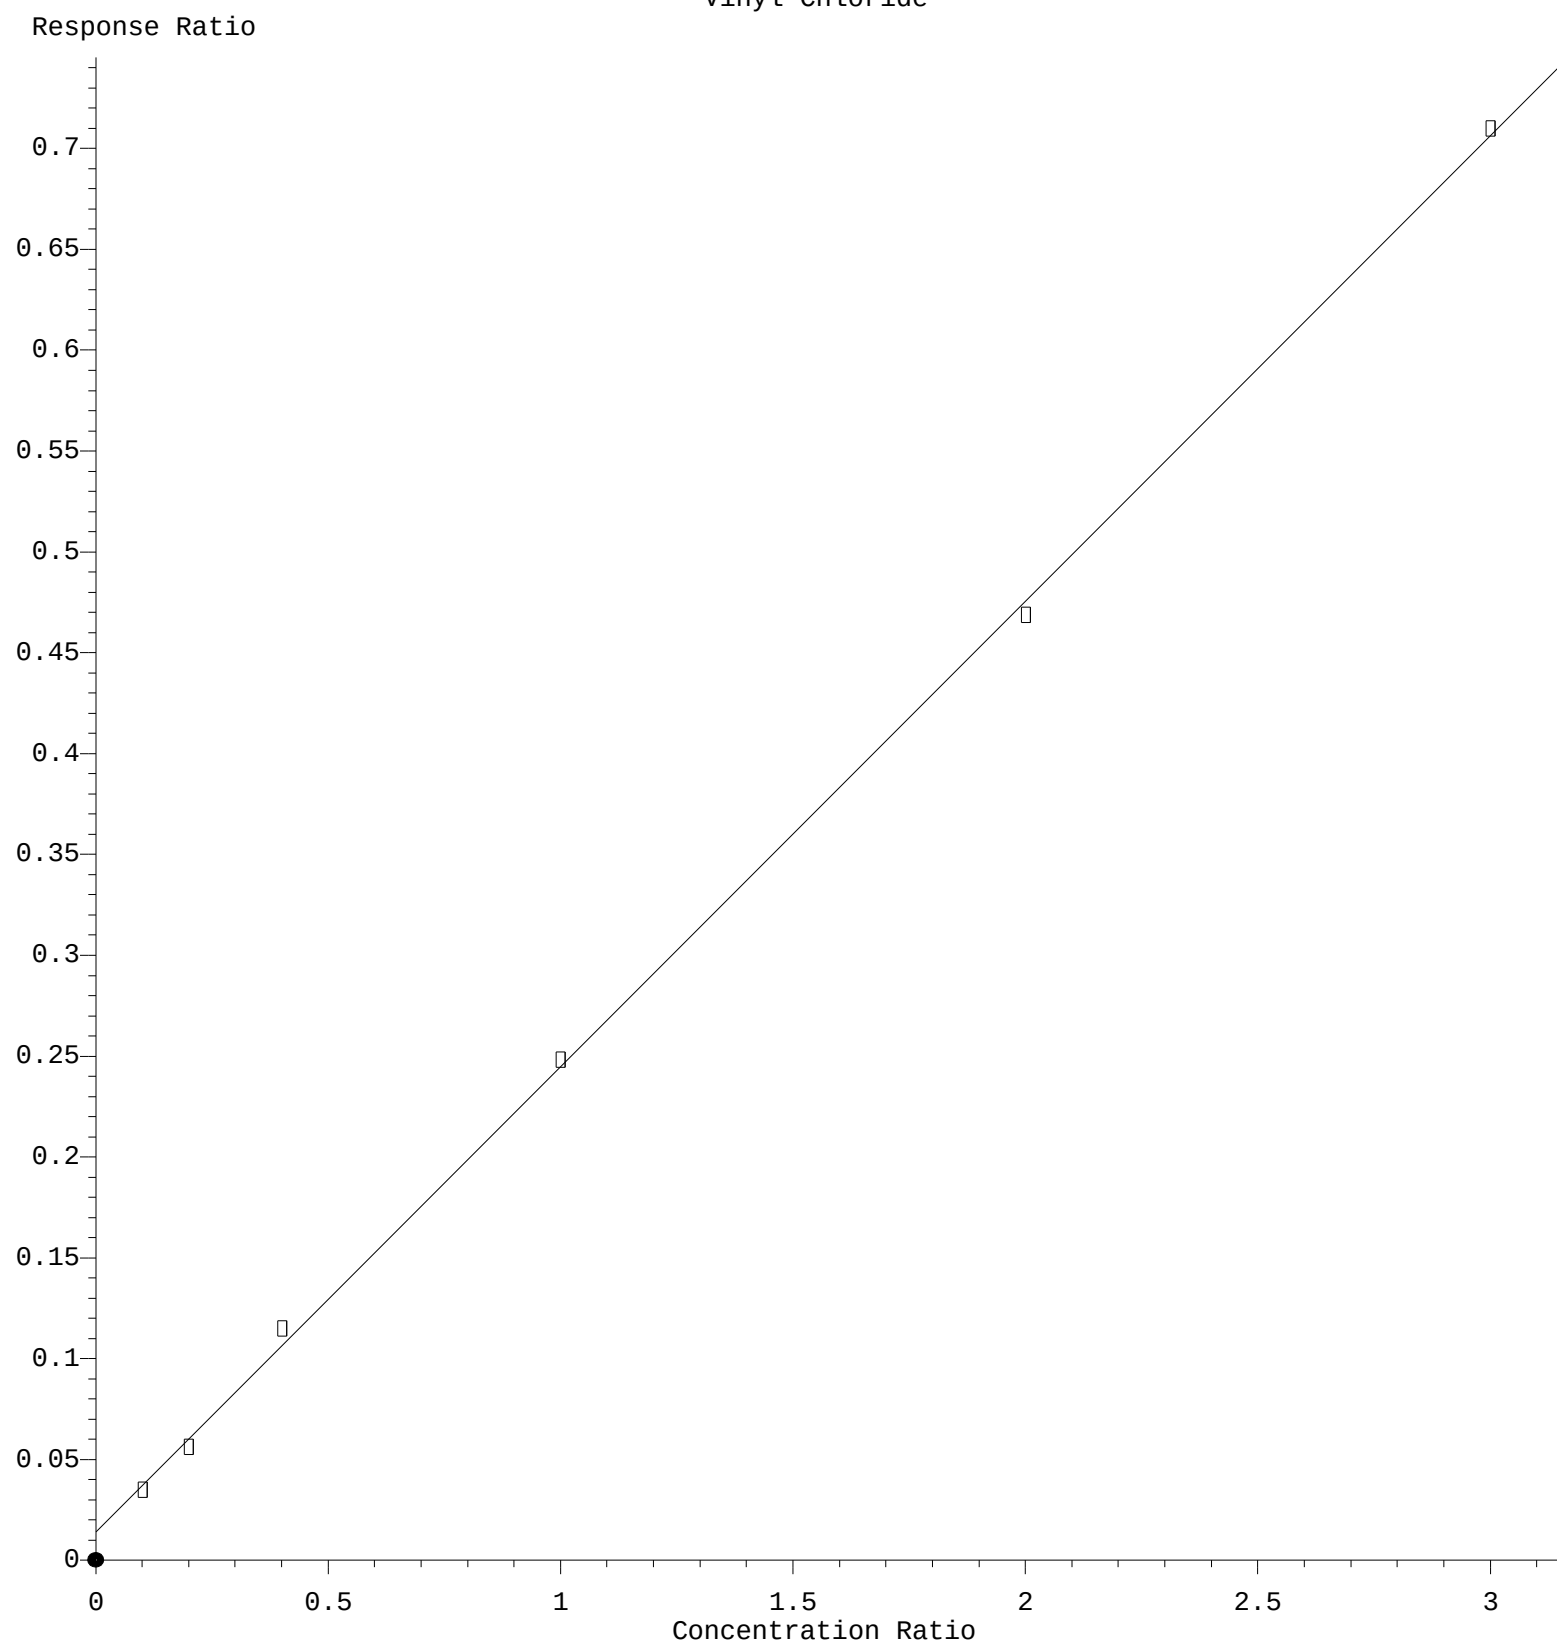

Response = 2.308e-001 * Amt + 1.436e-002
 Coef of Det (r^2) = 0.999548 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D062722S.M
 Calibration Table Last Updated: Mon Jun 27 16:20:04 2022

Bromomethane

Response Ratio

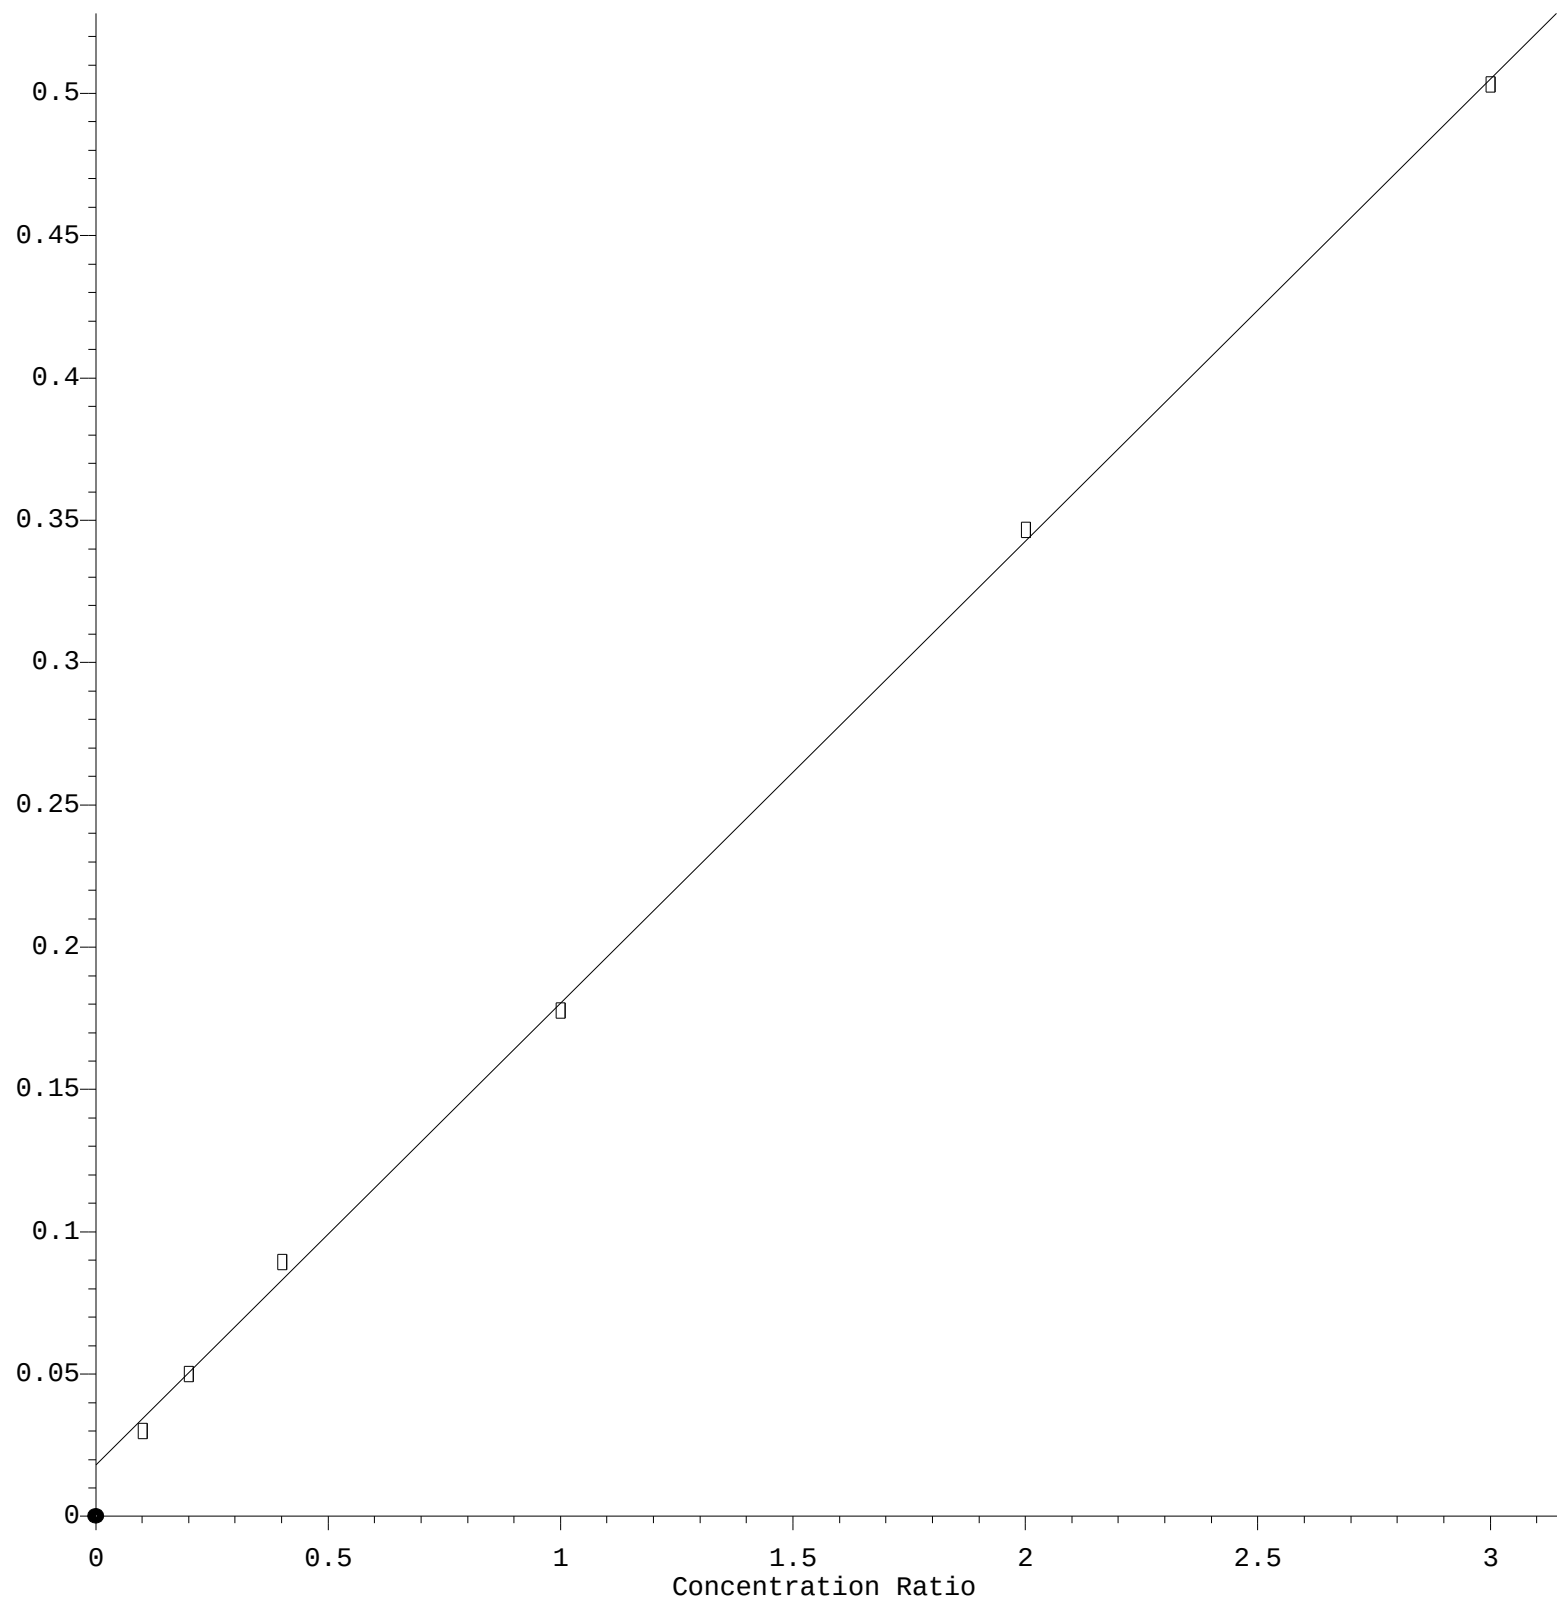


$$\text{Response} = 1.624\text{e-}001 * \text{Amt} + 1.808\text{e-}002$$

Coef of Det (r^2) = 0.999520 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D062722S.M

Calibration Table Last Updated: Mon Jun 27 16:20:04 2022


Tert butylalcohol

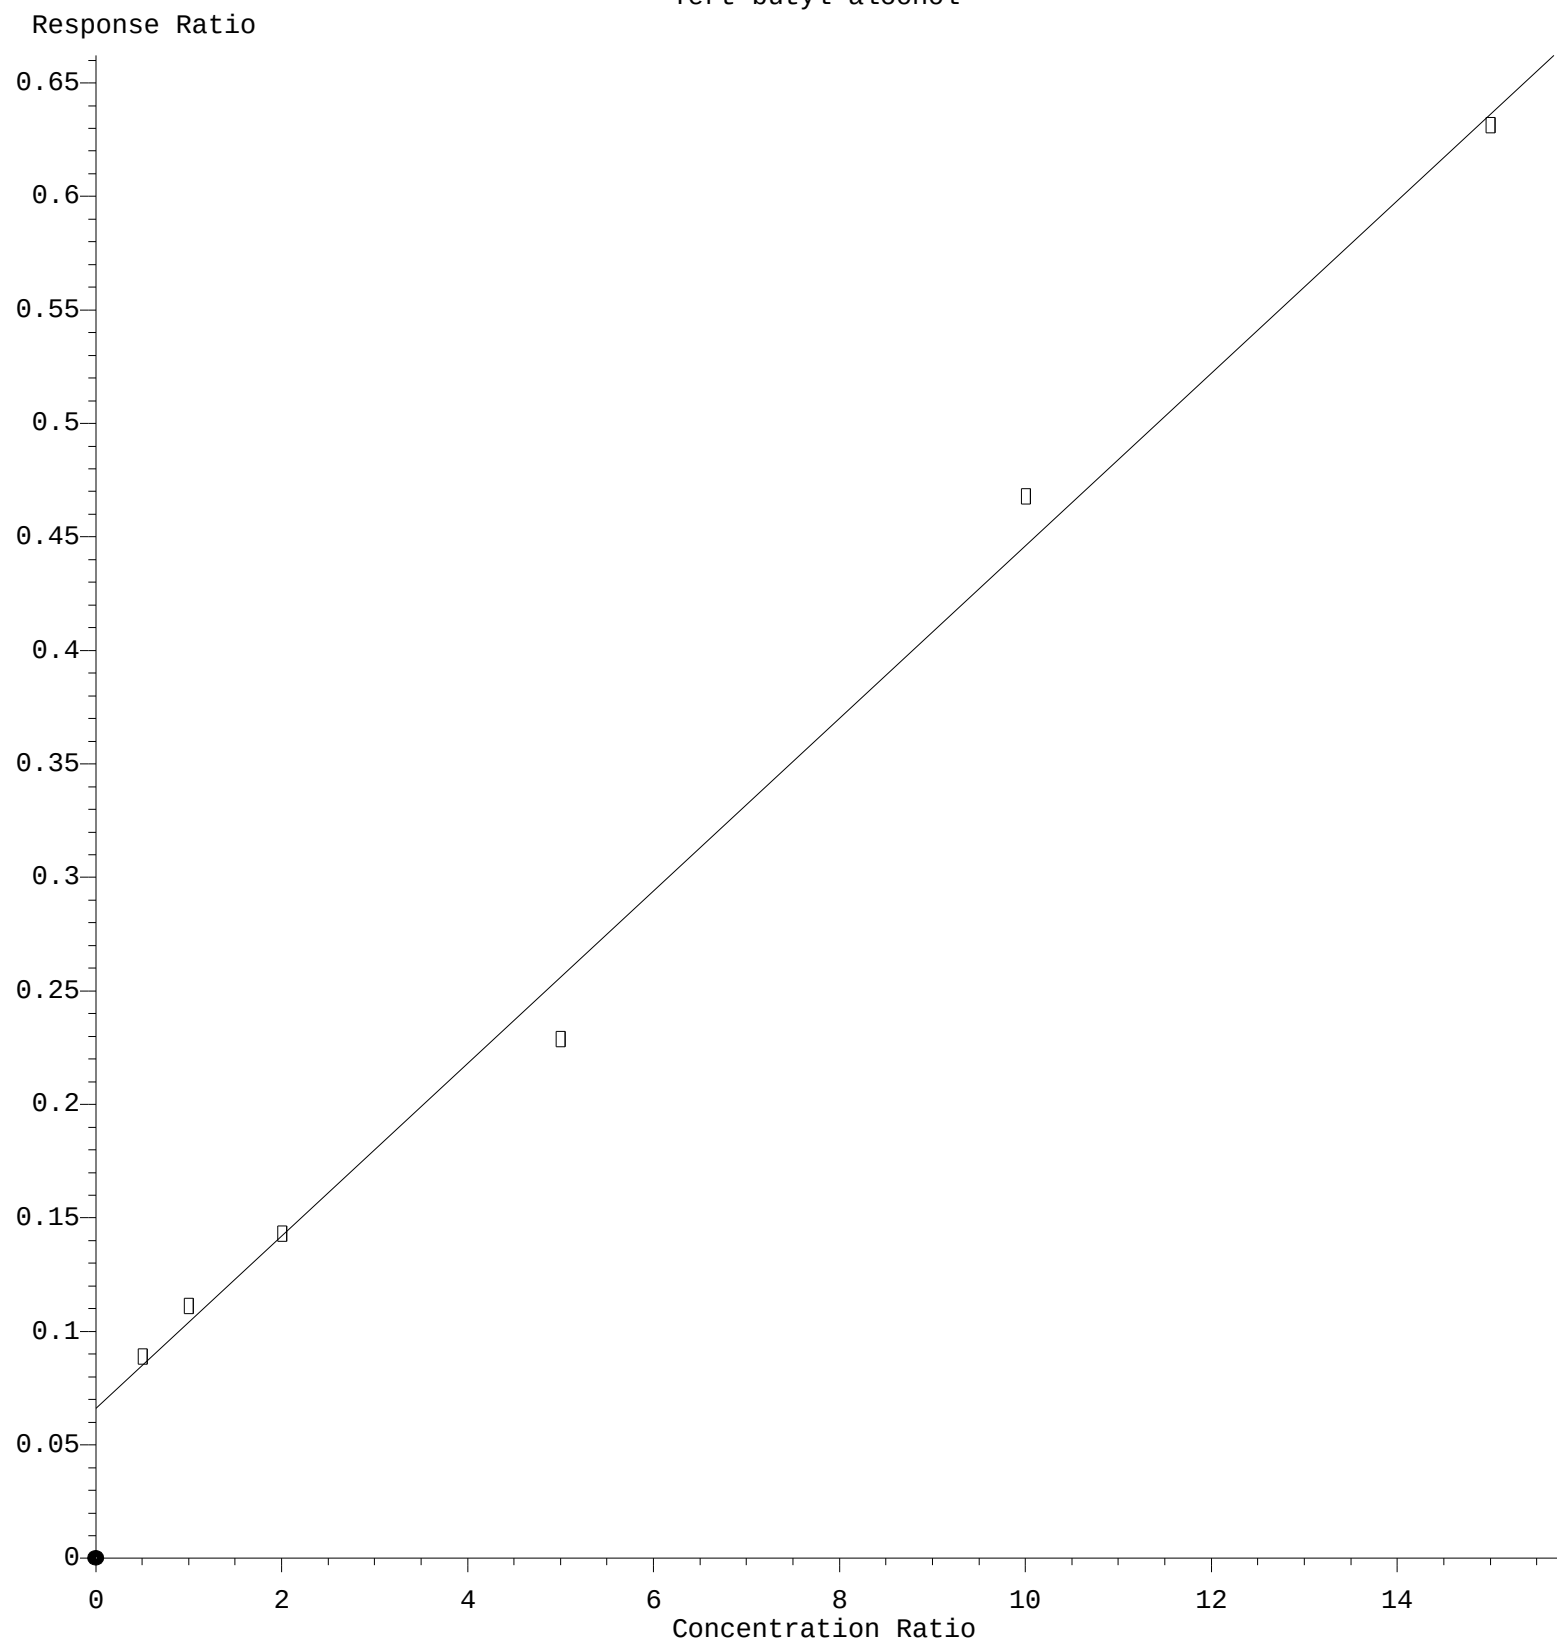

Response = $3.808 \times 10^{-2} \times \text{Amt} + 6.579 \times 10^{-2}$
 Coef of Det (r^2) = 0.994646 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D062722S.M
 Calibration Table Last Updated: Mon Jun 27 16:20:04 2022

Methyl Acetate

Response Ratio

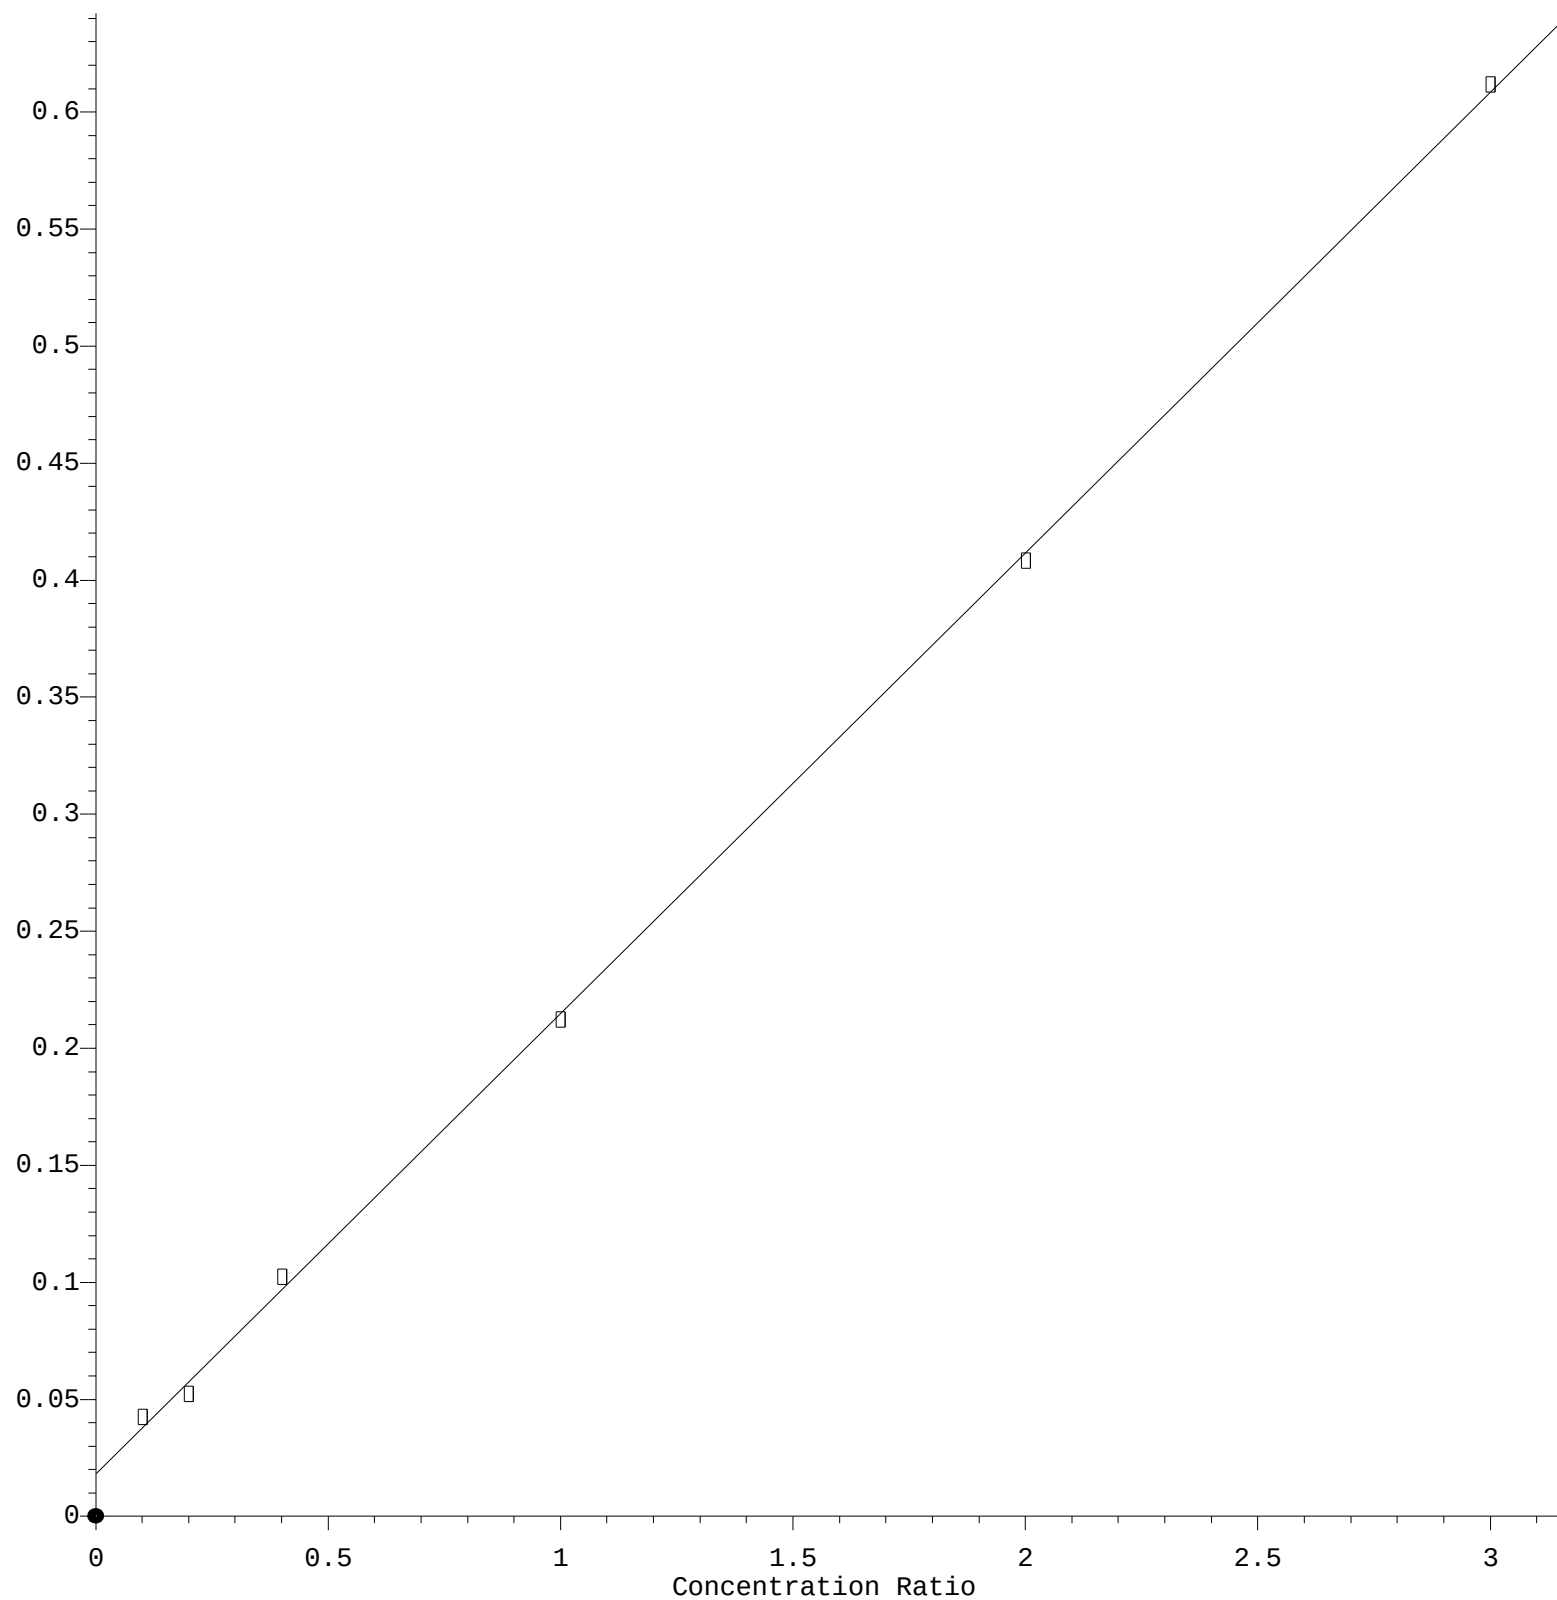

$$\text{Response} = 1.967\text{e-}001 * \text{Amt} + 1.845\text{e-}002$$


Coef of Det (r^2) = 0.999589 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D062722S.M

Calibration Table Last Updated: Mon Jun 27 16:20:04 2022

Methylene Chloride

Response Ratio

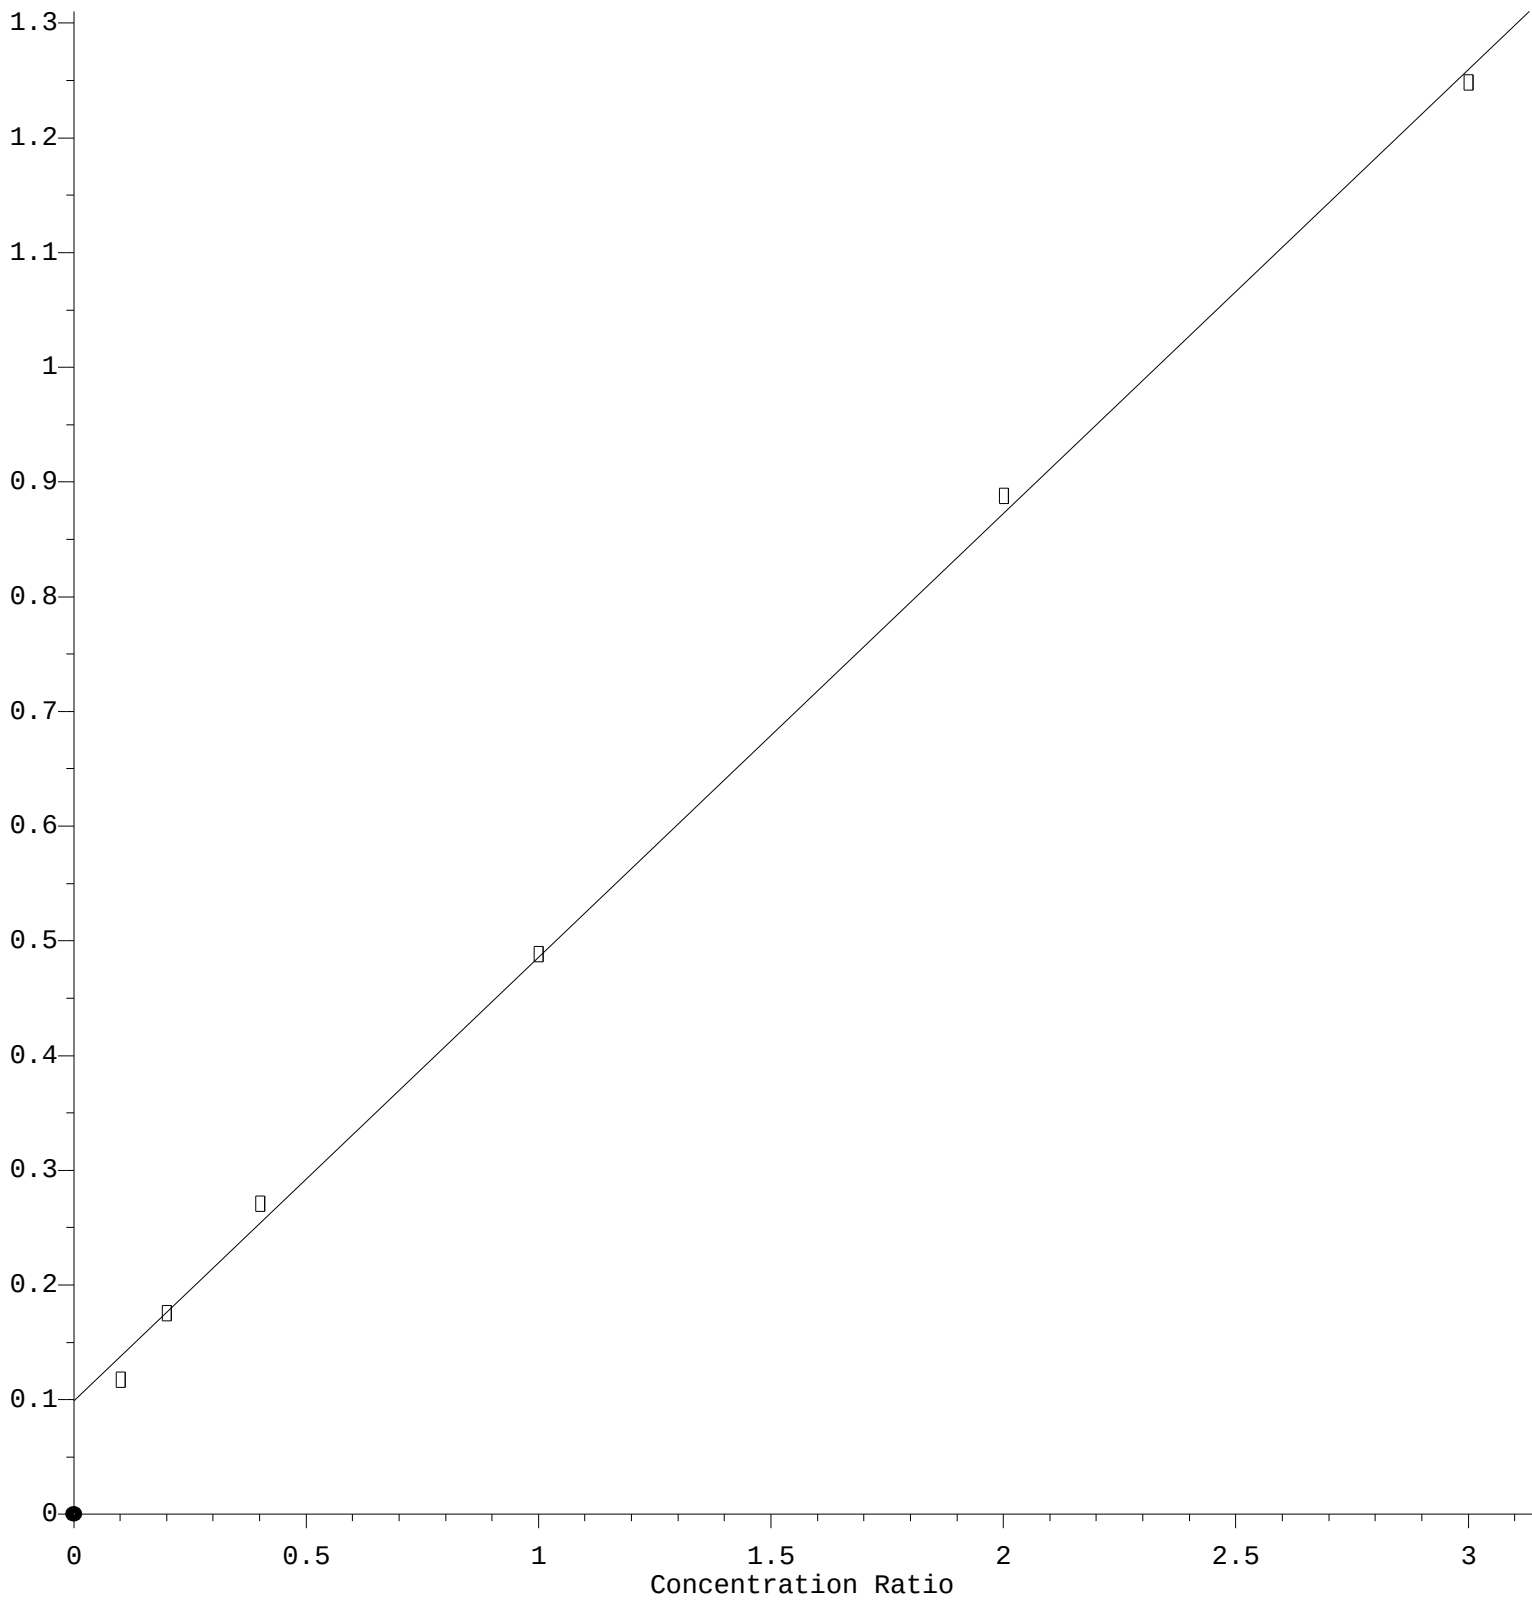

$$\text{Response} = 3.871\text{e-}001 * \text{Amt} + 9.879\text{e-}002$$


Coef of Det (r^2) = 0.998962 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D062722S.M

Calibration Table Last Updated: Mon Jun 27 16:20:04 2022

Cyclohexane

Response Ratio

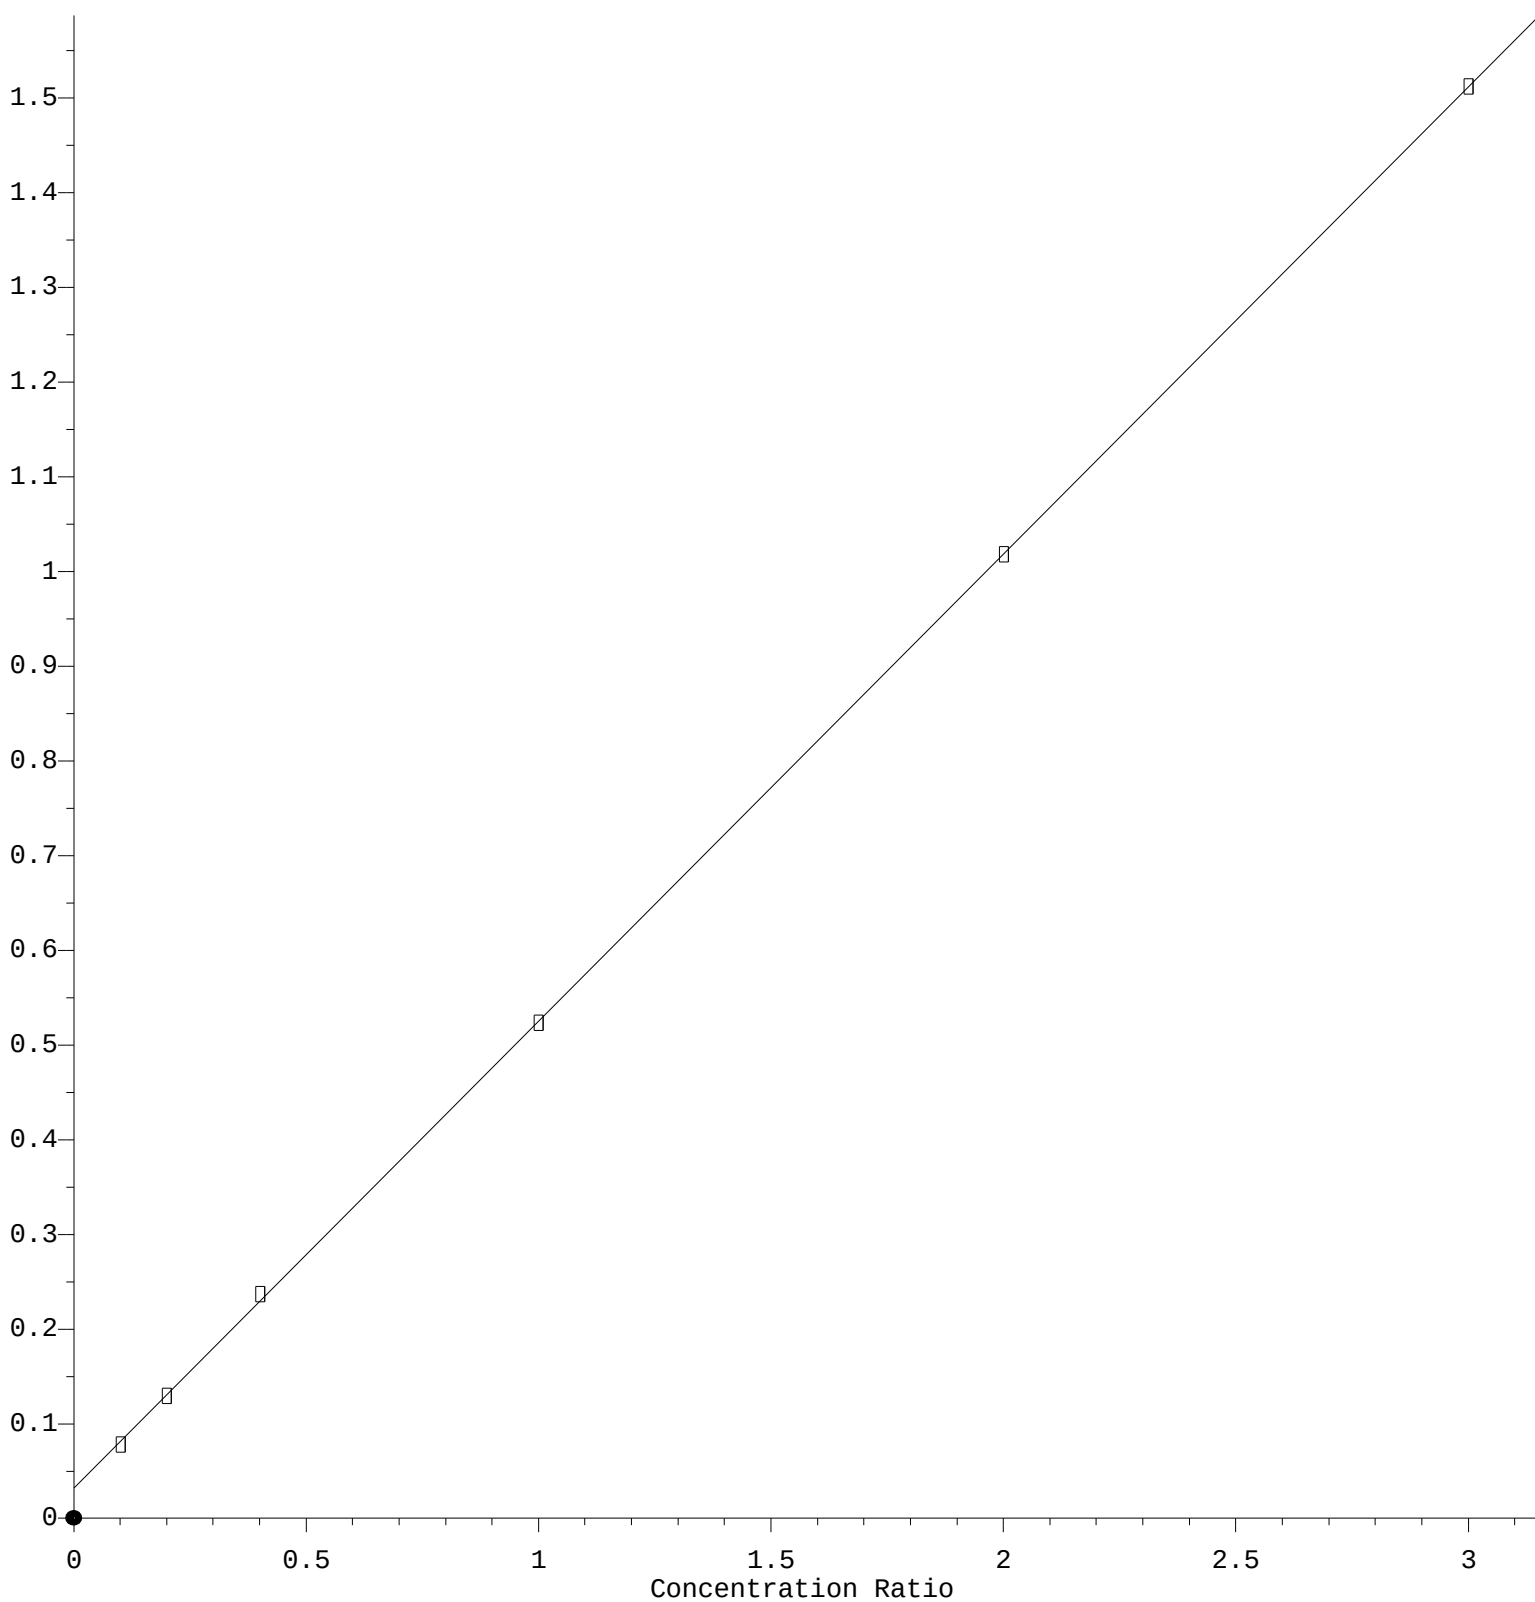

$$\text{Response} = 4.932\text{e-}001 * \text{Amt} + 3.206\text{e-}002$$


Coef of Det (r^2) = 0.999955 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D062722S.M

Calibration Table Last Updated: Mon Jun 27 16:20:04 2022

1,2-Dichloroethane-d4

Response Ratio

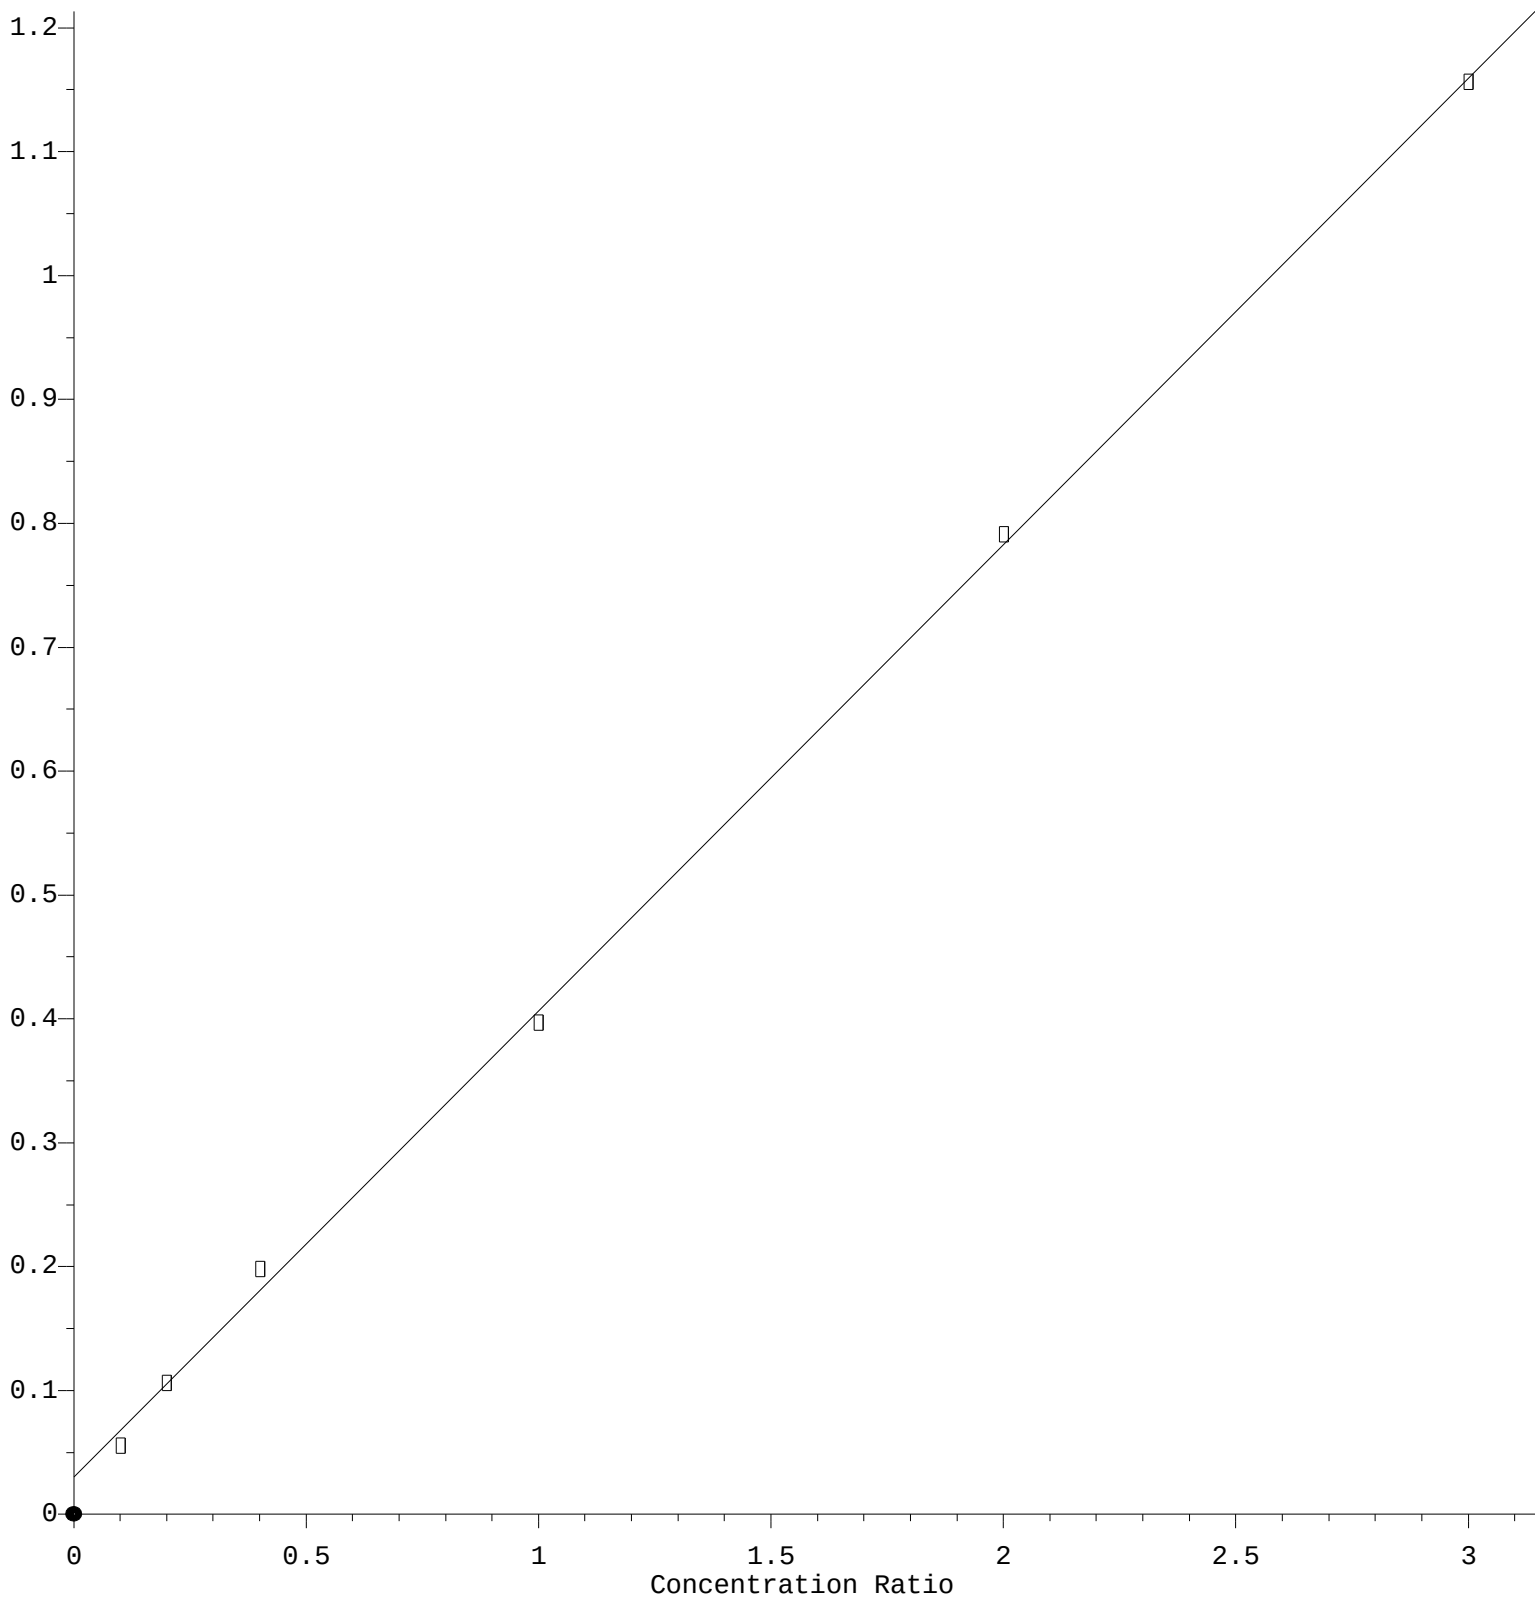

$$\text{Response} = 3.767\text{e-}001 * \text{Amt} + 2.975\text{e-}002$$

Coef of Det (r^2) = 0.999361 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D062722S.M

Calibration Table Last Updated: Mon Jun 27 16:20:04 2022