
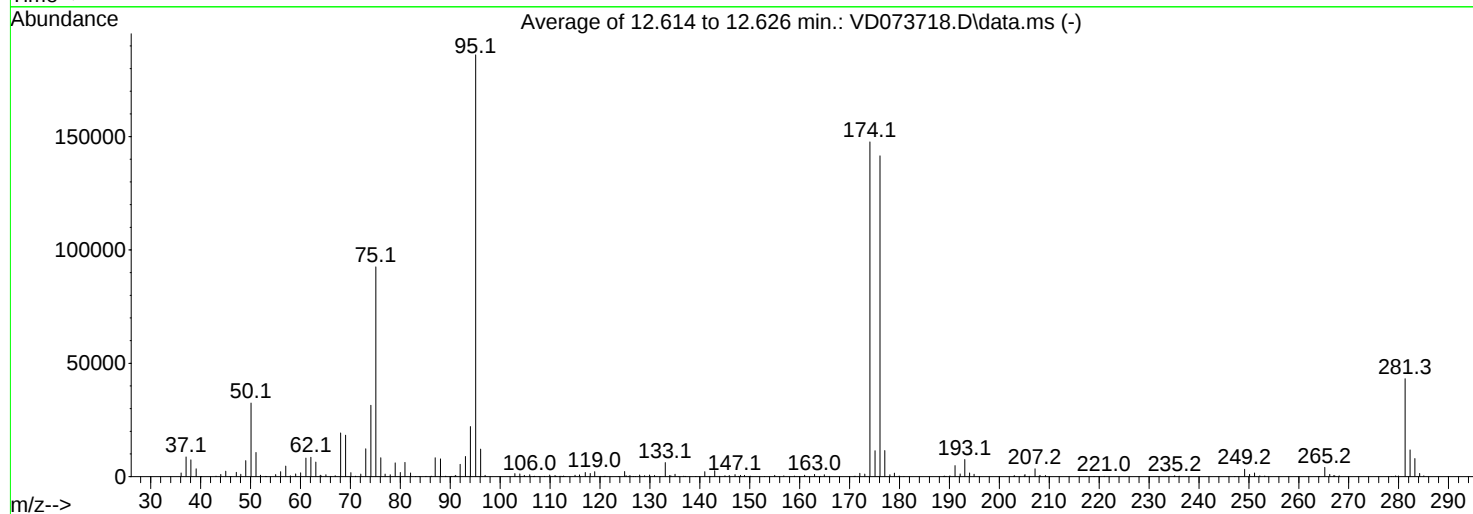


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD062722\
 Data File : VD073718.D
 Acq On : 27 Jun 2022 09:17
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D062722S.M
 Title : SW846 8260
 Last Update : Mon Jun 27 16:20:04 2022

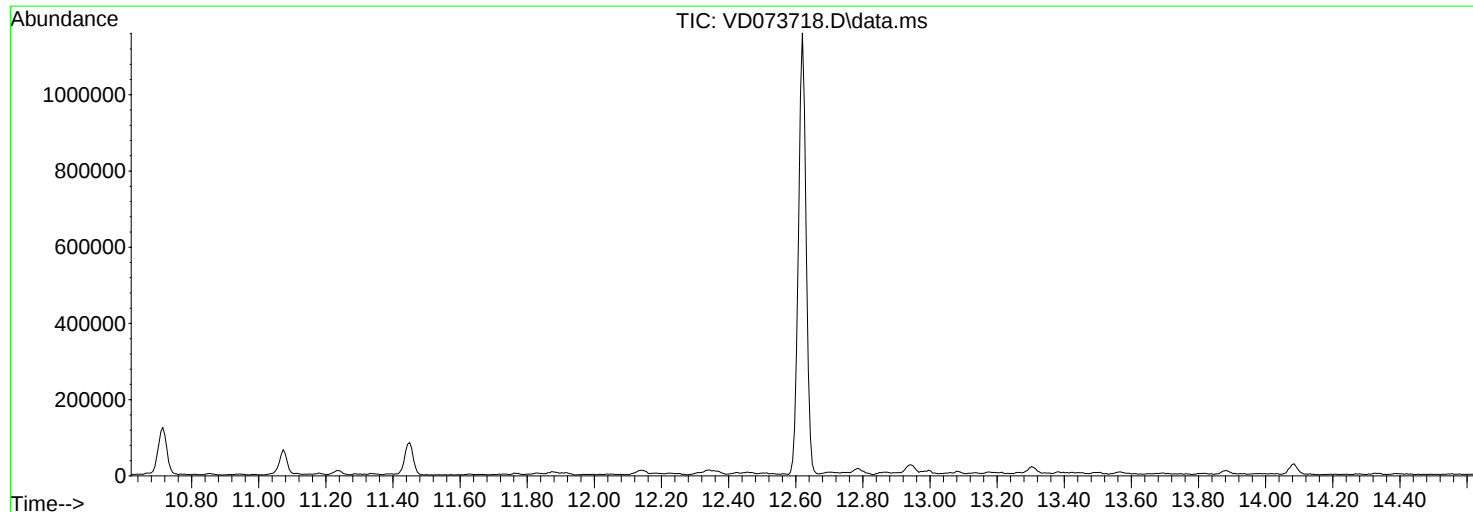

AutoFind: Scans 1818, 1819, 1820; Background Corrected with Scan 1803

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.4	32443	PASS
75	95	30	60	49.7	92525	PASS
95	95	100	100	100.0	186069	PASS
96	95	5	9	6.5	12164	PASS
173	174	0.00	2	0.8	1150	PASS
174	95	50	100	79.4	147648	PASS
175	174	5	9	7.7	11422	PASS
176	174	95	101	95.9	141552	PASS
177	176	5	9	8.1	11487	PASS