
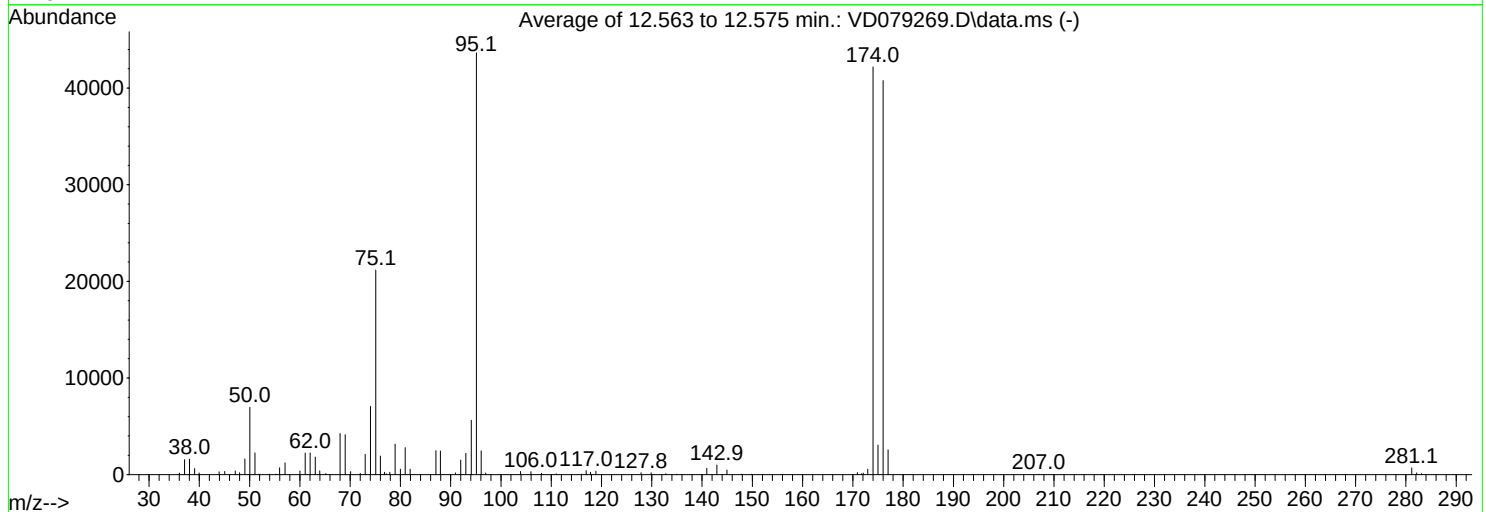


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD062724\
Data File : VD079269.D
Acq On : 27 Jun 2024 11:38
Operator : RP/MD
Sample : BFB816
Misc : 5.00G/10ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB816

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM062724SMA.M
Title : SFAM01.0
Last Update : Fri Jun 28 06:29:36 2024

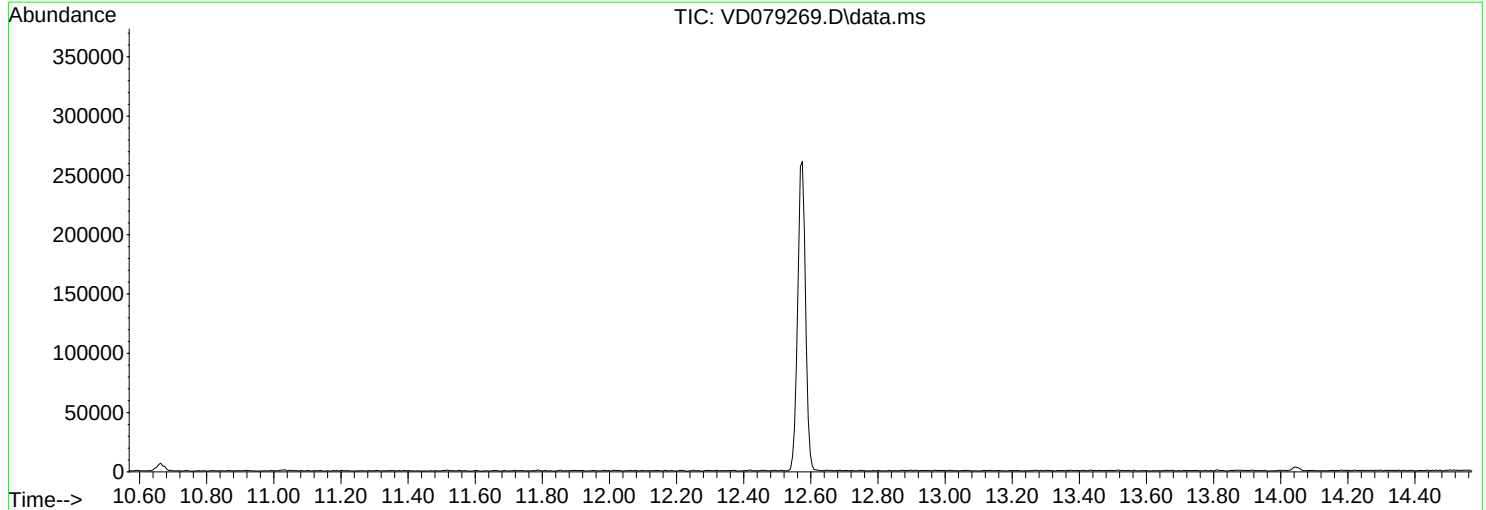

AutoFind: Scans 1866, 1867, 1868; Background Corrected with Scan 1860

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.0	6977	PASS
75	95	30	80	48.5	21184	PASS
95	95	100	100	100.0	43648	PASS
96	95	5	9	5.7	2470	PASS
173	174	0.00	2	1.3	565	PASS
174	95	50	120	96.7	42189	PASS
175	174	5	9	7.2	3058	PASS
176	174	95	105	96.7	40789	PASS
177	176	5	10	6.3	2562	PASS

m/z	Abundance
40.00	507.0
44.00	418.0

Instrument :
MSVOA_D
ClientSampleId :
BFB816

m/z	Abundance
37.10	1030.0
38.10	1243.0
39.10	517.0
39.90	617.0
43.90	504.0
45.10	223.0
47.10	218.0
48.00	190.0
49.10	1022.0
50.00	5230.0
51.00	1701.0
51.90	220.0
55.90	379.0
57.00	1036.0
60.00	256.0
61.10	2174.0
62.10	2168.0
63.10	1475.0
64.00	194.0
68.00	3036.0
69.00	3026.0
72.10	243.0
73.00	1602.0
74.00	5000.0
75.10	17432.0
76.00	1653.0
77.00	249.0
77.90	150.0
79.00	2728.0
80.00	321.0
81.00	2136.0
81.90	379.0
87.00	2052.0
87.90	2212.0
92.00	1120.0
93.00	1943.0
94.10	4203.0
95.10	33288.0
96.10	1958.0
103.90	166.0
106.00	209.0
117.00	308.0
117.80	321.0
119.00	201.0
127.80	180.0
140.90	458.0
142.90	610.0
145.10	273.0
147.80	156.0
172.00	152.0
173.00	455.0
174.00	29856.0
175.00	2604.0
176.00	31504.0
177.00	1898.0
207.00	154.0
281.10	383.0

Instrument :
MSVOA_D
ClientSampleId :
BFB816

m/z	Abundance
36.10	218.0
37.10	1914.0
38.00	2075.0
39.00	608.0
40.00	747.0
44.00	696.0
45.00	446.0
47.20	512.0
47.90	206.0
49.00	1934.0
50.10	7660.0
51.10	2255.0
55.20	160.0
56.00	1077.0
57.10	1334.0
60.00	441.0
61.00	1938.0
62.00	2058.0
63.10	2358.0
64.00	509.0
65.10	179.0
68.00	4913.0
69.00	4762.0
70.10	519.0
73.00	2319.0
74.00	8170.0
75.10	22872.0
76.00	1981.0
76.80	153.0
77.20	236.0
78.00	252.0
78.90	3049.0
80.00	667.0
81.00	3427.0
82.00	647.0
87.00	2582.0
88.00	2773.0
90.90	250.0
92.00	1709.0
93.00	2412.0
94.10	6703.0
95.10	49832.0
96.00	3282.0
97.00	245.0
103.80	480.0
106.00	482.0
108.00	228.0
117.00	368.0
117.80	412.0
118.90	513.0
127.90	254.0
129.80	267.0
135.00	165.0
141.00	811.0
143.00	1062.0
144.90	572.0
149.90	176.0
170.90	280.0
173.00	524.0
174.00	46720.0
175.00	3001.0
176.00	44520.0
177.00	2676.0
281.00	631.0
282.10	201.0

Instrument :
MSVOA_D
ClientSampleId :
BFB816

m/z	Abundance
36.00	270.0
37.00	1740.0
38.00	1509.0
39.00	756.0
40.00	728.0
44.00	948.0
45.00	337.0
47.20	403.0
48.10	204.0
49.10	1937.0
50.10	8040.0
51.00	2810.0
53.90	218.0
55.90	680.0
57.00	1291.0
60.00	445.0
61.00	2576.0
62.00	2534.0
63.00	1653.0
63.90	485.0
65.20	187.0
68.00	4800.0
69.00	4659.0
70.10	439.0
71.90	178.0
73.00	2403.0
74.10	7998.0
75.10	23248.0
76.00	2119.0
76.80	367.0
77.80	324.0
78.90	3697.0
80.00	726.0
80.90	2831.0
82.00	686.0
87.10	2799.0
87.90	2355.0
91.00	278.0
92.00	1713.0
93.00	2275.0
94.10	6003.0
95.10	47824.0
96.00	2171.0
96.90	244.0
104.00	326.0
105.80	232.0
108.10	157.0
111.00	247.0
116.10	185.0
116.90	560.0
118.80	366.0
127.90	178.0
129.90	310.0
132.80	285.0
140.90	737.0
143.00	1286.0
145.00	610.0
170.90	368.0
171.70	312.0
172.10	336.0
172.90	715.0
174.00	49992.0
175.00	3570.0
176.00	46344.0
177.00	3112.0
281.20	1057.0
282.20	345.0
283.10	282.0

Instrument :
MSVOA_D
ClientSampleId :
BFB816