


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD062818\
 Data File : VD059460.D
 Acq On : 28 Jun 2018 12:43
 Operator : VA/AP
 Sample : BFB
 Misc : 5.00µl/5ml/MSVOA D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D062518S.M
 Title : SW846 8260
 Last Update : Mon Jun 25 07:29:35 2018

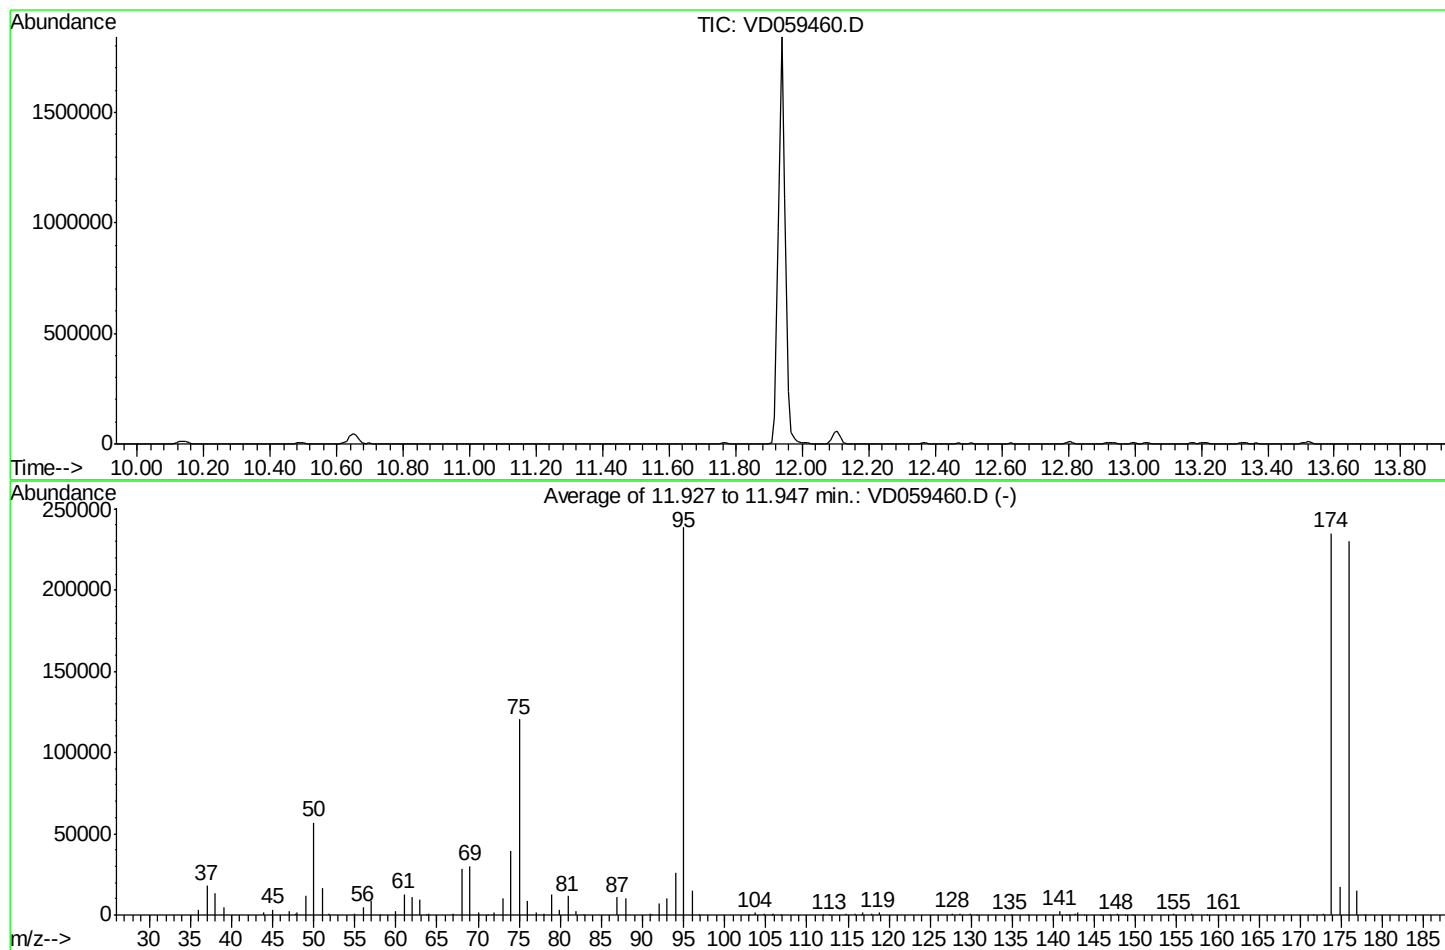

AutoFind: Scans 1189, 1190, 1191; Background Corrected with Scan 1184

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.8	56845	PASS
75	95	30	60	50.4	120288	PASS
95	95	100	100	100.0	238634	PASS
96	95	5	9	6.2	14817	PASS
173	174	0.00	2	0.3	617	PASS
174	95	50	100	98.5	235144	PASS
175	174	5	9	7.5	17563	PASS
176	174	95	101	97.8	229952	PASS
177	176	5	9	6.7	15340	PASS