
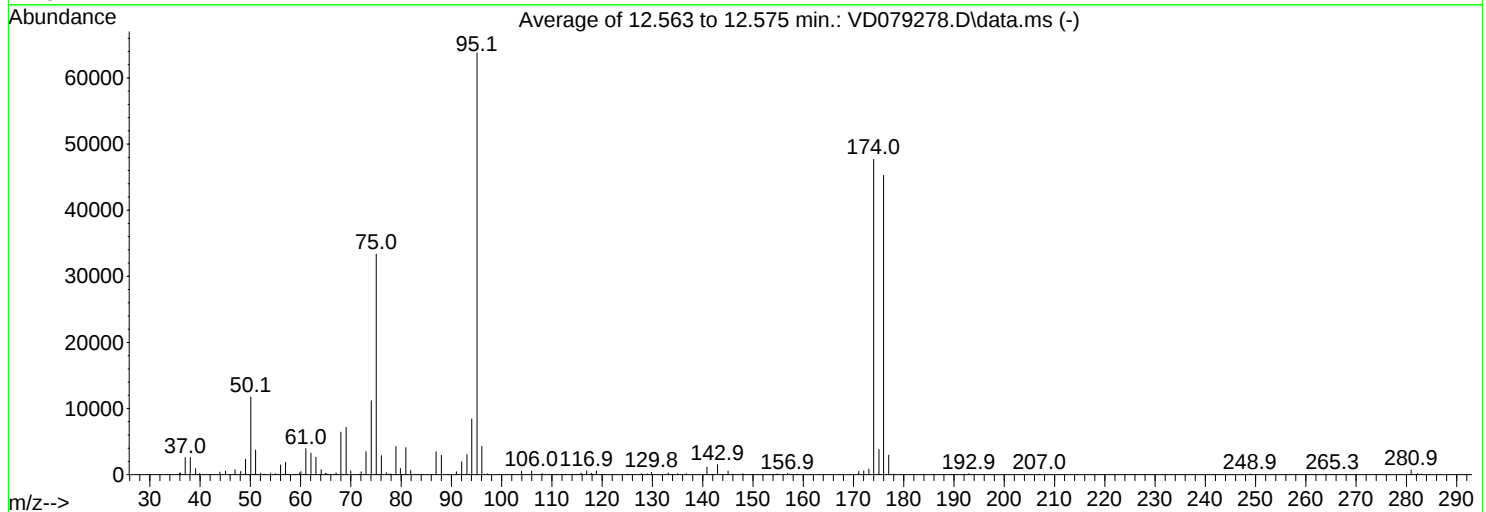


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD062824\
Data File : VD079278.D
Acq On : 28 Jun 2024 11:57
Operator : RP/MD
Sample : BFB
Misc : 5.00G/5.0ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D062824S.M
Title : SW846 8260
Last Update : Sat Jun 29 06:28:31 2024

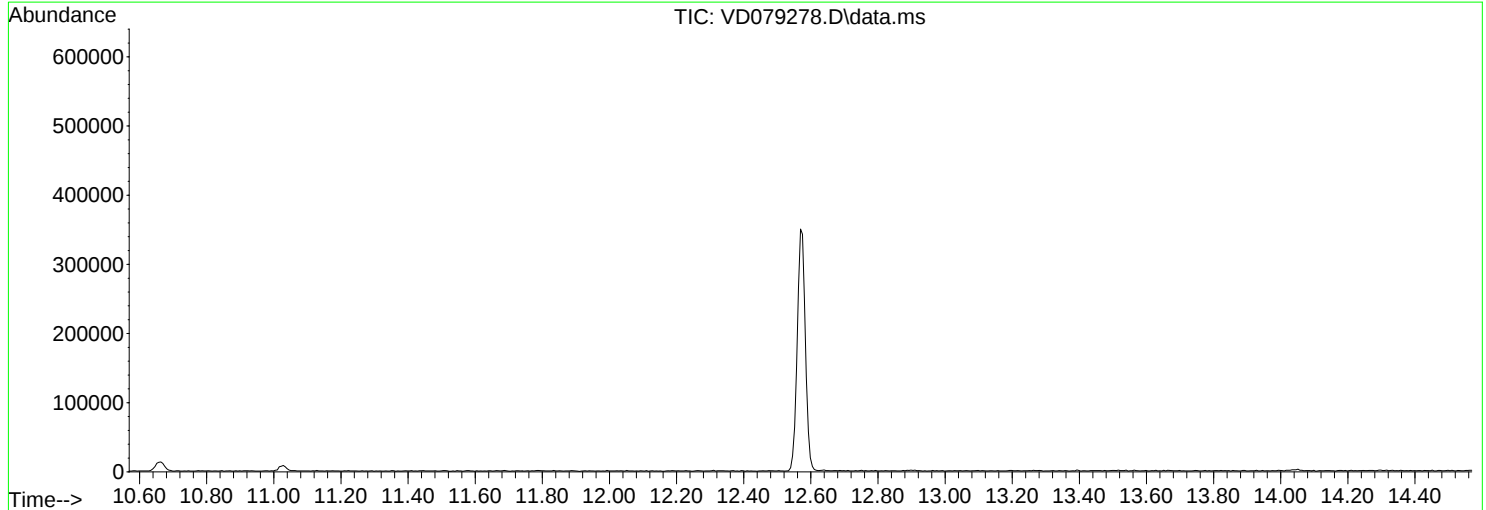

AutoFind: Scans 1866, 1867, 1868; Background Corrected with Scan 1858

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.4	11736	PASS
75	95	30	60	52.3	33357	PASS
95	95	100	100	100.0	63800	PASS
96	95	5	9	6.7	4287	PASS
173	174	0.00	2	1.8	847	PASS
174	95	50	100	74.7	47677	PASS
175	174	5	9	8.0	3798	PASS
176	174	95	101	94.9	45251	PASS
177	176	5	9	6.5	2957	PASS