


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD062918\
Data File : VD059483.D
Acq On : 29 Jun 2018 9:52
Operator : VA/AP
Sample : BFB
Misc : 5.00µl/5ml/MSVOA D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D062518S.M
Title : SW846 8260
Last Update : Mon Jun 25 07:29:35 2018

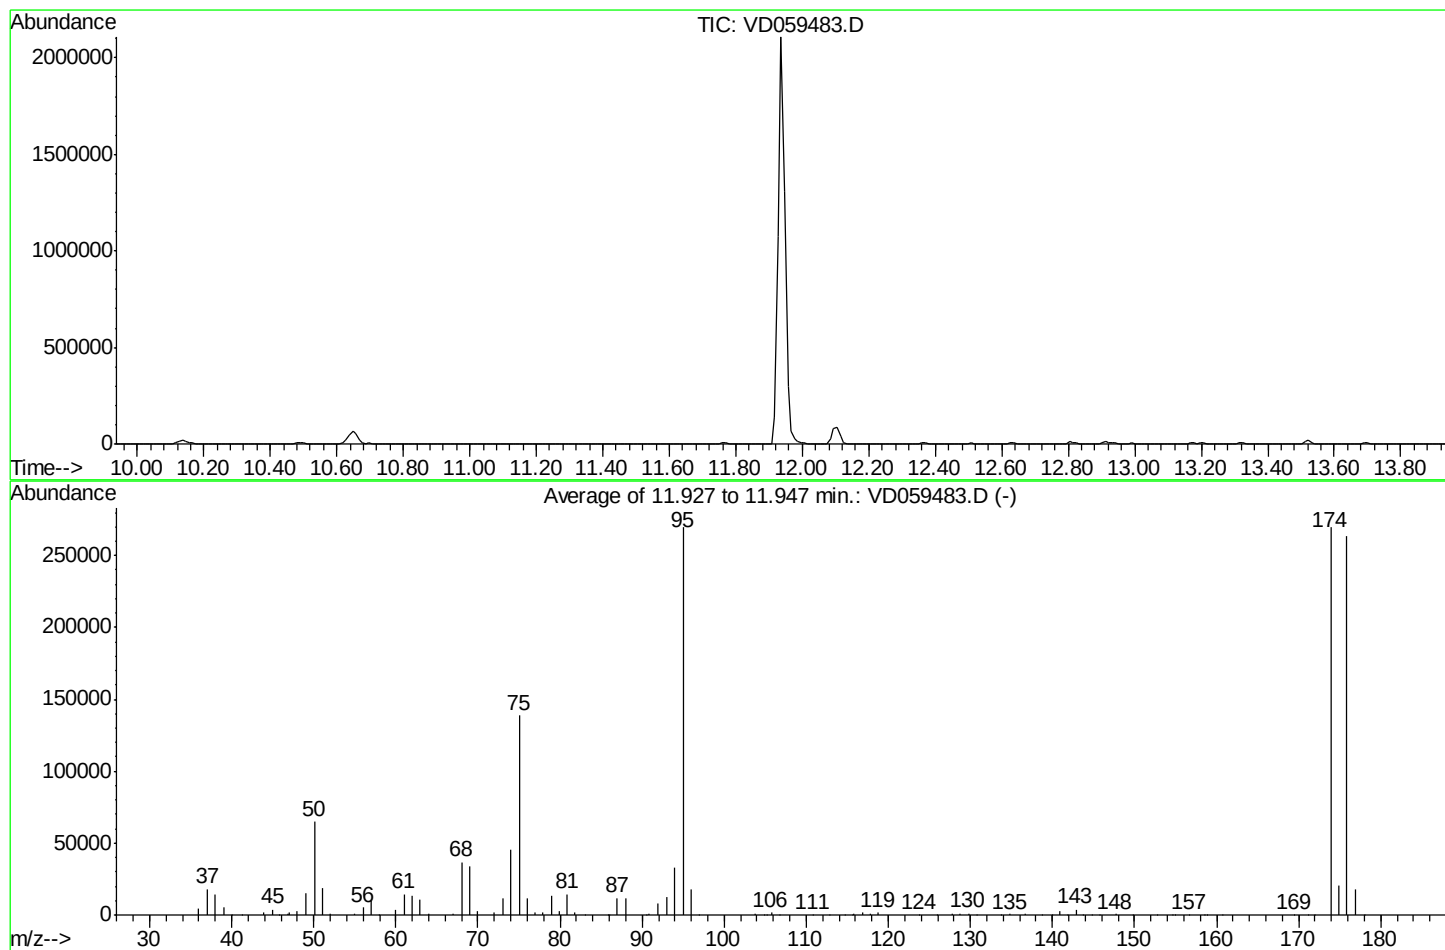

AutoFind: Scans 1189, 1190, 1191; Background Corrected with Scan 1184

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.1	64853	PASS
75	95	30	60	51.5	138784	PASS
95	95	100	100	100.0	269610	PASS
96	95	5	9	6.7	18048	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	99.9	269418	PASS
175	174	5	9	7.5	20307	PASS
176	174	95	101	97.9	263722	PASS
177	176	5	9	6.6	17443	PASS