
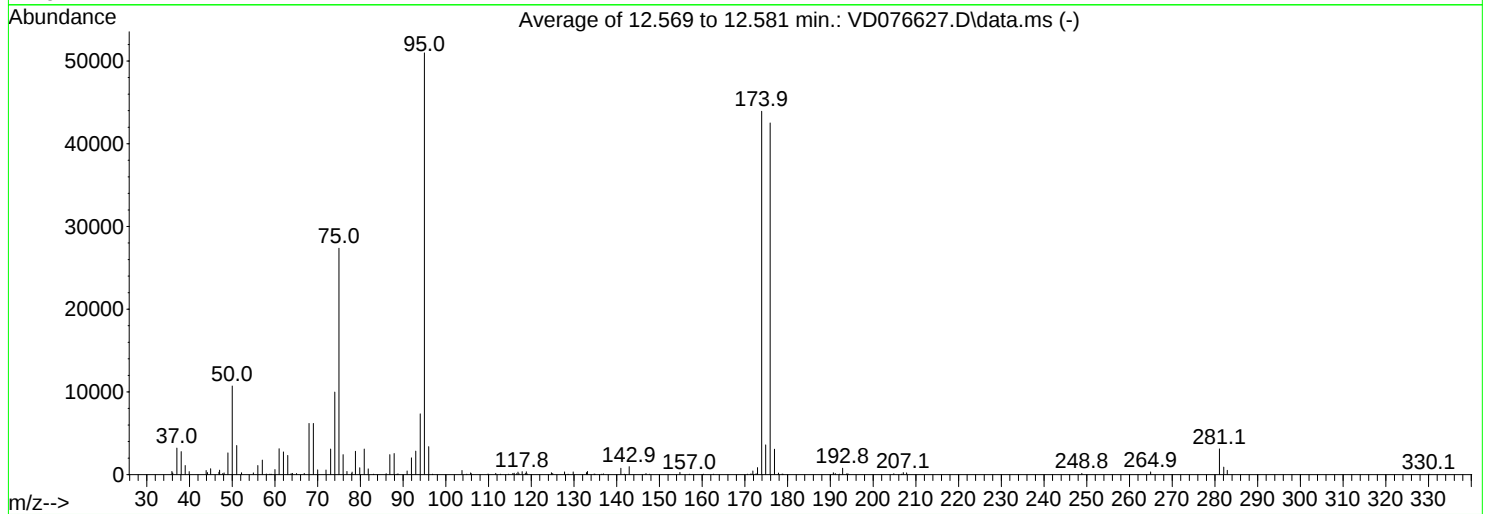


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD062923\
 Data File : VD076627.D
 Acq On : 29 Jun 2023 08:54
 Operator : KP/SY
 Sample : BFB148
 Misc : 5.00G/10.0ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB148

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM061523SMA.M
 Title : SFAM01.0
 Last Update : Fri Jun 16 01:50:34 2023

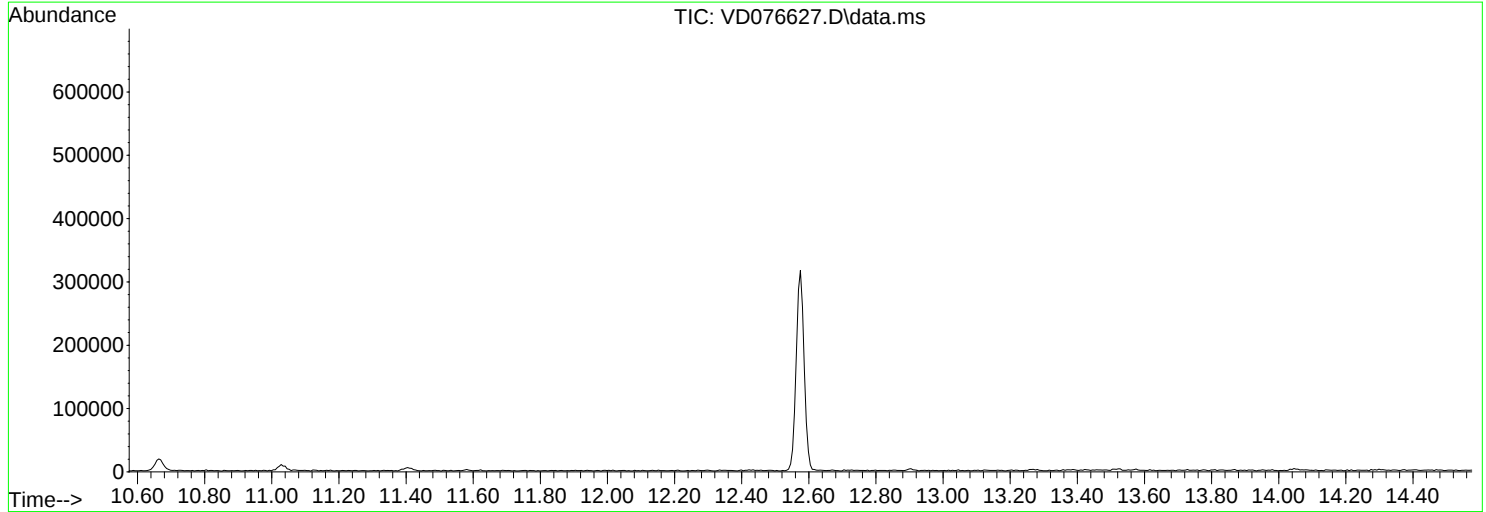

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1860

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.0	10717	PASS
75	95	30	80	53.7	27371	PASS
95	95	100	100	100.0	50989	PASS
96	95	5	9	6.6	3382	PASS
173	174	0.00	2	1.9	851	PASS
174	95	50	120	86.1	43920	PASS
175	174	5	9	8.2	3604	PASS
176	174	95	105	96.8	42512	PASS
177	176	5	10	7.2	3078	PASS

m/z	Abundance
40.00	706.0
43.80	508.0
50.00	208.0
52.90	272.0

Instrument :
MSVOA_D
ClientSampleId :
BFB148

m/z	Abundance
35.90	546.0
37.00	3288.0
38.10	3414.0
39.00	1249.0
39.90	1245.0
43.90	772.0
44.20	767.0
44.90	511.0
46.90	901.0
47.80	428.0
49.00	3088.0
50.00	11534.0
51.10	3273.0
52.20	307.0
55.00	279.0
56.00	1121.0
57.10	1967.0
58.00	255.0
60.00	704.0
61.00	3903.0
62.00	3207.0
63.00	2132.0
64.20	194.0
65.10	184.0
66.80	228.0
68.00	7092.0
69.00	6515.0
70.00	630.0
71.90	498.0
73.00	2646.0
74.00	9576.0
75.00	27368.0
76.00	2838.0
77.00	312.0
77.90	356.0
78.90	2962.0
79.80	689.0
80.90	3221.0
81.80	634.0
86.00	199.0
86.90	2906.0
87.90	2941.0
88.60	199.0
91.00	608.0
91.90	2002.0
93.00	2514.0
94.00	7693.0
95.00	52120.0
96.00	2966.0
96.90	155.0
103.80	571.0
105.80	347.0
111.80	264.0
112.80	189.0
115.70	443.0
117.00	403.0
117.90	450.0
118.90	596.0
124.70	333.0
127.80	475.0
129.80	320.0
132.90	746.0
134.70	217.0
141.00	668.0
142.90	837.0
146.80	186.0
147.70	169.0
154.90	343.0
170.60	153.0
171.40	294.0
171.80	353.0
172.90	917.0
173.90	40120.0
174.80	3801.0
175.90	40936.0
176.90	2962.0
178.00	159.0
190.70	375.0
192.80	427.0
194.10	195.0
206.70	196.0
207.80	172.0
249.00	153.0
265.00	219.0
281.00	2408.0
282.00	623.0
282.90	374.0

Instrument :
MSVOA_D
ClientSampleId :
BFB148

m/z	Abundance
36.10	630.0
37.10	3559.0
38.10	2503.0
39.00	1376.0
40.00	1026.0
44.00	1181.0
45.00	854.0
47.10	836.0
48.10	377.0
49.00	2689.0
50.10	11979.0
51.00	3969.0
52.20	223.0
54.90	346.0
56.00	1058.0
57.00	1734.0
58.80	173.0
60.00	494.0
61.00	2960.0
62.00	2691.0
63.00	2845.0
64.00	281.0
66.90	230.0
68.00	6587.0
69.00	7114.0
70.00	748.0
72.00	529.0
73.10	3765.0
74.00	11035.0
75.00	30952.0
75.90	2712.0
76.80	652.0
78.10	499.0
78.80	3324.0
79.90	780.0
80.90	3269.0
81.90	550.0
83.10	153.0
86.10	177.0
86.90	2704.0
87.90	2797.0
90.80	327.0
91.90	2230.0
92.90	3501.0
94.00	8050.0
95.00	56272.0
96.00	4304.0
103.80	633.0
104.90	159.0
106.00	301.0
111.60	206.0
114.70	165.0
116.00	368.0
116.80	554.0
117.70	366.0
118.80	472.0
124.70	387.0
127.80	327.0
129.80	447.0
133.20	553.0
134.90	202.0
136.90	268.0
141.00	916.0
142.80	1082.0
146.90	240.0
154.80	316.0
157.00	161.0
160.30	151.0
171.90	542.0
173.00	1208.0
173.90	48792.0
174.80	3970.0
175.90	47728.0
176.90	3204.0
177.80	184.0
178.70	215.0
191.20	193.0
192.90	923.0
194.10	185.0
204.80	211.0
207.00	419.0
207.90	204.0
265.00	392.0
281.10	2816.0
282.10	1152.0
283.00	443.0
330.10	157.0

Instrument :
MSVOA_D
ClientSampleId :
BFB148

m/z	Abundance
35.90	603.0
37.00	2759.0
38.00	2422.0
38.90	695.0
40.00	933.0
44.00	1100.0
44.90	783.0
47.00	771.0
48.10	264.0
49.00	2112.0
50.00	9262.0
51.00	3301.0
52.10	163.0
56.00	1127.0
57.10	1587.0
59.10	204.0
60.00	657.0
61.00	2544.0
62.00	2350.0
63.00	1986.0
63.80	349.0
65.00	247.0
68.00	4892.0
69.00	4967.0
70.00	341.0
71.80	366.0
72.00	286.0
73.00	2903.0
74.00	9309.0
75.00	23792.0
75.90	1727.0
76.90	170.0
78.00	436.0
78.90	2181.0
79.90	1038.0
80.90	2812.0
81.80	879.0
86.80	1662.0
87.90	1933.0
88.80	297.0
90.90	395.0
92.00	1857.0
93.00	2510.0
94.00	6296.0
95.00	44576.0
96.00	2877.0
103.90	310.0
105.80	297.0
109.90	228.0
116.00	182.0
116.60	376.0
117.10	347.0
117.90	285.0
118.60	400.0
119.10	257.0
125.00	407.0
127.90	164.0
128.60	169.0
129.90	238.0
133.10	584.0
136.50	198.0
140.90	744.0
141.80	204.0
143.00	960.0
154.70	157.0
162.70	153.0
171.80	437.0
172.60	367.0
173.00	429.0
173.90	42848.0
174.90	3040.0
175.90	38872.0
176.90	3067.0
177.80	231.0
178.90	194.0
190.70	330.0
191.10	225.0
192.10	177.0
192.80	952.0
193.80	263.0
204.90	169.0
207.10	314.0
207.80	287.0
248.80	326.0
264.90	386.0
281.00	4148.0
282.00	954.0
282.80	743.0

Instrument :
MSVOA_D
ClientSampleId :
BFB148