



Bromomethane

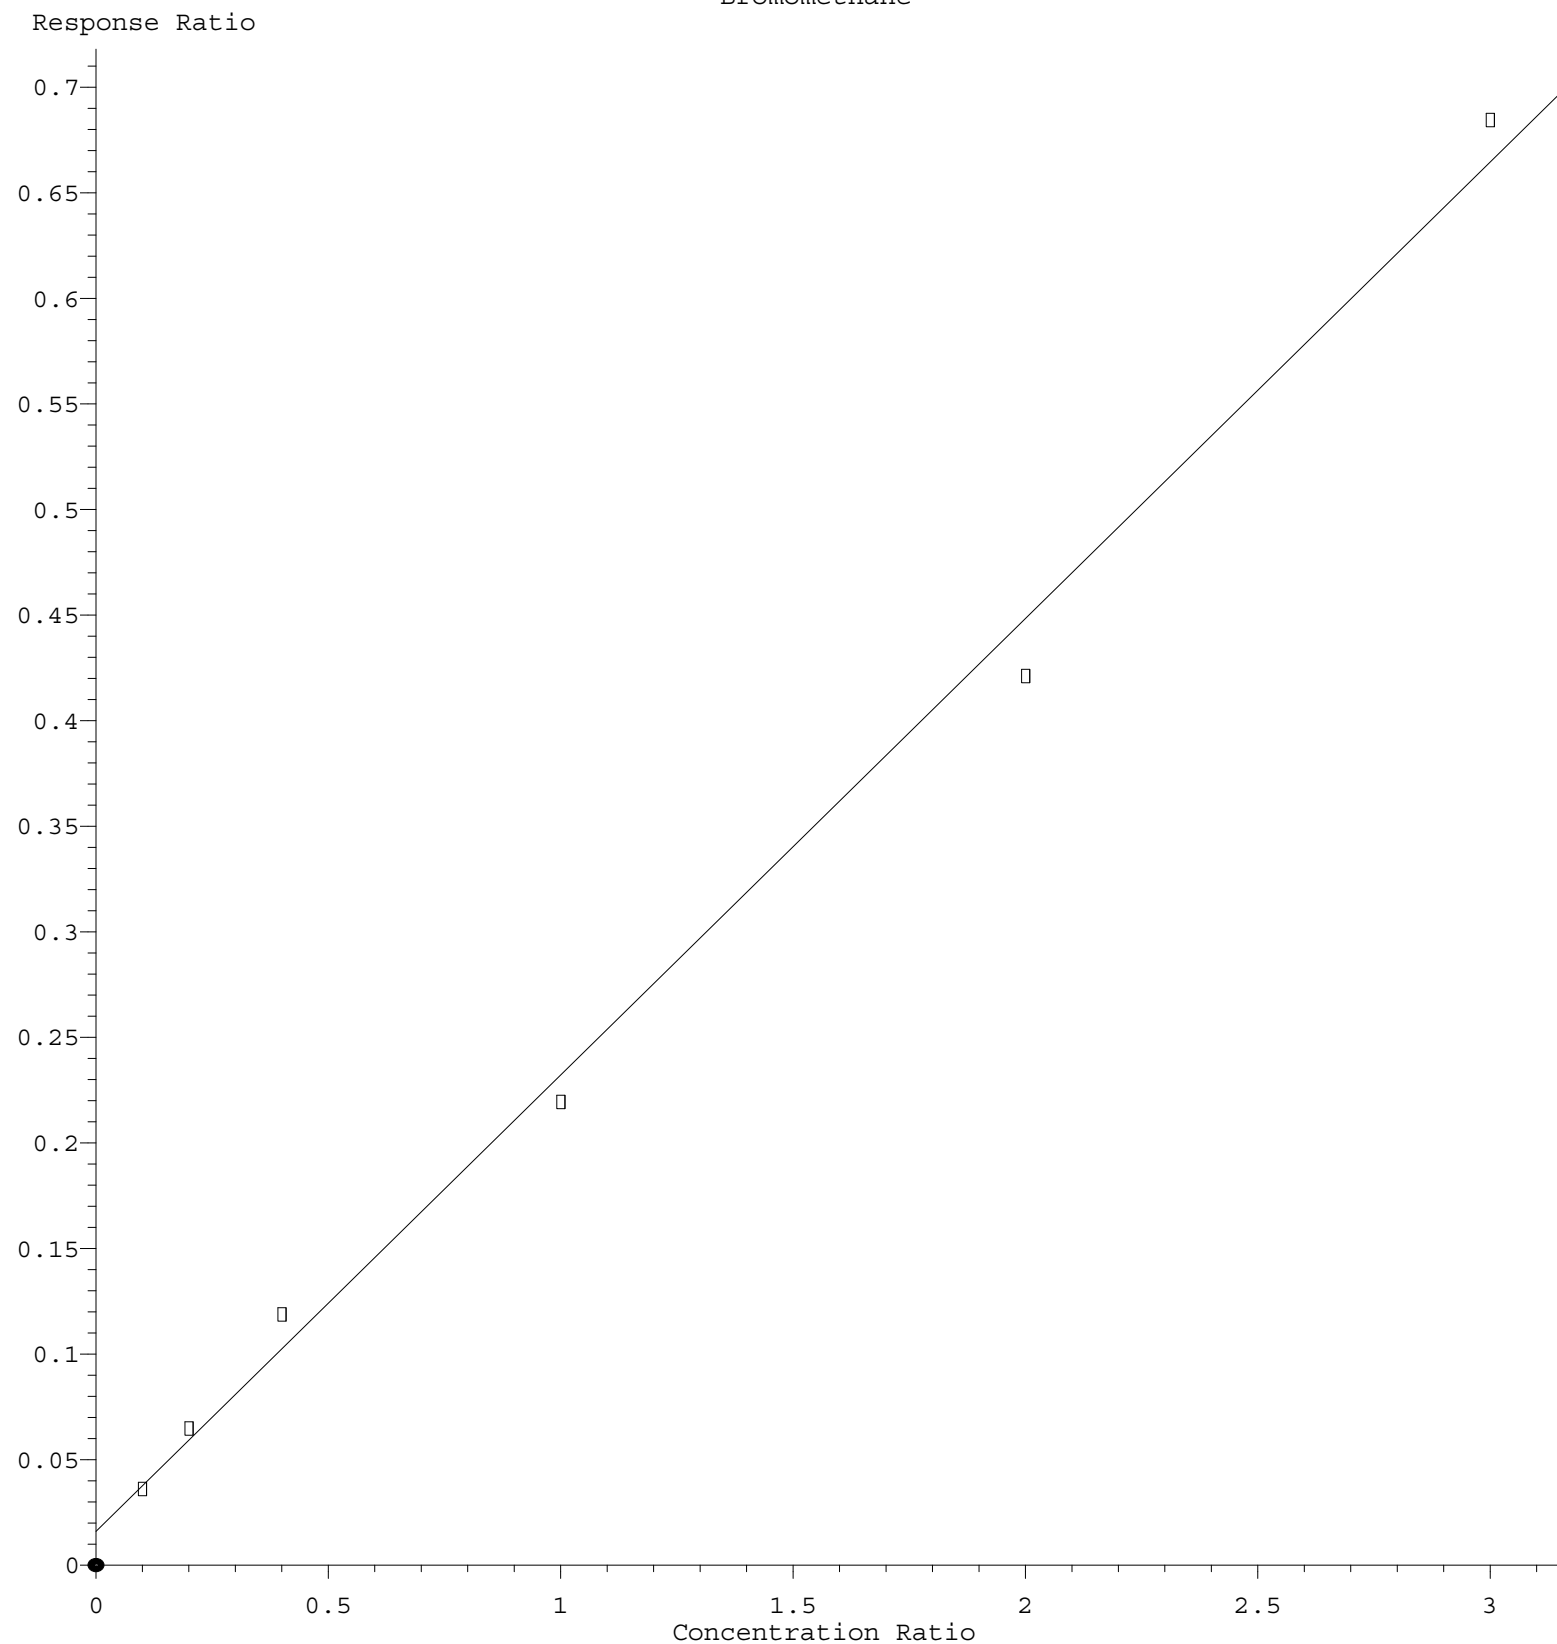

Response = $2.161 \times 10^{-1} \times \text{Amt} + 1.603 \times 10^{-2}$
 Coef of Det (r^2) = 0.994934 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D063022S.M
 Calibration Table Last Updated: Tue Jul 05 10:05:34 2022

Cyclohexane

Response Ratio

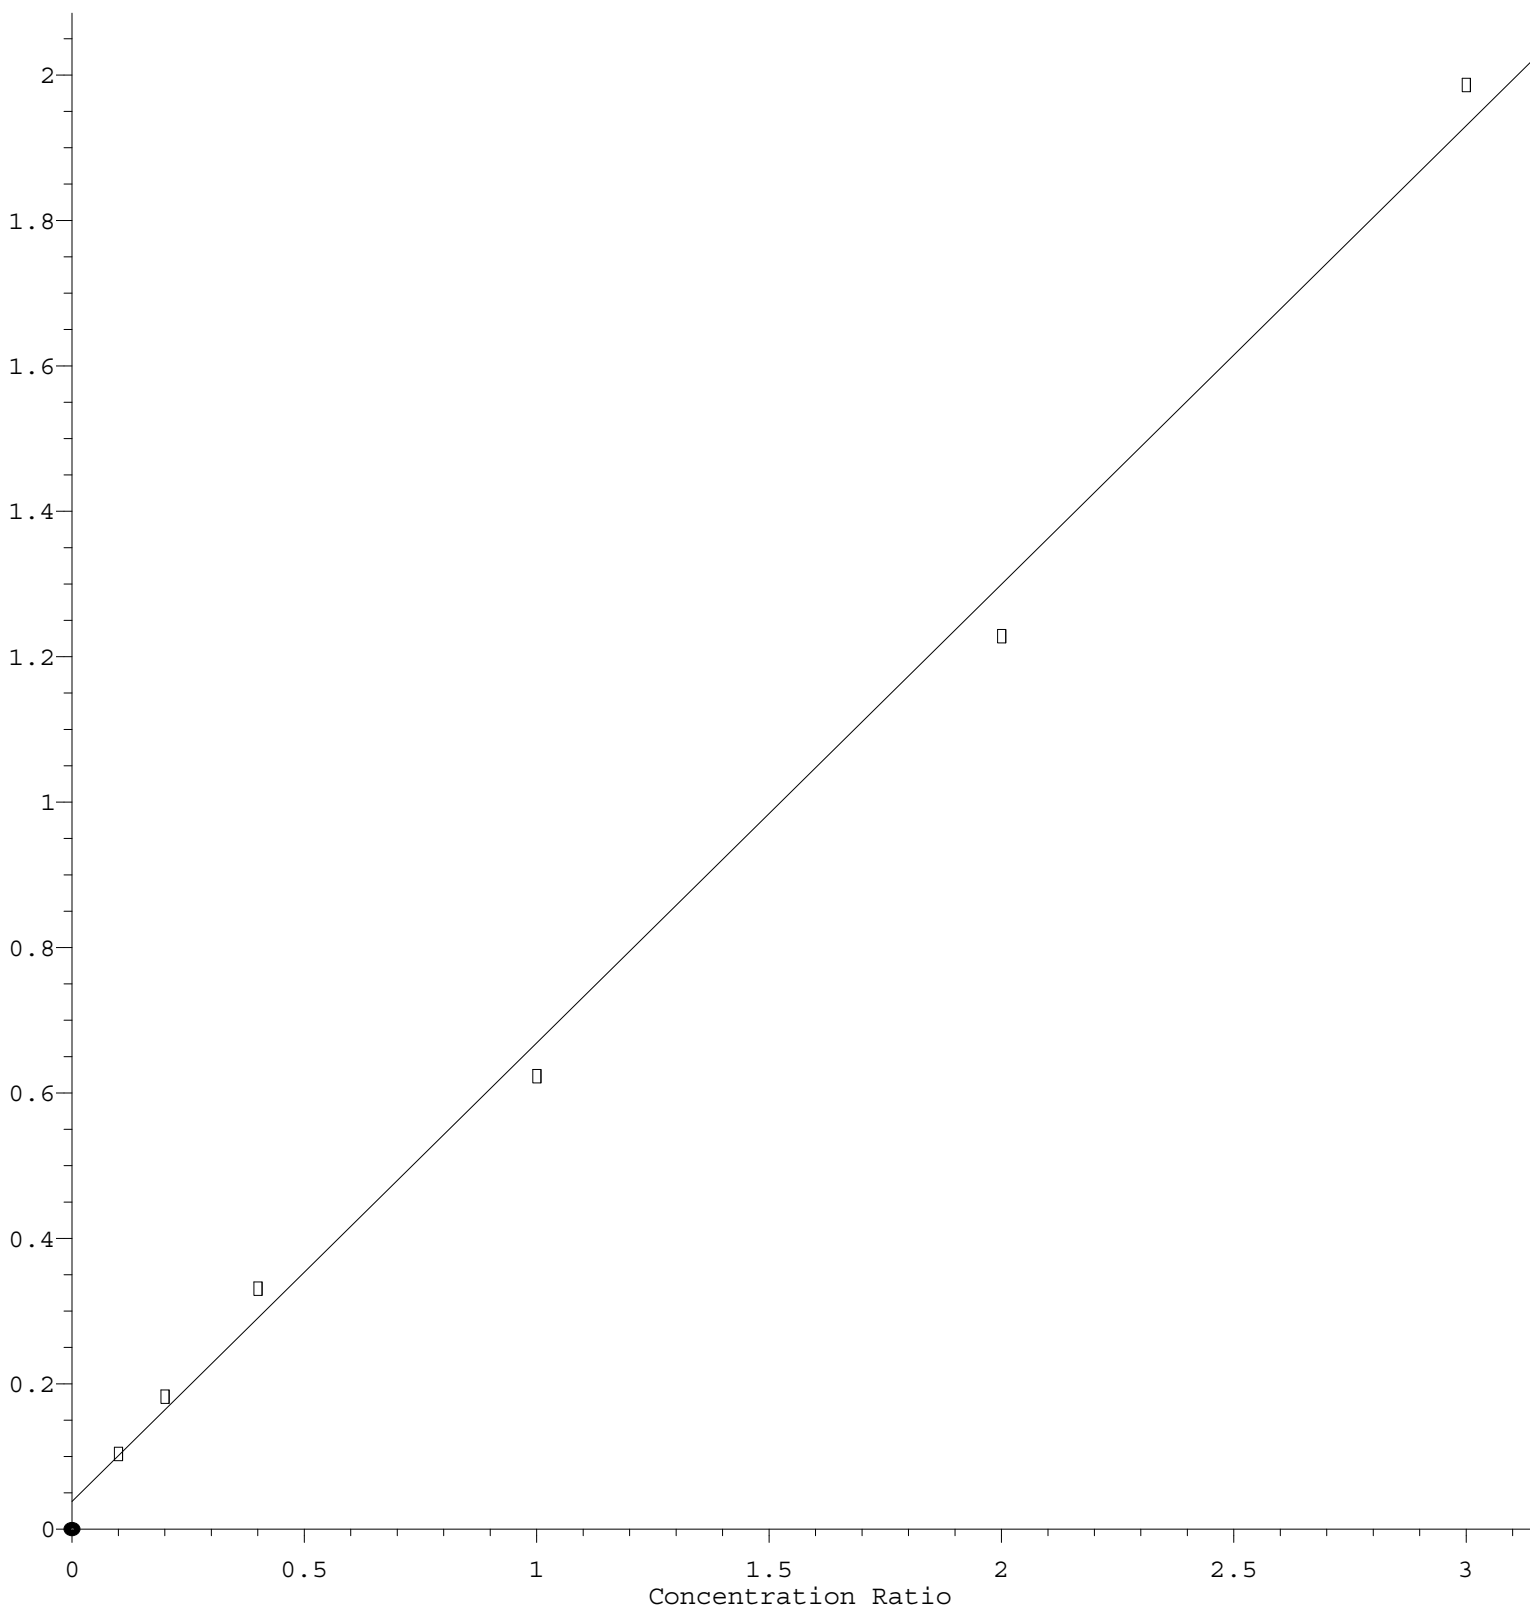

$$\text{Response} = 6.307\text{e-}001 * \text{Amt} + 3.794\text{e-}002$$


Coef of Det (r^2) = 0.995432 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D063022S.M

Calibration Table Last Updated: Tue Jul 05 10:05:34 2022

Methylene Chloride

Response Ratio

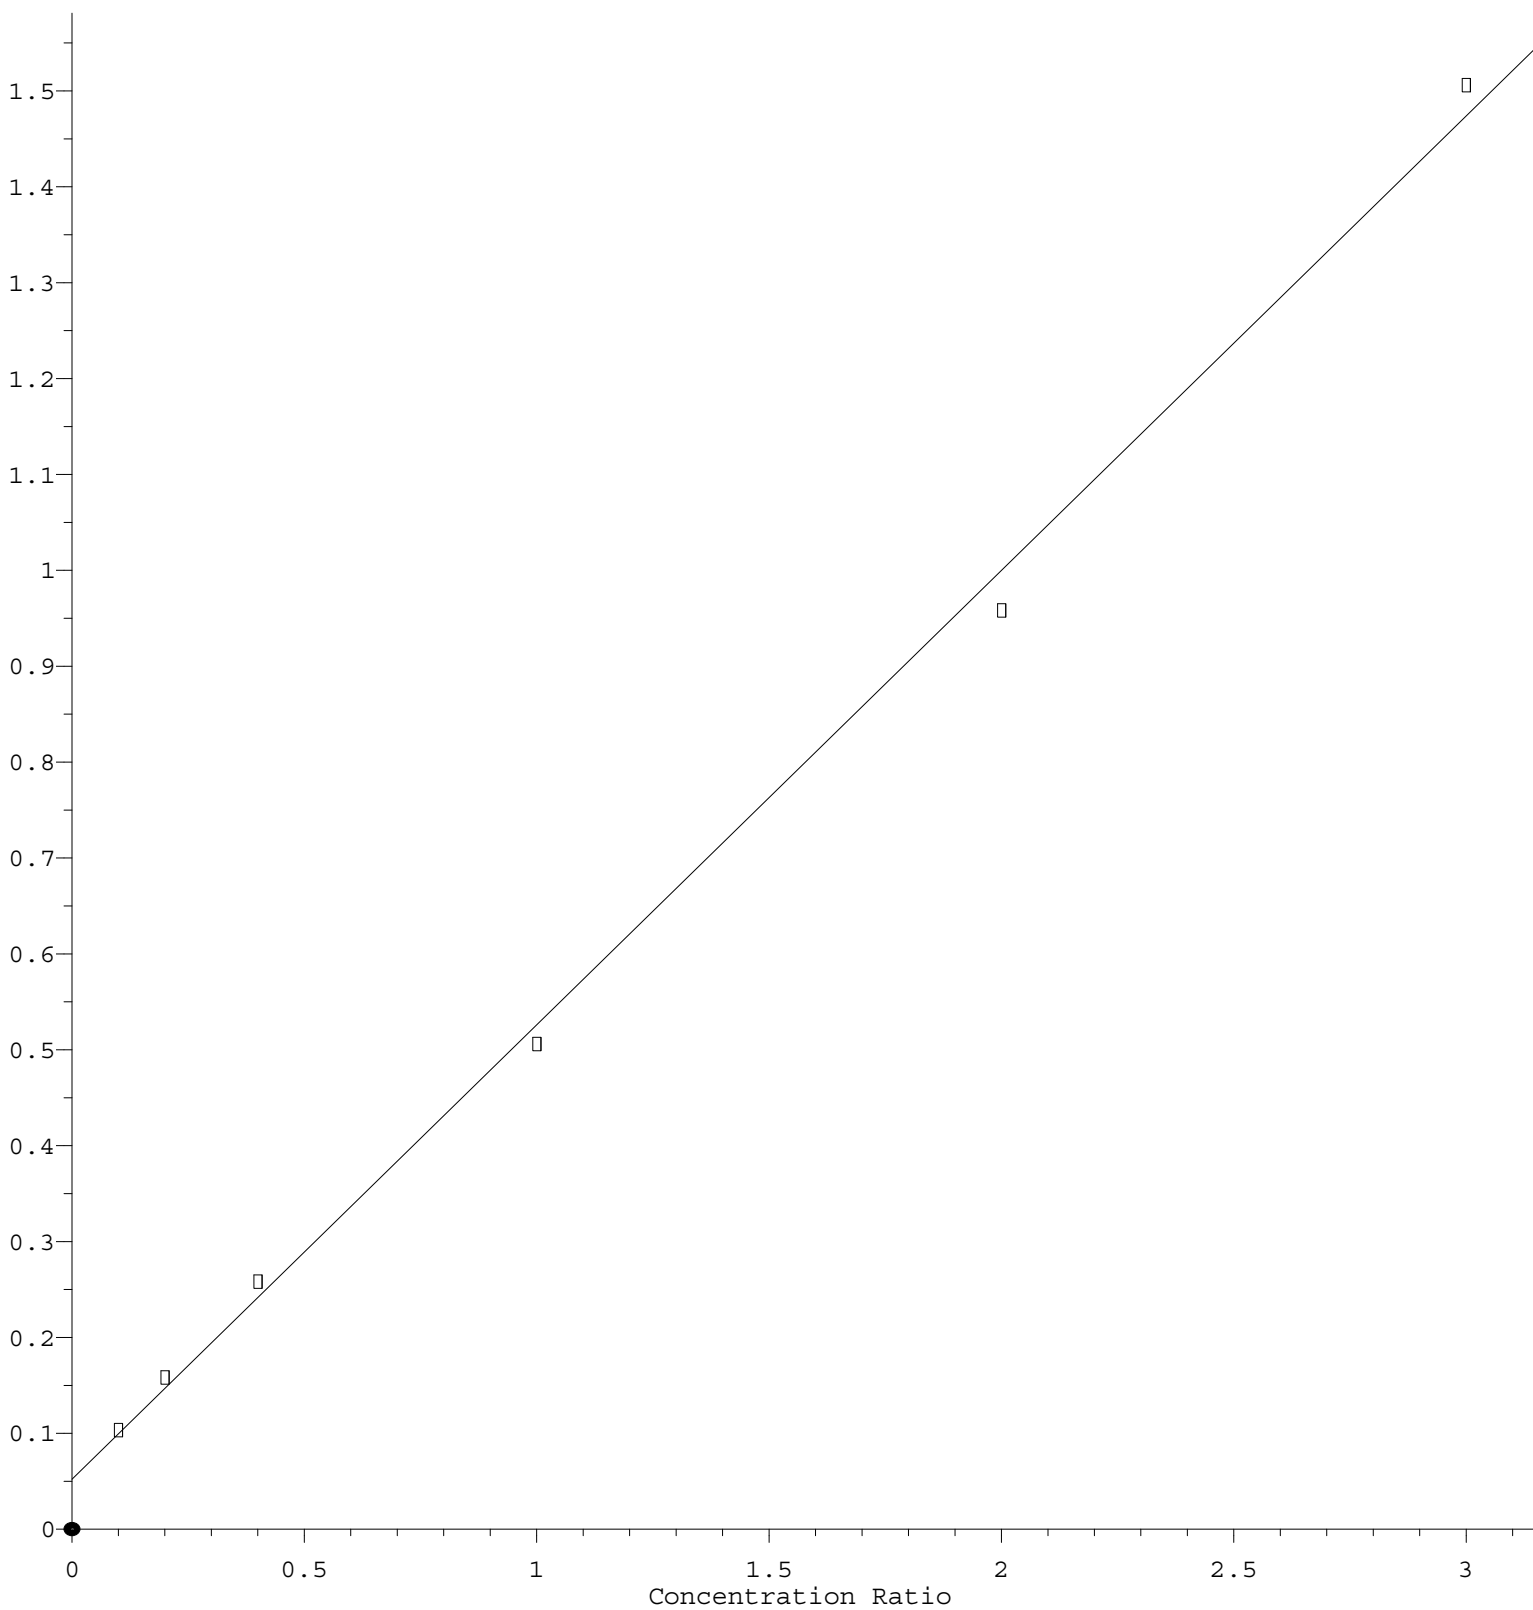

$$\text{Response} = 4.739\text{e-}001 * \text{Amt} + 5.239\text{e-}002$$


Coef of Det (r^2) = 0.997626 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D063022S.M

Calibration Table Last Updated: Tue Jul 05 10:05:34 2022

Methyl Acetate

Response Ratio

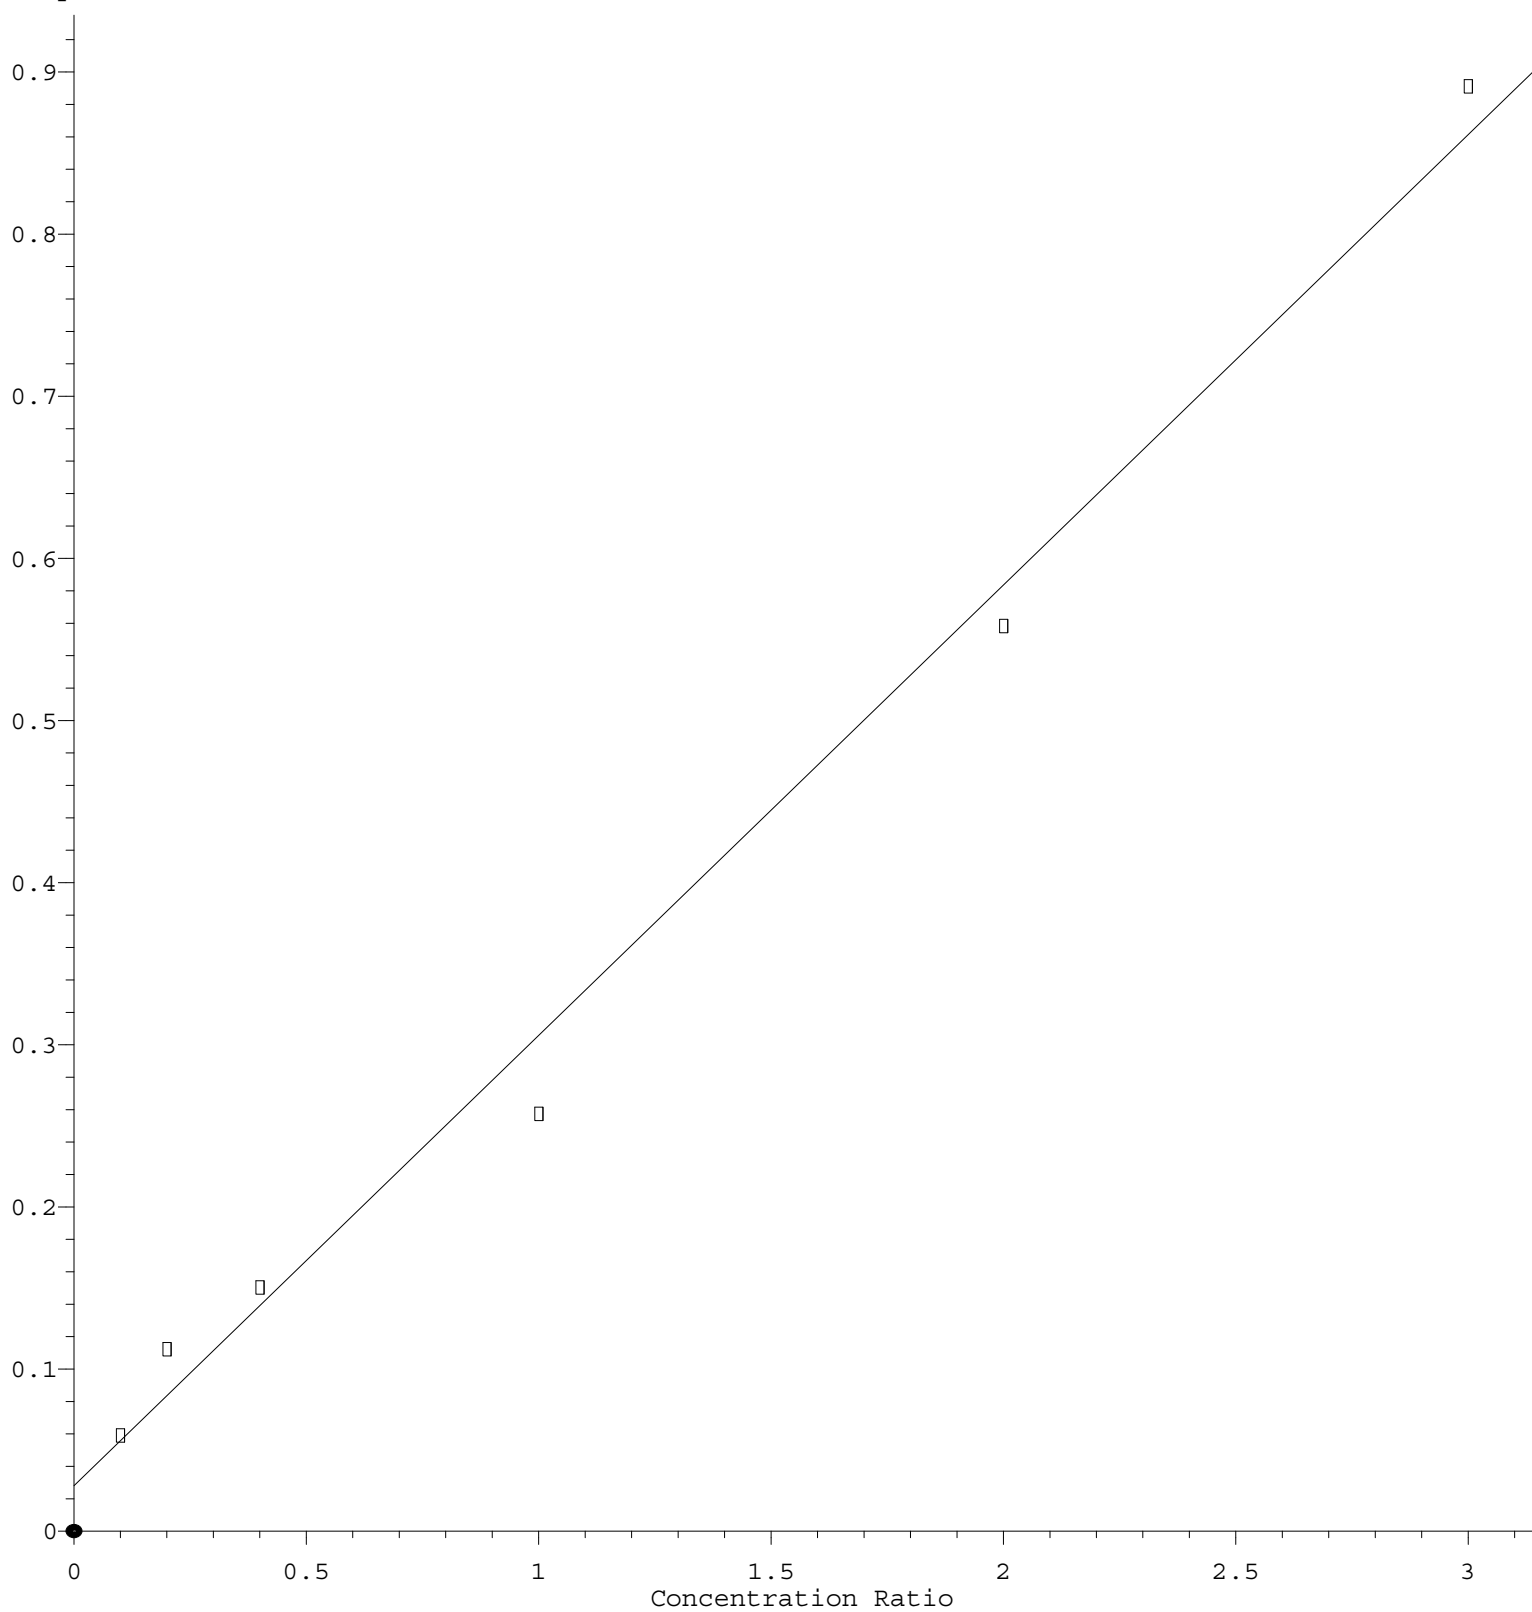

$$\text{Response} = 2.780\text{e-}001 * \text{Amt} + 2.753\text{e-}002$$

Coef of Det (r^2) = 0.990808 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D063022S.M

Calibration Table Last Updated: Tue Jul 05 10:05:34 2022