


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD063023\
Data File : VD076668.D
Acq On : 30 Jun 2023 17:54
Operator : KP/SY
Sample : 03472-22
Misc : 4.30G/10.0ml/MSVOA_D/SOIL
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
A46R3

Manual IntegrationsAPPROVED

Quant Time: Jul 03 01:31:36 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM061523SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jun 16 01:50:34 2023
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 07/03/2023
Supervised By :Mahesh Dadoda 07/07/2023

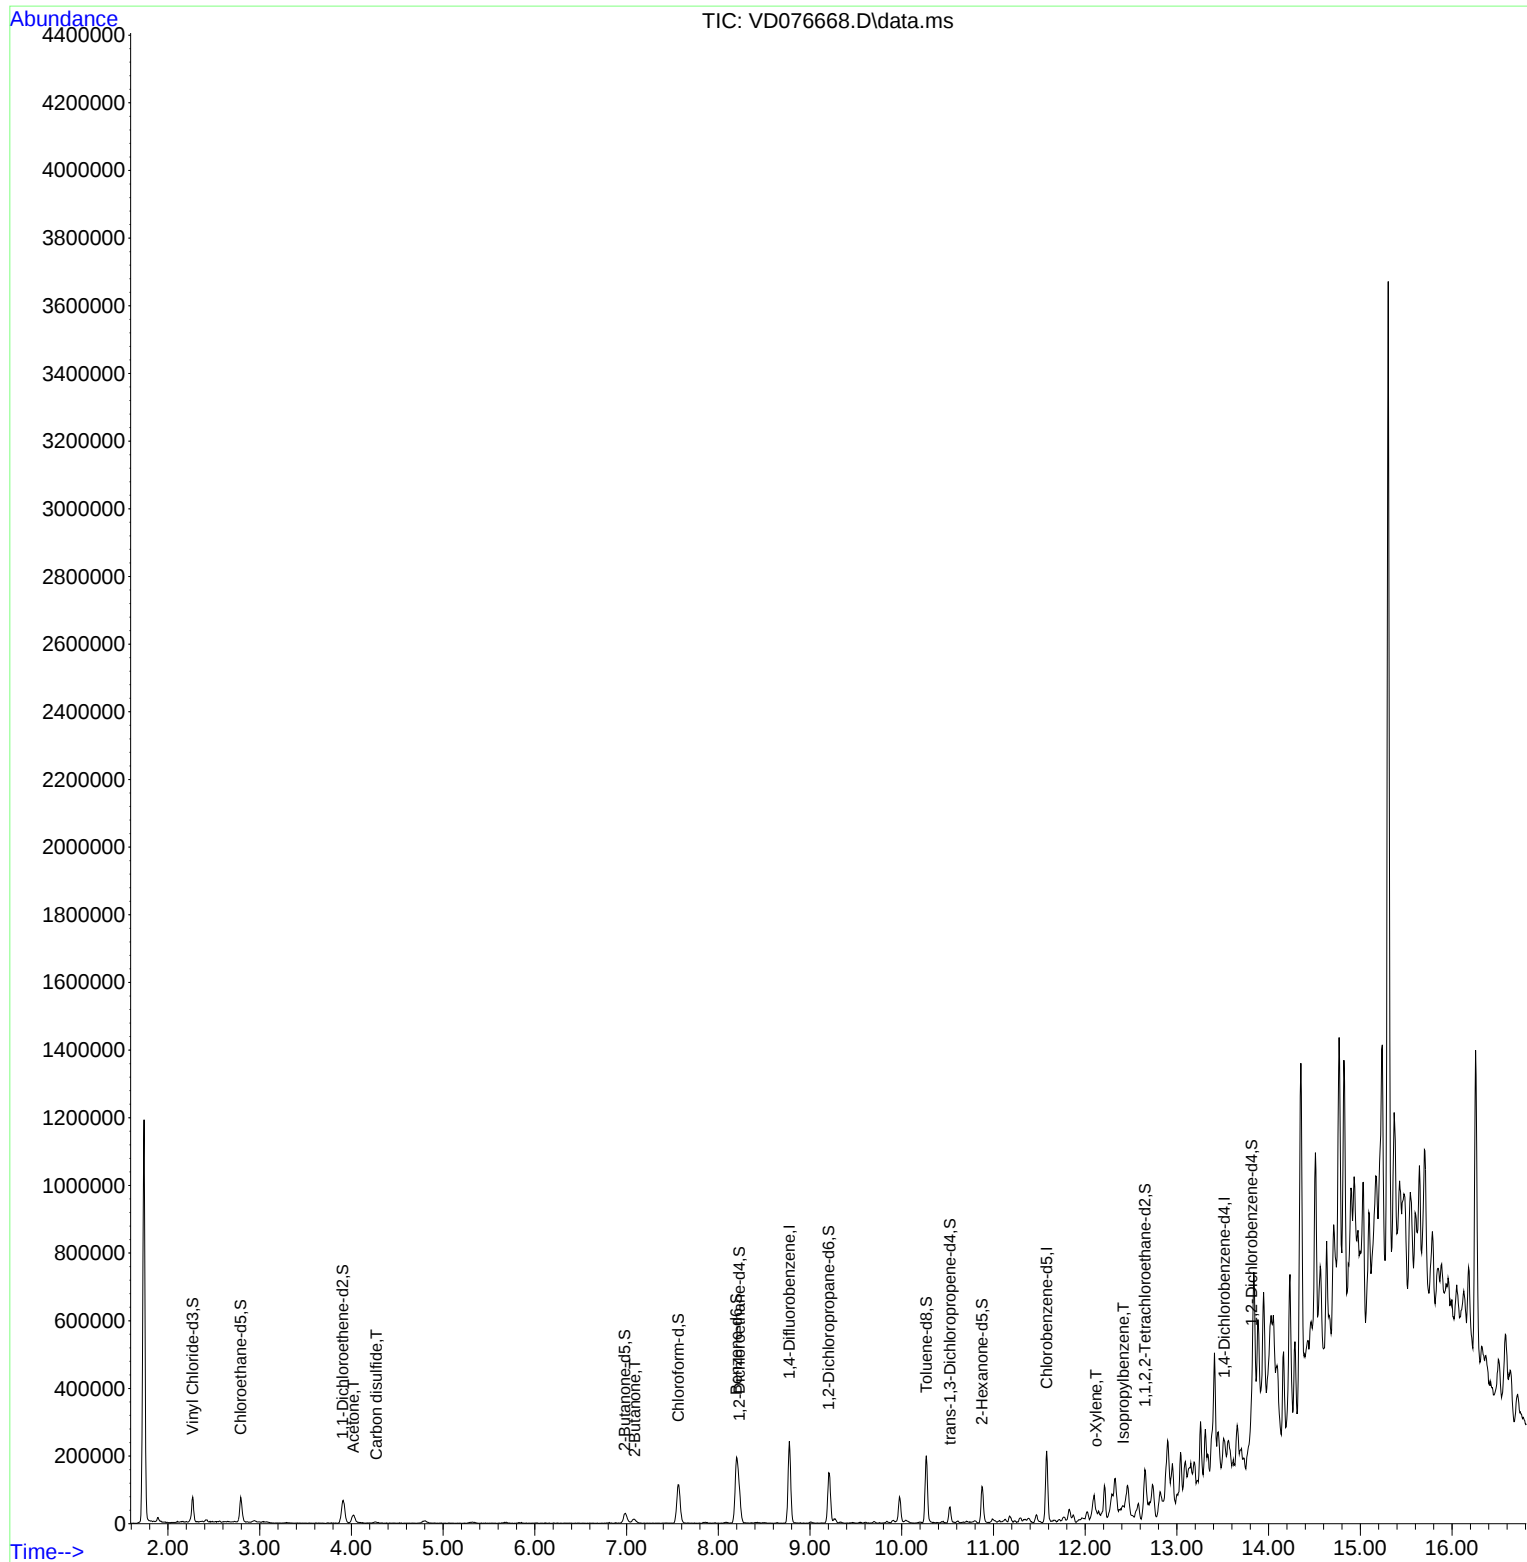




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD063023\
Data File : VD076668.D
Acq On : 30 Jun 2023 17:54
Operator : KP/SY
Sample : 03472-22
Misc : 4.30G/10.0ml/MSVOA_D/SOIL
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
A46R3

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 07/03/2023
Supervised By :Mahesh Dadoda 07/07/2023

Quant Time: Jul 03 01:31:36 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM061523SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jun 16 01:50:34 2023
Response via : Initial Calibration

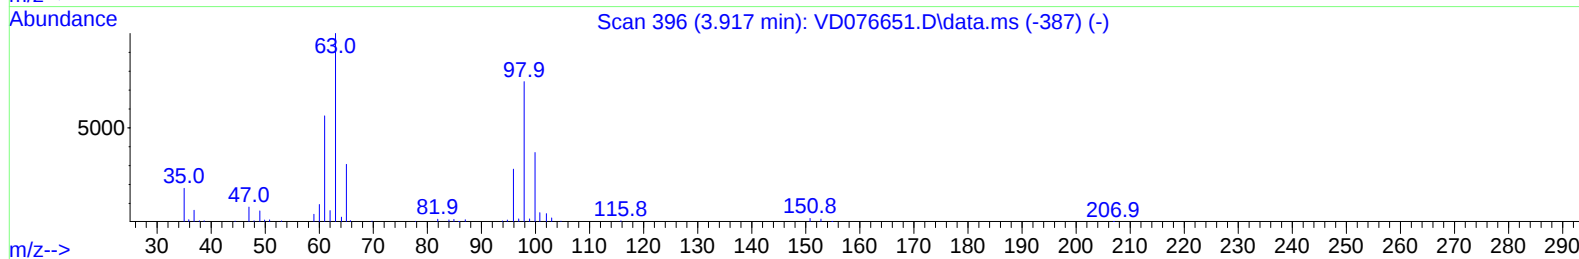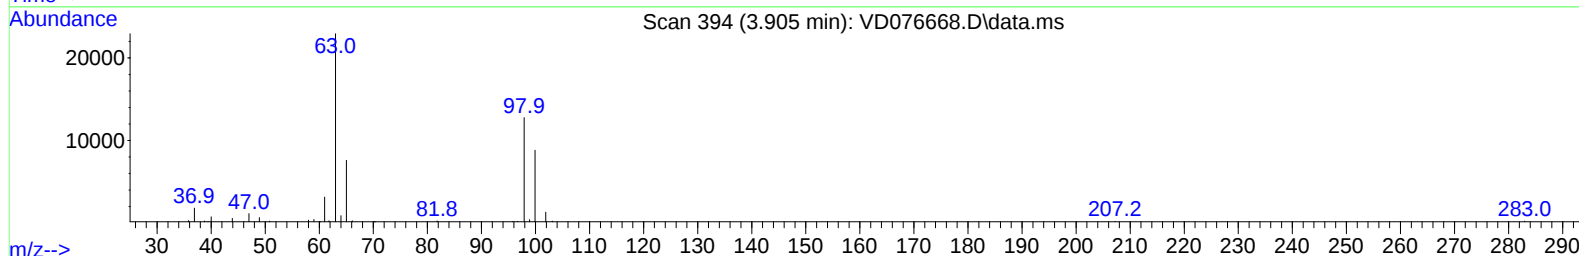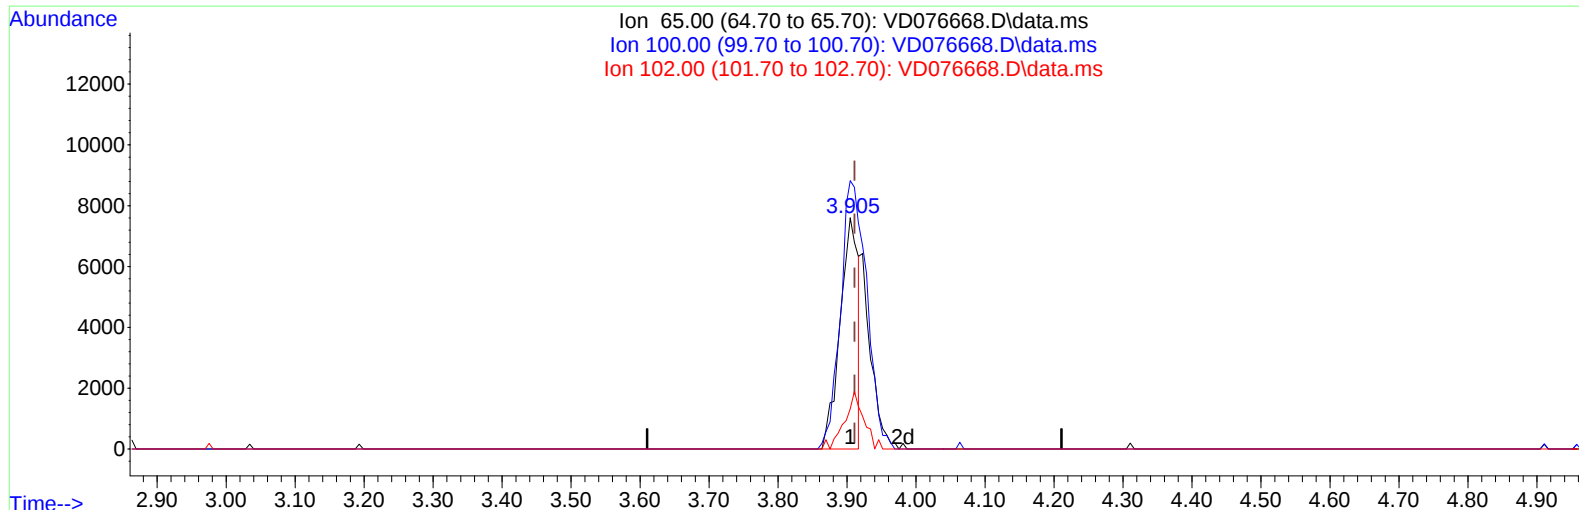

TIC: VD076668.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

3.905min (-0.006) 10.70 ug/L

response 13851

Ion	Exp%	Act%
65.00	100.00	100.00
100.00	143.00	167.95
102.00	21.10	24.62
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD063023\
Data File : VD076668.D
Acq On : 30 Jun 2023 17:54
Operator : KP/SY
Sample : 03472-22
Misc : 4.30G/10.0ml/MSVOA_D/SOIL
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
A46R3

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 07/03/2023
Supervised By :Mahesh Dadoda 07/07/2023

Quant Time: Jul 03 01:31:36 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM061523SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jun 16 01:50:34 2023
Response via : Initial Calibration

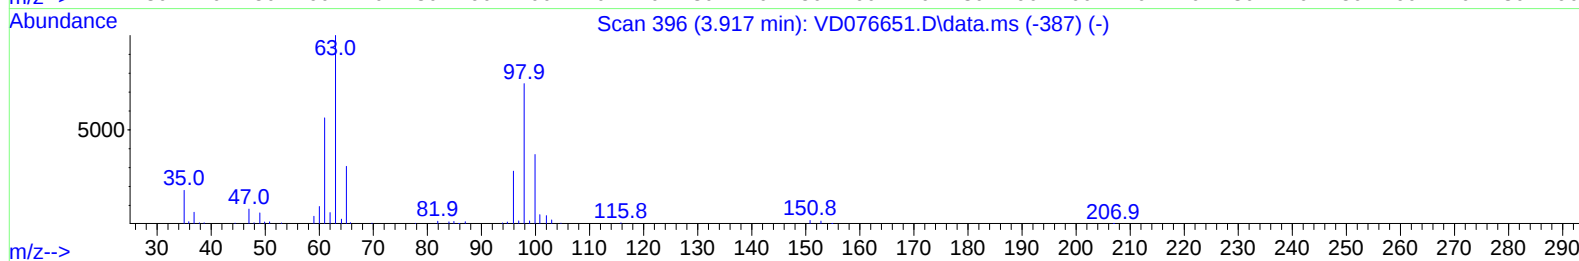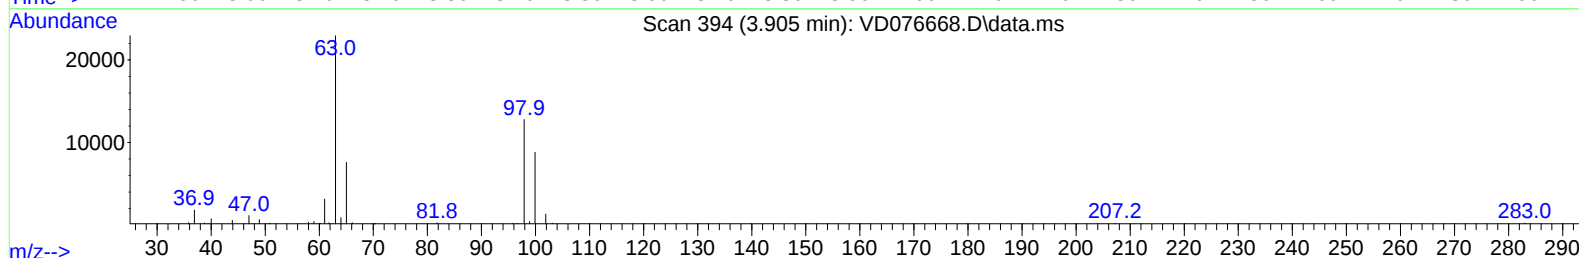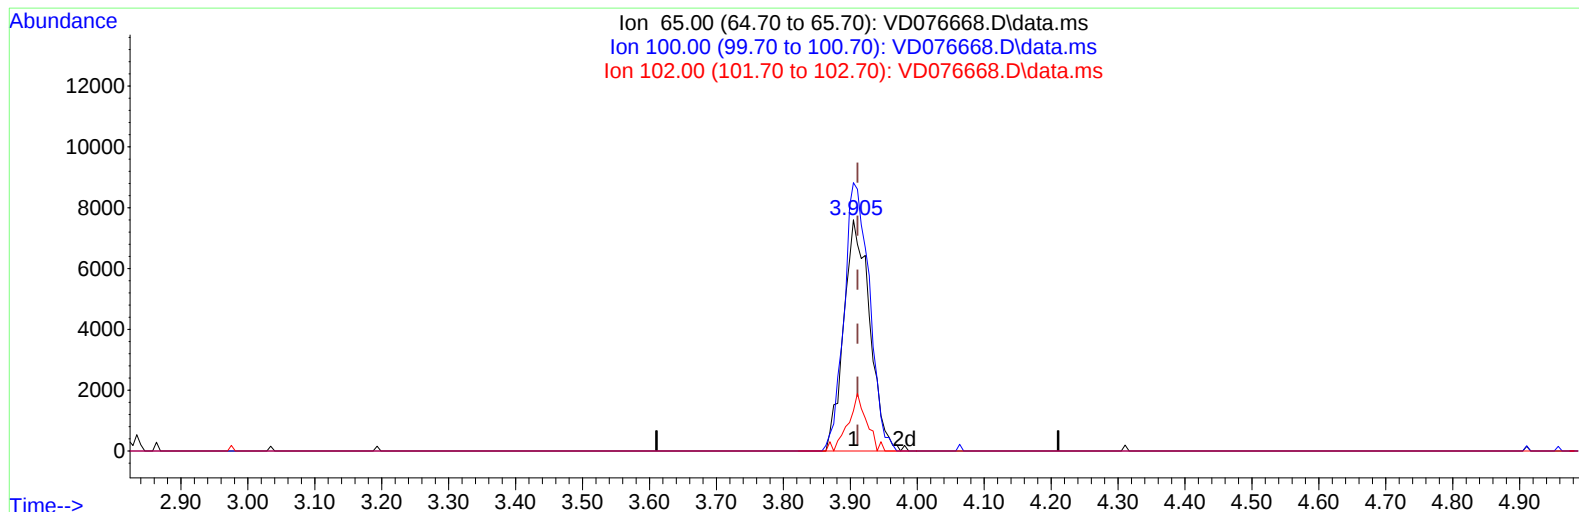

TIC: VD076668.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

3.905min (-0.006) 15.88 ug/L m

response 20572

Ion	Exp%	Act%
65.00	100.00	100.00
100.00	143.00	113.08
102.00	21.10	16.58
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD063023\
 Data File : VD076668.D
 Acq On : 30 Jun 2023 17:54
 Operator : KP/SY
 Sample : 03472-22
 Misc : 4.30G/10.0ml/MSVOA_D/SOIL
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 A46R3

Manual IntegrationsAPPROVED

Quant Time: Jul 03 01:31:36 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM061523SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 16 01:50:34 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 07/03/2023
 Supervised By :Mahesh Dadoda 07/07/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.775	114	203728	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.581	117	116257	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.516	152	33214	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.269	65	64821	13.065	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	52.280%		
7) Chloroethane-d5	2.793	69	70648	17.610	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	70.440%		
11) 1,1-Dichloroethene-d2	3.905	65	20572m	15.885	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	63.520%		
21) 2-Butanone-d5	6.981	46	52904	70.408	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	140.820%#		
24) Chloroform-d	7.563	84	116157	21.641	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	86.560%		
26) 1,2-Dichloroethane-d4	8.228	65	67823	25.614	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	102.440%		
32) Benzene-d6	8.199	84	196269	27.598	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	110.400%		
36) 1,2-Dichloropropane-d6	9.204	67	73546	32.399	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	129.600%#		
41) Toluene-d8	10.269	98	129095	19.604	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	78.400%		
43) trans-1,3-Dichloroprop...	10.528	79	25929	27.462	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	109.840%		
47) 2-Hexanone-d5	10.875	63	35534	100.842	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	201.680%#		
56) 1,1,2,2-Tetrachloroeth...	12.651	84	51042	31.605	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	126.400%#		
66) 1,2-Dichlorobenzene-d4	13.816	152	24162	19.847	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	79.400%		
Target Compounds					Qvalue	
13) Acetone	4.022	43	41856	68.968	ug/L	72
14) Carbon disulfide	4.269	76	7053	0.736	ug/L	97
22) 2-Butanone	7.087	43	19577	19.989	ug/L	90
54) o-Xylene	12.116	106	1311	0.395	ug/L	88
60) Isopropylbenzene	12.416	105	3646	0.718	ug/L #	57

(#) = qualifier out of range (m) = manual integration (+) = signals summed