

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD063023\
 Data File : VD076672.D
 Acq On : 30 Jun 2023 19:40
 Operator : KP/SY
 Sample : 03472-16
 Misc : 5.14G/10.0ml/MSVOA_D/SOIL
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 A46T0

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 07/03/2023
 Supervised By :Mahesh Dadoda 07/07/2023

Quant Time: Jul 03 01:32:09 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM061523SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 16 01:50:34 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.775	114	316361	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.581	117	266456	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.516	152	110862	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.269	65	78727	10.219	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	40.880%		
7) Chloroethane-d5	2.787	69	88487	14.204	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	56.800%		
11) 1,1-Dichloroethene-d2	3.904	65	28745	14.293	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	57.160%		
21) 2-Butanone-d5	6.981	46	127993	109.696	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	219.400%#		
24) Chloroform-d	7.563	84	176700	21.200	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	84.800%		
26) 1,2-Dichloroethane-d4	8.228	65	114097	27.749	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	111.000%		
32) Benzene-d6	8.198	84	313407	19.228	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	76.920%		
36) 1,2-Dichloropropane-d6	9.210	67	114998	22.103	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	88.400%		
41) Toluene-d8	10.269	98	265870	17.616	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	70.480%		
43) trans-1,3-Dichloroprop...	10.522	79	47845	22.109	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	88.440%		
47) 2-Hexanone-d5	10.875	63	88404	109.462	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	218.920%#		
56) 1,1,2,2-Tetrachloroeth...	12.651	84	145486	39.305	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	157.200%#		
66) 1,2-Dichlorobenzene-d4	13.816	152	91843	22.602	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	90.400%		
Target Compounds						Qvalue
5) Vinyl chloride	2.275	62	44833	5.071	ug/L	88
12) 1,1-Dichloroethene	3.928	96	3503	0.853	ug/L #	1
13) Acetone	4.016	43	11147	11.828	ug/L	89
14) Carbon disulfide	4.257	76	6943	0.466	ug/L #	76
20) cis-1,2-Dichloroethene	7.069	96	40976	8.015	ug/L	93
22) 2-Butanone	7.093	43	4978m	3.273	ug/L	
34) Trichloroethene	9.028	95	8835	1.950	ug/L	89
46) Tetrachloroethene	10.810	164	2782	0.781	ug/L	78

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD063023\
Data File : VD076672.D
Acq On : 30 Jun 2023 19:40
Operator : KP/SY
Sample : 03472-16
Misc : 5.14G/10.0ml/MSVOA_D/SOIL
ALS Vial : 24 Sample Multiplier: 1


Instrument :
MSVOA_D
ClientSampleId :
A46T0

Quant Time: Jul 03 01:32:09 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM061523SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jun 16 01:50:34 2023
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 07/03/2023
Supervised By :Mahesh Dadoda 07/07/2023

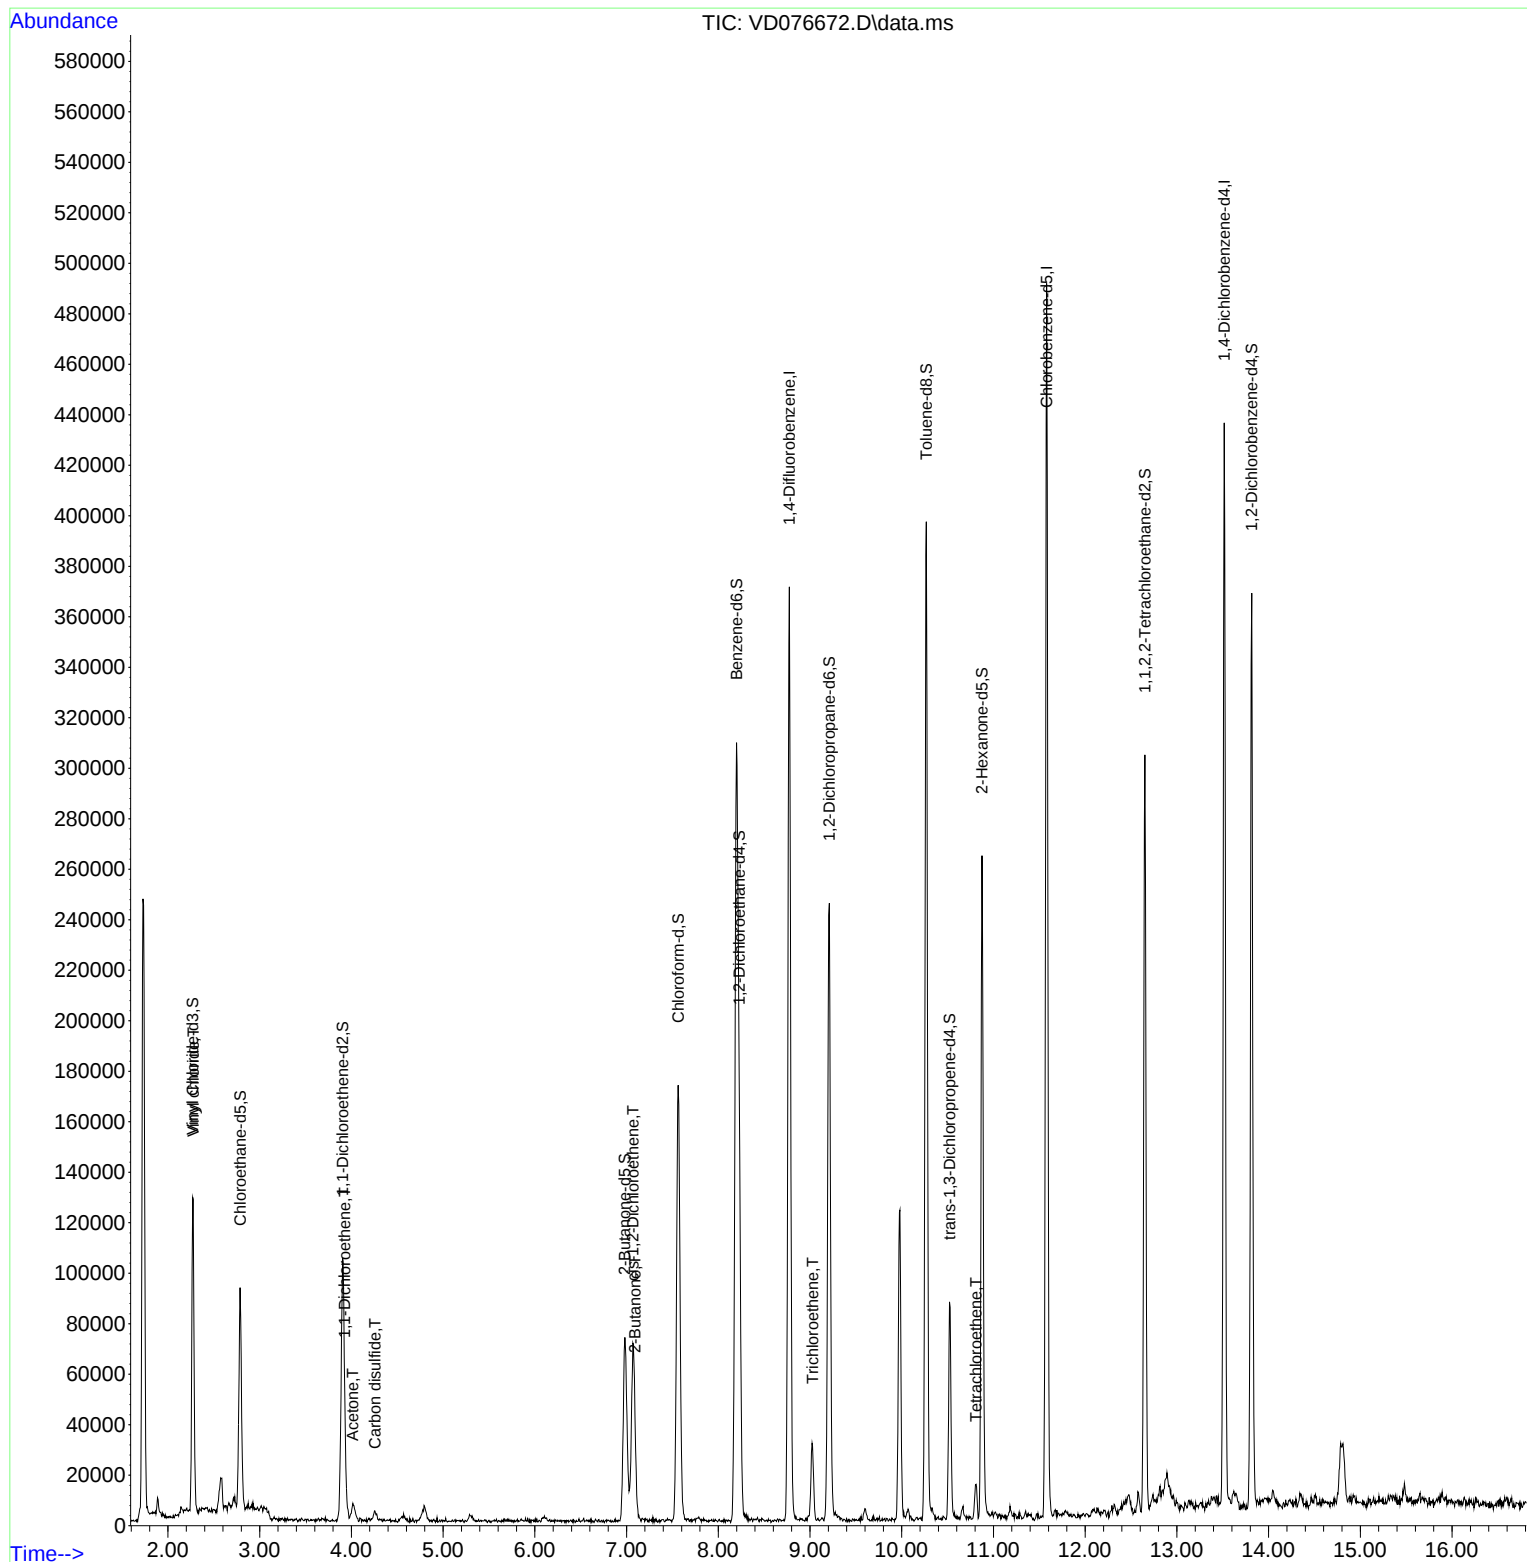

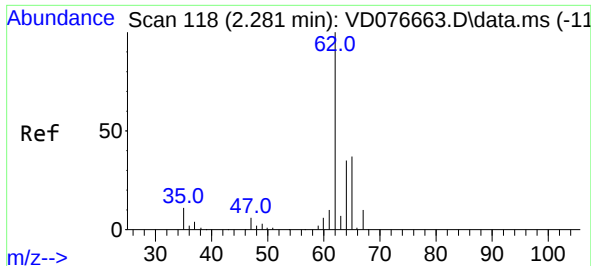





#5
Vinyl chloride
Concen: 5.071 ug/L
RT: 2.275 min Scan# 11
Delta R.T. -0.000 min
Lab File: VD076672.D
Acq: 30 Jun 2023 19:40

Instrument :
MSVOA_D
ClientSampleId :
A46T0

Tgt Ion: 62 Resp: 4483
Ion Ratio Lower Upper
62 100
64 36.6 21.1 39.1




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 07/03/2023
Supervised By :Mahesh Dadoda 07/07/2023

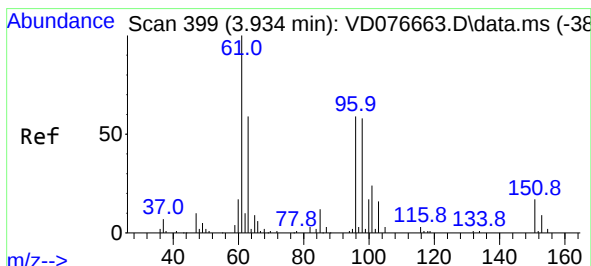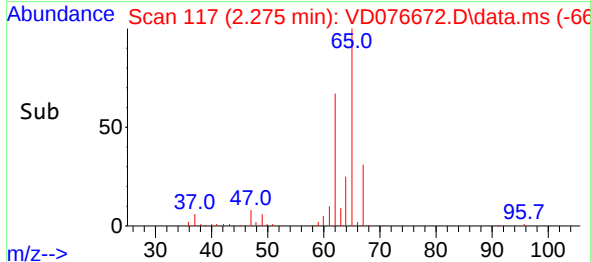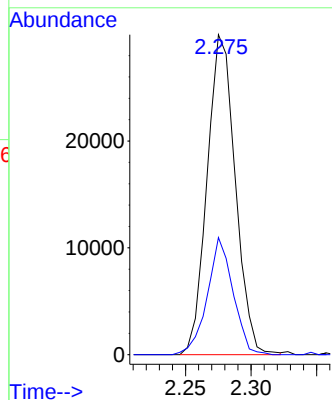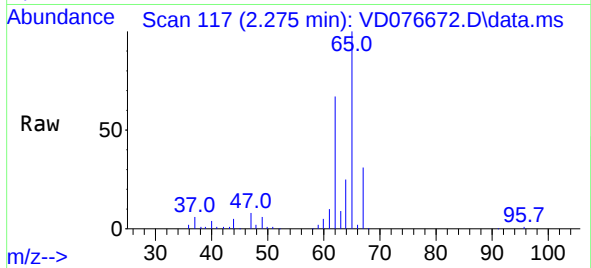

#12
1,1-Dichloroethene
Concen: 0.853 ug/L
RT: 3.928 min Scan# 398
Delta R.T. -0.000 min
Lab File: VD076672.D
Acq: 30 Jun 2023 19:40

Tgt Ion: 96 Resp: 3503
Ion Ratio Lower Upper
96 100
61 247.5 113.0 209.8#
63 917.5 83.6 155.2#

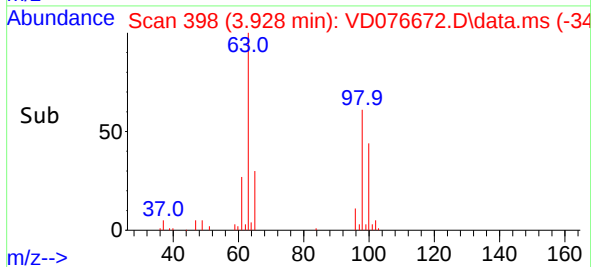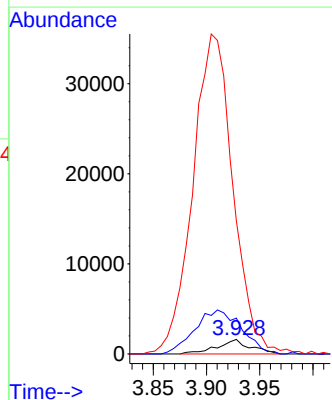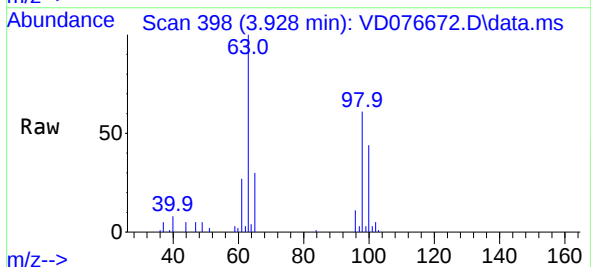

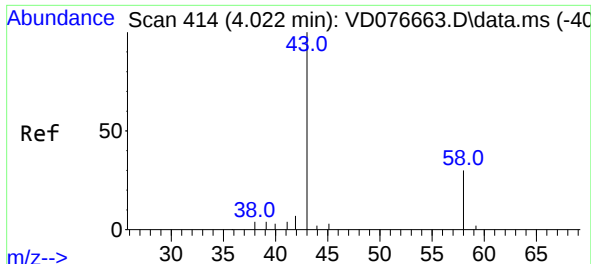





#13
Acetone
Concen: 11.828 ug/L
RT: 4.016 min Scan# 41
Delta R.T. -0.006 min
Lab File: VD076672.D
Acq: 30 Jun 2023 19:40

Instrument :
MSVOA_D
ClientSampleId :
A46T0

Tgt Ion: 43 Resp: 1114
Ion Ratio Lower Upper
43 100
58 27.4 0.0 67.4




Manual Integrations
APPROVED


Reviewed By :Semsettin Yesilyurt 07/03/2023
Supervised By :Mahesh Dadoda 07/07/2023

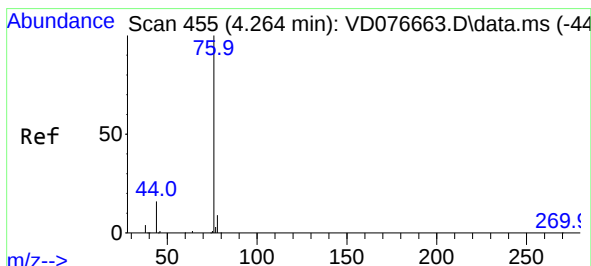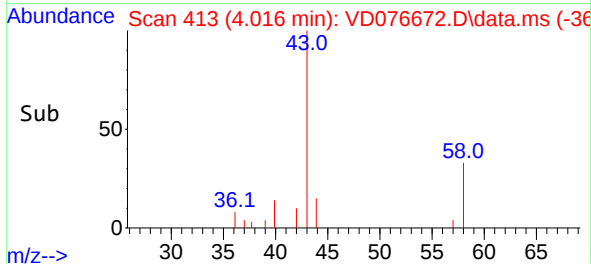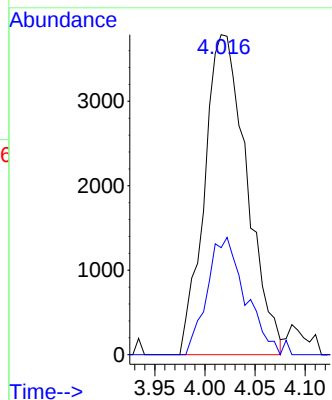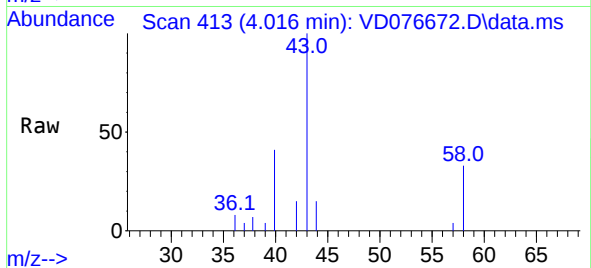

#14
Carbon disulfide
Concen: 0.466 ug/L
RT: 4.257 min Scan# 454
Delta R.T. -0.006 min
Lab File: VD076672.D
Acq: 30 Jun 2023 19:40


Tgt Ion: 76 Resp: 6943
Ion Ratio Lower Upper
76 100
78 17.4 7.0 10.4#

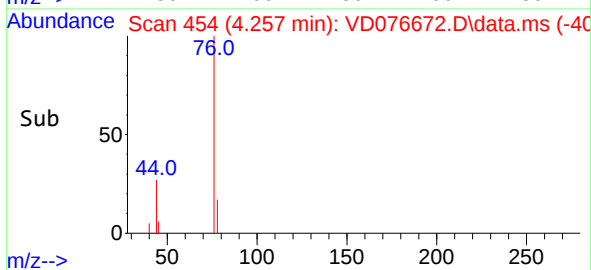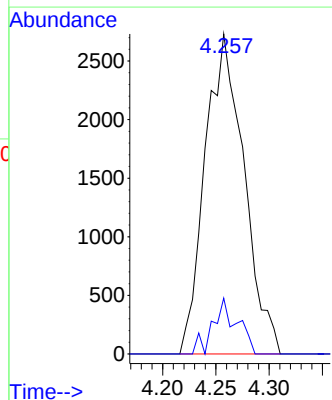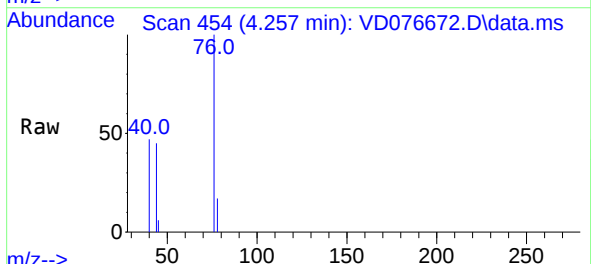

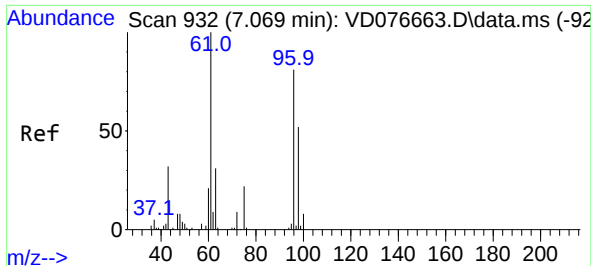

#20
cis-1,2-Dichloroethene
Concen: 8.015 ug/L
RT: 7.069 min Scan# 91
Delta R.T. -0.006 min
Lab File: VD076672.D
Acq: 30 Jun 2023 19:40




Instrument :
MSVOA_D
ClientSampleId :
A46T0

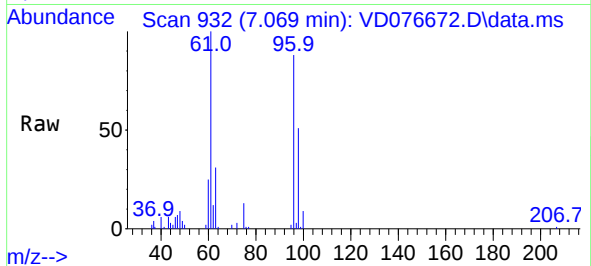


Tgt Ion: 96 Resp: 40970
Ion Ratio Lower Upper
96 100
61 113.1 86.0 159.6
98 58.0 42.2 78.4

Manual Integrations
APPROVED



Reviewed By :Semsettin Yesilyurt 07/03/2023
Supervised By :Mahesh Dadoda 07/07/2023

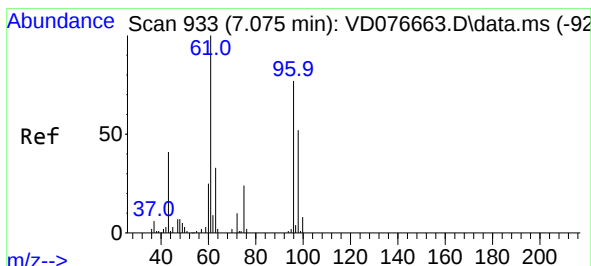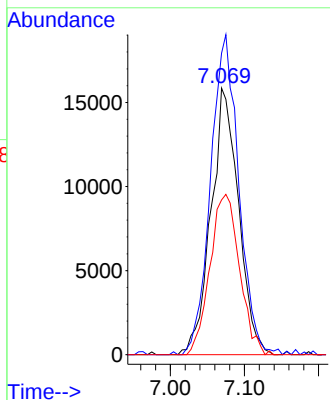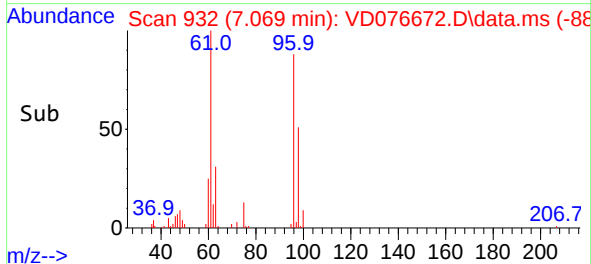


#22
2-Butanone
Concen: 3.273 ug/L m
RT: 7.093 min Scan# 936
Delta R.T. 0.011 min
Lab File: VD076672.D
Acq: 30 Jun 2023 19:40

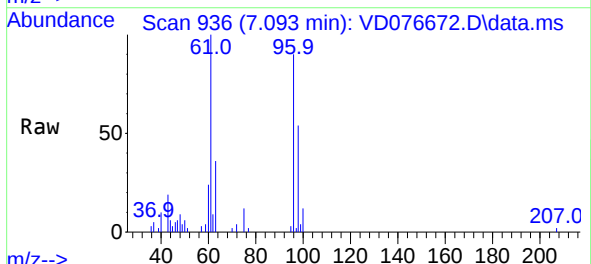


Tgt Ion: 43 Resp: 4978
Ion Ratio Lower Upper
43 100
72 25.1 12.9 38.7

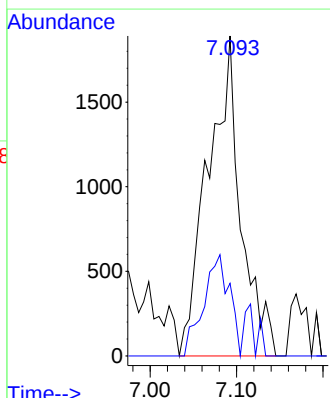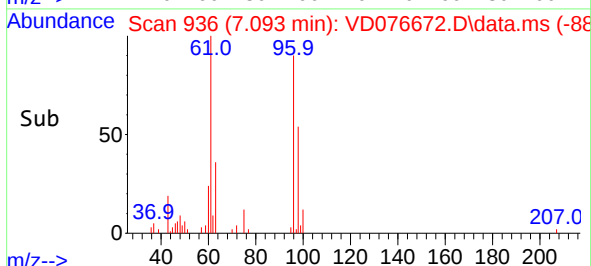

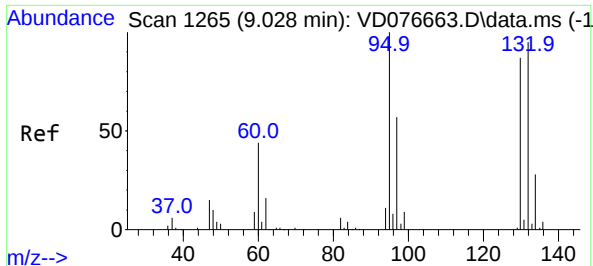

#34
Trichloroethene
Concen: 1.950 ug/L
RT: 9.028 min Scan# 1265
Delta R.T. -0.000 min
Lab File: VD076672.D
Acq: 30 Jun 2023 19:40




Instrument :
MSVOA_D
ClientSampleId :
A46T0

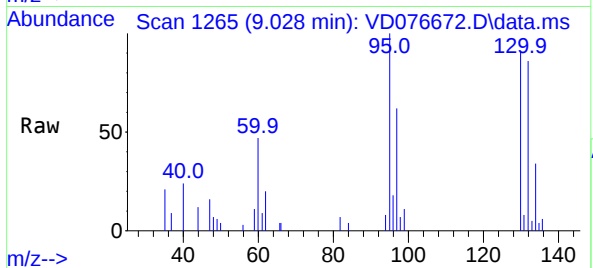


Tgt Ion: 95 Resp: 883
Ion Ratio Lower Upper
95 100
97 62.4 43.1 80.1
132 85.8 71.8 133.4
130 90.6 71.9 133.5

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 07/03/2023
Supervised By :Mahesh Dadoda 07/07/2023

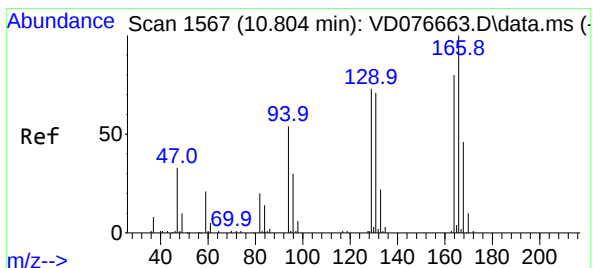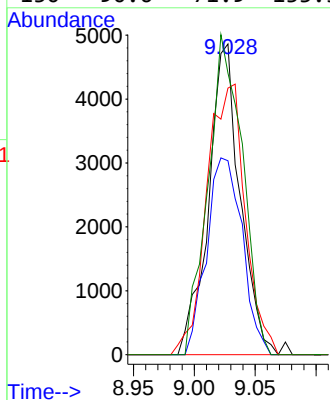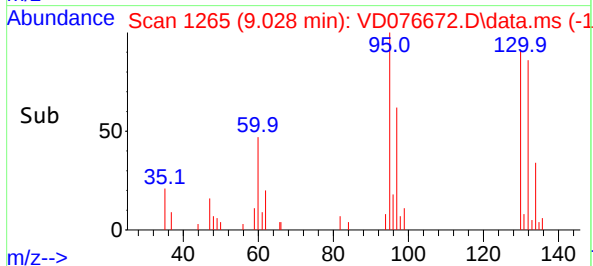

#46
Tetrachloroethene
Concen: 0.781 ug/L
RT: 10.810 min Scan# 1568
Delta R.T. -0.000 min
Lab File: VD076672.D
Acq: 30 Jun 2023 19:40

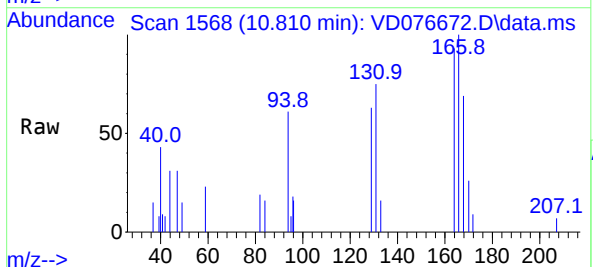

Tgt Ion:164 Resp: 2782
Ion Ratio Lower Upper
164 100
129 67.8 65.5 121.6
131 81.0 64.8 120.3
166 107.7 97.2 180.4

