
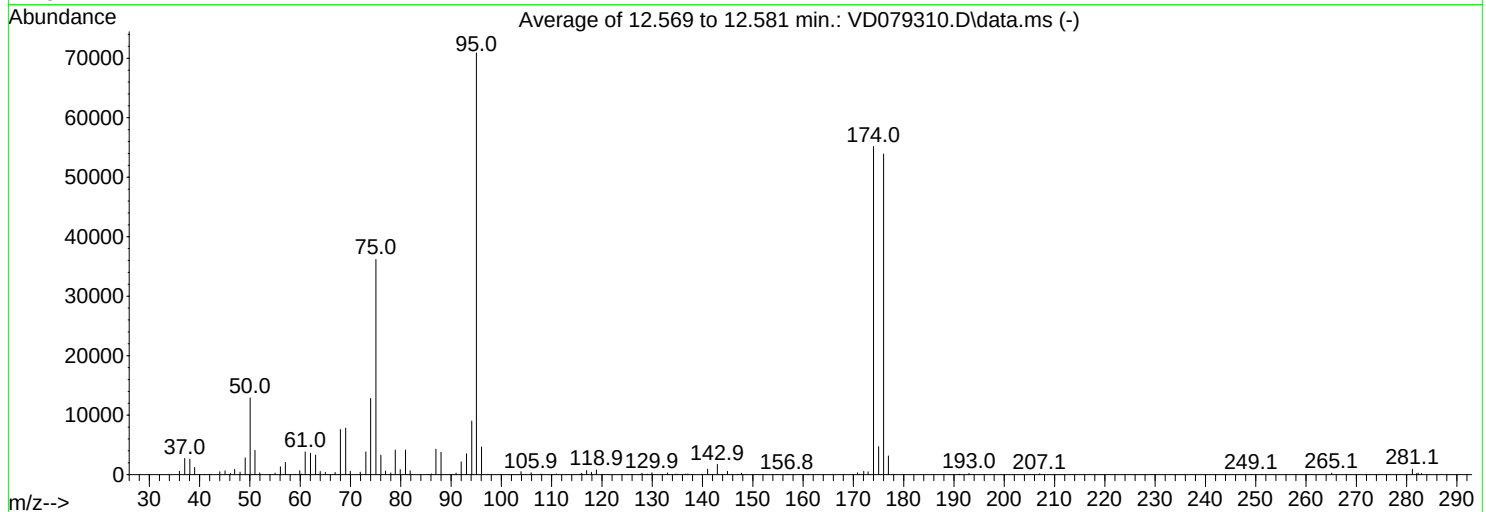


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD070224\
Data File : VD079310.D
Acq On : 02 Jul 2024 08:17
Operator : RP/MD
Sample : BFB
Misc : 5.00G/5.0ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D062824S.M
Title : SW846 8260
Last Update : Sat Jun 29 06:28:31 2024

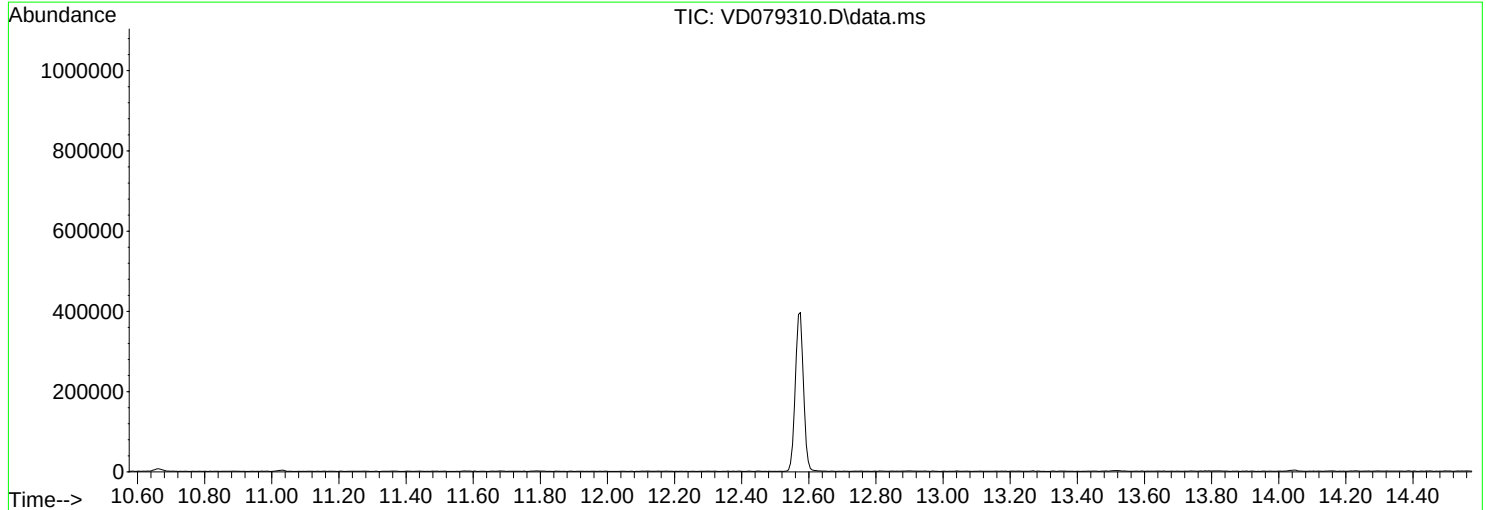

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1858

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.2	12926	PASS
75	95	30	60	51.0	36195	PASS
95	95	100	100	100.0	70912	PASS
96	95	5	9	6.6	4650	PASS
173	174	0.00	2	0.9	494	PASS
174	95	50	100	77.8	55165	PASS
175	174	5	9	8.6	4720	PASS
176	174	95	101	97.7	53896	PASS
177	176	5	9	5.9	3155	PASS