

Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD070319\
 Data File : VD063022.D
 Acq On : 3 Jul 2019 13:46
 Operator : VA/AP
 Sample : K3650-02
 Misc : 4.20g/5ml/MSVOA D/SOIL
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 FK-PS-01-051

Quant Time: Jul 04 01:56:05 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D061919S.M
 Quant Title : SW846 8260
 QLast Update : Thu Jun 20 01:50:56 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.05	168	824955	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.23	114	1099193	50.00	ug/l	0.00
63) Chlorobenzene-d5	12.37	117	744946	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	14.52	152	241991	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	7.46	65	431893	48.16	ug/l	0.00
Spiked Amount			Recovery	=	96.32%	
35) Dibromofluoromethane	6.93	113	459560	49.58	ug/l	0.00
Spiked Amount			Recovery	=	99.16%	
50) Toluene-d8	10.41	98	835187	41.40	ug/l	0.00
Spiked Amount			Recovery	=	82.80%	
62) 4-Bromofluorobenzene	13.55	95	252318	27.51	ug/l	0.00
Spiked Amount			Recovery	=	55.02%	


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA D\DATA\VD070319\
Data File : VD063022.D
Acq On : 3 Jul 2019 13:46
Operator : VA/AP
Sample : K3650-02
Misc : 4.20g/5ml/MSVOA D/SOIL
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
FK-PS-01-051

Quant Time: Jul 04 01:56:05 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_D\METHOD\82D061919S.M
Quant Title : SW846 8260
QLast Update : Thu Jun 20 01:50:56 2019
Response via : Initial Calibration

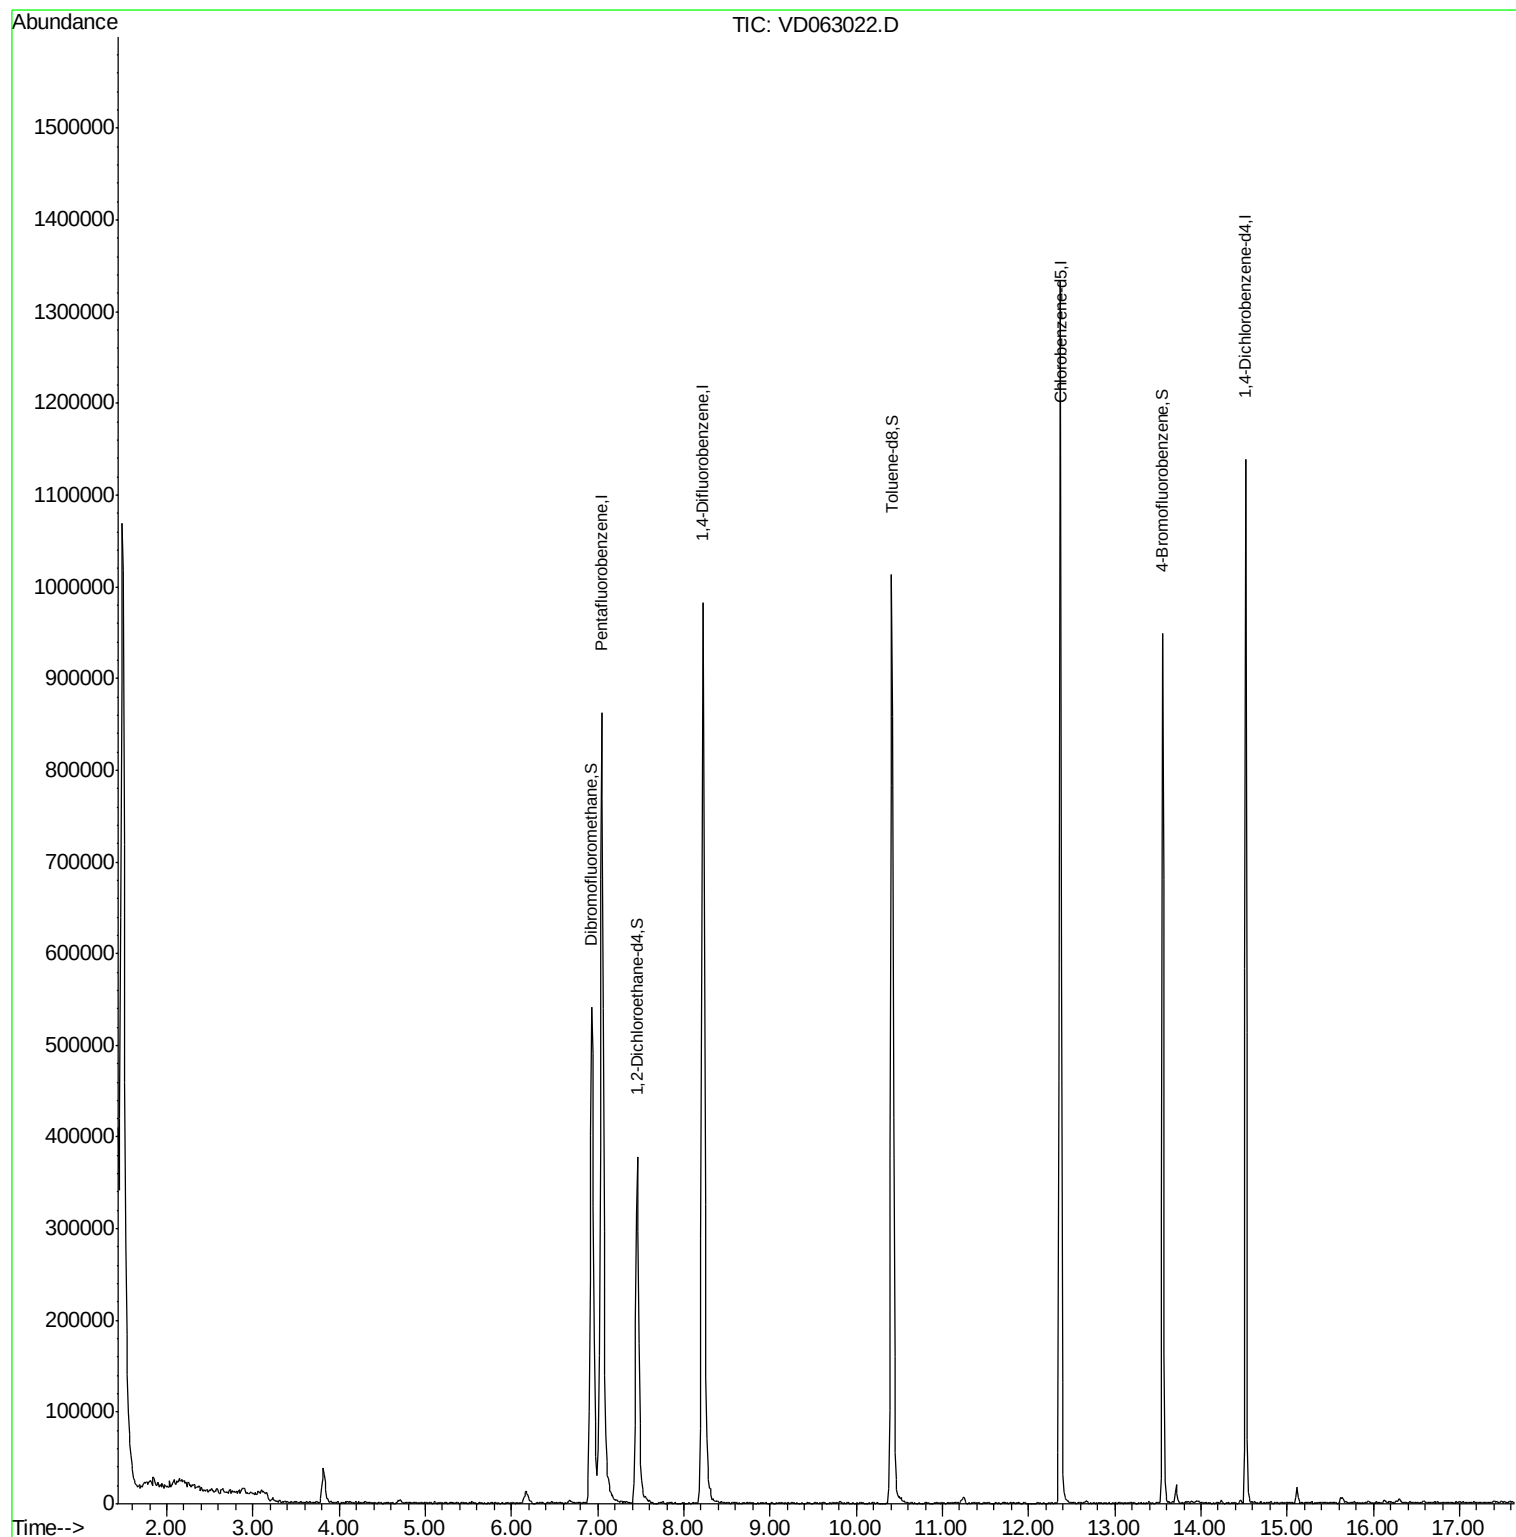

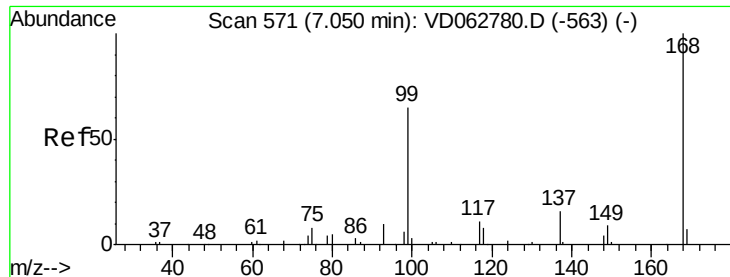

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.05 min Scan# 571

Delta R.T. -0.00 min

Lab File: VD063022.D

Acq: 3 Jul 2019 13:46

Instrument :

MSVOA_D

ClientSampleId :


FK-PS-01-051

Tot Ion:168 Resp: 824955

Ion Ratio Lower Upper




168 100

99 62.8 53.0 79.6

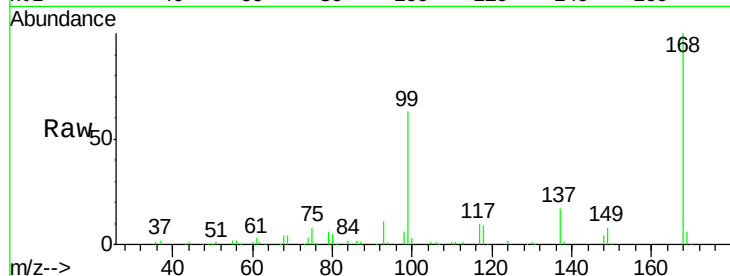

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.95 (98.65 to 99.65): VDC

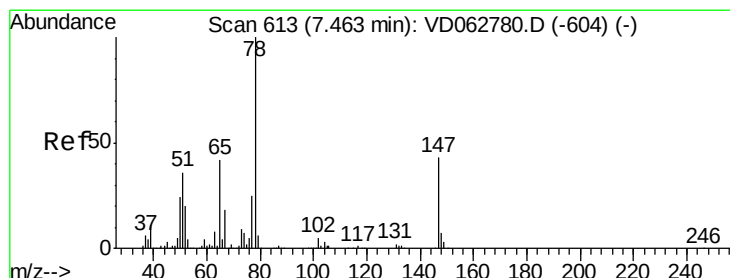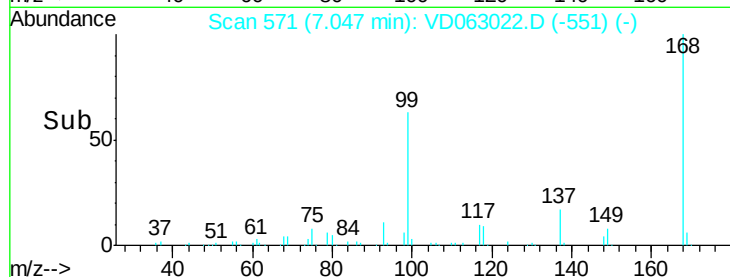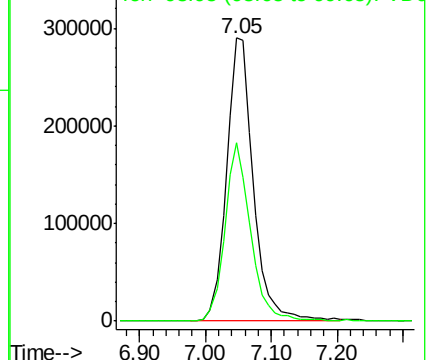

#33

1,2-Dichloroethane-d4

Concen: 48.164 ug/l

RT: 7.46 min Scan# 613

Delta R.T. -0.00 min

Lab File: VD063022.D


Acq: 3 Jul 2019 13:46

Tgt Ion: 65 Resp: 431893

Ion Ratio Lower Upper



65 100


67 43.1 0.0 87.4

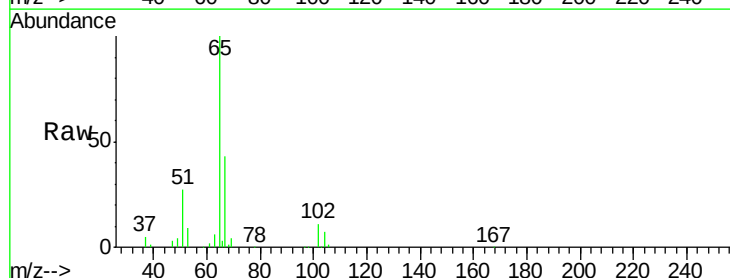

Abundance Ion 64.95 (64.65 to 65.65): VDC

Ion 66.90 (66.60 to 67.60): VDC

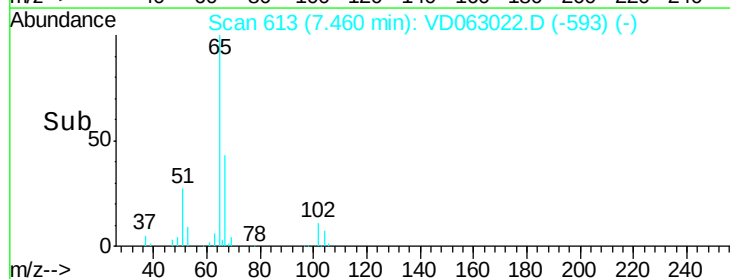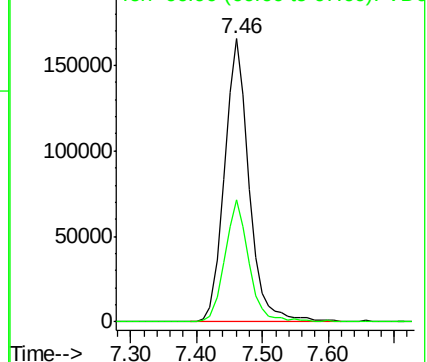


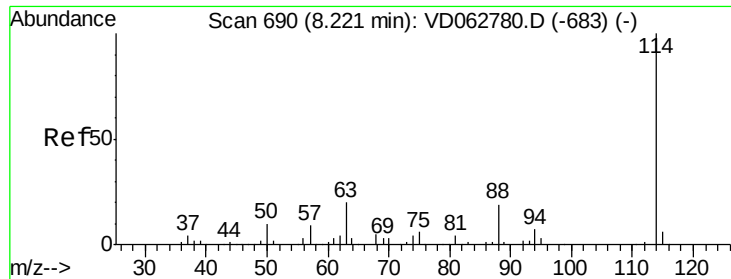




#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.23 min Scan# 691
 Delta R.T. 0.01 min
 Lab File: VD063022.D
 Acq: 3 Jul 2019 13:46

Instrument :
 MSVOA_D
 ClientSampleId :
 FK-PS-01-051

Tot Ion:114 Resp: 1099193
 Ion Ratio Lower Upper
 114 100
 63 17.7 0.0 40.0
 88 16.6 0.0 38.8

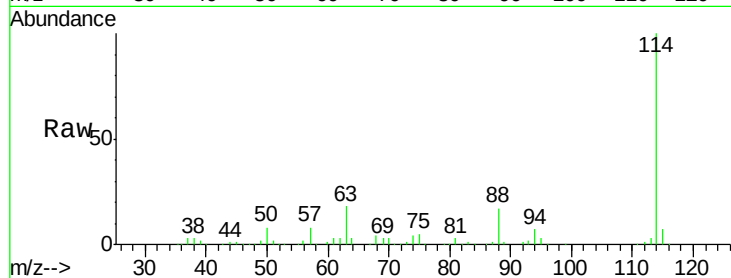


Abundance Ion 114.00 (113.70 to 114.70): V
 Ion 62.95 (62.65 to 63.65): VDC
 Ion 87.90 (87.60 to 88.60): VDC

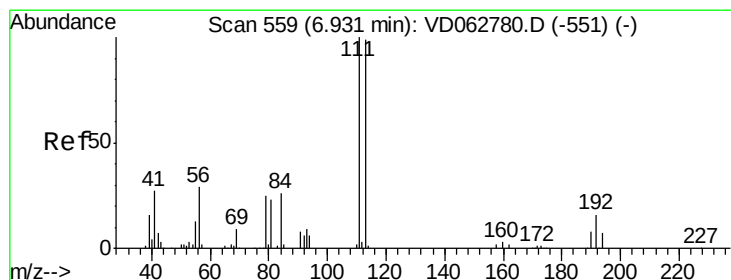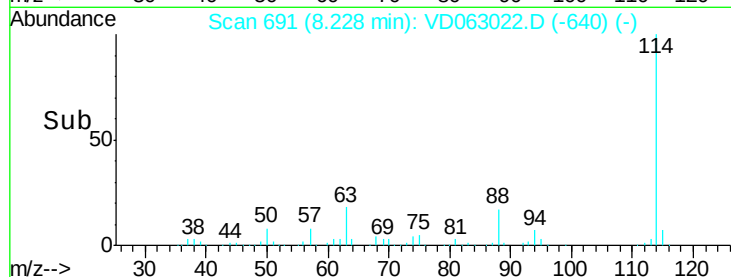
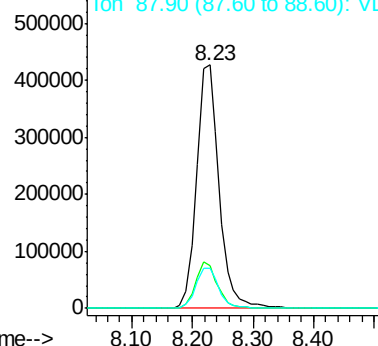



#35
 Dibromofluoromethane
 Concen: 49.584 ug/l
 RT: 6.93 min Scan# 559
 Delta R.T. -0.00 min
 Lab File: VD063022.D
 Acq: 3 Jul 2019 13:46

Tgt Ion:113 Resp: 459560
 Ion Ratio Lower Upper
 113 100
 111 96.5 81.2 121.8
 192 14.3 12.9 19.3

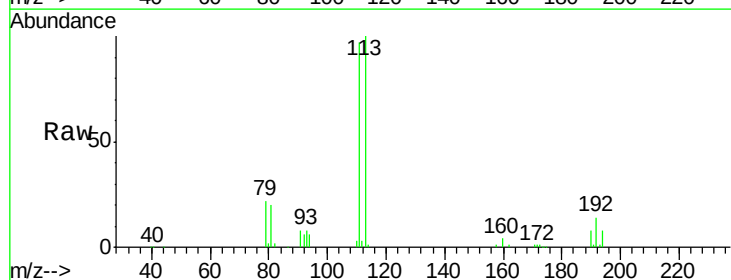

Abundance Ion 112.90 (112.60 to 113.60): V
 Ion 110.90 (110.60 to 111.60): V
 Ion 191.80 (191.50 to 192.50): V



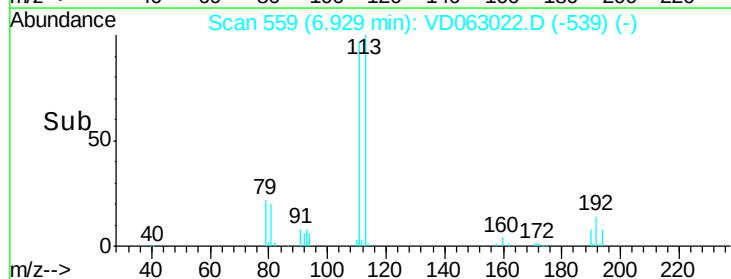
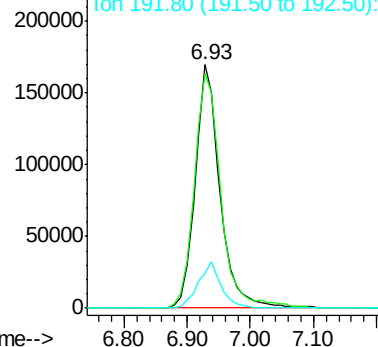


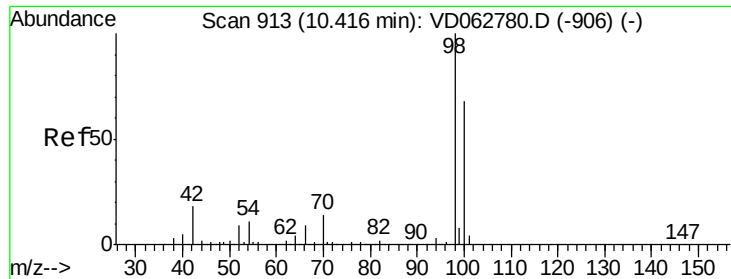

#50
Toluene-d8
Concen: 41.403 ug/l
RT: 10.41 min Scan# 913
Delta R.T. -0.00 min
Lab File: VD063022.D
Acq: 3 Jul 2019 13:46




Instrument :
MSVOA_D
ClientSampleId :
FK-PS-01-051


Tot Ion: 98 Resp: 835187
Ion Ratio Lower Upper
98 100
100 65.0 54.7 82.1

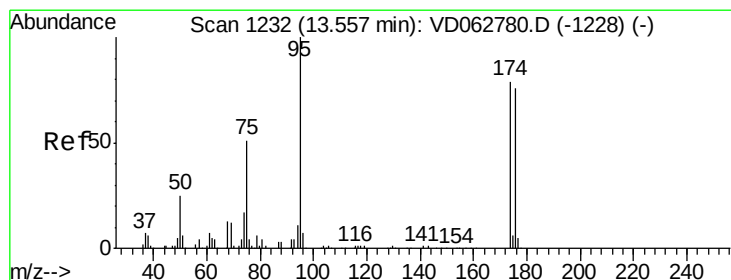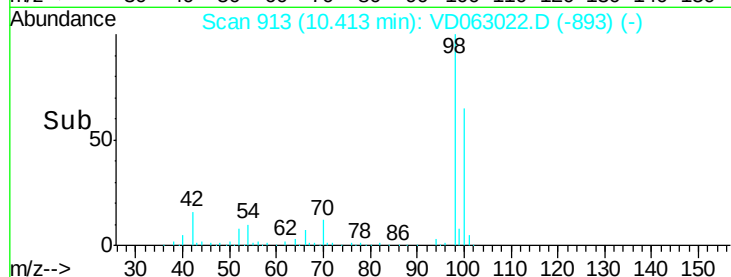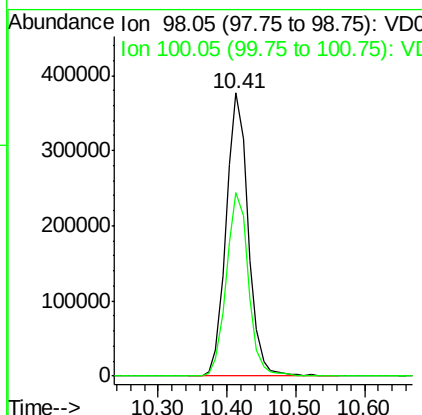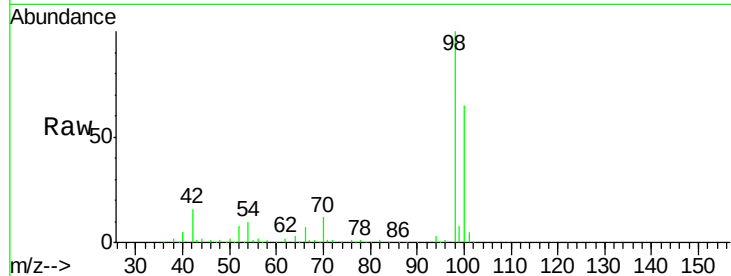

#62
4-Bromofluorobenzene
Concen: 27.508 ug/l
RT: 13.55 min Scan# 1232
Delta R.T. -0.00 min
Lab File: VD063022.D
Acq: 3 Jul 2019 13:46

Tgt Ion: 95 Resp: 252318
Ion Ratio Lower Upper
95 100
174 78.1 0.0 158.0
176 75.6 0.0 151.6


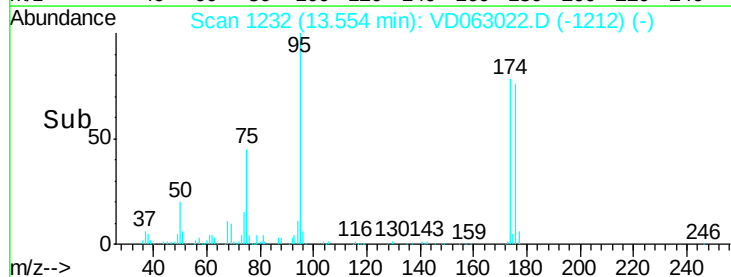
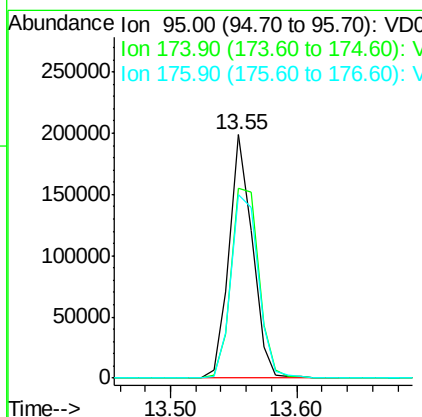
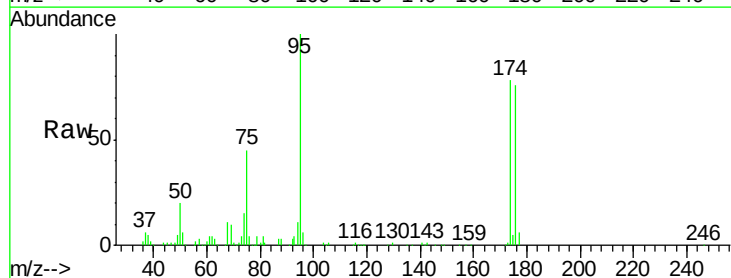


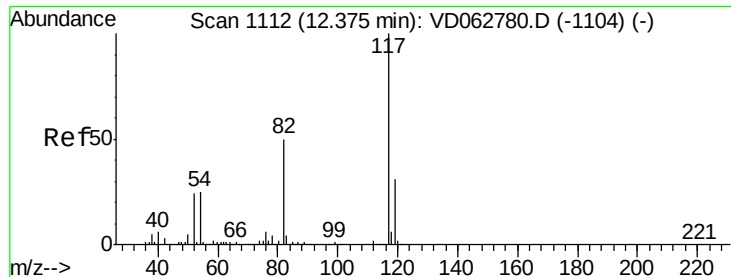

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 12.37 min Scan# 1112
Delta R.T. -0.00 min
Lab File: VD063022.D
Acq: 3 Jul 2019 13:46

Instrument :
MSVOA_D
ClientSampleId :
FK-PS-01-051

Tot Ion:117 Resp: 744946
Ion Ratio Lower Upper
117 100
82 48.9 40.4 60.6
119 31.6 25.2 37.8

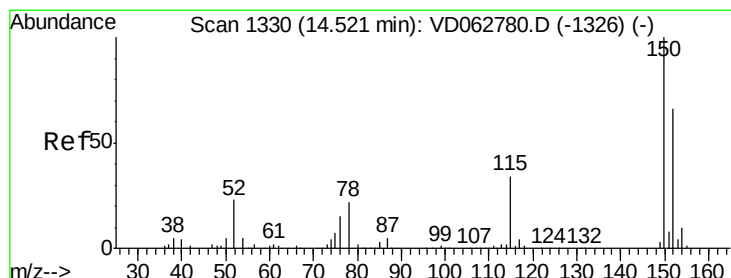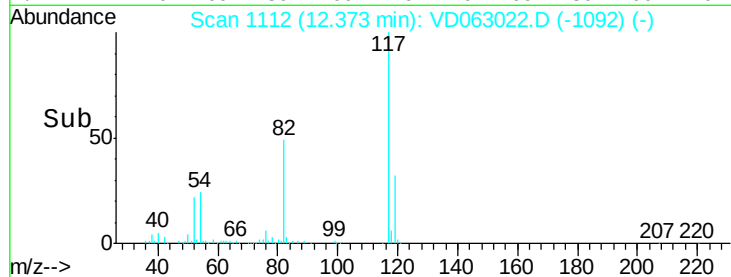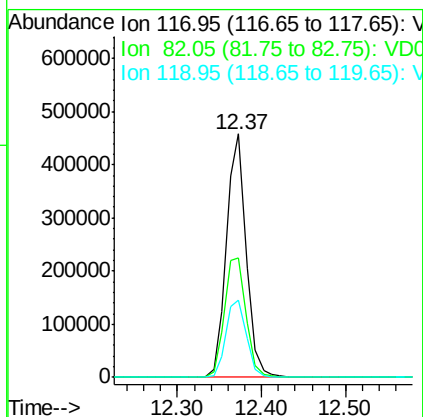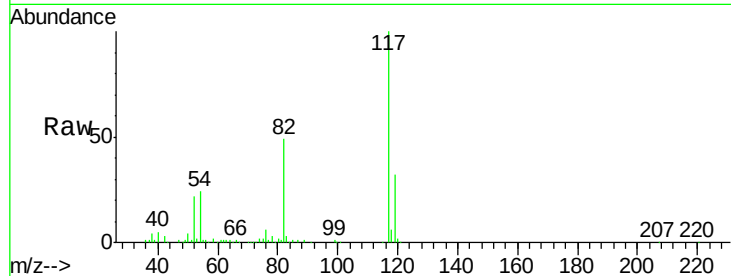

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 14.52 min Scan# 1330
Delta R.T. -0.00 min
Lab File: VD063022.D
Acq: 3 Jul 2019 13:46

Tgt Ion:152 Resp: 241991
Ion Ratio Lower Upper
152 100
115 60.0 29.2 87.6
150 153.8 0.0 305.8

