

Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD070319\
Data File : VD063030.D
Acq On : 3 Jul 2019 17:52
Operator : VA/AP
Sample : VSTDCCC050
Misc : 5.00µl/5ml/MSVOA D/SOIL
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
VSTDCCC050EC


Manual Integrations
APPROVED

MMDadoda
7/9/2019 8:54:07 AM

Quant Time: Jul 04 02:12:19 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D061919S.M
Quant Title : SW846 8260
QLast Update : Thu Jun 20 01:50:56 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
93) 1,2,4-Trichlorobenzene	15.95	180	655055	54.814	ug/l	97
94) Hexachlorobutadiene	16.04	225	462918	50.704	ug/l	97
95) Naphthalene	16.13	128	1014081	60.542	ug/l	99
96) 1,2,3-Trichlorobenzene	16.27	180	521822	56.830	ug/l	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

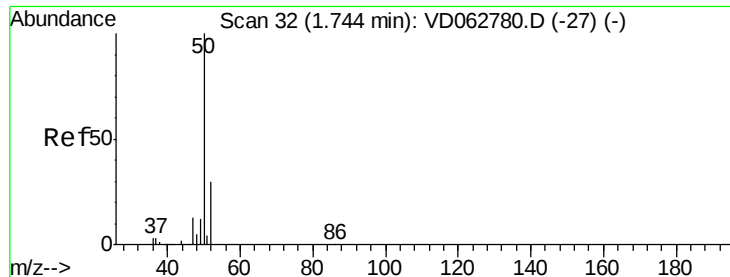

#3

Chloromethane

Concen: 43.904 ug/l

RT: 1.75 min Scan# 33

Delta R.T. 0.01 min

Lab File: VD063030.D

Acq: 3 Jul 2019 17:52

Instrument :

MSVOA_D

ClientSampleId :

VSTDCCC050EC

Tot Ion: 50 Resp: 395160

Ion Ratio Lower Upper

50 100


52 31.8 23.6 35.4

Manual Integrations

APPROVED




MMDadoda

7/9/2019 8:54:07 AM

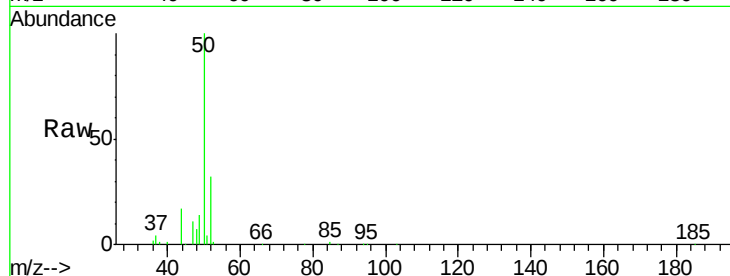

Abundance Ion 49.90 (49.60 to 50.60): VDC

Ion 51.90 (51.60 to 52.60): VDC

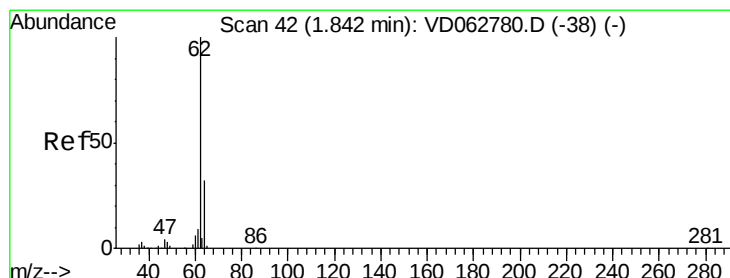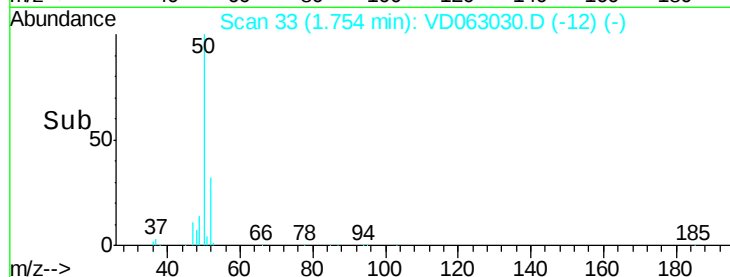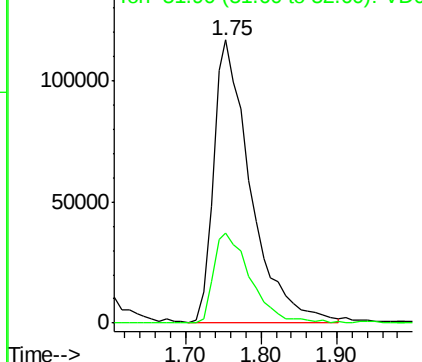

#4

Vinyl Chloride

Concen: 46.489 ug/l

RT: 1.85 min Scan# 43

Delta R.T. 0.01 min

Lab File: VD063030.D


Acq: 3 Jul 2019 17:52

Tgt Ion: 62 Resp: 414872

Ion Ratio Lower Upper



62 100


64 32.0 25.6 38.4

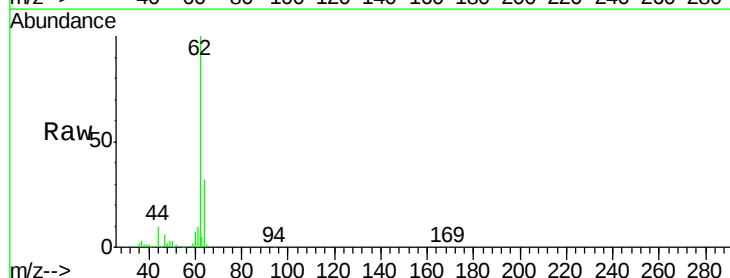

Abundance Ion 61.95 (61.65 to 62.65): VDC

Ion 63.95 (63.65 to 64.65): VDC

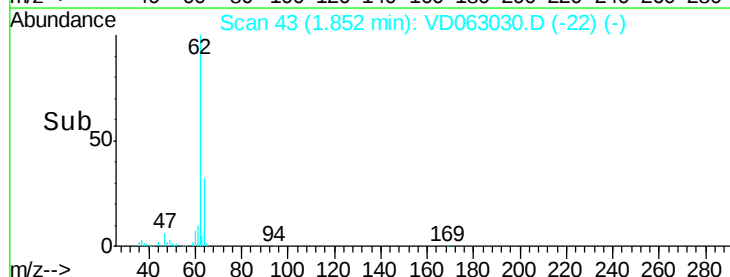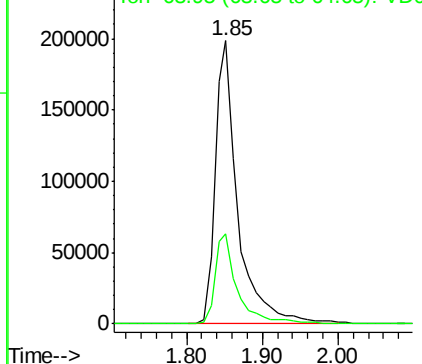

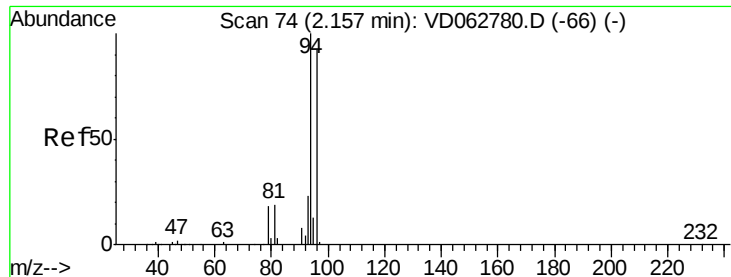

#5

Bromomethane

Concen: 46.586 ug/l

RT: 2.16 min Scan# 74

Delta R.T. 0.00 min

Lab File: VD063030.D

Acq: 3 Jul 2019 17:52

Instrument :

MSVOA_D





ClientSampleId :

VSTDCCC050EC

Tot Ion:	94	Resp:	194694
Ion	Ratio	Lower	Upper
94	100		
96	97.9	73.4	110.2
93	20.4	18.2	27.4

Manual Integrations
APPROVED

MMDadoda
7/9/2019 8:54:07 AM

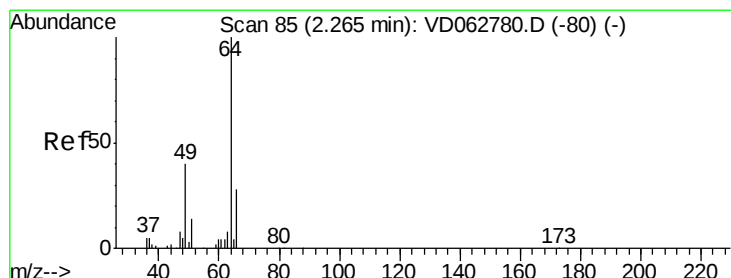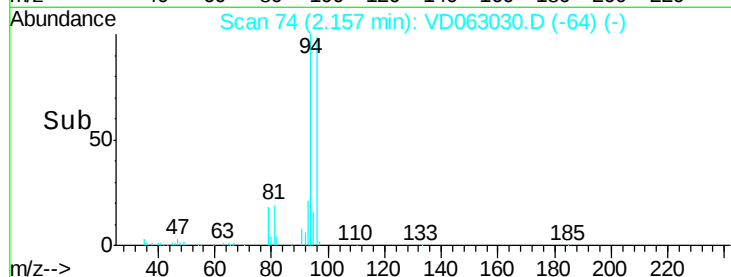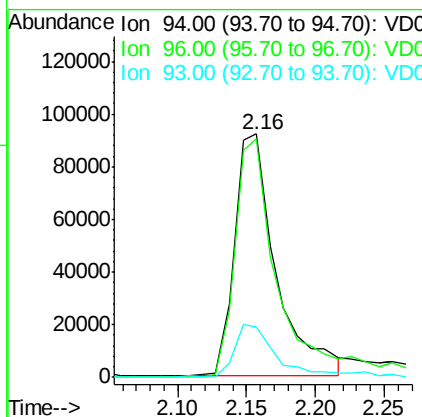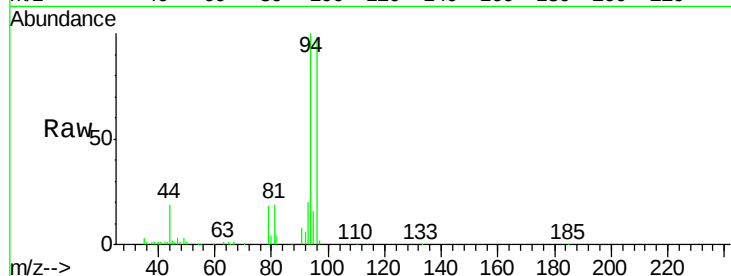

#6

Chloroethane

Concen: 49.452 ug/l

RT: 2.27 min Scan# 85

Delta R.T. 0.00 min

Lab File: VD063030.D

Acq: 3 Jul 2019 17:52

Tgt Ion:	64	Resp:	199797
Ion	Ratio	Lower	Upper
64	100		
66	33.2	23.0	34.4

