


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD070323\
Data File : VD076695.D
Acq On : 03 Jul 2023 16:28
Operator : KP/SY
Sample : 03444-12RE
Misc : 5.03G/10.0ml/MSVOA_D/SOIL
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
A46T6RE

Manual IntegrationsAPPROVED

Quant Time: Jul 04 01:11:17 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM061523SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jun 16 01:50:34 2023
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 07/05/2023
Supervised By :Mahesh Dadoda 07/07/2023

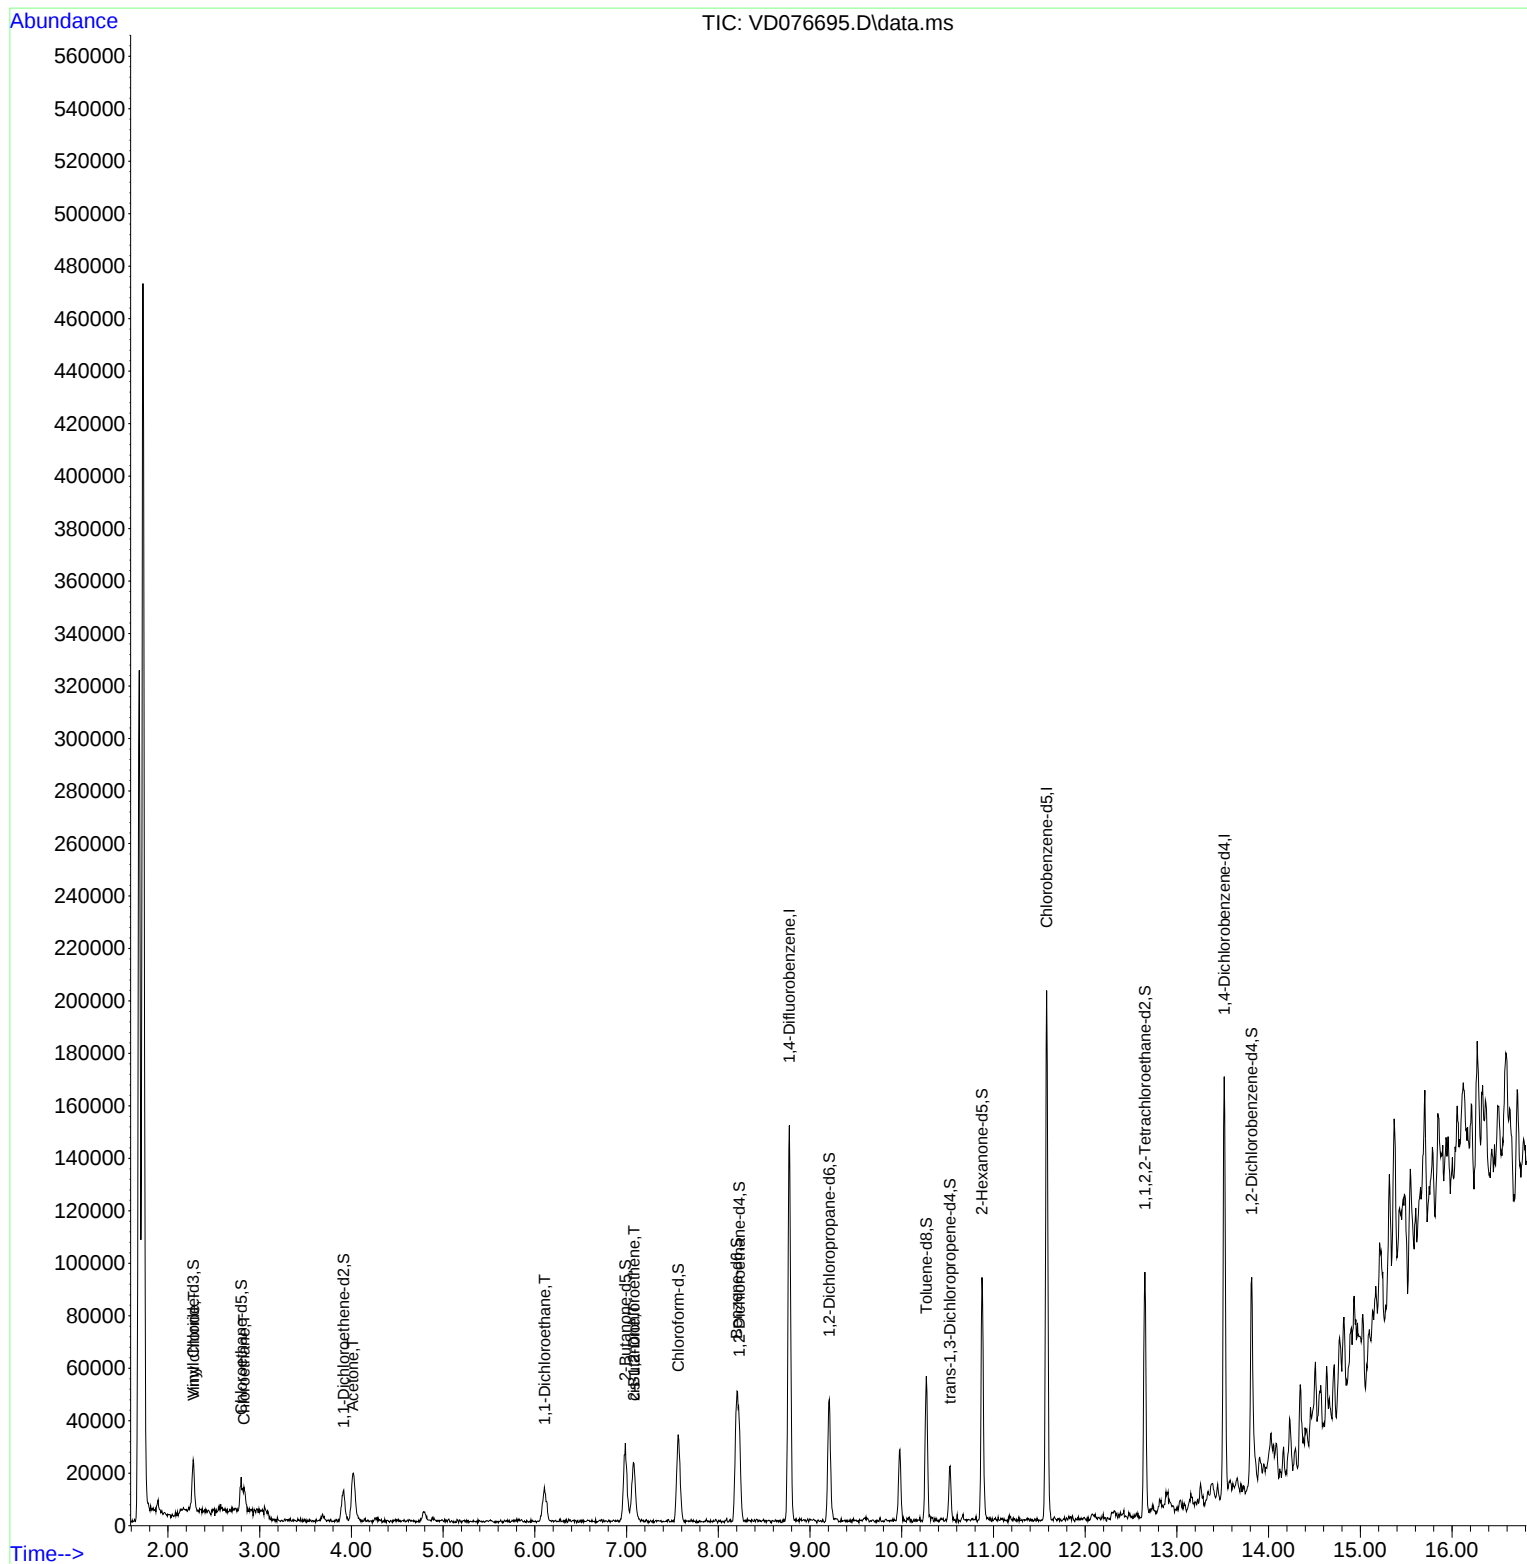




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD070323\
 Data File : VD076695.D
 Acq On : 03 Jul 2023 16:28
 Operator : KP/SY
 Sample : 03444-12RE
 Misc : 5.03G/10.0ml/MSVOA_D/SOIL
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 A46T6RE

Manual IntegrationsAPPROVED

Quant Time: Jul 04 01:11:17 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM061523SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 16 01:50:34 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 07/05/2023
 Supervised By :Mahesh Dadoda 07/07/2023

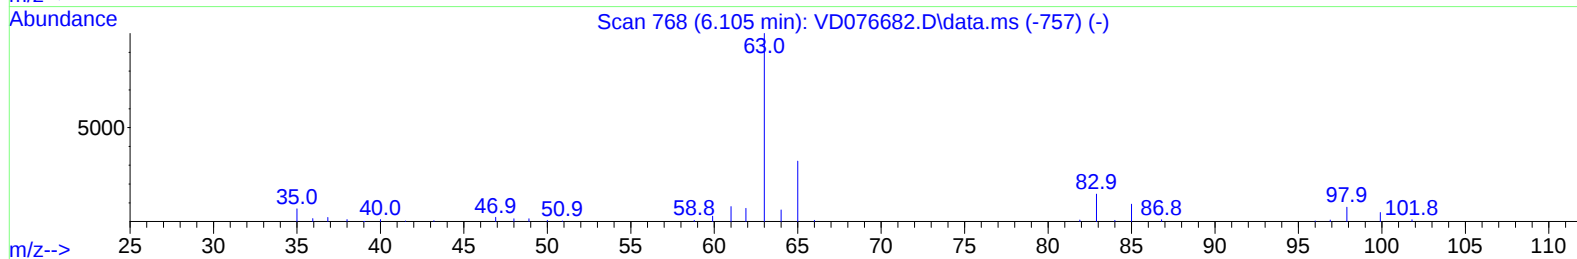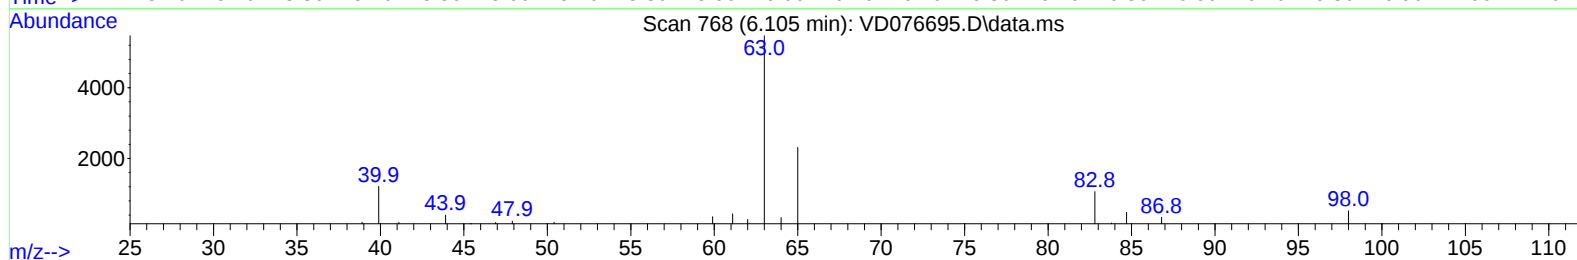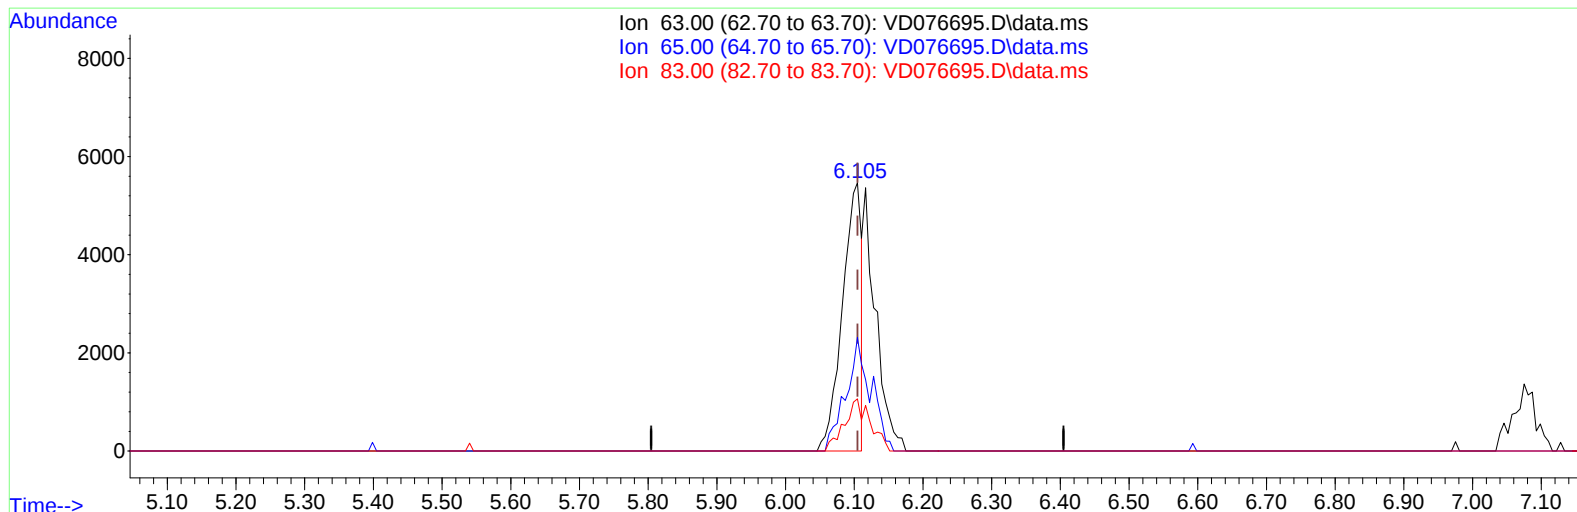

TIC: VD076695.D\data.ms

(19) 1,1-Dichloroethane (T)

6.105min (-0.000) 3.05 ug/L

response 10553

Ion	Exp%	Act%
63.00	100.00	100.00
65.00	29.70	42.26#
83.00	12.70	19.47#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD070323\
 Data File : VD076695.D
 Acq On : 03 Jul 2023 16:28
 Operator : KP/SY
 Sample : 03444-12RE
 Misc : 5.03G/10.0ml/MSVOA_D/SOIL
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 A46T6RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 07/05/2023
 Supervised By :Mahesh Dadoda 07/07/2023

Quant Time: Jul 04 01:11:17 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM061523SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 16 01:50:34 2023
 Response via : Initial Calibration

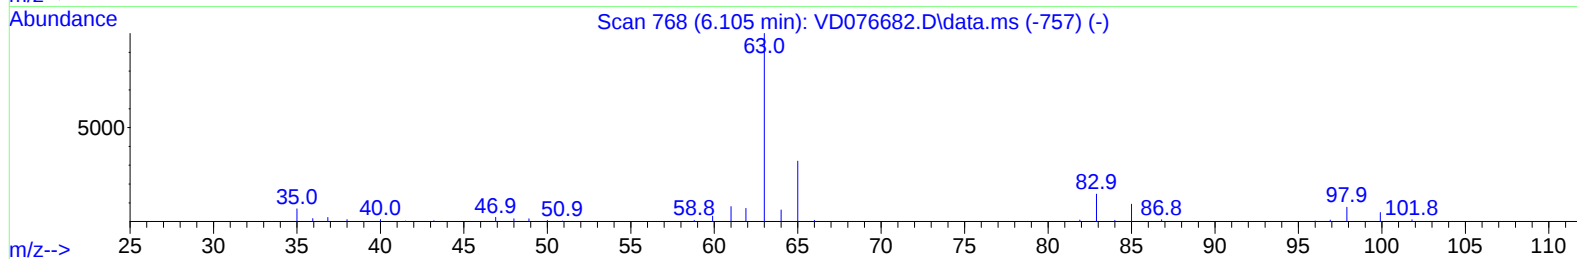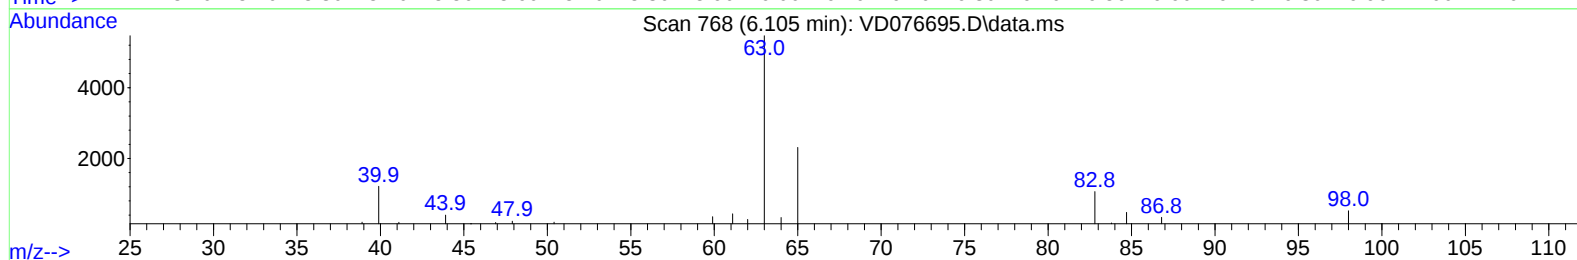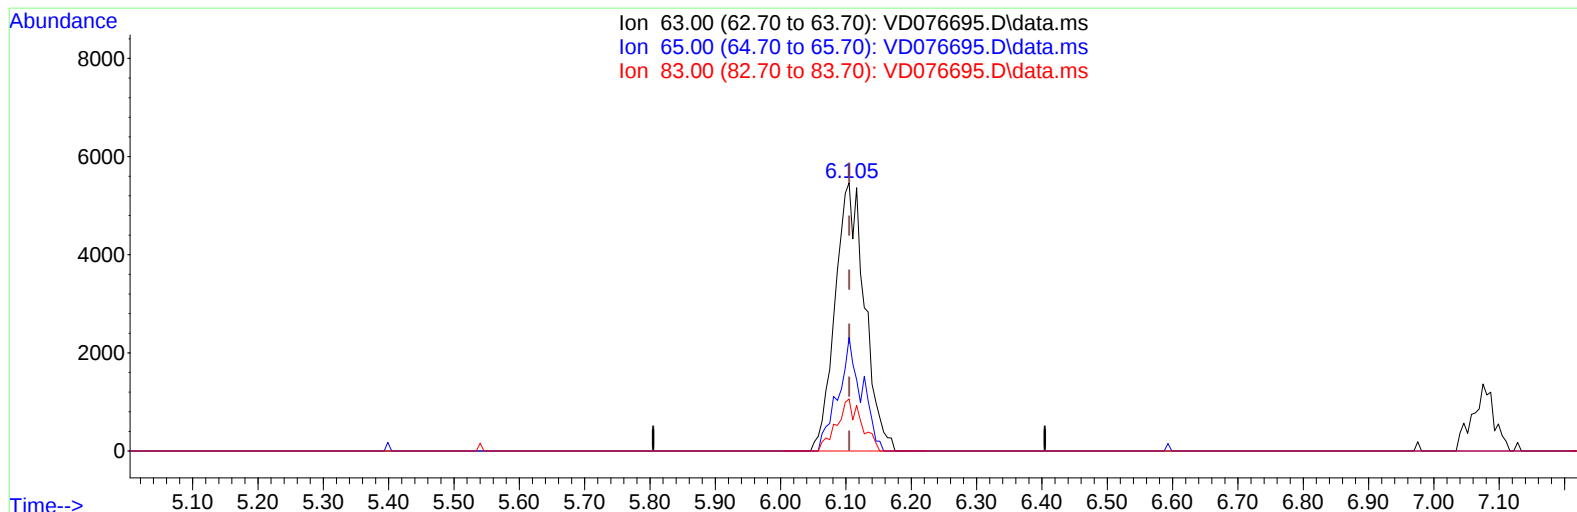

TIC: VD076695.D\data.ms

(19) 1,1-Dichloroethane (T)

6.105min (-0.000) 4.95 ug/L m

response 17154

Ion	Exp%	Act%
63.00	100.00	100.00
65.00	29.70	42.26#
83.00	12.70	19.47#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD070323\
 Data File : VD076695.D
 Acq On : 03 Jul 2023 16:28
 Operator : KP/SY
 Sample : 03444-12RE
 Misc : 5.03G/10.0ml/MSVOA_D/SOIL
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 A46T6RE

Manual IntegrationsAPPROVED

Quant Time: Jul 04 01:11:17 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM061523SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 16 01:50:34 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 07/05/2023
 Supervised By :Mahesh Dadoda 07/07/2023

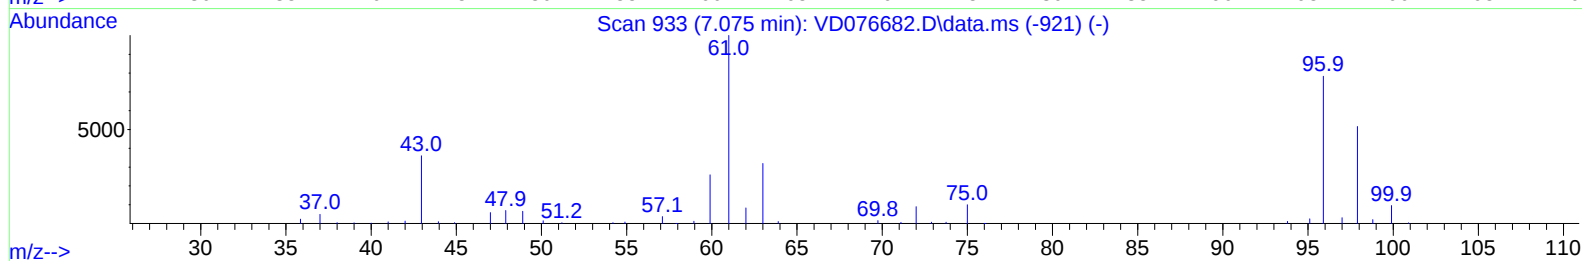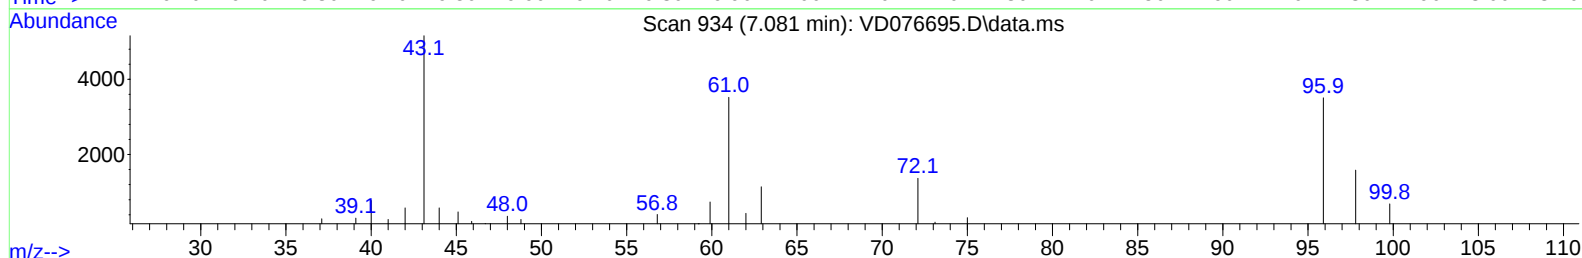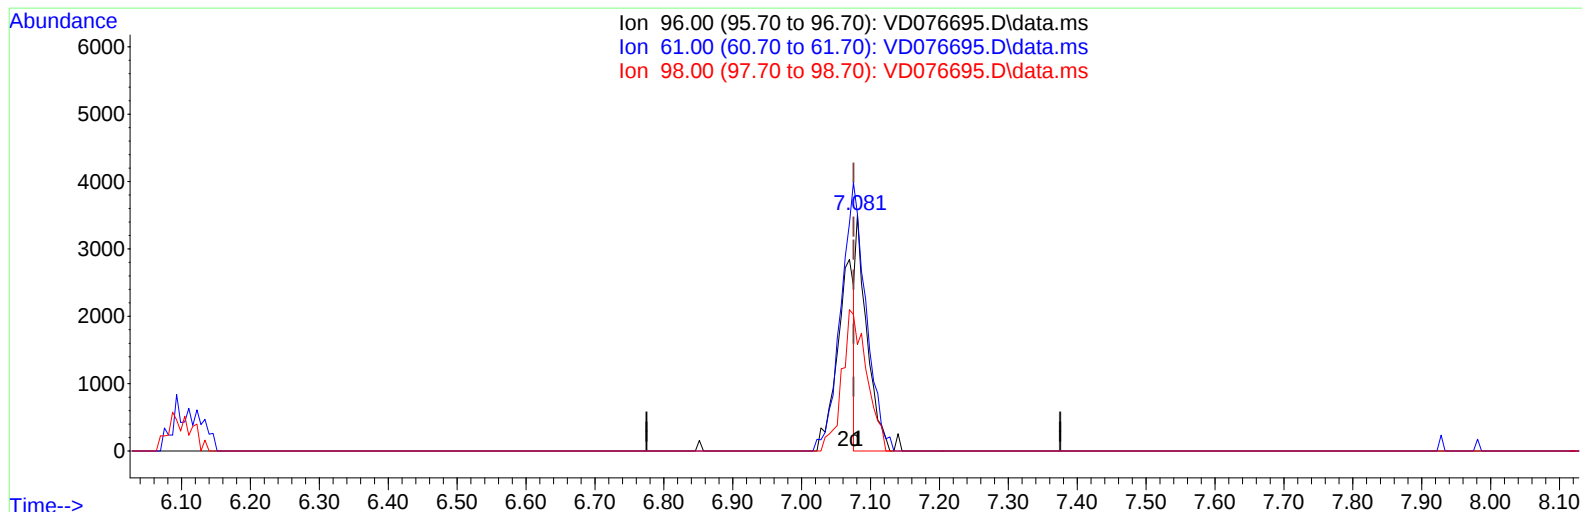

TIC: VD076695.D\data.ms

(20) cis-1,2-Dichloroethene (T)

7.081min (+ 0.006) 1.87 ug/L

response 3966

Ion	Exp%	Act%
96.00	100.00	100.00
61.00	122.80	100.34
98.00	60.30	45.11
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD070323\
 Data File : VD076695.D
 Acq On : 03 Jul 2023 16:28
 Operator : KP/SY
 Sample : 03444-12RE
 Misc : 5.03G/10.0ml/MSVOA_D/SOIL
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 A46T6RE

Manual IntegrationsAPPROVED

Quant Time: Jul 04 01:11:17 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM061523SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 16 01:50:34 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 07/05/2023
 Supervised By :Mahesh Dadoda 07/07/2023

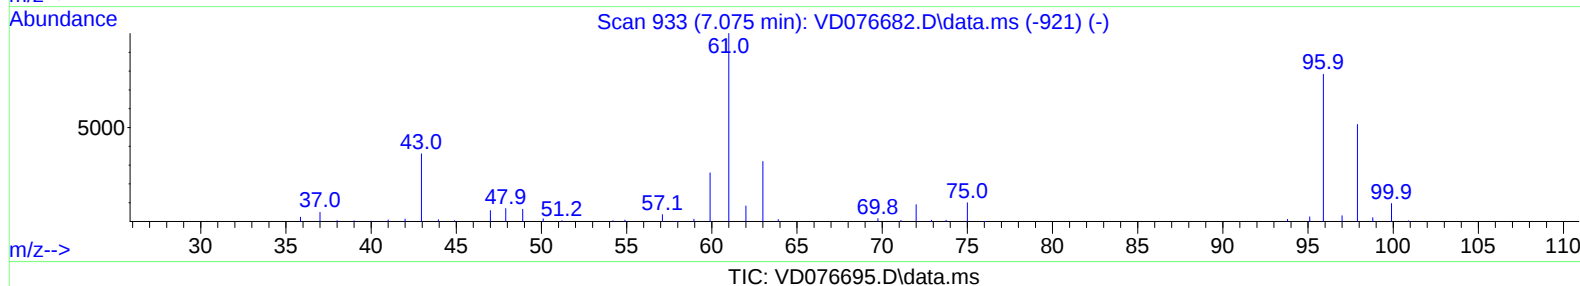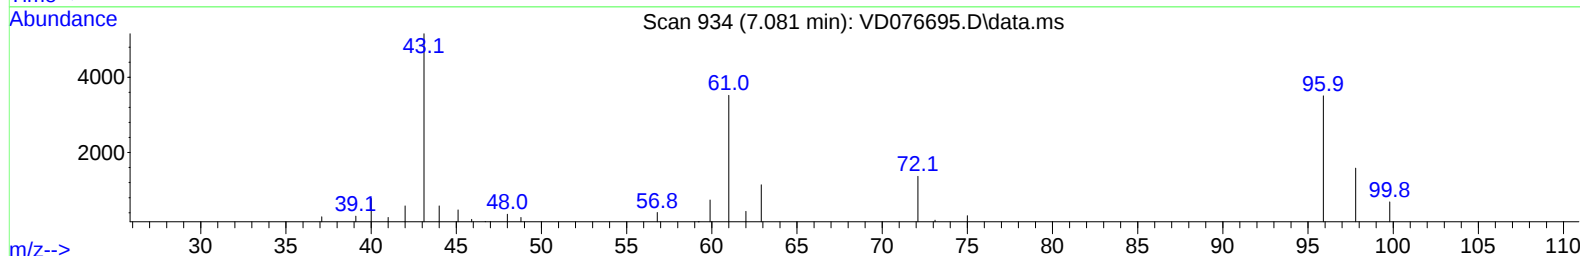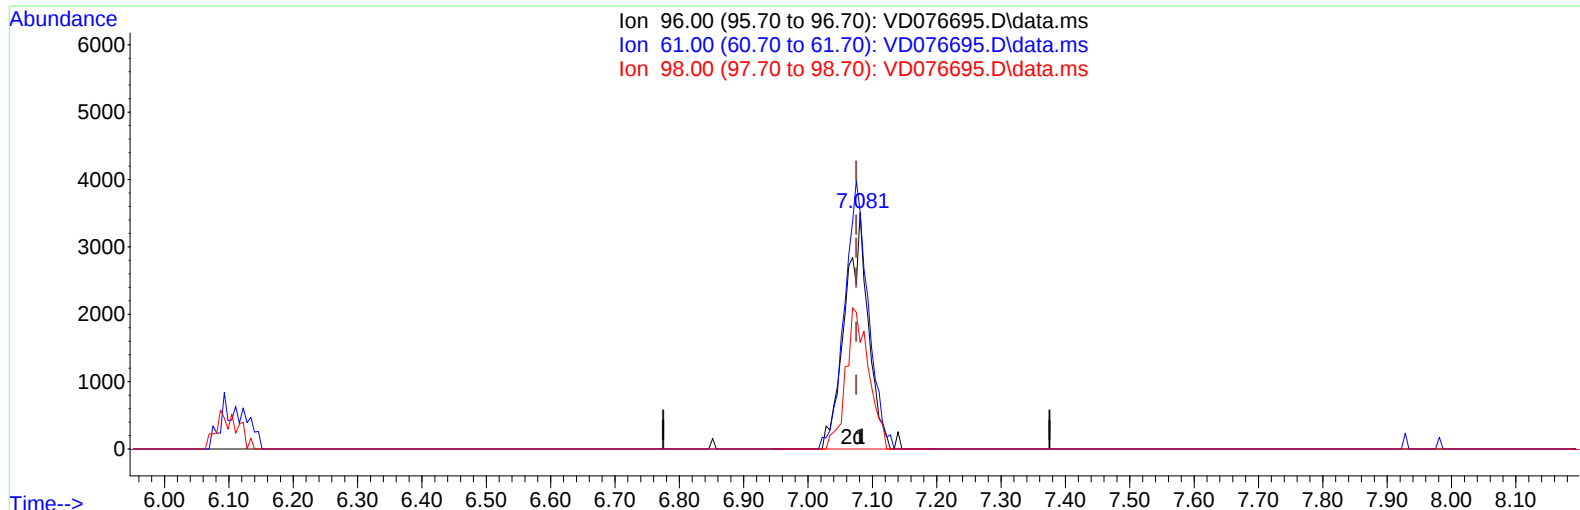

TIC: VD076695.D\data.ms

(20) cis-1,2-Dichloroethene (T)

7.081min (+ 0.006) 4.20 ug/L m

response 8885

Ion	Exp%	Act%
96.00	100.00	100.00
61.00	122.80	100.34
98.00	60.30	45.11
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD070323\
 Data File : VD076695.D
 Acq On : 03 Jul 2023 16:28
 Operator : KP/SY
 Sample : 03444-12RE
 Misc : 5.03G/10.0ml/MSVOA_D/SOIL
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 A46T6RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 07/05/2023
 Supervised By :Mahesh Dadoda 07/07/2023

Quant Time: Jul 04 01:11:17 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM061523SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 16 01:50:34 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.775	114	130937	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.581	117	110948	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.516	152	43876	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.275	65	8699	2.728	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	10.920%#
7) Chloroethane-d5	2.799	69	12039	4.669	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	18.680%#
11) 1,1-Dichloroethene-d2	3.916	65	3348	4.022	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	16.080%#
21) 2-Butanone-d5	6.987	46	49951	103.435	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	206.880%#
24) Chloroform-d	7.563	84	34086	9.881	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	39.520%#
26) 1,2-Dichloroethane-d4	8.228	65	23636	13.889	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	55.560%#
32) Benzene-d6	8.199	84	47108	6.941	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	27.760%
36) 1,2-Dichloropropane-d6	9.210	67	21626	9.983	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	39.920%#
41) Toluene-d8	10.269	98	36344	5.783	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	23.120%#
43) trans-1,3-Dichloroprop...	10.528	79	11510	12.774	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	51.080%
47) 2-Hexanone-d5	10.875	63	32633	97.041	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	194.080%#
56) 1,1,2,2-Tetrachloroeth...	12.651	84	46310	30.047	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	120.200%#
66) 1,2-Dichlorobenzene-d4	13.816	152	19347	12.030	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	48.120%#
Target Compounds						Qvalue
5) Vinyl chloride	2.281	62	10463	2.860	ug/L	96
8) Chloroethane	2.828	64	7065	3.152	ug/L	97
13) Acetone	4.016	43	33457	85.776	ug/L	92
19) 1,1-Dichloroethane	6.105	63	17154m	4.952	ug/L	
20) cis-1,2-Dichloroethene	7.081	96	8885m	4.199	ug/L	
22) 2-Butanone	7.081	43	14276	22.680	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed