
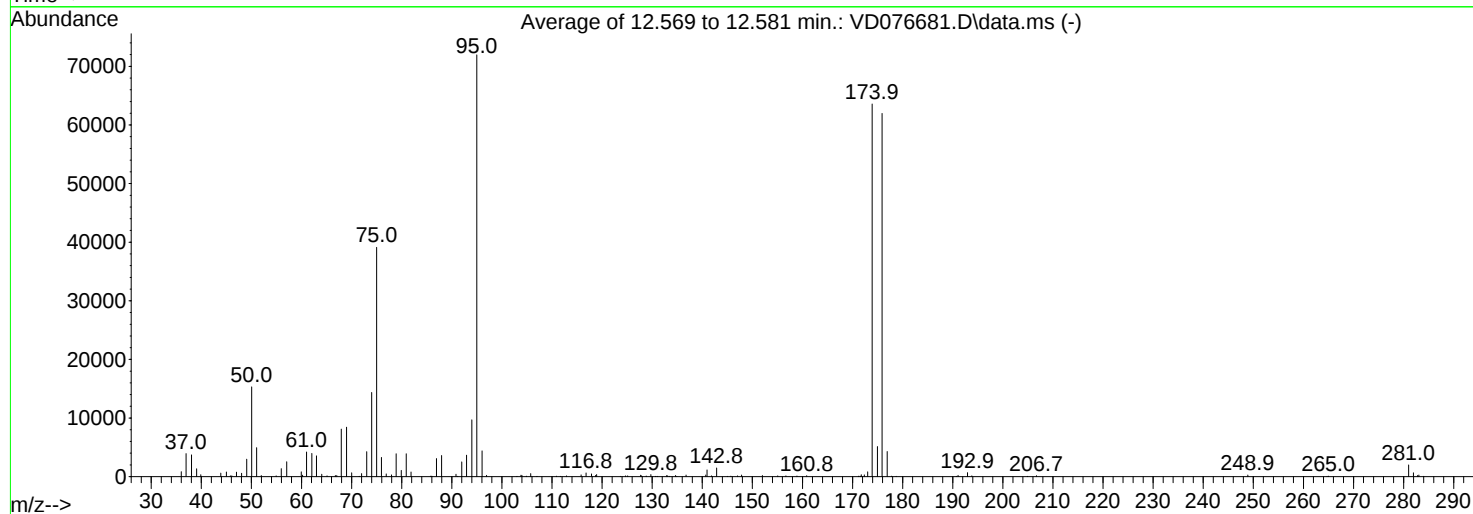


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD070323\
Data File : VD076681.D
Acq On : 03 Jul 2023 09:31
Operator : KP/SY
Sample : BFB150
Misc : 5.00G/10.0ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB150

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM061523SMA.M
Title : SFAM01.0
Last Update : Fri Jun 16 01:50:34 2023

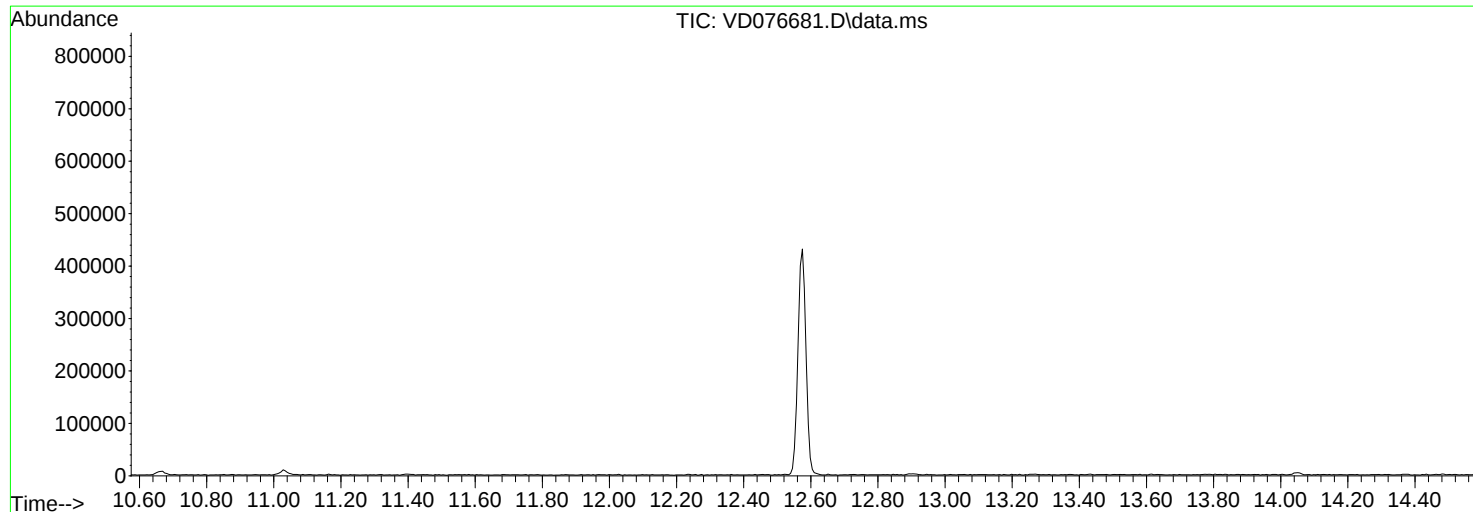

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1859

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.3	15306	PASS
75	95	30	80	54.4	39131	PASS
95	95	100	100	100.0	71965	PASS
96	95	5	9	6.1	4407	PASS
173	174	0.00	2	1.3	815	PASS
174	95	50	120	88.3	63568	PASS
175	174	5	9	8.1	5139	PASS
176	174	95	105	97.5	61979	PASS
177	176	5	10	6.9	4299	PASS

m/z	Abundance
36.80	181.0
39.90	886.0
41.10	189.0
42.10	305.0
43.90	593.0
55.00	161.0
153.00	169.0
187.90	220.0
207.20	213.0

Instrument :
MSVOA_D
ClientSampleId :
BFB150

m/z	Abundance
36.10	882.0
37.00	4397.0
38.00	3934.0
39.10	1629.0
39.90	1078.0
43.90	1300.0
45.00	950.0
45.80	191.0
46.90	804.0
48.10	622.0
49.00	3097.0
50.00	16263.0
51.00	5039.0
52.00	207.0
55.10	214.0
55.90	1626.0
57.10	2312.0
59.90	889.0
61.00	4673.0
62.00	4389.0
63.00	3663.0
64.00	343.0
65.10	191.0
66.80	242.0
67.90	8246.0
69.00	10095.0
70.10	786.0
72.00	812.0
73.00	4322.0
74.00	15301.0
75.00	38696.0
76.00	3079.0
76.90	308.0
78.00	257.0
78.90	3885.0
79.90	1161.0
80.90	4068.0
81.80	801.0
85.80	266.0
87.10	3151.0
87.90	3394.0
90.90	319.0
92.10	2061.0
92.90	4116.0
94.00	10397.0
95.00	70720.0
96.10	5148.0
96.90	250.0
103.00	160.0
103.80	377.0
104.90	222.0
105.80	643.0
107.00	186.0
111.70	164.0
112.90	257.0
115.80	304.0
116.80	608.0
117.90	319.0
118.70	554.0
123.70	168.0
124.70	371.0
127.70	465.0
128.80	180.0
129.70	340.0
131.00	170.0
132.90	356.0
134.60	296.0
136.80	494.0
140.70	800.0
141.00	824.0
142.90	1249.0
147.80	213.0
152.00	184.0
155.10	165.0
156.80	253.0
159.00	195.0
160.90	345.0
171.20	251.0
171.90	355.0
172.40	333.0
173.10	1257.0
173.90	64760.0
174.90	4844.0
175.90	59656.0
176.90	3885.0
177.80	261.0
191.10	213.0
193.00	339.0
206.70	169.0
249.00	218.0
264.70	201.0
281.00	1573.0

Instrument :
MSVOA_D
ClientSampleId :
BFB150

282.00	374.0
282.80	392.0
284.00	198.0

Instrument :
MSVOA_D
ClientSampleId :
BFB150

m/z	Abundance
35.90	920.0
37.00	4765.0
38.00	3884.0
39.00	1490.0
40.00	1359.0
44.00	1025.0
45.00	985.0
46.10	194.0
47.00	824.0
48.10	653.0
49.00	3223.0
50.00	16440.0
51.10	4852.0
52.00	163.0
54.90	377.0
56.00	1387.0
57.00	2601.0
59.90	772.0
60.20	714.0
61.00	4317.0
62.10	4577.0
63.00	3851.0
64.00	532.0
65.10	193.0
66.70	373.0
67.10	244.0
68.00	8726.0
69.00	8632.0
69.90	766.0
71.50	159.0
72.00	393.0
73.00	5041.0
74.00	15933.0
75.00	43728.0
76.00	3510.0
77.00	536.0
77.80	294.0
78.90	3997.0
79.90	946.0
80.90	4268.0
81.90	781.0
86.00	288.0
86.90	3174.0
88.00	4449.0
90.80	692.0
91.90	2846.0
92.90	3558.0
94.00	10958.0
95.00	78928.0
96.00	4507.0
96.90	229.0
104.00	662.0
105.70	620.0
110.90	272.0
115.70	378.0
116.90	741.0
118.00	581.0
118.90	674.0
125.20	162.0
127.90	433.0
129.80	421.0
130.70	181.0
132.90	206.0
133.50	189.0
134.90	165.0
136.60	160.0
140.90	1260.0
141.80	191.0
142.80	1704.0
145.00	163.0
145.70	216.0
147.20	151.0
147.90	247.0
152.00	171.0
152.80	171.0
156.60	155.0
158.80	160.0
160.70	188.0
171.70	604.0
172.90	1189.0
173.90	66576.0
175.00	5983.0
175.90	69064.0
176.90	5135.0
190.70	180.0
191.10	202.0
192.80	500.0
193.10	512.0
193.80	196.0
206.70	182.0
249.00	268.0
281.00	2243.0

Instrument :
MSVOA_D
ClientSampleId :
BFB150

282.00	752.0
282.80	186.0
283.20	236.0

Instrument :
MSVOA_D
ClientSampleId :
BFB150

m/z	Abundance
36.00	754.0
37.00	3212.0
38.10	3358.0
39.00	930.0
39.90	1216.0
44.00	1285.0
45.00	438.0
45.80	212.0
46.10	244.0
47.10	683.0
48.00	452.0
49.10	2620.0
50.10	13214.0
51.00	4907.0
51.90	187.0
55.00	289.0
55.90	1110.0
57.00	2719.0
60.00	836.0
61.00	3666.0
62.00	2882.0
63.00	3109.0
64.10	360.0
67.00	369.0
68.00	7360.0
69.00	6595.0
70.00	449.0
72.00	360.0
73.00	3436.0
74.00	11849.0
75.00	34968.0
75.90	3253.0
76.80	543.0
78.00	341.0
78.90	3795.0
79.90	1051.0
80.90	3368.0
81.90	777.0
86.90	2943.0
87.90	2940.0
90.80	220.0
91.20	207.0
92.00	2626.0
93.00	3319.0
94.00	7736.0
95.00	66248.0
96.00	3567.0
97.00	188.0
103.80	357.0
105.70	285.0
112.90	158.0
115.90	218.0
116.70	556.0
117.80	461.0
118.90	401.0
125.00	230.0
127.70	321.0
128.80	156.0
129.80	284.0
133.10	433.0
134.70	268.0
136.80	201.0
140.90	1399.0
141.90	251.0
142.90	1455.0
147.00	295.0
147.90	332.0
152.00	198.0
155.00	289.0
171.50	282.0
172.30	551.0
173.90	59368.0
174.90	4590.0
175.90	57216.0
176.90	3878.0
178.70	185.0
191.00	212.0
192.90	671.0
193.80	212.0
204.90	198.0
206.70	187.0
207.10	199.0
248.80	376.0
265.00	225.0
281.00	2150.0
281.90	867.0
283.00	593.0

Instrument :
MSVOA_D
ClientSampleId :
BFB150