
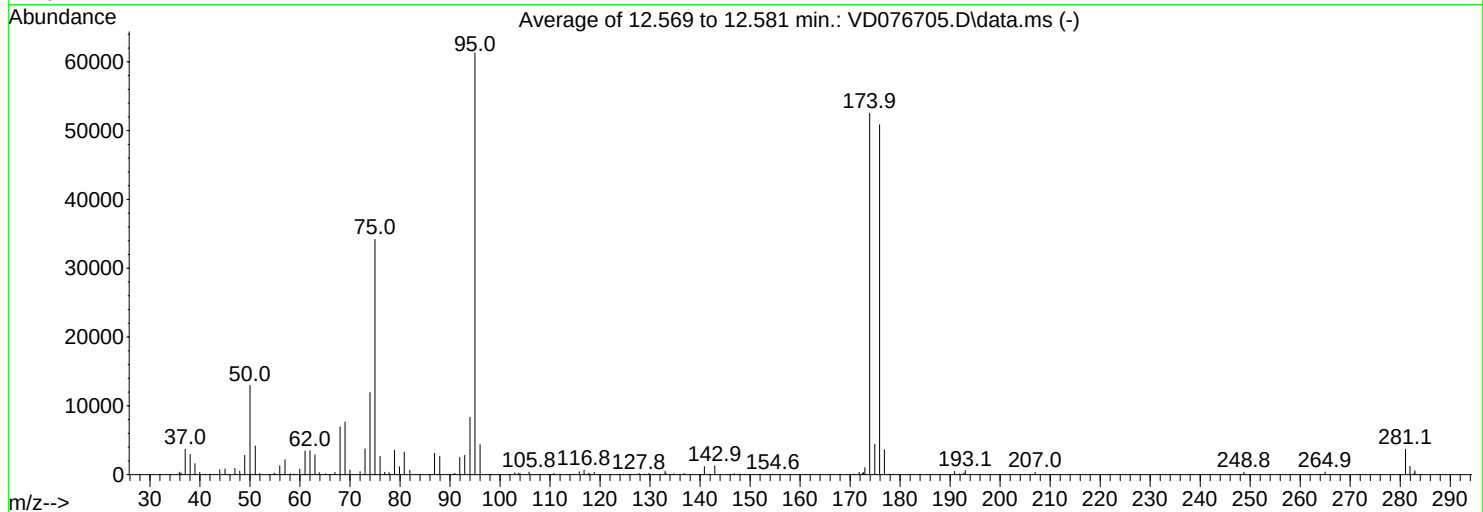


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD070523\
Data File : VD076705.D
Acq On : 05 Jul 2023 08:34
Operator : KP/SY
Sample : BFB151
Misc : 5.00G/10.0ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB151

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM061523SMA.M
Title : SFAM01.0
Last Update : Fri Jun 16 01:50:34 2023

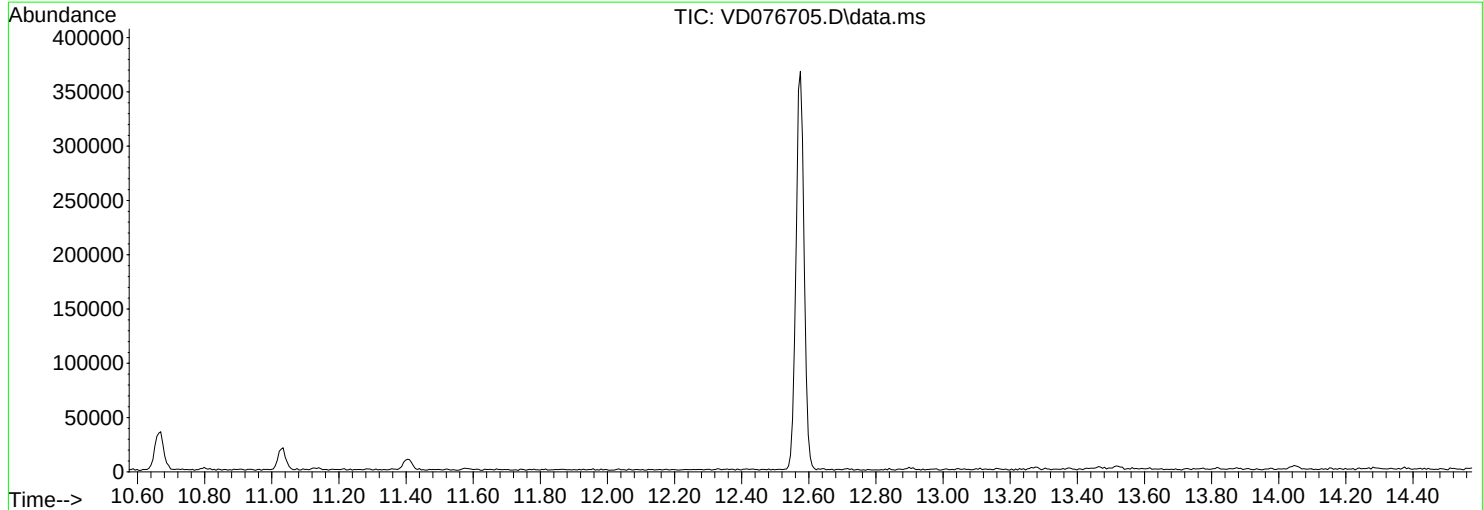

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1859

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.1	12946	PASS
75	95	30	80	55.8	34195	PASS
95	95	100	100	100.0	61317	PASS
96	95	5	9	7.1	4369	PASS
173	174	0.00	2	1.9	1021	PASS
174	95	50	120	85.7	52552	PASS
175	174	5	9	8.4	4428	PASS
176	174	95	105	96.8	50864	PASS
177	176	5	10	7.1	3631	PASS

m/z	Abundance
36.70	153.0
40.00	1044.0
42.90	189.0
44.00	419.0
72.70	157.0
207.10	168.0

Instrument :
MSVOA_D
ClientSampleId :
BFB151

m/z	Abundance
35.80	504.0
36.20	686.0
37.00	3456.0
38.10	3099.0
39.00	1801.0
39.90	1234.0
41.10	171.0
42.90	214.0
43.90	825.0
45.00	688.0
46.90	1213.0
47.90	474.0
49.00	3264.0
50.00	14190.0
51.00	4675.0
52.00	294.0
54.90	383.0
56.00	1291.0
57.00	1975.0
58.10	243.0
59.90	817.0
61.00	3906.0
62.00	3407.0
63.00	3365.0
63.80	160.0
65.10	207.0
67.10	220.0
68.00	6947.0
69.00	8463.0
70.10	642.0
72.10	479.0
73.00	4298.0
74.00	11986.0
75.00	35888.0
76.00	2827.0
77.00	382.0
77.90	342.0
78.90	3240.0
79.90	1173.0
80.90	2943.0
82.00	616.0
86.90	3494.0
87.90	2574.0
90.70	205.0
92.00	2981.0
93.00	3305.0
94.00	8902.0
95.00	62784.0
96.00	5002.0
103.00	264.0
103.80	407.0
105.90	465.0
110.90	338.0
115.80	473.0
116.80	416.0
117.70	297.0
118.80	292.0
123.90	152.0
127.90	255.0
129.70	382.0
130.60	173.0
133.10	707.0
134.70	167.0
136.80	239.0
140.90	1032.0
142.00	236.0
143.00	1320.0
146.90	173.0
147.70	215.0
169.90	182.0
171.80	502.0
172.50	636.0
173.00	885.0
173.90	50920.0
174.90	4530.0
175.90	53120.0
176.90	3590.0
190.90	440.0
191.90	183.0
192.80	670.0
204.80	154.0
207.00	842.0
248.70	388.0
249.80	152.0
265.00	184.0
281.00	2750.0
281.90	538.0
282.80	703.0

Instrument :
MSVOA_D
ClientSampleId :
BFB151

m/z	Abundance
35.90	632.0
37.10	3721.0
38.00	3185.0
39.00	1820.0
40.00	1489.0
44.00	1342.0
45.10	827.0
47.00	831.0
47.90	566.0
49.00	2742.0
50.00	14014.0
51.00	4211.0
51.90	184.0
54.80	284.0
56.00	1211.0
57.00	2771.0
58.70	196.0
60.00	870.0
61.00	3583.0
62.00	3842.0
63.00	3115.0
63.80	299.0
65.10	223.0
67.00	392.0
68.00	7422.0
69.00	8181.0
70.00	642.0
71.90	602.0
73.00	3239.0
74.00	13527.0
75.00	37536.0
76.00	3057.0
77.00	391.0
77.70	214.0
78.90	3695.0
79.90	1198.0
80.80	4098.0
81.90	686.0
86.90	3654.0
88.00	2917.0
91.00	348.0
92.00	2437.0
92.90	3357.0
94.00	8878.0
95.00	67136.0
96.00	4455.0
98.20	162.0
102.90	231.0
103.70	283.0
105.70	483.0
109.60	191.0
115.80	373.0
116.80	800.0
117.90	317.0
118.90	323.0
125.60	153.0
127.70	276.0
128.90	194.0
129.90	453.0
132.90	792.0
134.90	215.0
140.80	1083.0
142.90	1229.0
145.60	178.0
146.80	257.0
148.90	210.0
154.60	160.0
161.10	152.0
170.90	187.0
171.70	313.0
173.00	1314.0
173.90	57888.0
174.90	5063.0
175.90	52912.0
176.80	4048.0
178.70	162.0
190.90	363.0
191.80	172.0
193.10	614.0
206.90	263.0
248.80	319.0
265.00	479.0
281.10	3979.0
282.00	1496.0
283.00	941.0

Instrument :
MSVOA_D
ClientSampleId :
BFB151

m/z	Abundance
36.00	544.0
37.10	3899.0
38.00	2494.0
39.10	1179.0
39.90	1431.0
42.00	232.0
44.00	1234.0
44.90	1022.0
47.10	694.0
48.00	496.0
48.90	2343.0
50.00	10634.0
51.10	3627.0
55.10	239.0
55.90	1345.0
57.00	1745.0
58.10	170.0
59.00	175.0
60.00	706.0
61.00	2874.0
62.00	3252.0
63.00	2120.0
63.90	487.0
66.90	359.0
68.00	6514.0
69.00	6324.0
69.90	746.0
71.90	229.0
73.00	3699.0
74.00	10285.0
75.00	29160.0
76.00	2116.0
76.90	306.0
77.80	333.0
78.90	3667.0
79.90	1079.0
80.90	2786.0
81.90	667.0
87.00	2137.0
87.90	2500.0
91.00	220.0
91.90	2067.0
92.90	1723.0
94.00	7239.0
95.00	54032.0
96.00	3649.0
102.90	298.0
104.00	490.0
105.70	190.0
106.00	199.0
110.70	260.0
114.80	215.0
115.90	410.0
116.80	733.0
117.70	197.0
118.90	403.0
124.70	199.0
126.20	207.0
133.20	573.0
134.80	153.0
136.80	228.0
140.80	1374.0
142.90	1265.0
148.00	266.0
171.90	259.0
172.70	943.0
172.90	863.0
173.90	48848.0
175.00	3692.0
175.90	46560.0
176.90	3254.0
177.80	235.0
190.90	567.0
193.00	1137.0
194.00	247.0
207.00	443.0
248.70	299.0
264.90	481.0
281.00	4361.0
281.90	1579.0
282.90	810.0
284.30	181.0

Instrument :
MSVOA_D
ClientSampleId :
BFB151