
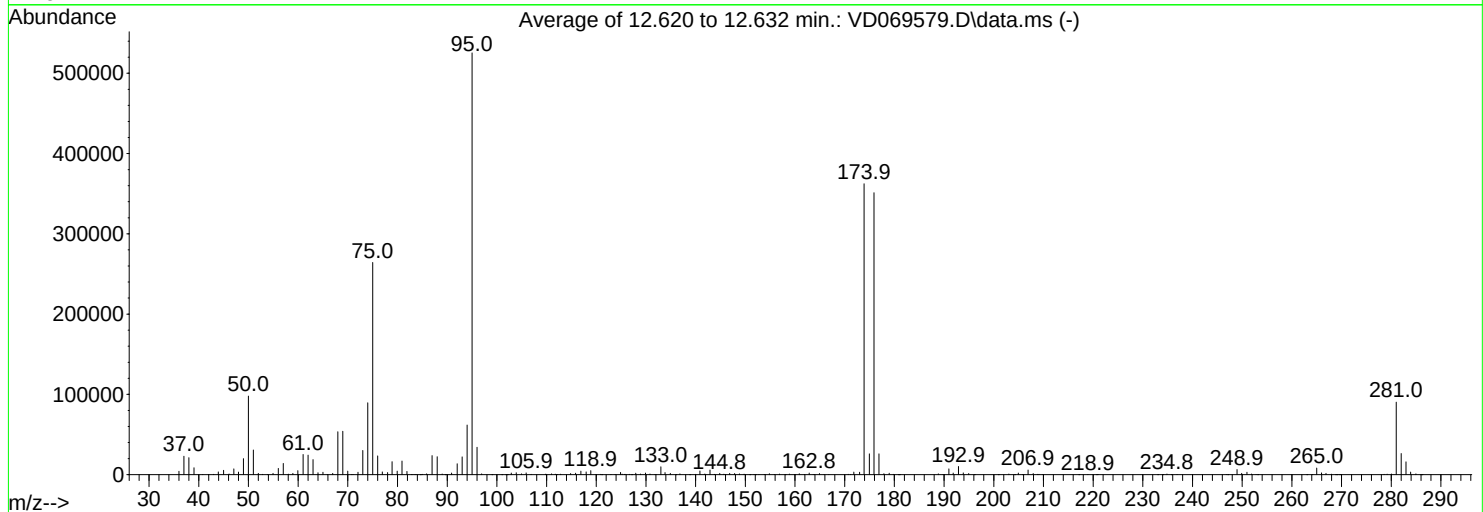


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD070621\
Data File : VD069579.D
Acq On : 06 Jul 2021 12:55
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D062121S.M
Title : SW846 8260
Last Update : Tue Jun 22 04:33:24 2021

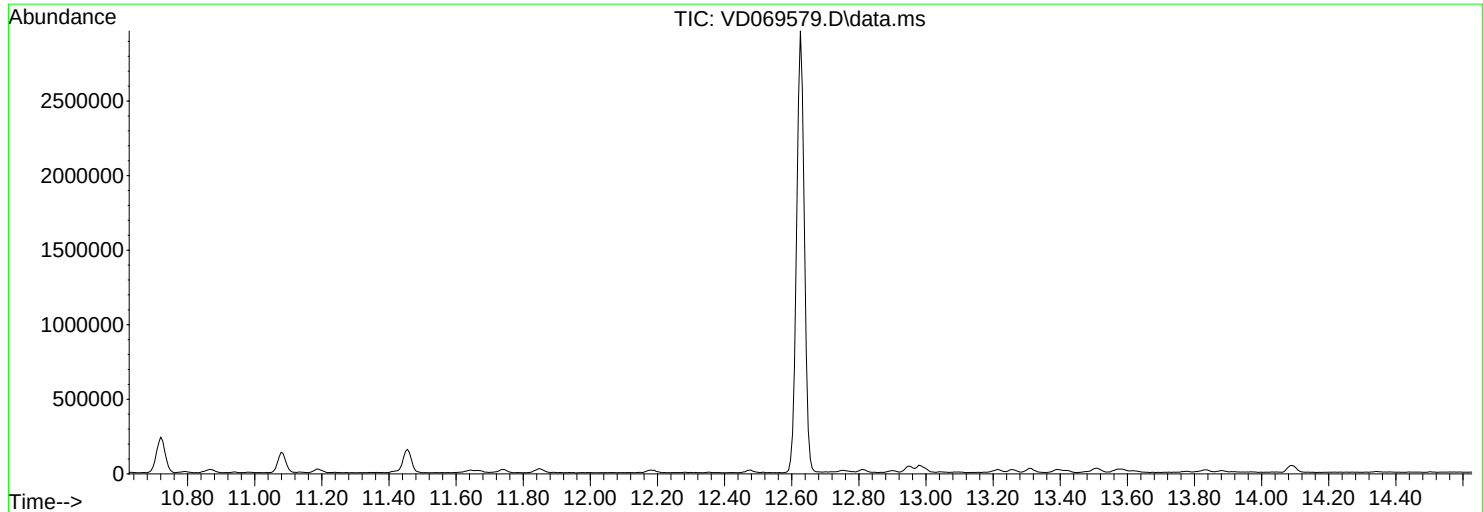

AutoFind: Scans 1819, 1820, 1821; Background Corrected with Scan 1810

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.6	97973	PASS
75	95	30	60	50.3	264235	PASS
95	95	100	100	100.0	525440	PASS
96	95	5	9	6.5	34024	PASS
173	174	0.00	2	0.8	2937	PASS
174	95	50	100	69.0	362304	PASS
175	174	5	9	7.2	26005	PASS
176	174	95	101	96.9	351189	PASS
177	176	5	9	7.4	25832	PASS