



Dichlorodifluoromethane

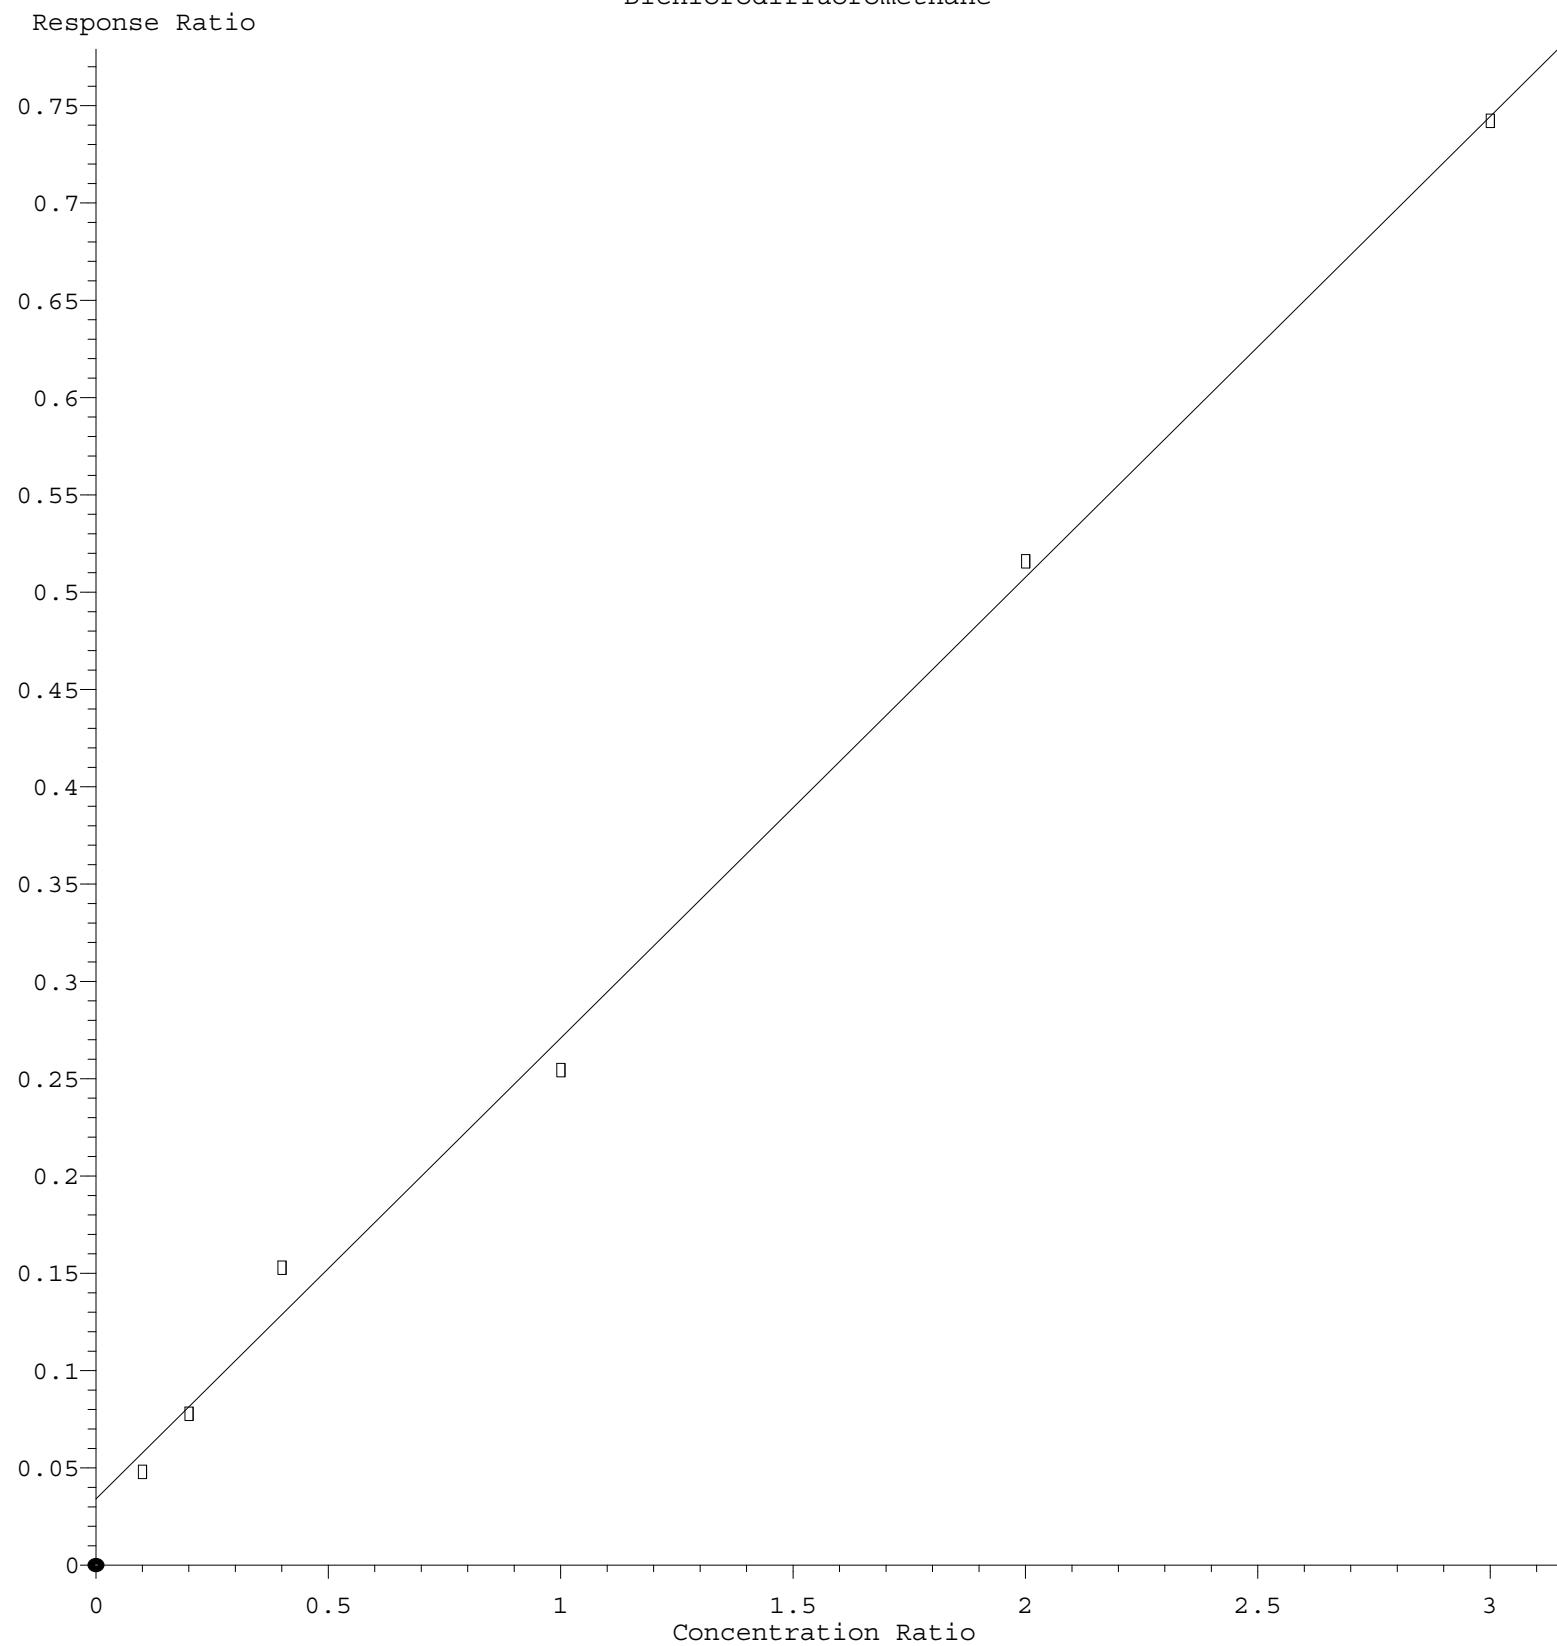

Response = 2.369e-001 * Amt + 3.390e-002
 Coef of Det (r^2) = 0.997279 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D070622S.M
 Calibration Table Last Updated: Mon Jul 11 11:42:28 2022

Chloromethane

Response Ratio

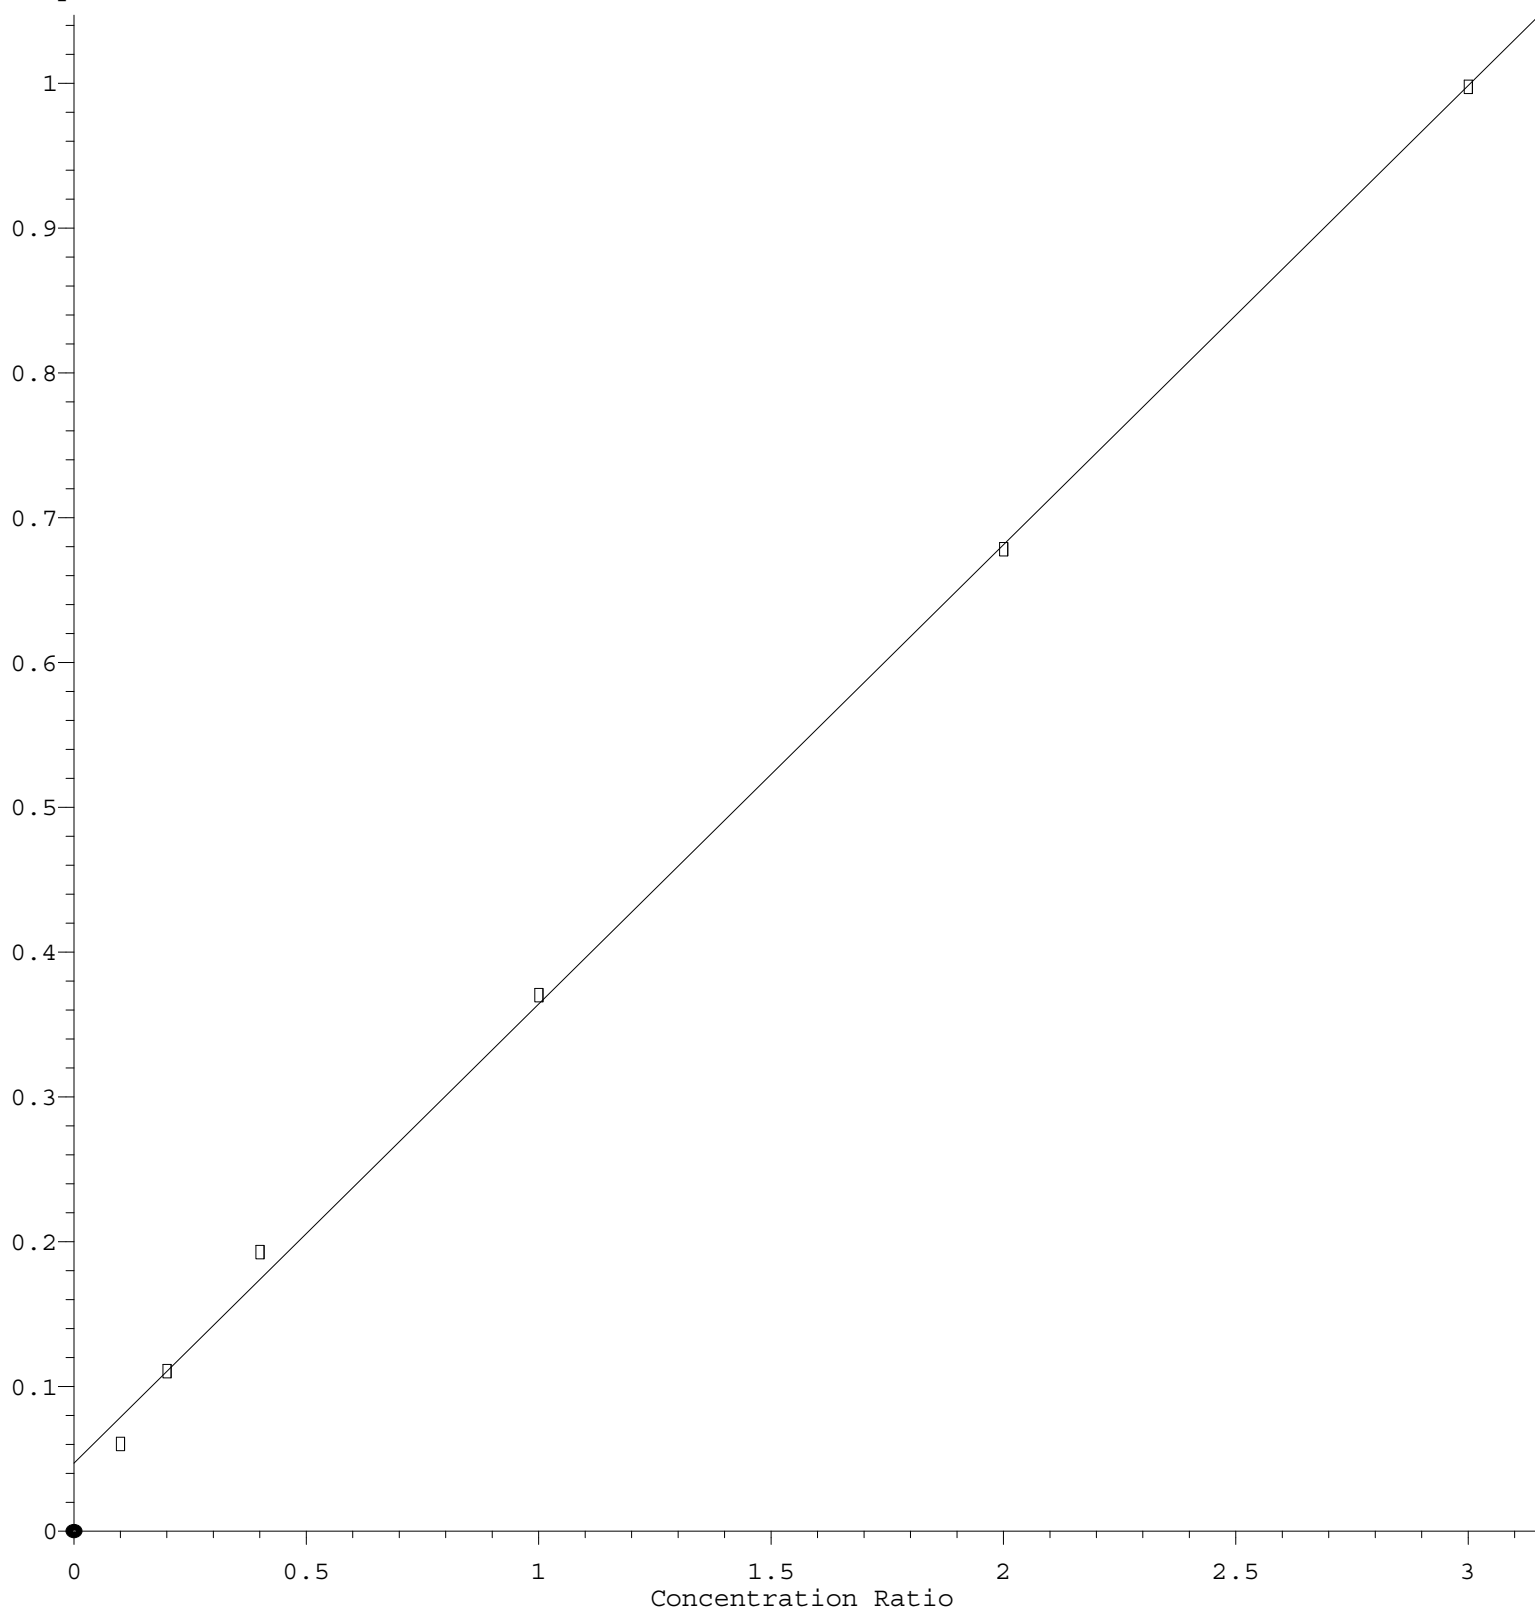

$$\text{Response} = 3.171\text{e-}001 * \text{Amt} + 4.738\text{e-}002$$


Coef of Det (r^2) = 0.998901 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D070622S.M

Calibration Table Last Updated: Mon Jul 11 11:42:28 2022

Vinyl Chloride

Response Ratio

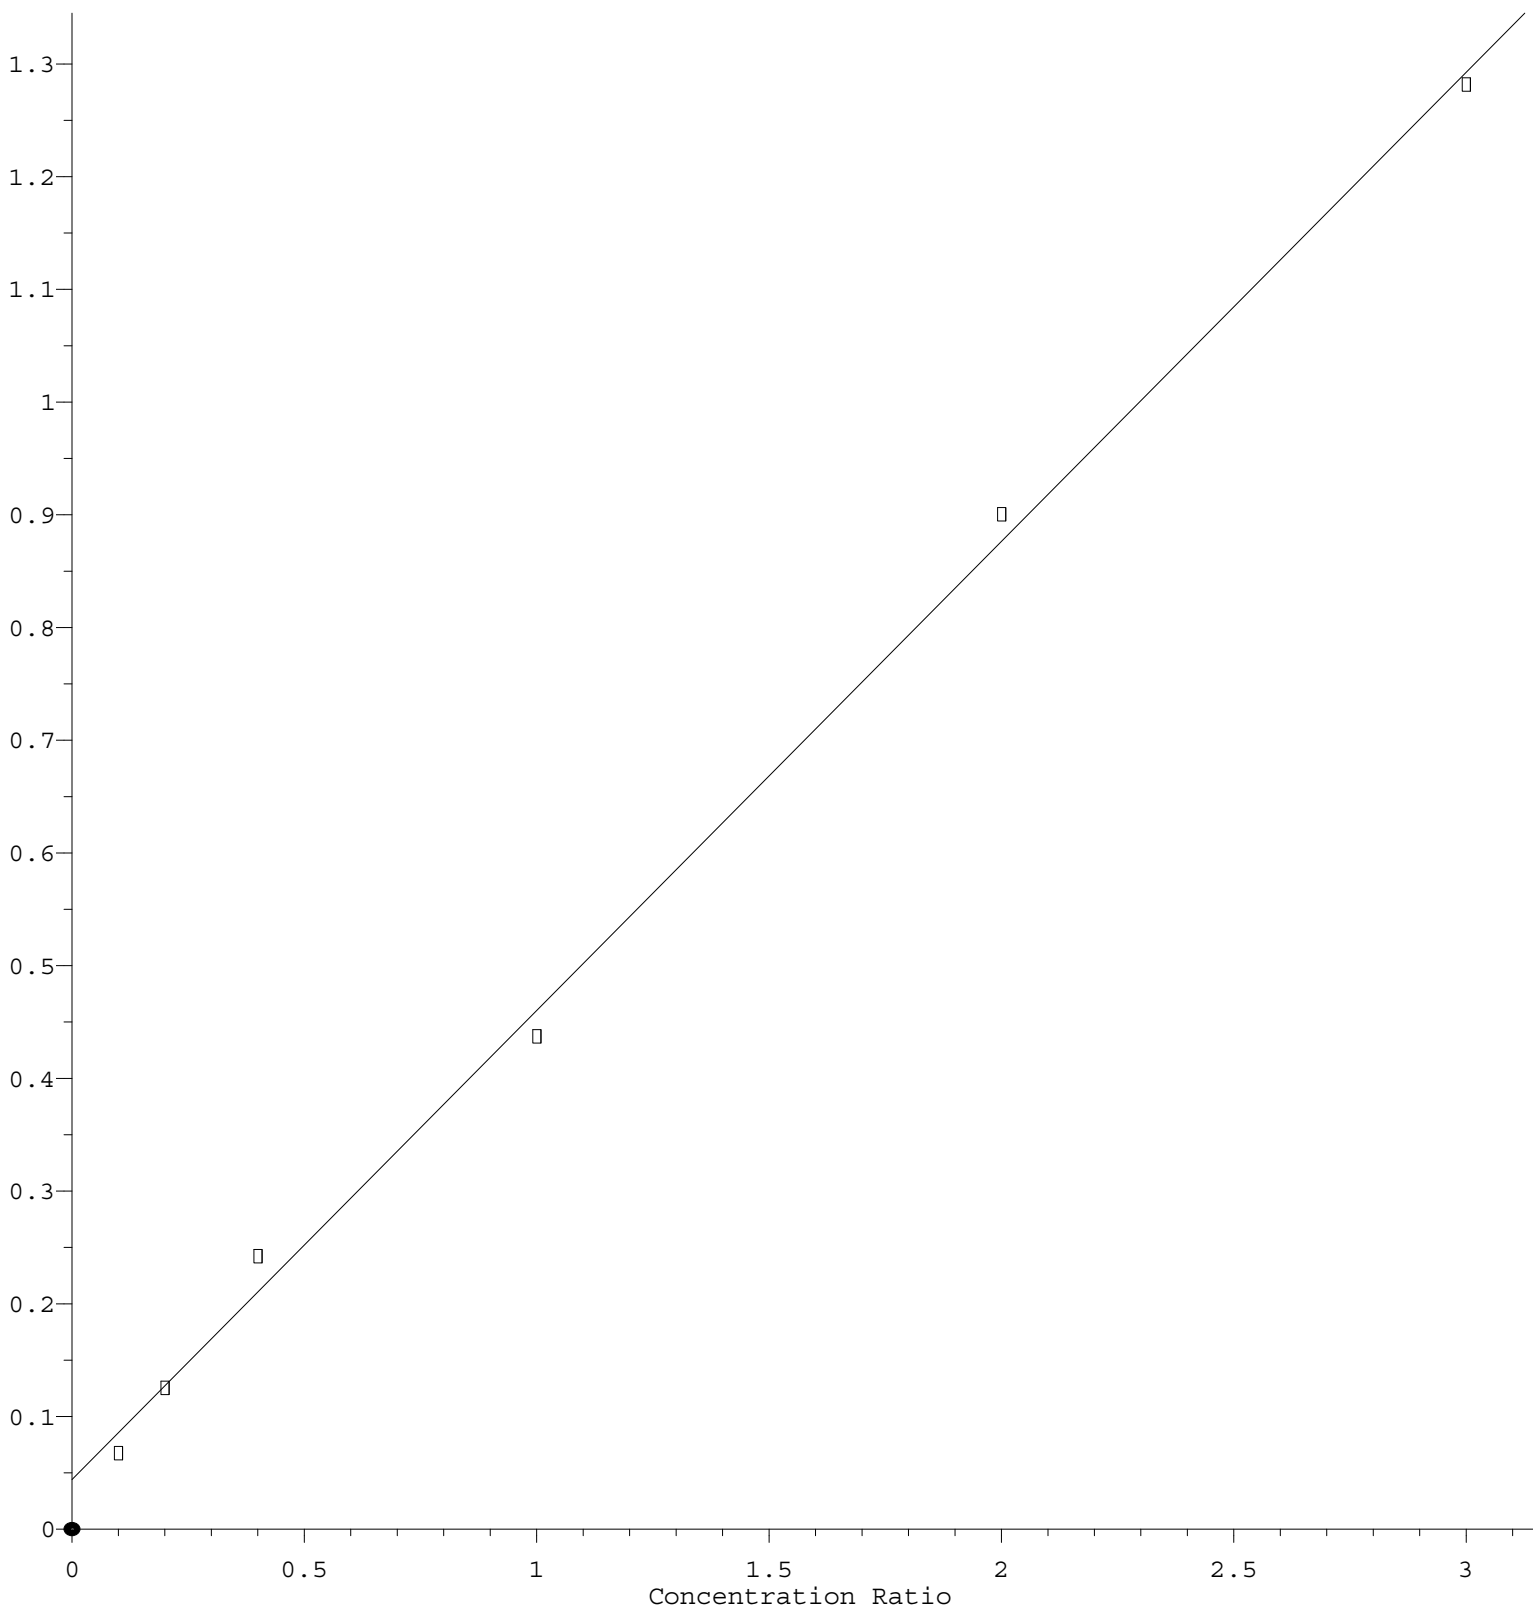

$$\text{Response} = 4.163\text{e-}001 * \text{Amt} + 4.417\text{e-}002$$


Coef of Det (r^2) = 0.997802 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D070622S.M

Calibration Table Last Updated: Mon Jul 11 11:42:28 2022

Bromomethane

Response Ratio

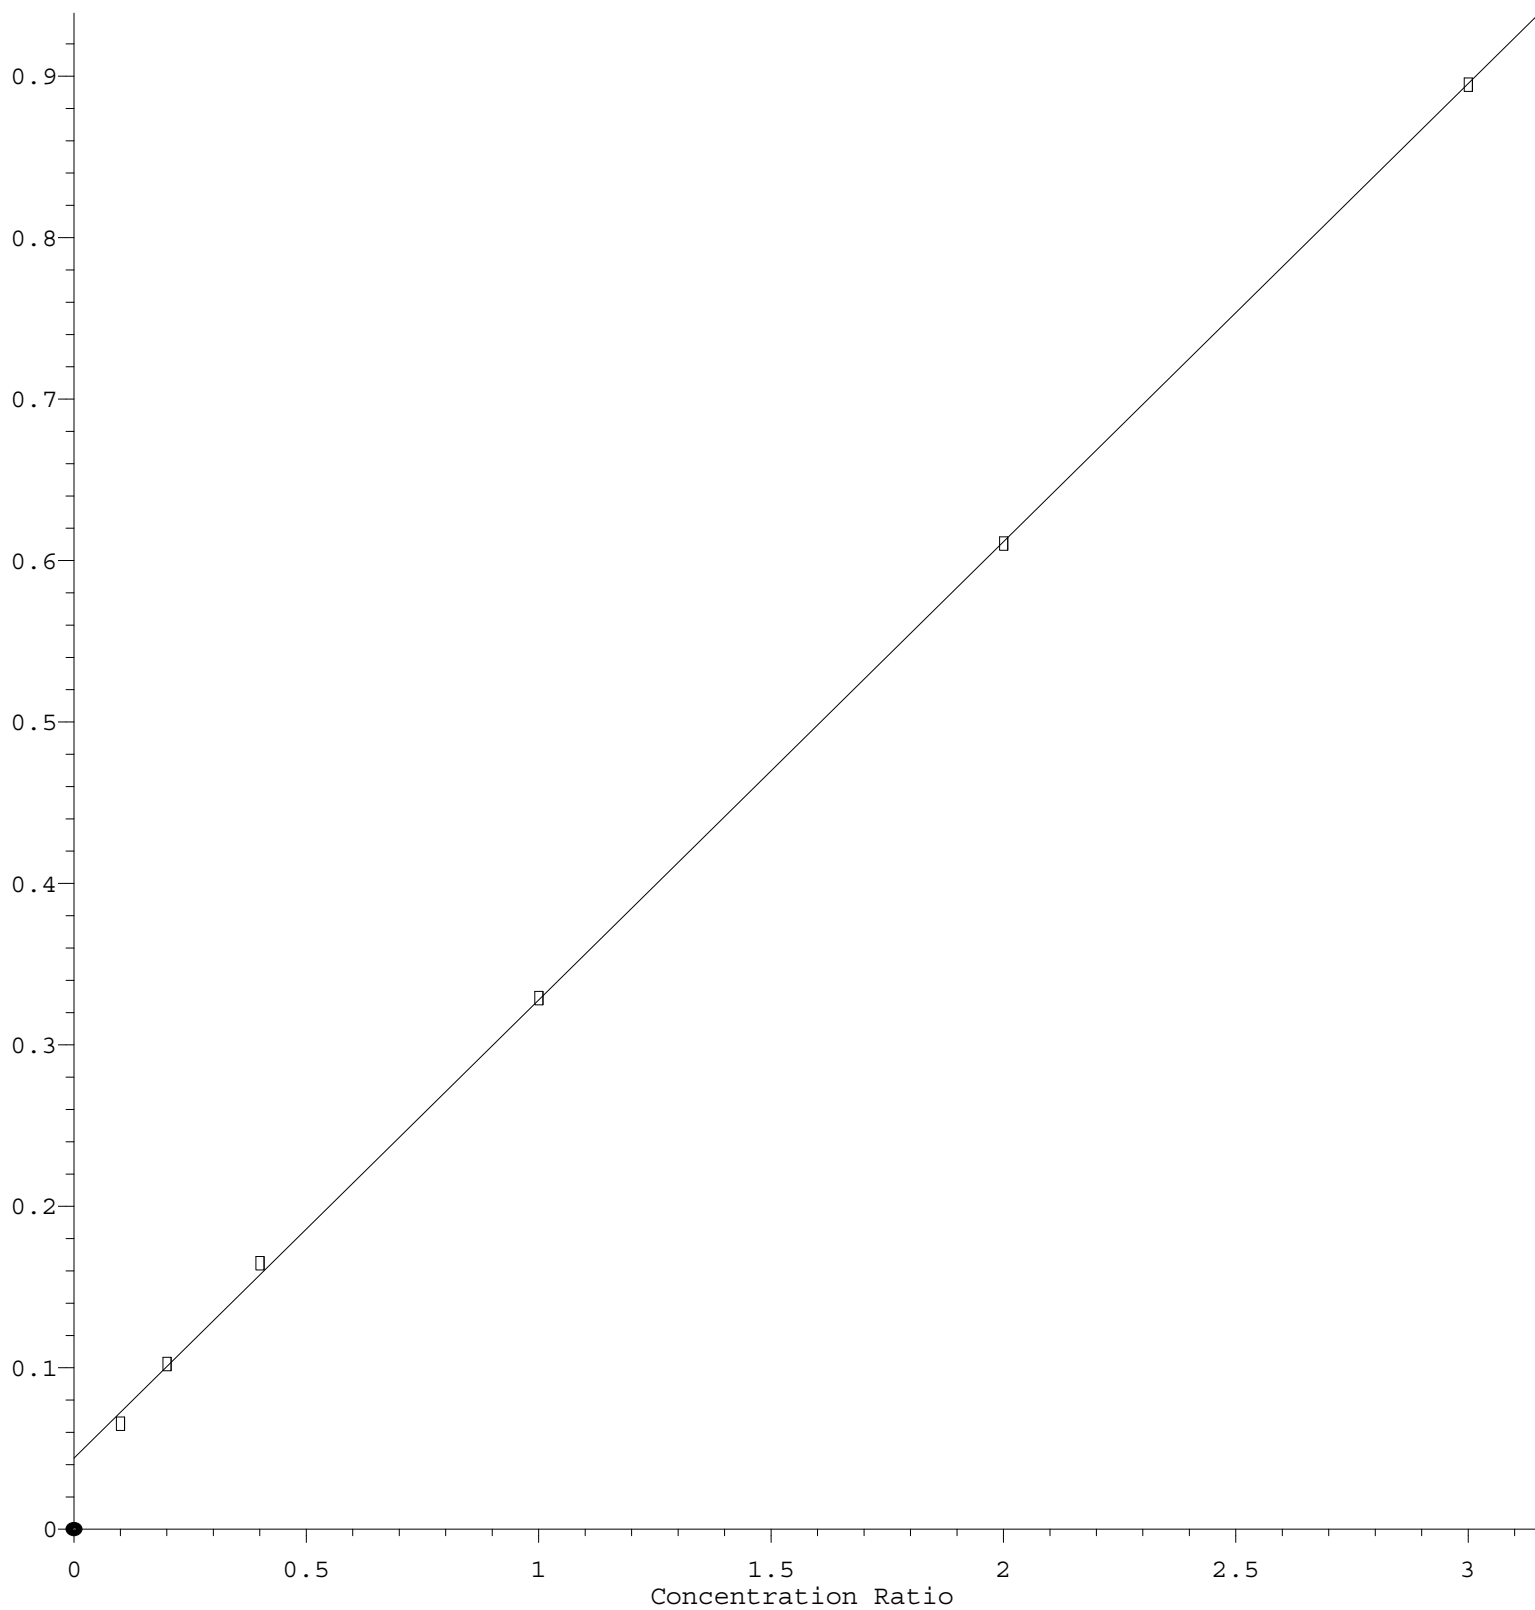


$$\text{Response} = 2.835\text{e-}001 * \text{Amt} + 4.446\text{e-}002$$

Coef of Det (r^2) = 0.999806 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D070622S.M

Calibration Table Last Updated: Mon Jul 11 11:42:28 2022


Tetrachloroethene

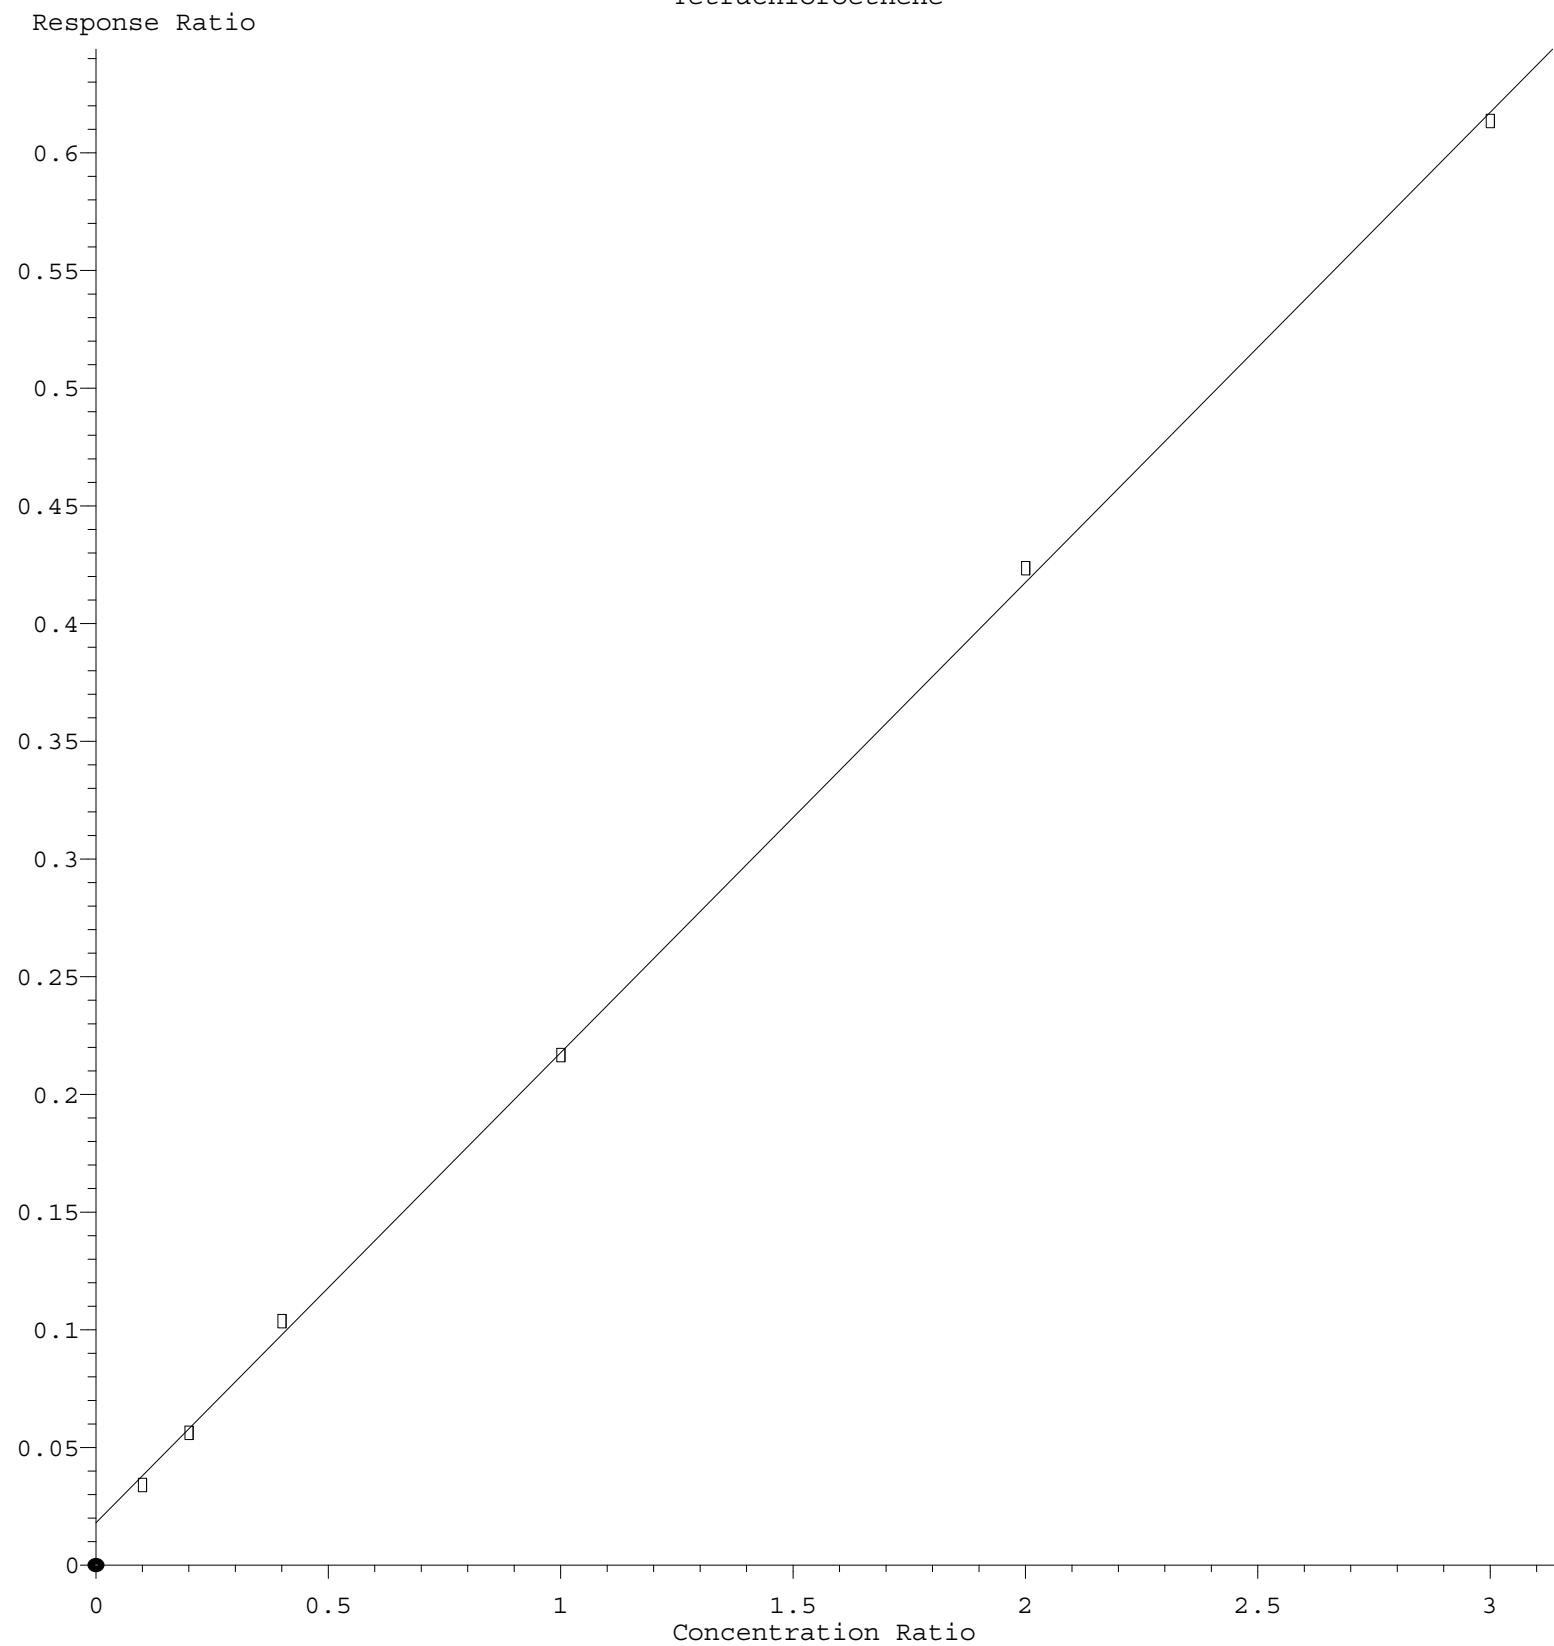

Response = $1.997\text{e-}001 \cdot \text{Amt} + 1.826\text{e-}002$
Coef of Det (r^2) = 0.999618 Curve Fit: Linear
Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D070622S.M
Calibration Table Last Updated: Mon Jul 11 11:42:28 2022

Cyclohexane

Response Ratio

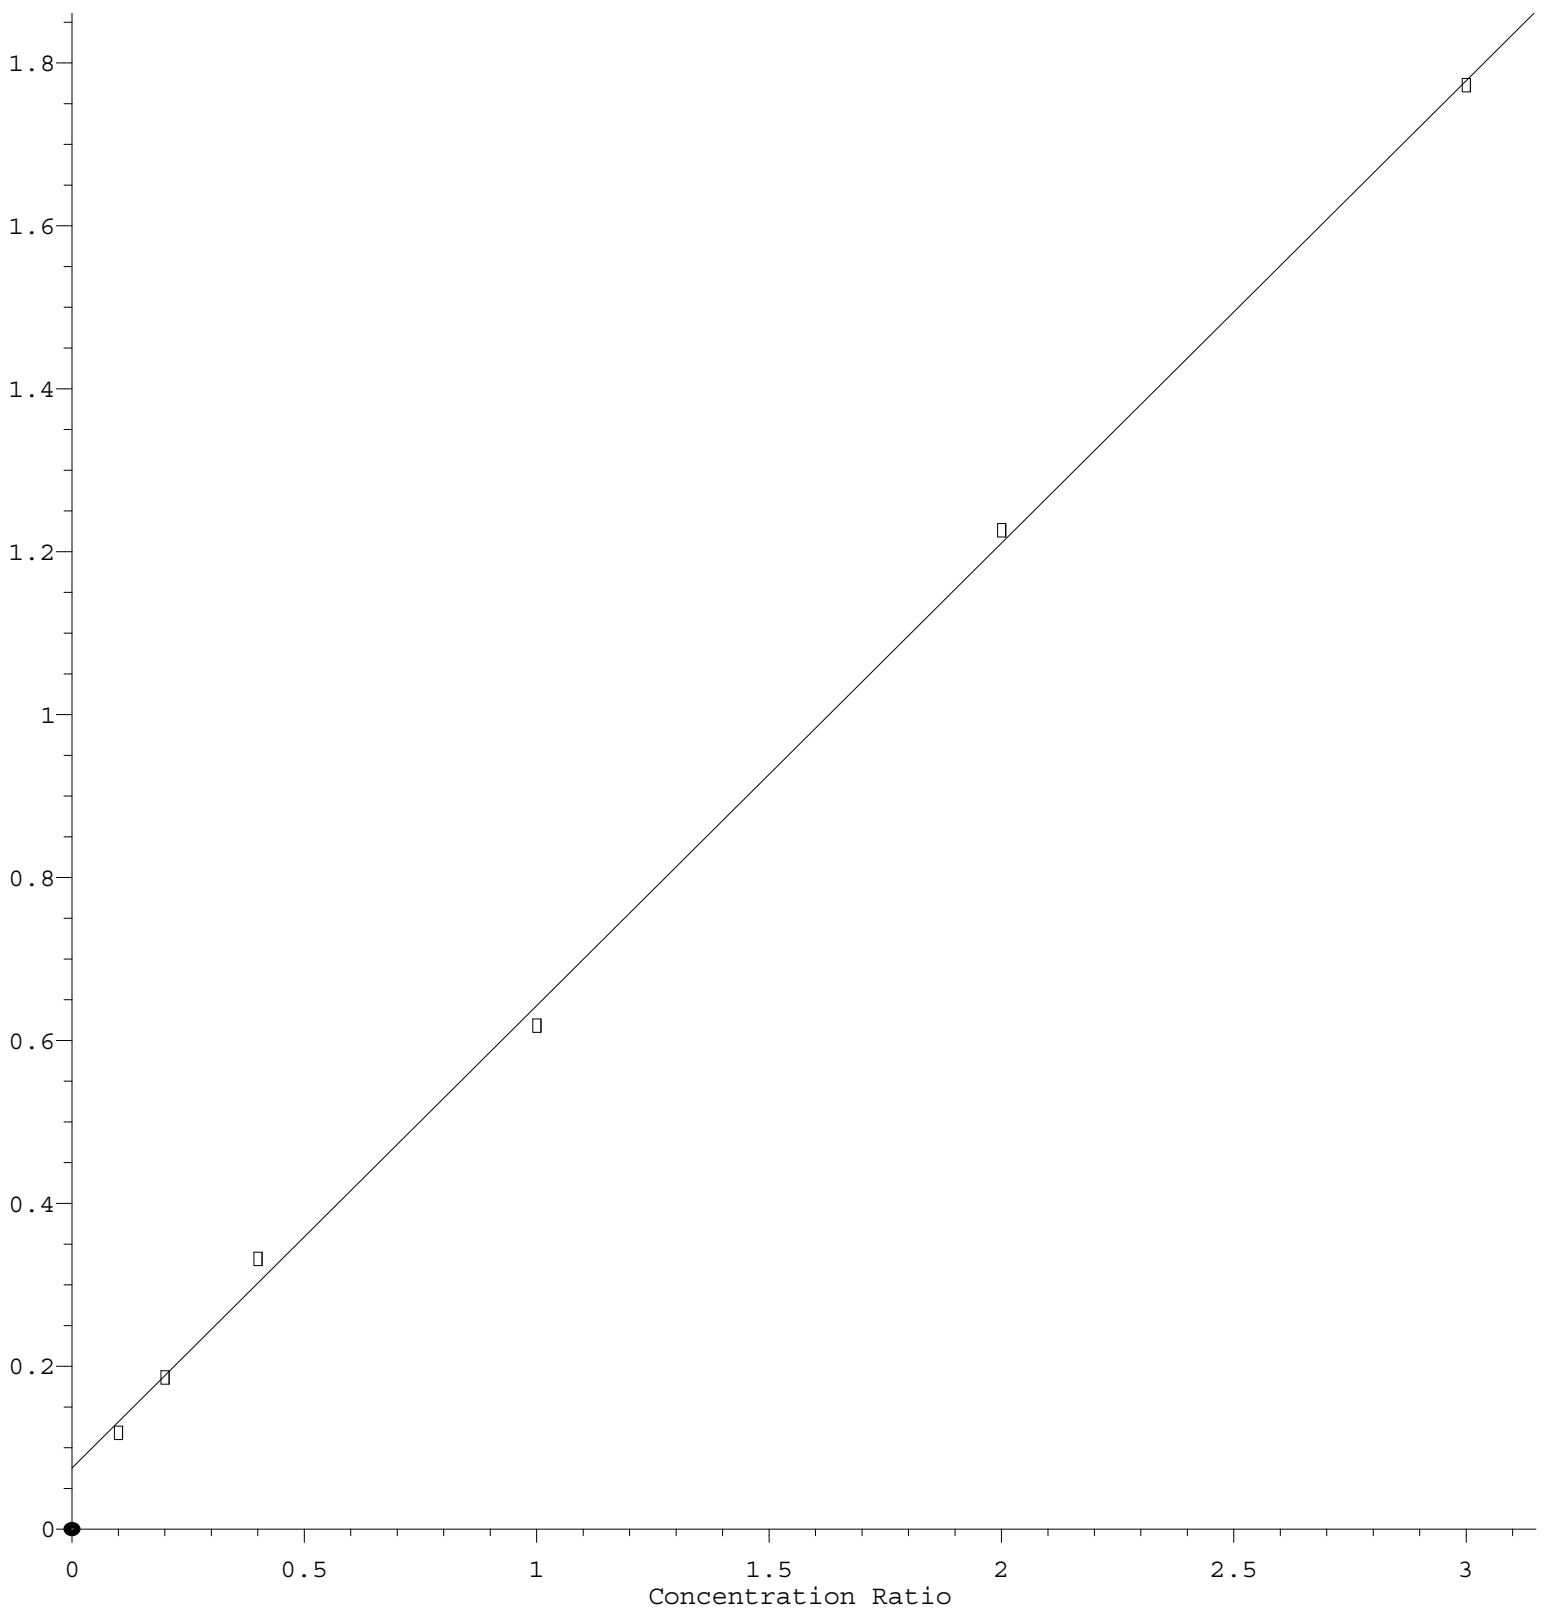

$$\text{Response} = 5.679\text{e-}001 * \text{Amt} + 7.474\text{e-}002$$


Coef of Det (r^2) = 0.999100 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D070622S.M

Calibration Table Last Updated: Mon Jul 11 11:42:28 2022

Methyl Acetate

Response Ratio

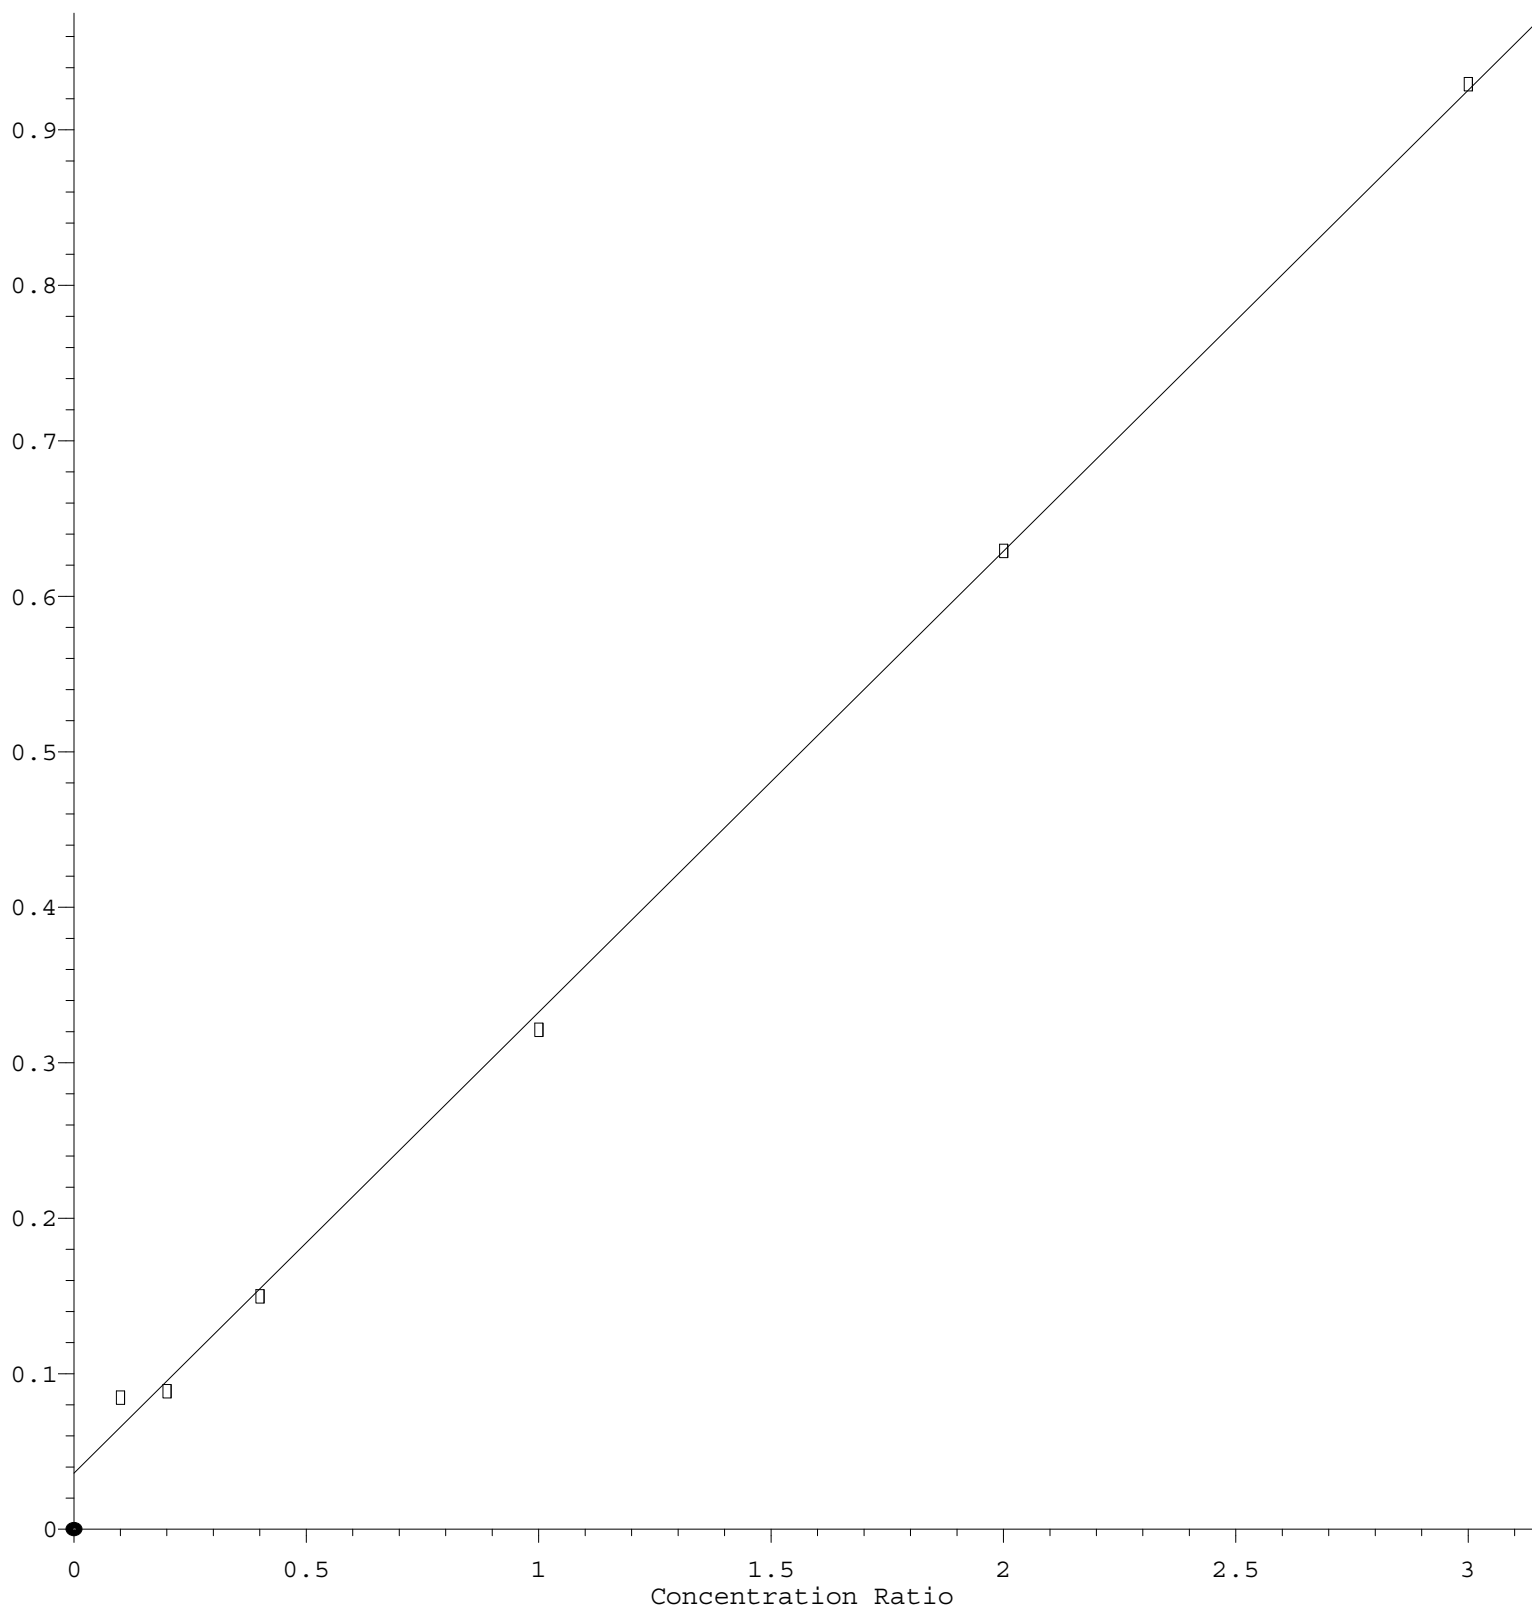

$$\text{Response} = 2.963\text{e-}001 * \text{Amt} + 3.622\text{e-}002$$


Coef of Det (r^2) = 0.999036 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D070622S.M

Calibration Table Last Updated: Mon Jul 11 11:42:28 2022

Methylene Chloride


Response Ratio

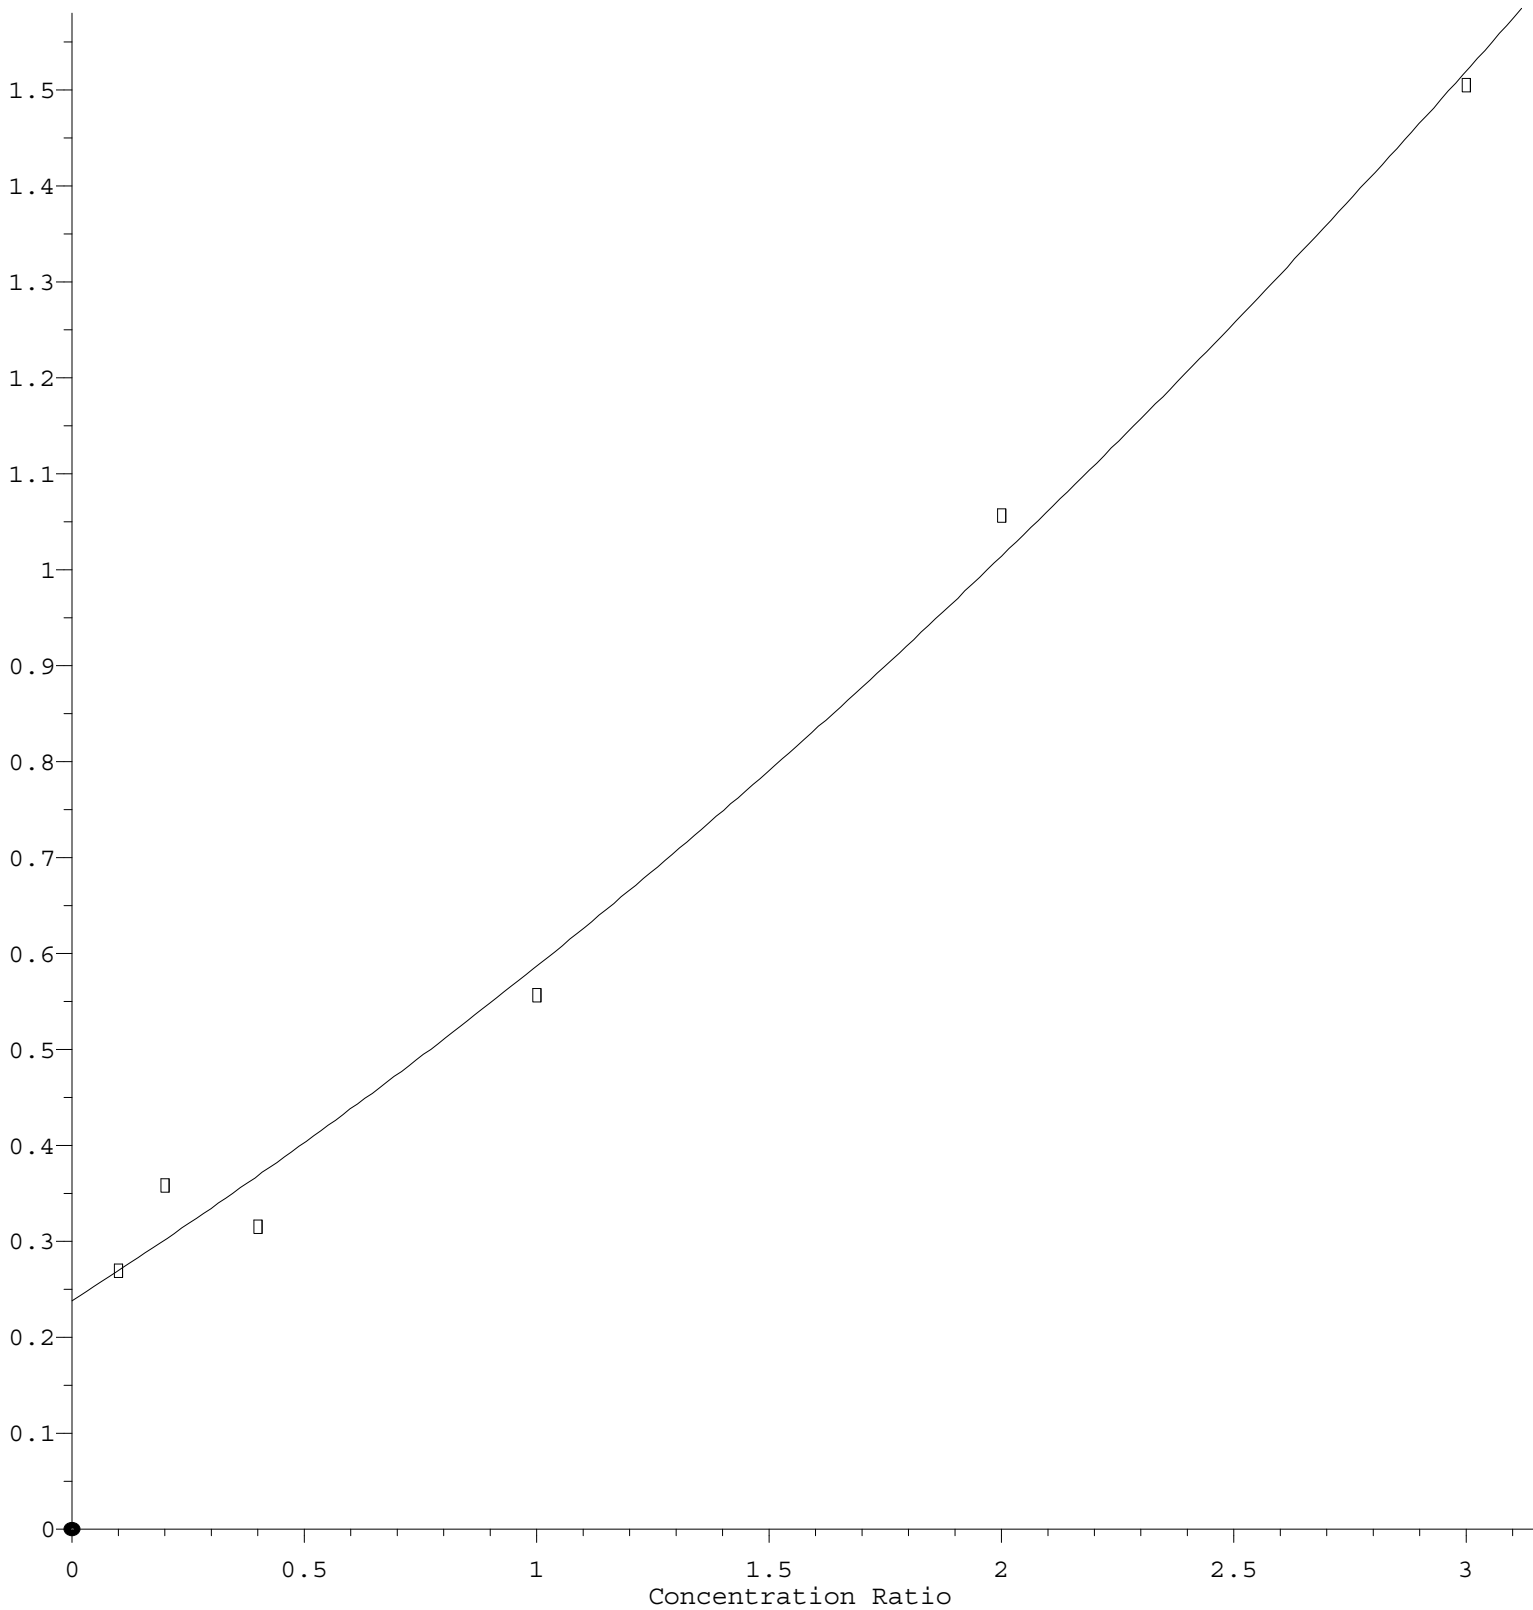

$R = 3.927e-002 A^2 + 3.093e-001 A + 2.384e-001$
 Coef of Det (r^2) = 0.992795 Curve Fit: Quadratic
 Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D070622S.M
 Calibration Table Last Updated: Mon Jul 11 11:42:28 2022

Carbon Disulfide

Response Ratio

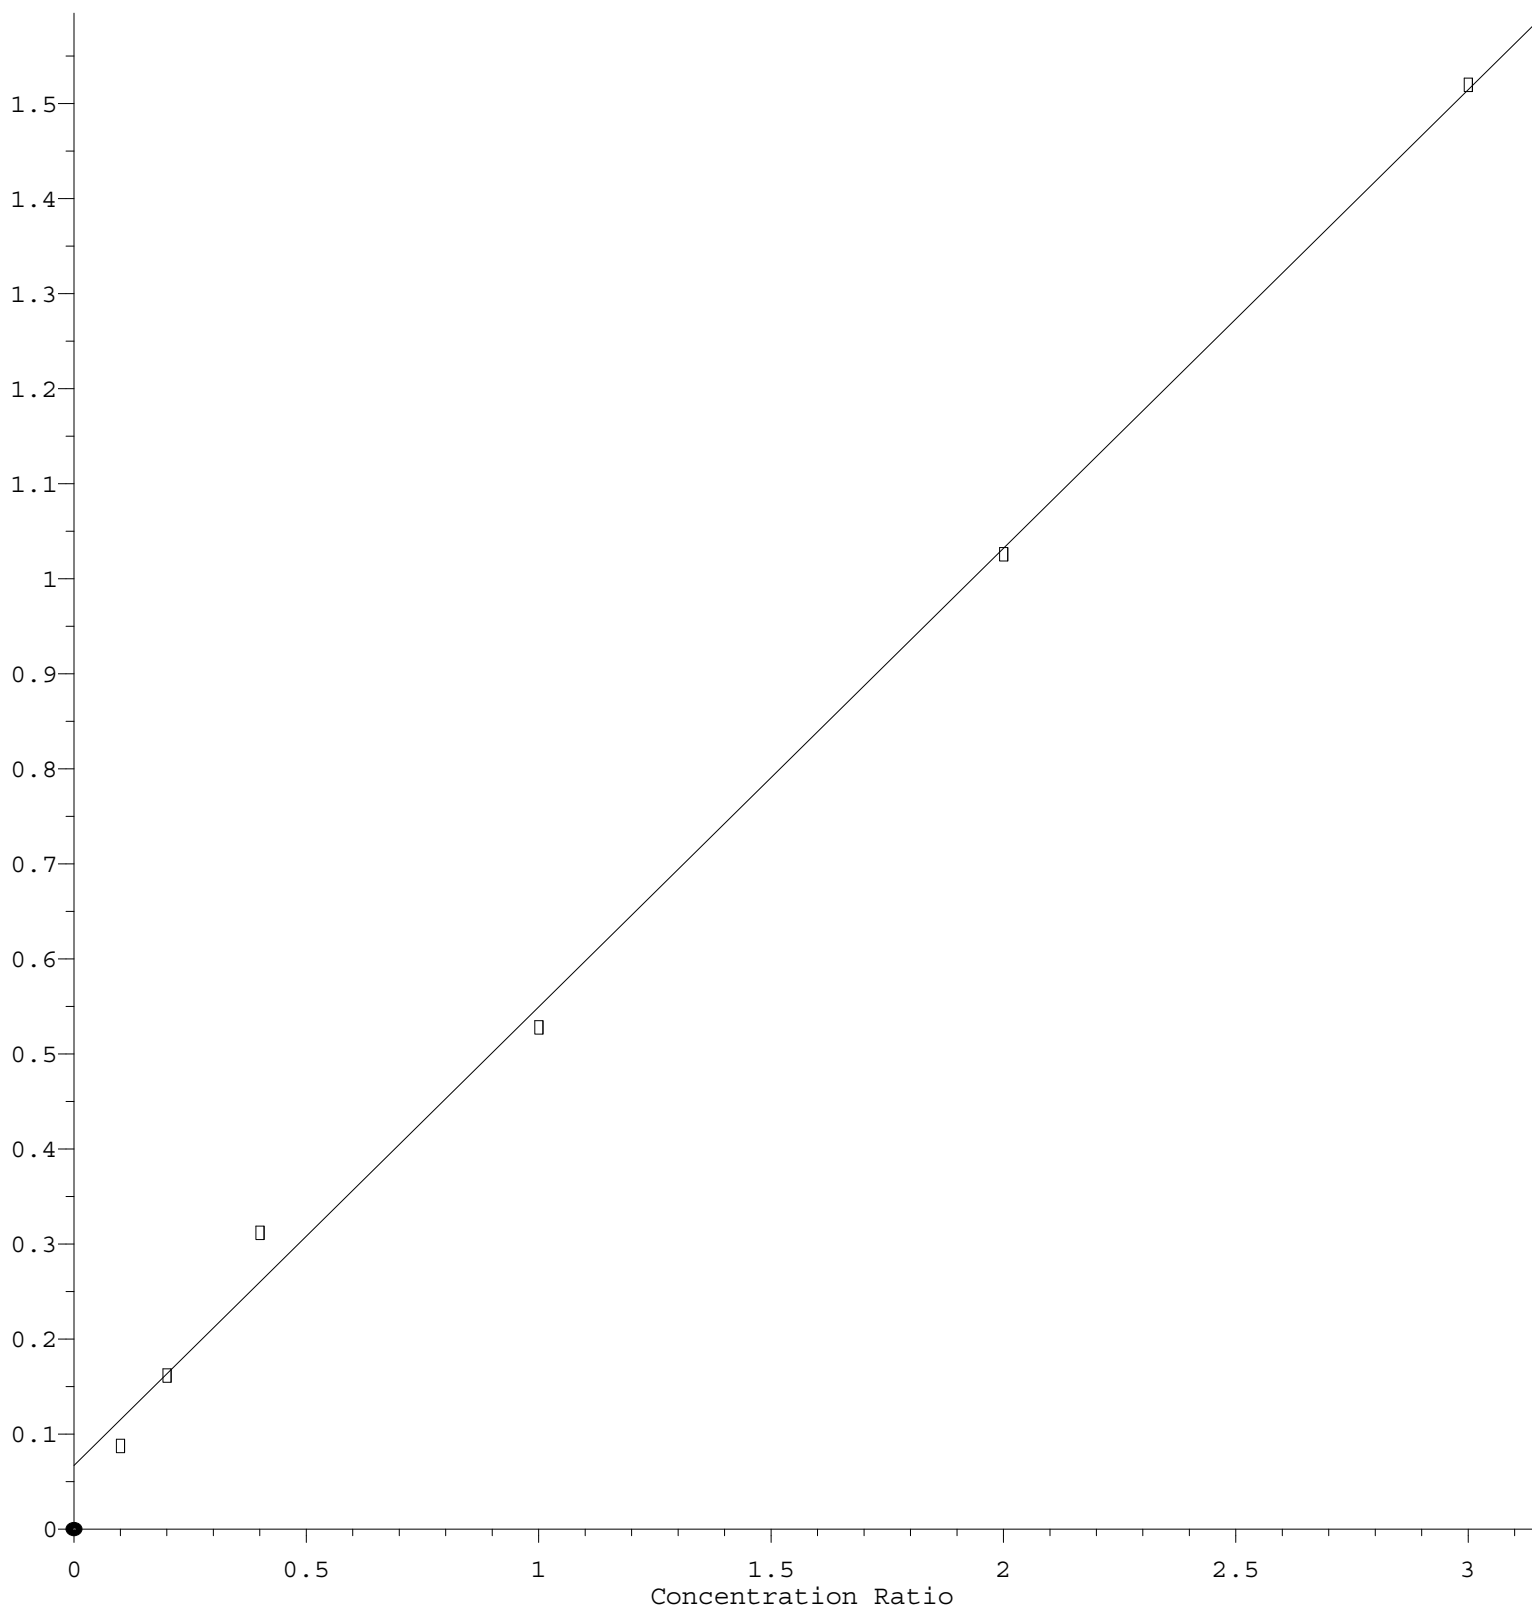

$$\text{Response} = 4.824\text{e-}001 * \text{Amt} + 6.701\text{e-}002$$


Coef of Det (r^2) = 0.997460 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D070622S.M

Calibration Table Last Updated: Mon Jul 11 11:42:28 2022

Acetone

Response Ratio

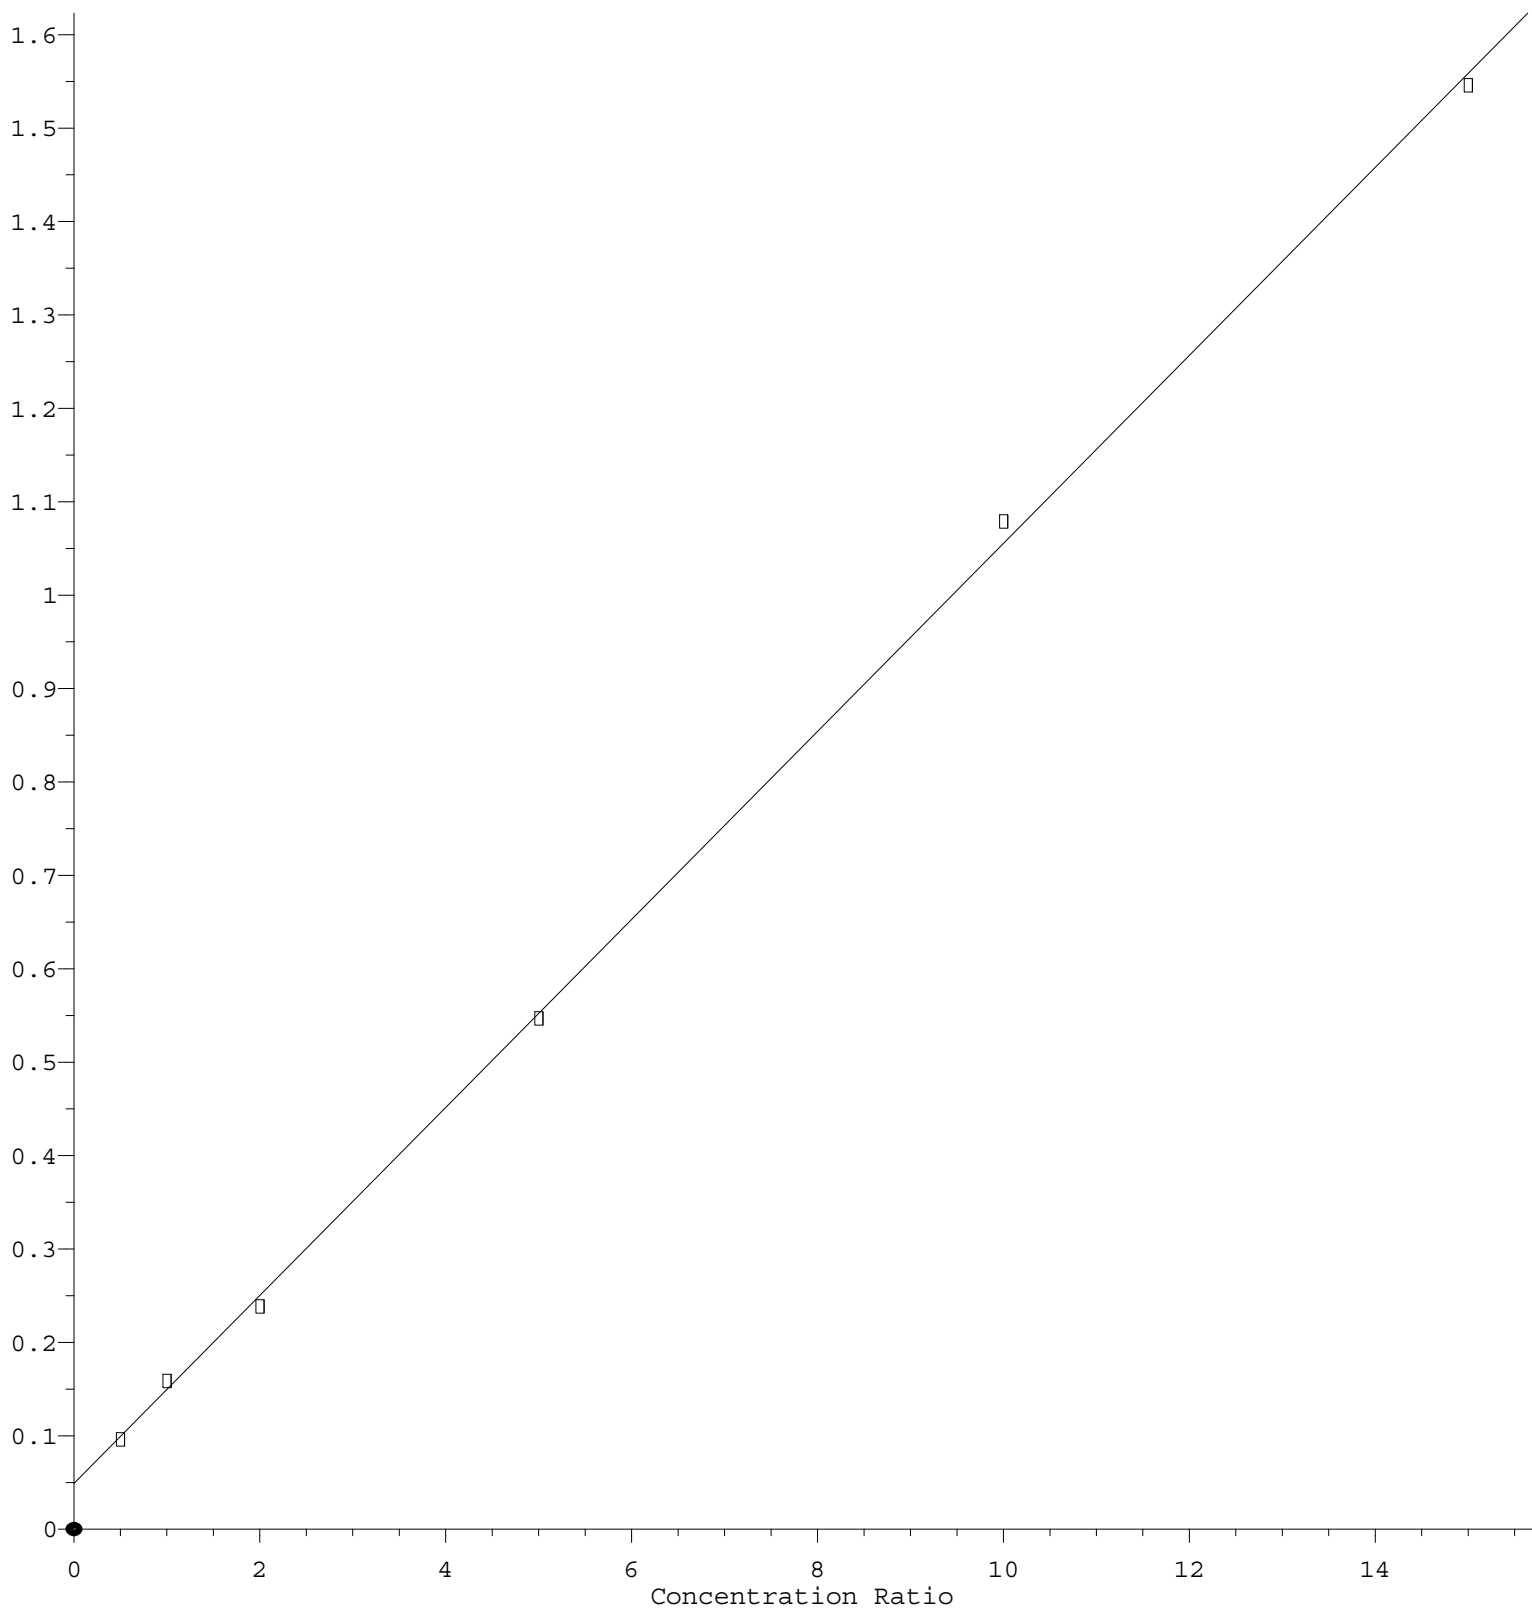


$$\text{Response} = 1.007\text{e-}001 * \text{Amt} + 4.869\text{e-}002$$

Coef of Det (r^2) = 0.999430 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D070622S.M

Calibration Table Last Updated: Mon Jul 11 11:42:28 2022

Acrolein

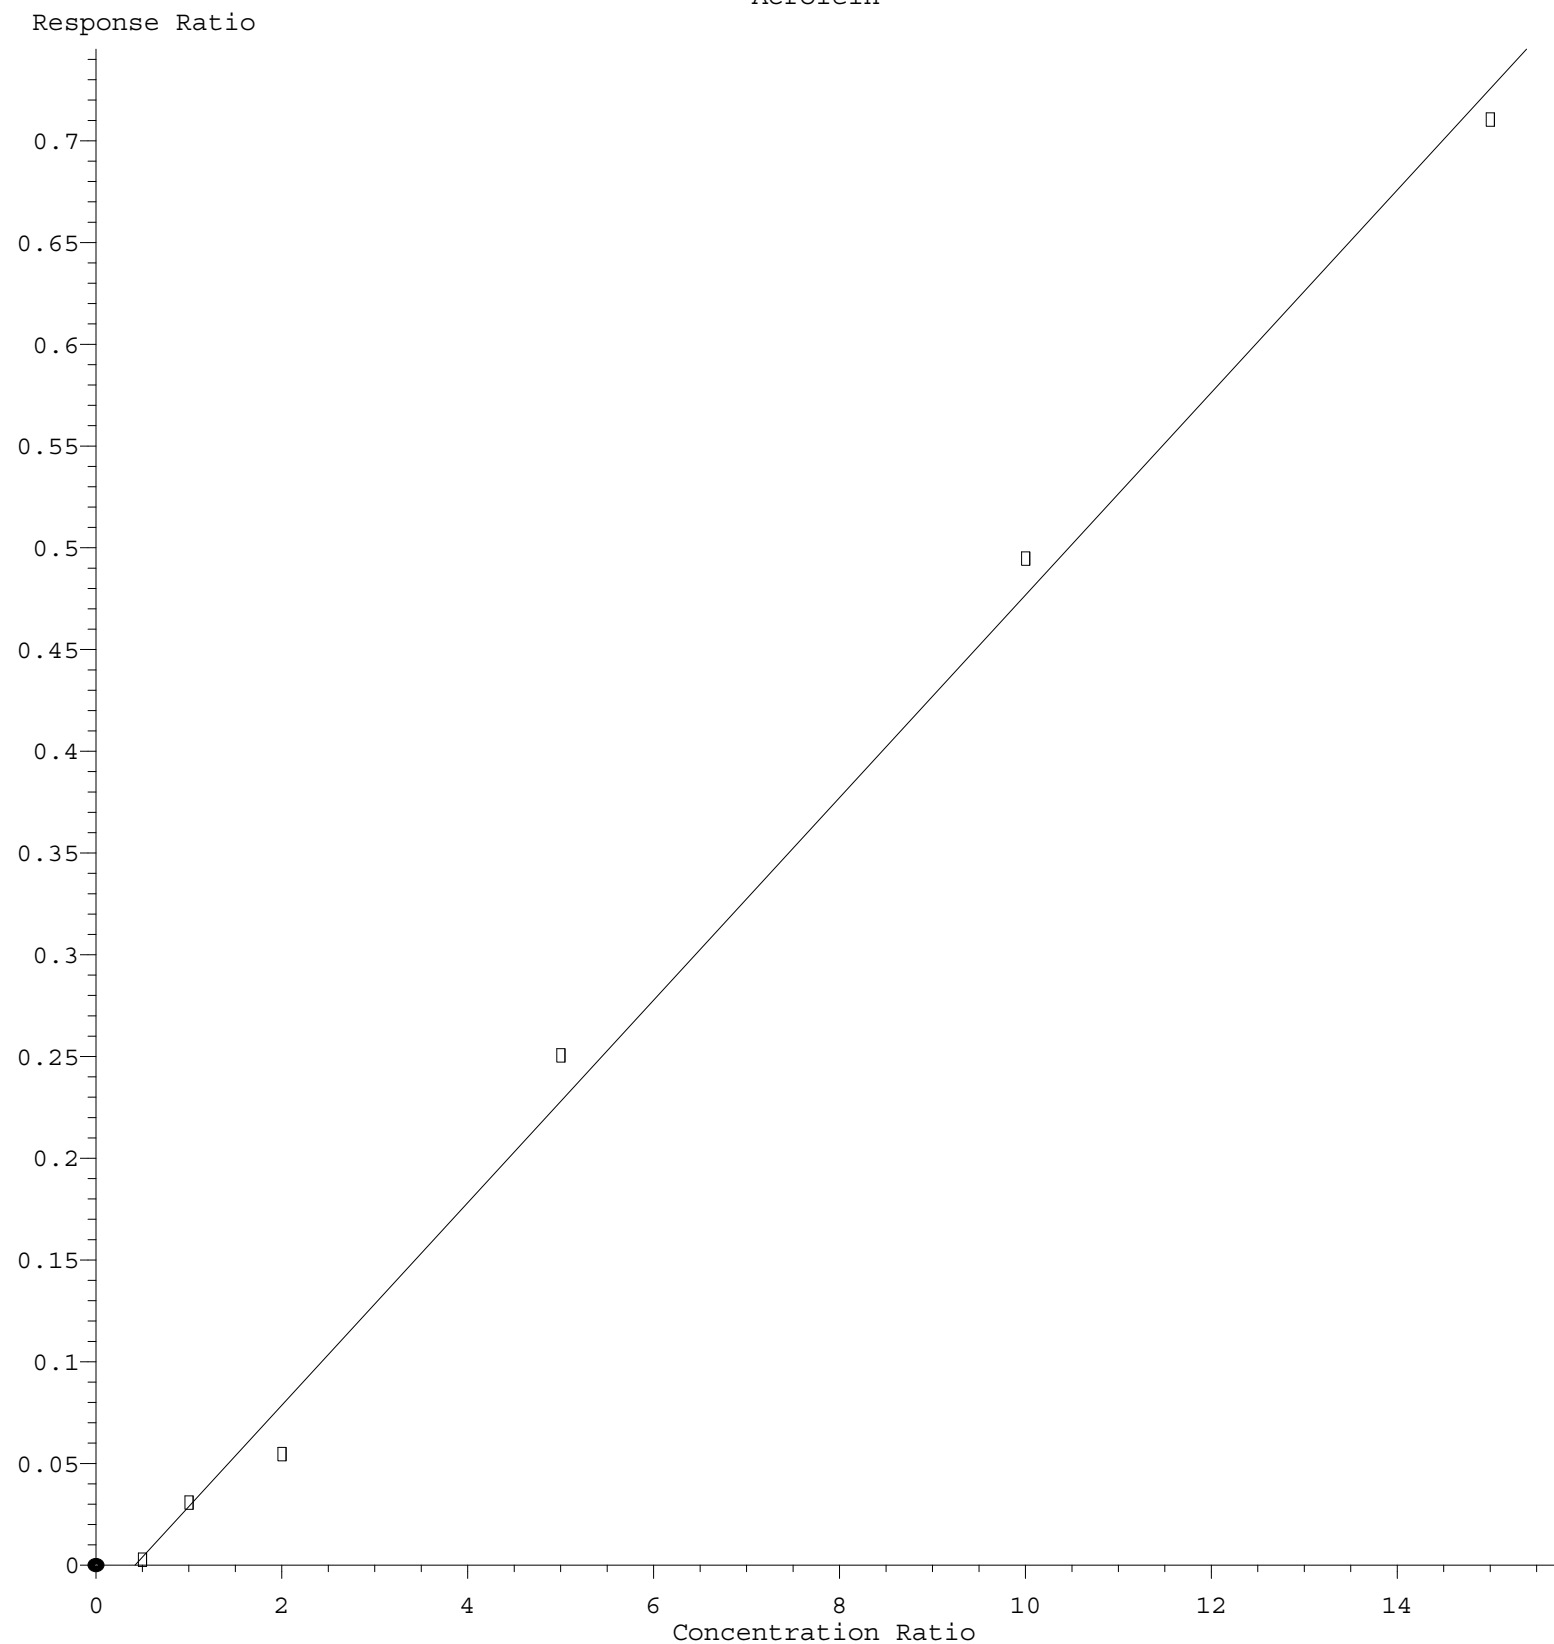

$\text{Response} = 4.981\text{e-}002 * \text{Amt} - 2.083\text{e-}002$
 Coef of Det (r^2) = 0.996075 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D070622S.M
 Calibration Table Last Updated: Mon Jul 11 11:42:28 2022