


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD070720\
Data File : VD065919.D
Acq On : 07 Jul 2020 11:41
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D070720S.M
Title : SW846 8260
Last Update : Wed Jul 08 09:45:47 2020

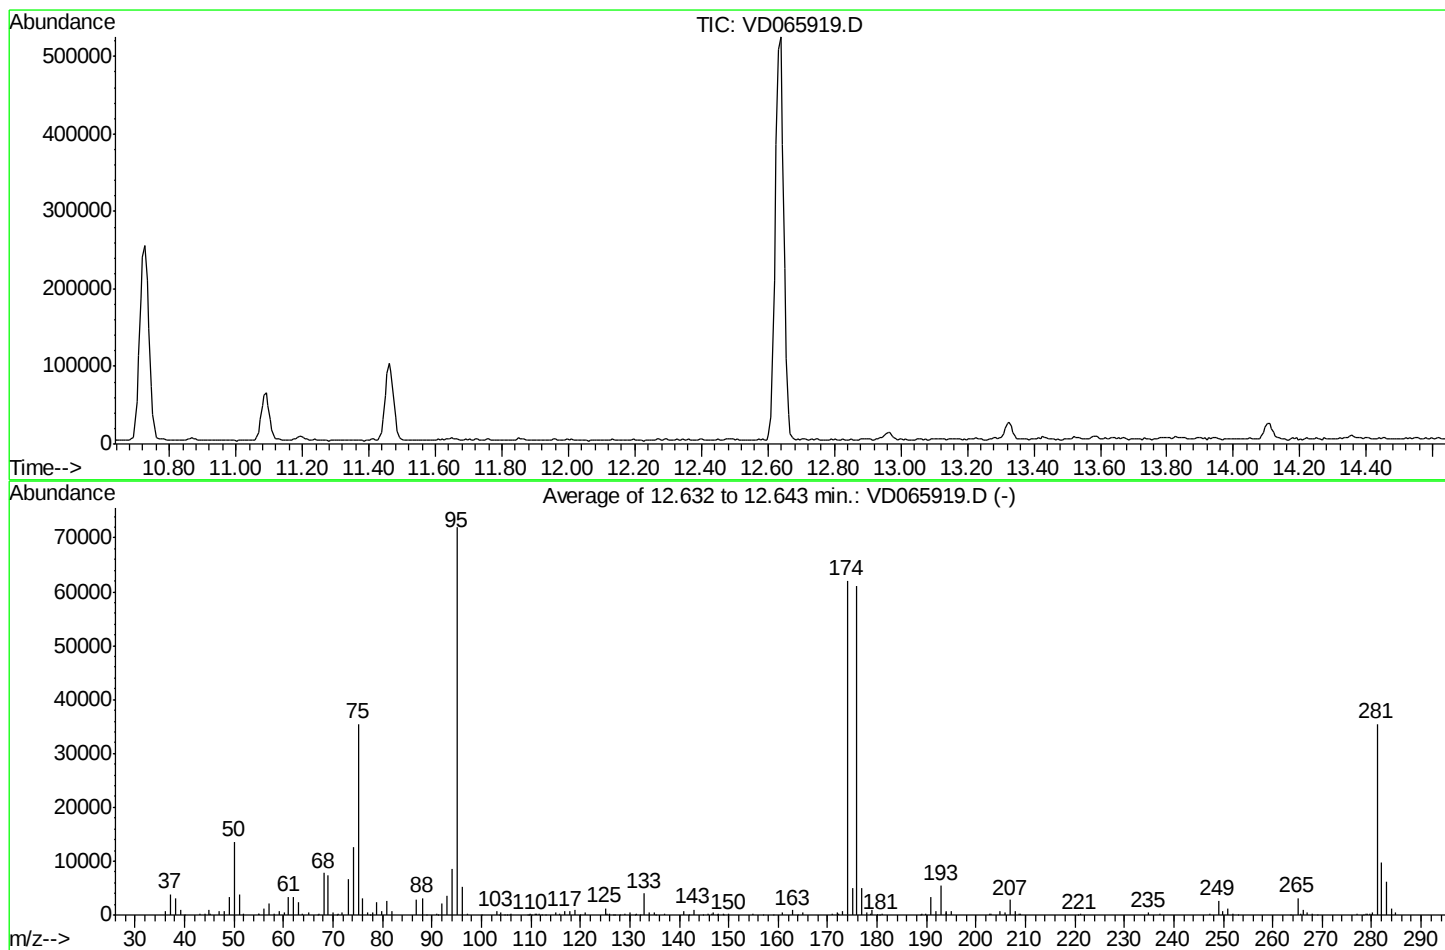

AutoFind: Scans 1821, 1822, 1823; Background Corrected with Scan 1812

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.9	13605	PASS
75	95	30	60	49.3	35480	PASS
95	95	100	100	100.0	71970	PASS
96	95	5	9	7.3	5284	PASS
173	174	0.00	2	1.2	716	PASS
174	95	50	100	86.3	62128	PASS
175	174	5	9	8.0	4974	PASS
176	174	95	101	98.4	61109	PASS
177	176	5	9	8.3	5047	PASS