


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD070721\
 Data File : VD069601.D
 Acq On : 07 Jul 2021 09:51
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D0621215.M
 Title : SW846 8260
 Last Update : Tue Jun 22 04:33:24 2021

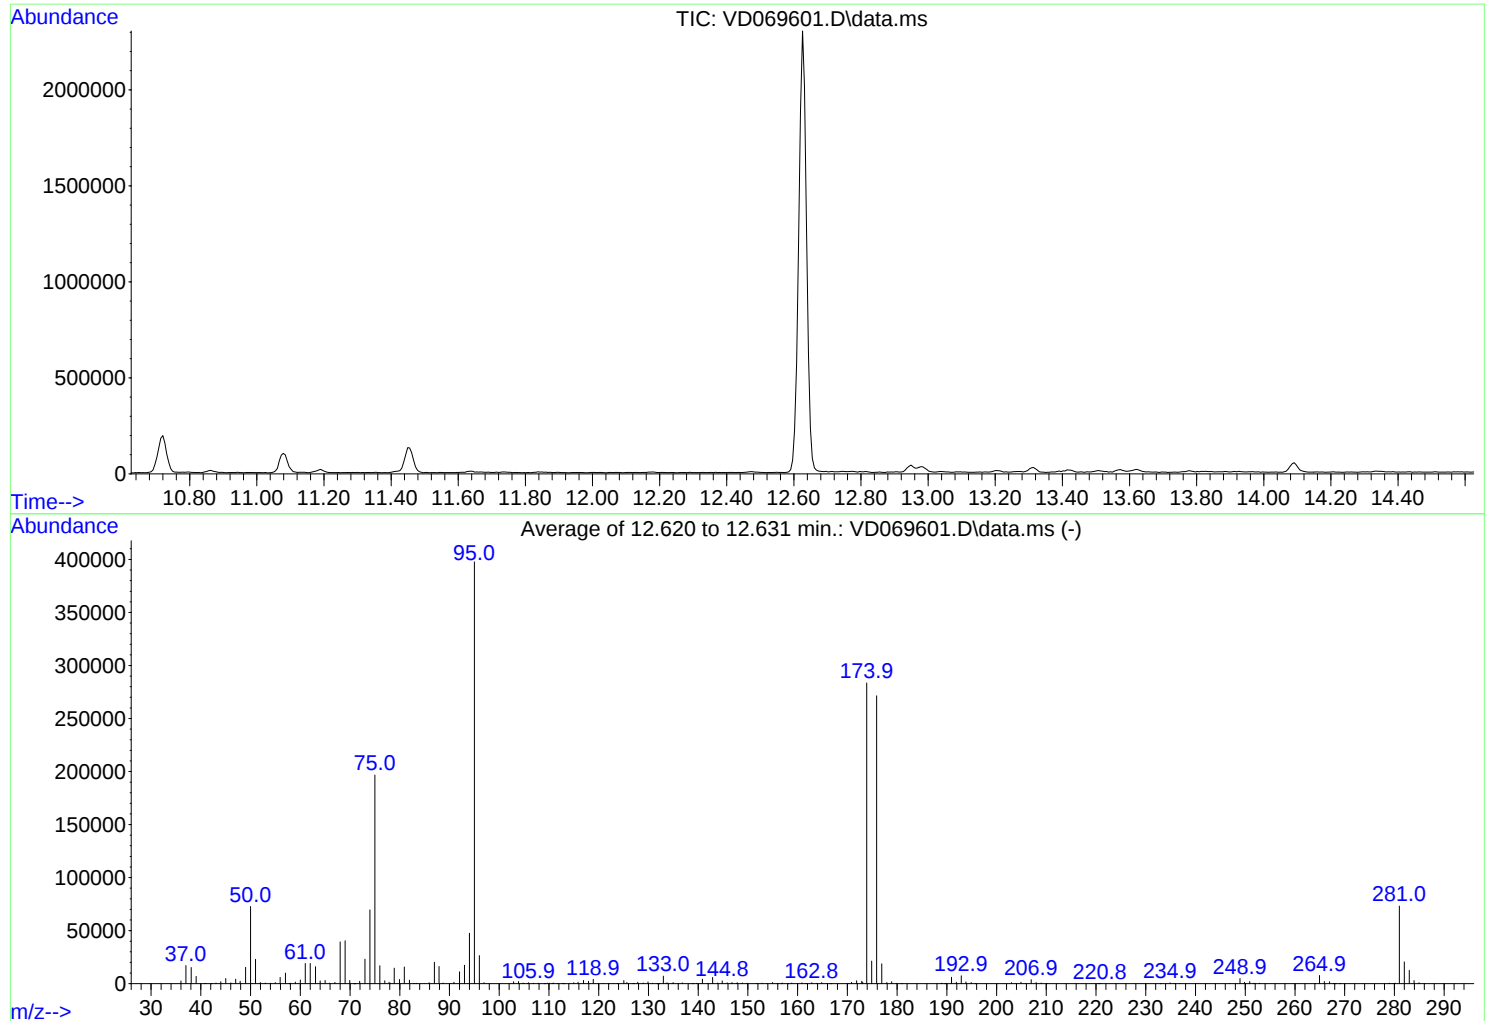

AutoFind: Scans 1819, 1820, 1821; Background Corrected with Scan 1809

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.3	72677	PASS
75	95	30	60	49.5	196757	PASS
95	95	100	100	100.0	397717	PASS
96	95	5	9	6.6	26376	PASS
173	174	0.00	2	0.8	2271	PASS
174	95	50	100	71.3	283499	PASS
175	174	5	9	7.5	21299	PASS
176	174	95	101	95.7	271445	PASS
177	176	5	9	6.9	18641	PASS