
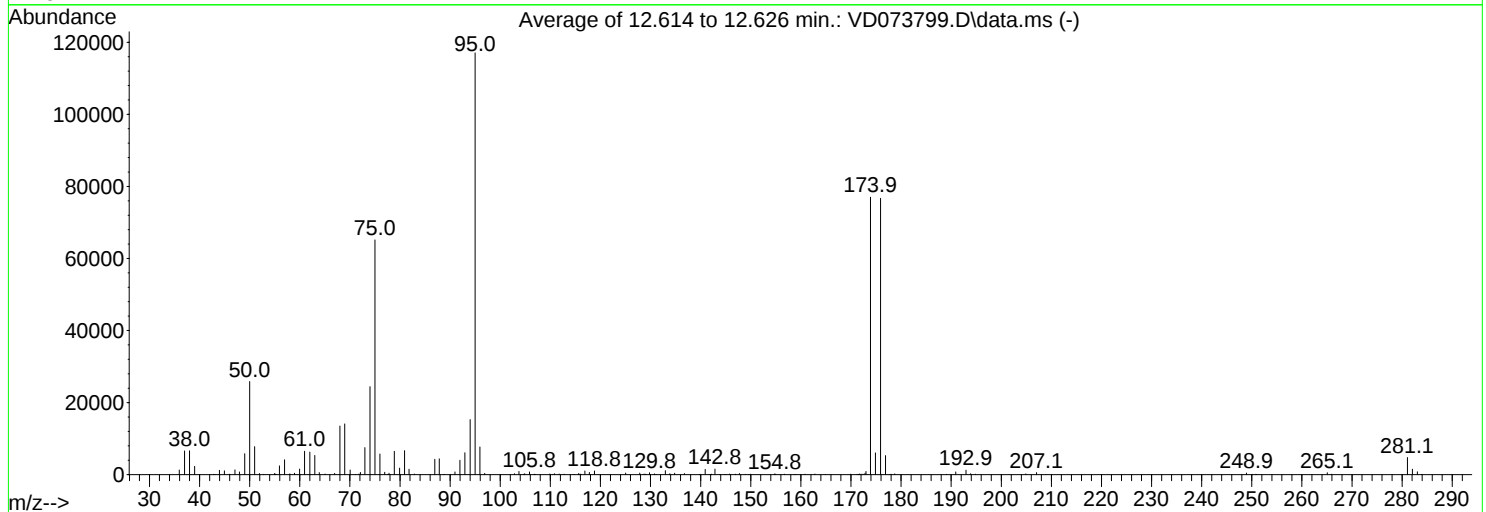


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD070722\
Data File : VD073799.D
Acq On : 07 Jul 2022 09:07
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D070622S.M
Title : SW846 8260
Last Update : Fri Jul 08 05:39:57 2022

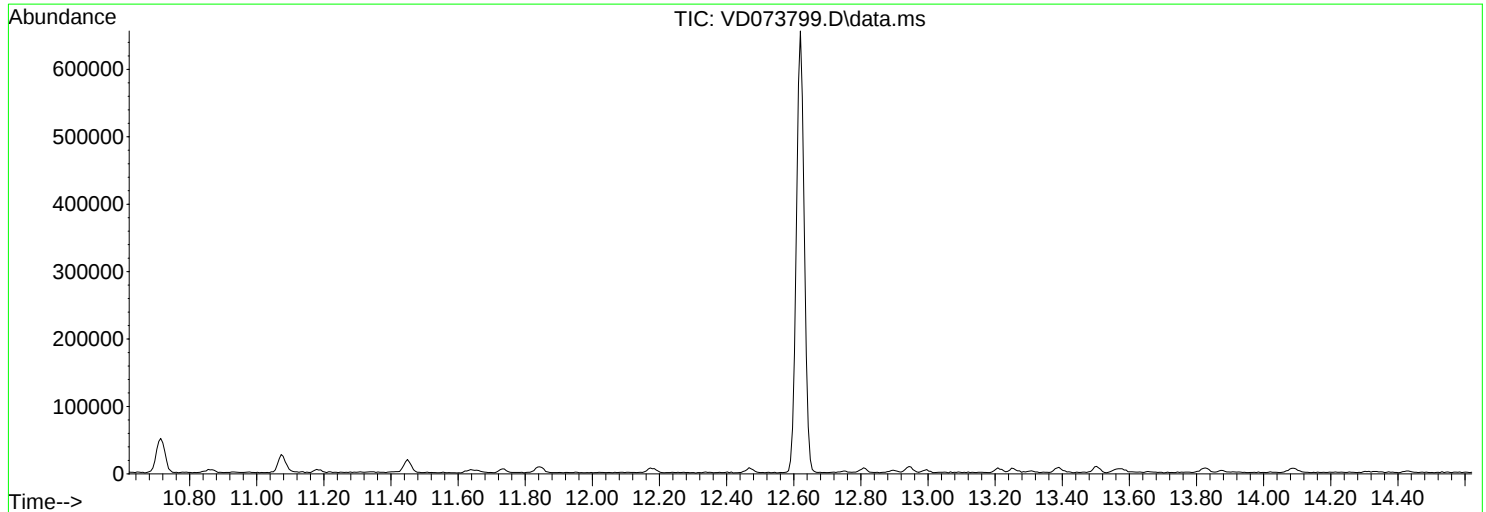

AutoFind: Scans 1818, 1819, 1820; Background Corrected with Scan 1809

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	22.1	25837	PASS
75	95	30	60	55.7	65171	PASS
95	95	100	100	100.0	117072	PASS
96	95	5	9	6.6	7696	PASS
173	174	0.00	2	1.2	896	PASS
174	95	50	100	65.8	77029	PASS
175	174	5	9	7.8	6042	PASS
176	174	95	101	99.6	76704	PASS
177	176	5	9	6.9	5288	PASS