


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD070820\
Data File : VD065934.D
Acq On : 08 Jul 2020 09:48
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D070720S.M
Title : SW846 8260
Last Update : Wed Jul 08 09:45:47 2020

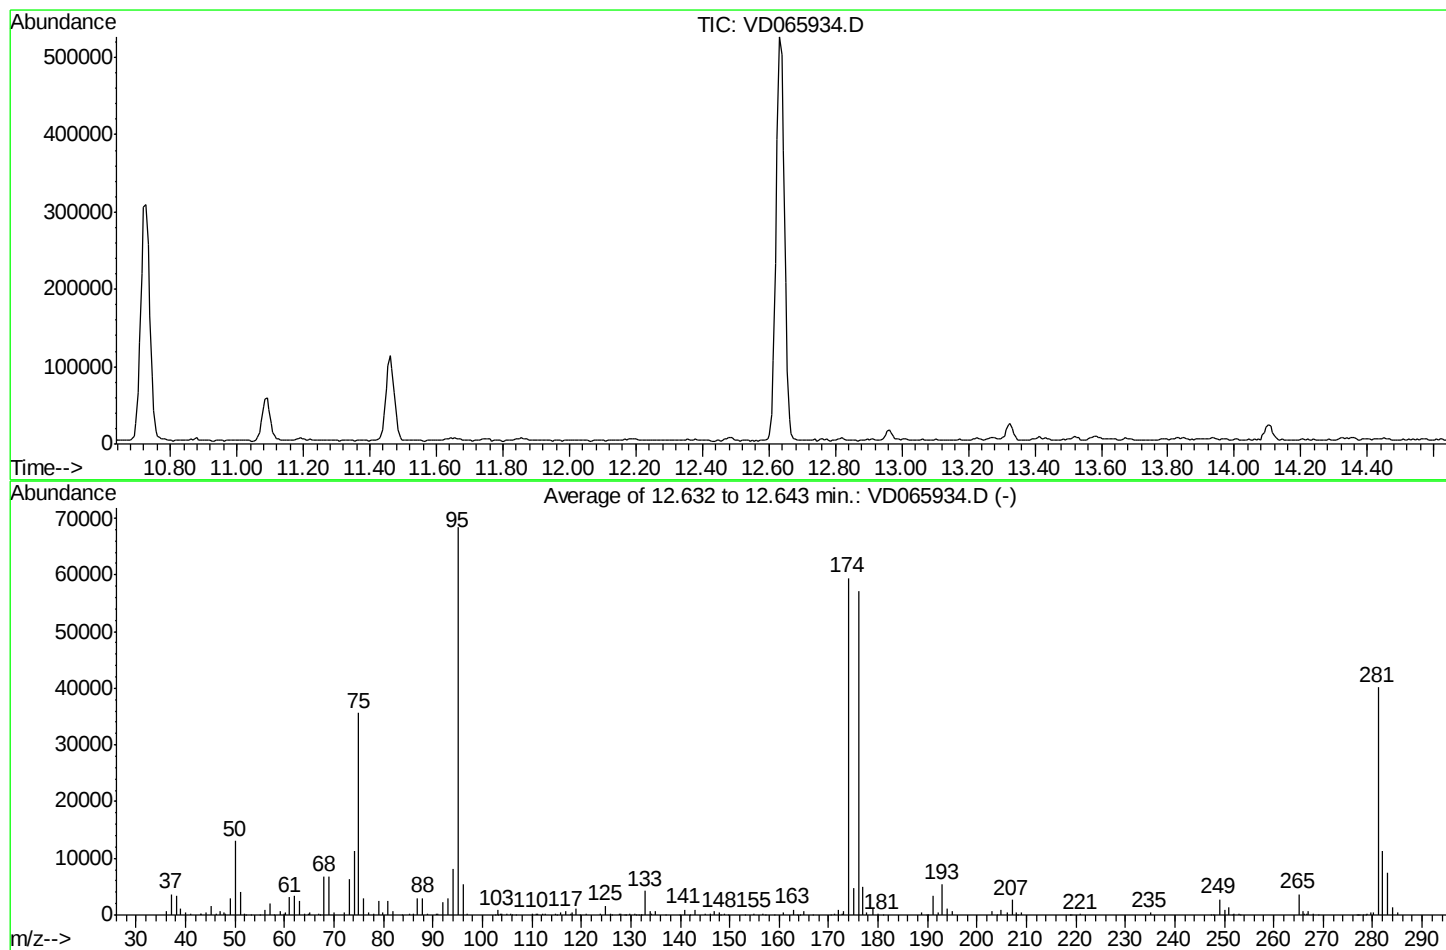

AutoFind: Scans 1821, 1822, 1823; Background Corrected with Scan 1812

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.1	13074	PASS
75	95	30	60	52.1	35594	PASS
95	95	100	100	100.0	68378	PASS
96	95	5	9	7.9	5397	PASS
173	174	0.00	2	1.1	635	PASS
174	95	50	100	87.0	59474	PASS
175	174	5	9	8.1	4804	PASS
176	174	95	101	96.1	57136	PASS
177	176	5	9	8.7	4976	PASS