
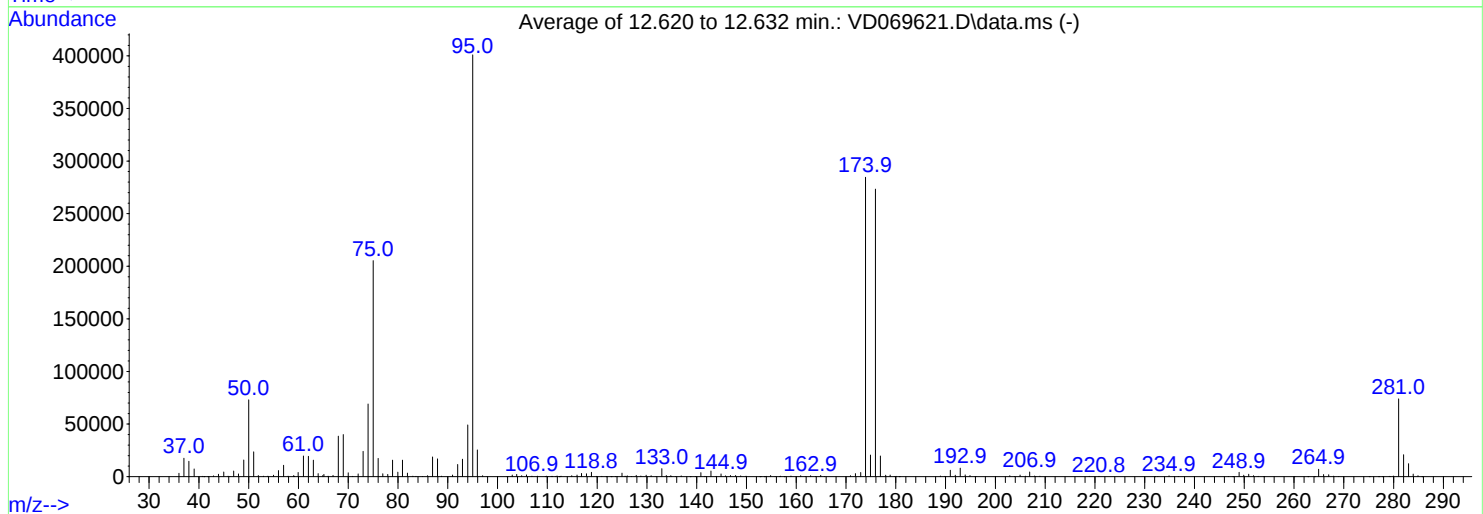


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD070821\
Data File : VD069621.D
Acq On : 08 Jul 2021 10:04
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D062121S.M
Title : SW846 8260
Last Update : Tue Jun 22 04:33:24 2021

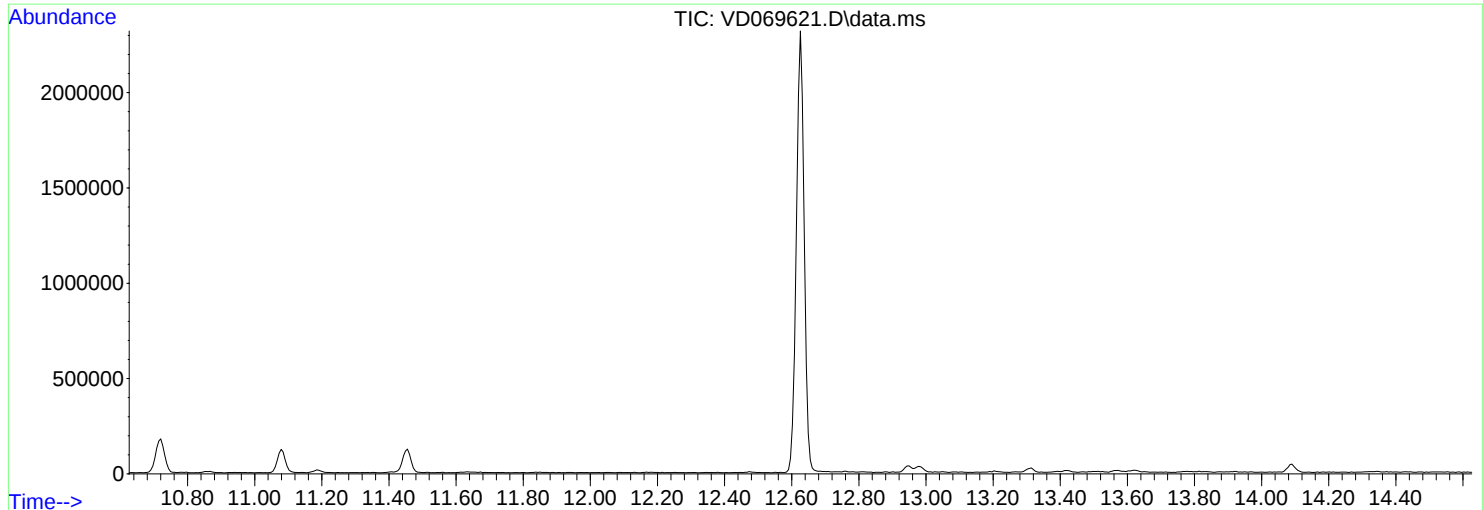

AutoFind: Scans 1819, 1820, 1821; Background Corrected with Scan 1810

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.2	73064	PASS
75	95	30	60	51.2	205333	PASS
95	95	100	100	100.0	400981	PASS
96	95	5	9	6.4	25487	PASS
173	174	0.00	2	1.4	3899	PASS
174	95	50	100	71.0	284587	PASS
175	174	5	9	7.2	20469	PASS
176	174	95	101	96.1	273365	PASS
177	176	5	9	7.2	19573	PASS