


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA D\DATA\VD071020\
Data File : VD065942.D
Acq On : 10 Jul 2020 09:34
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\V0ASRV\HPCHEM1\MSVOA_D\METHOD\82D070720S.M
Title : SW846 8260
Last Update : Wed Jul 08 09:45:47 2020

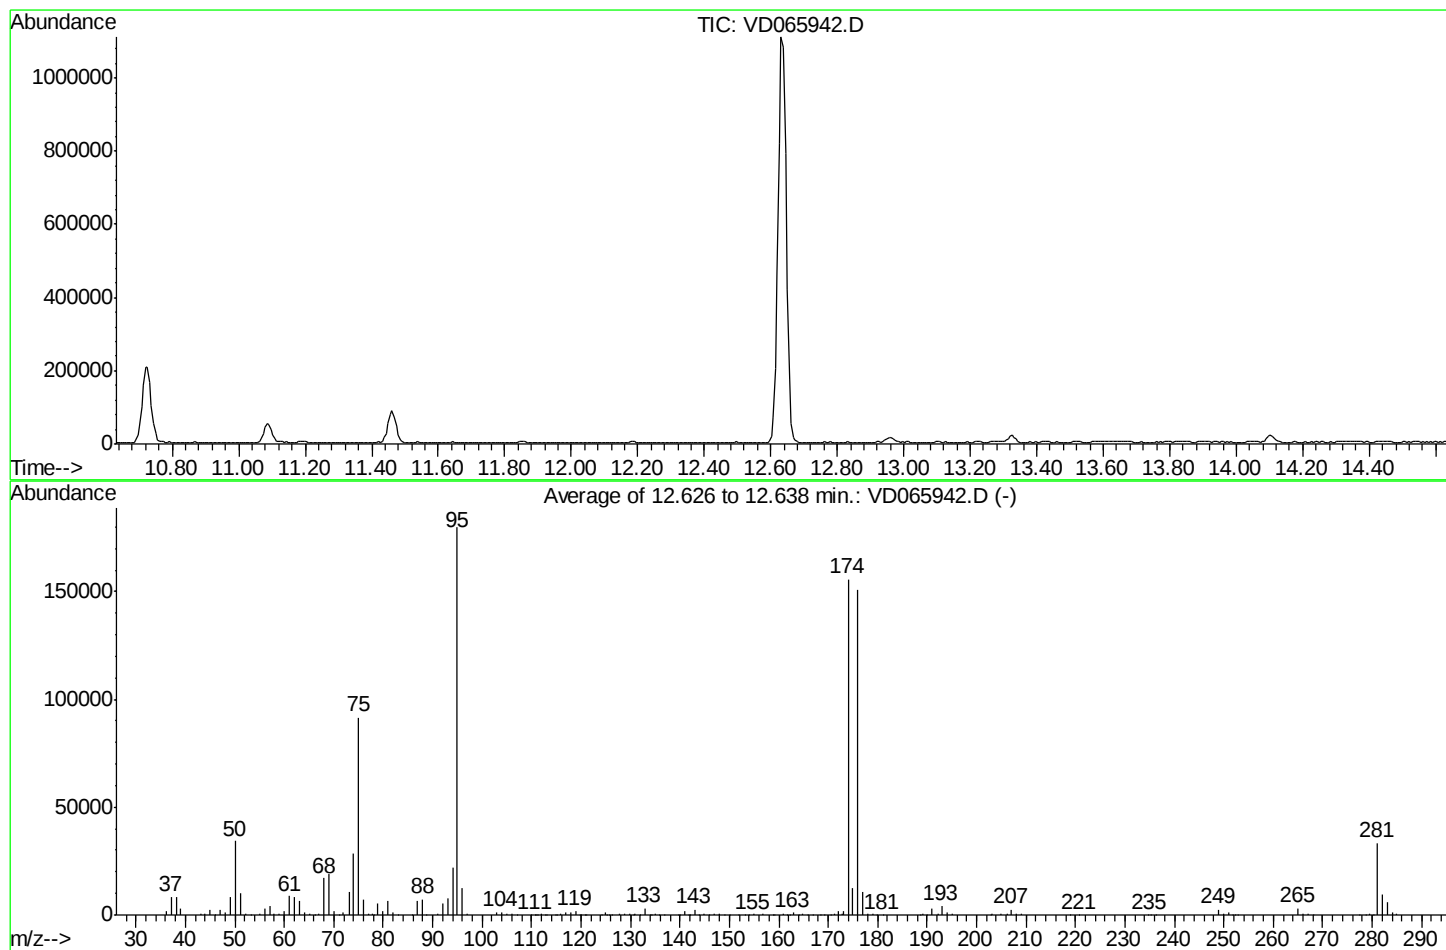

AutoFind: Scans 1820, 1821, 1822; Background Corrected with Scan 1812

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.0	34218	PASS
75	95	30	60	50.9	91501	PASS
95	95	100	100	100.0	179797	PASS
96	95	5	9	6.9	12452	PASS
173	174	0.00	2	1.2	1889	PASS
174	95	50	100	86.7	155840	PASS
175	174	5	9	8.1	12591	PASS
176	174	95	101	96.7	150746	PASS
177	176	5	9	7.0	10515	PASS