



Chloromethane

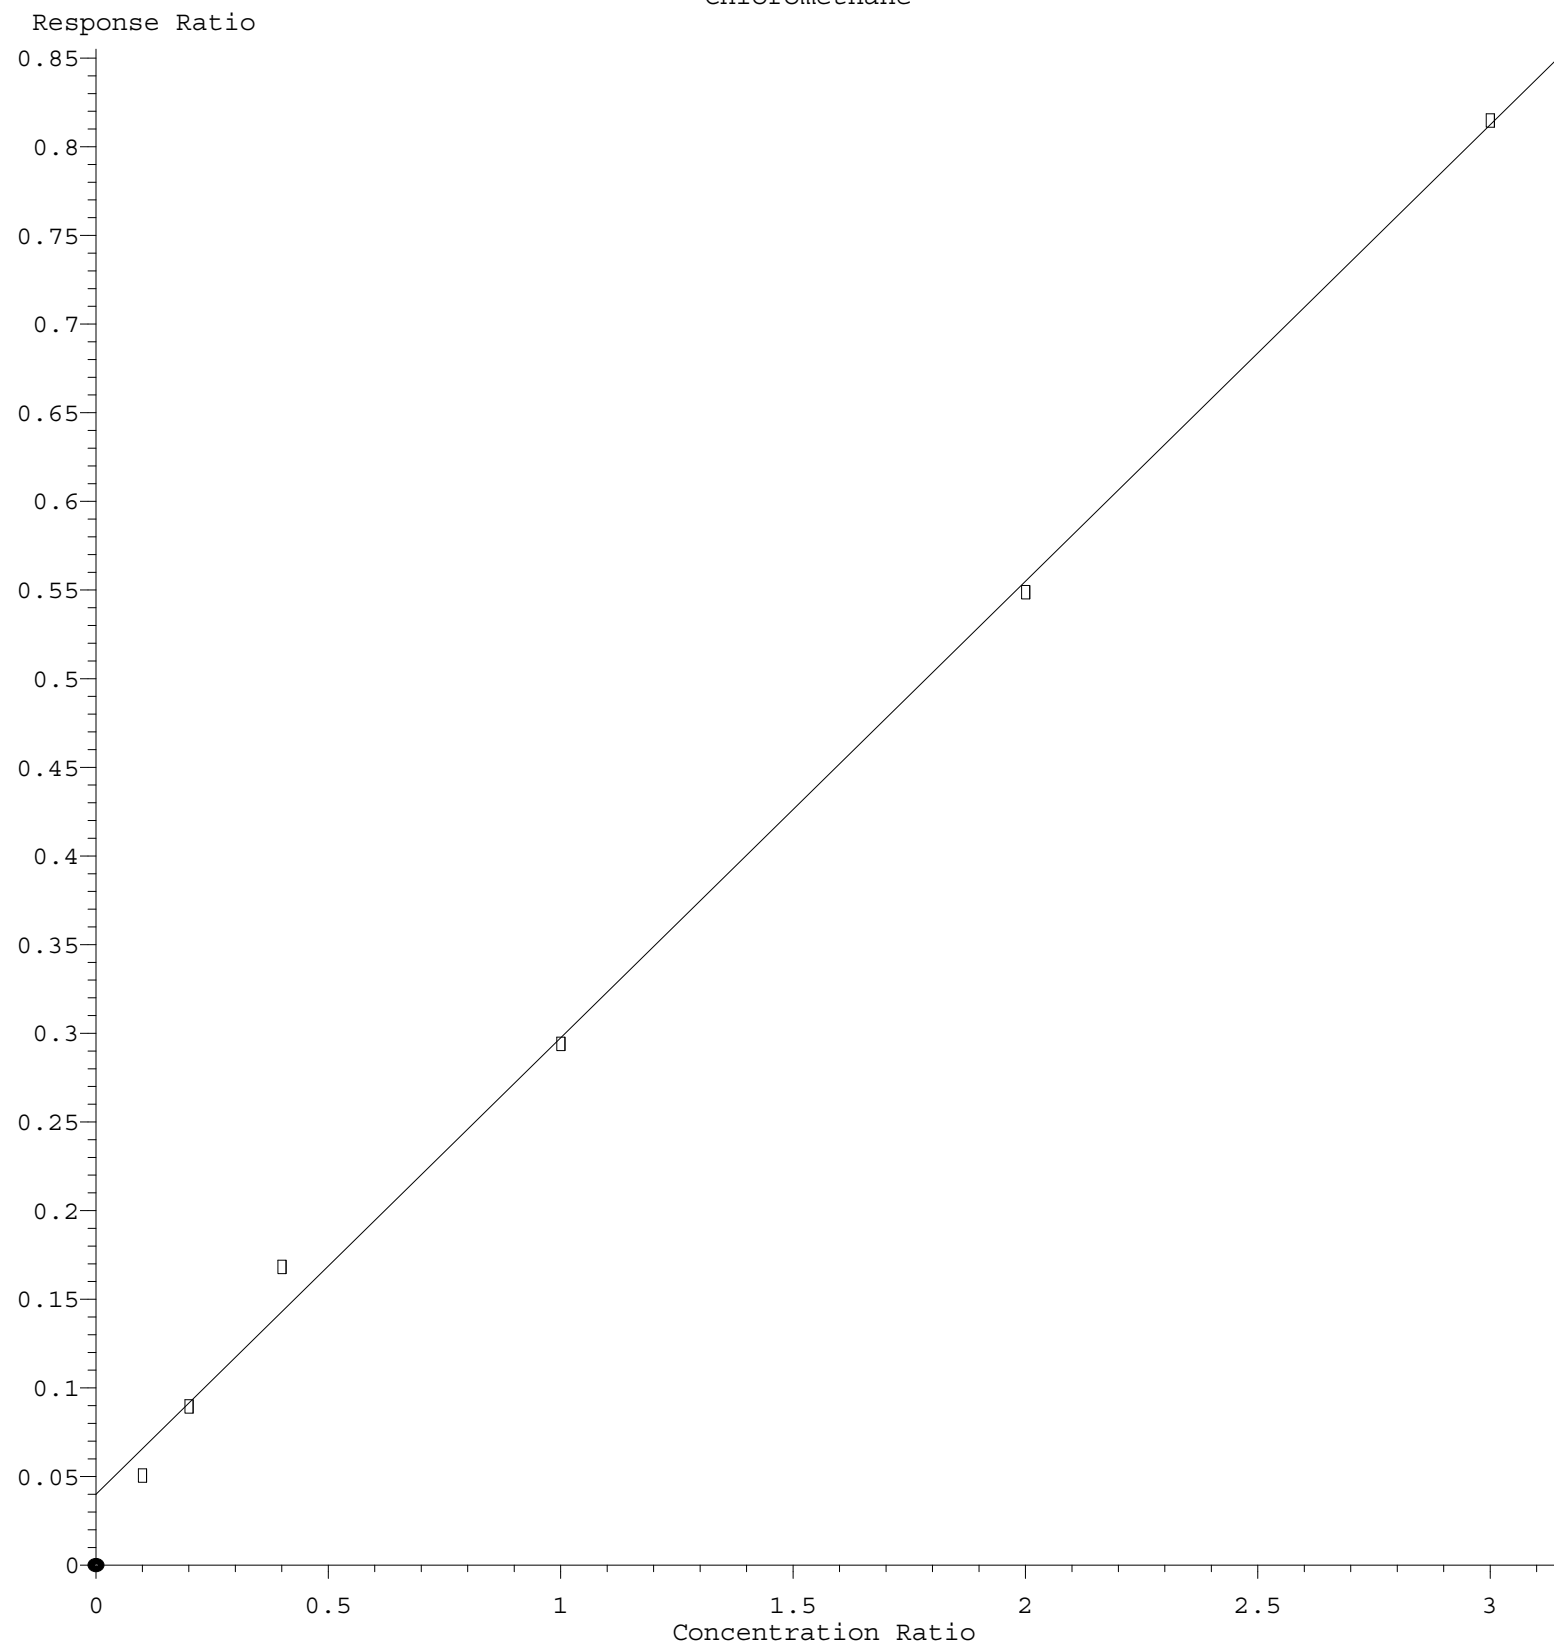

Response = 2.573e-001 * Amt + 4.034e-002
Coef of Det (r^2) = 0.997925 Curve Fit: Linear
Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D071122S.M
Calibration Table Last Updated: Tue Jul 12 07:04:44 2022

Cyclohexane

Response Ratio

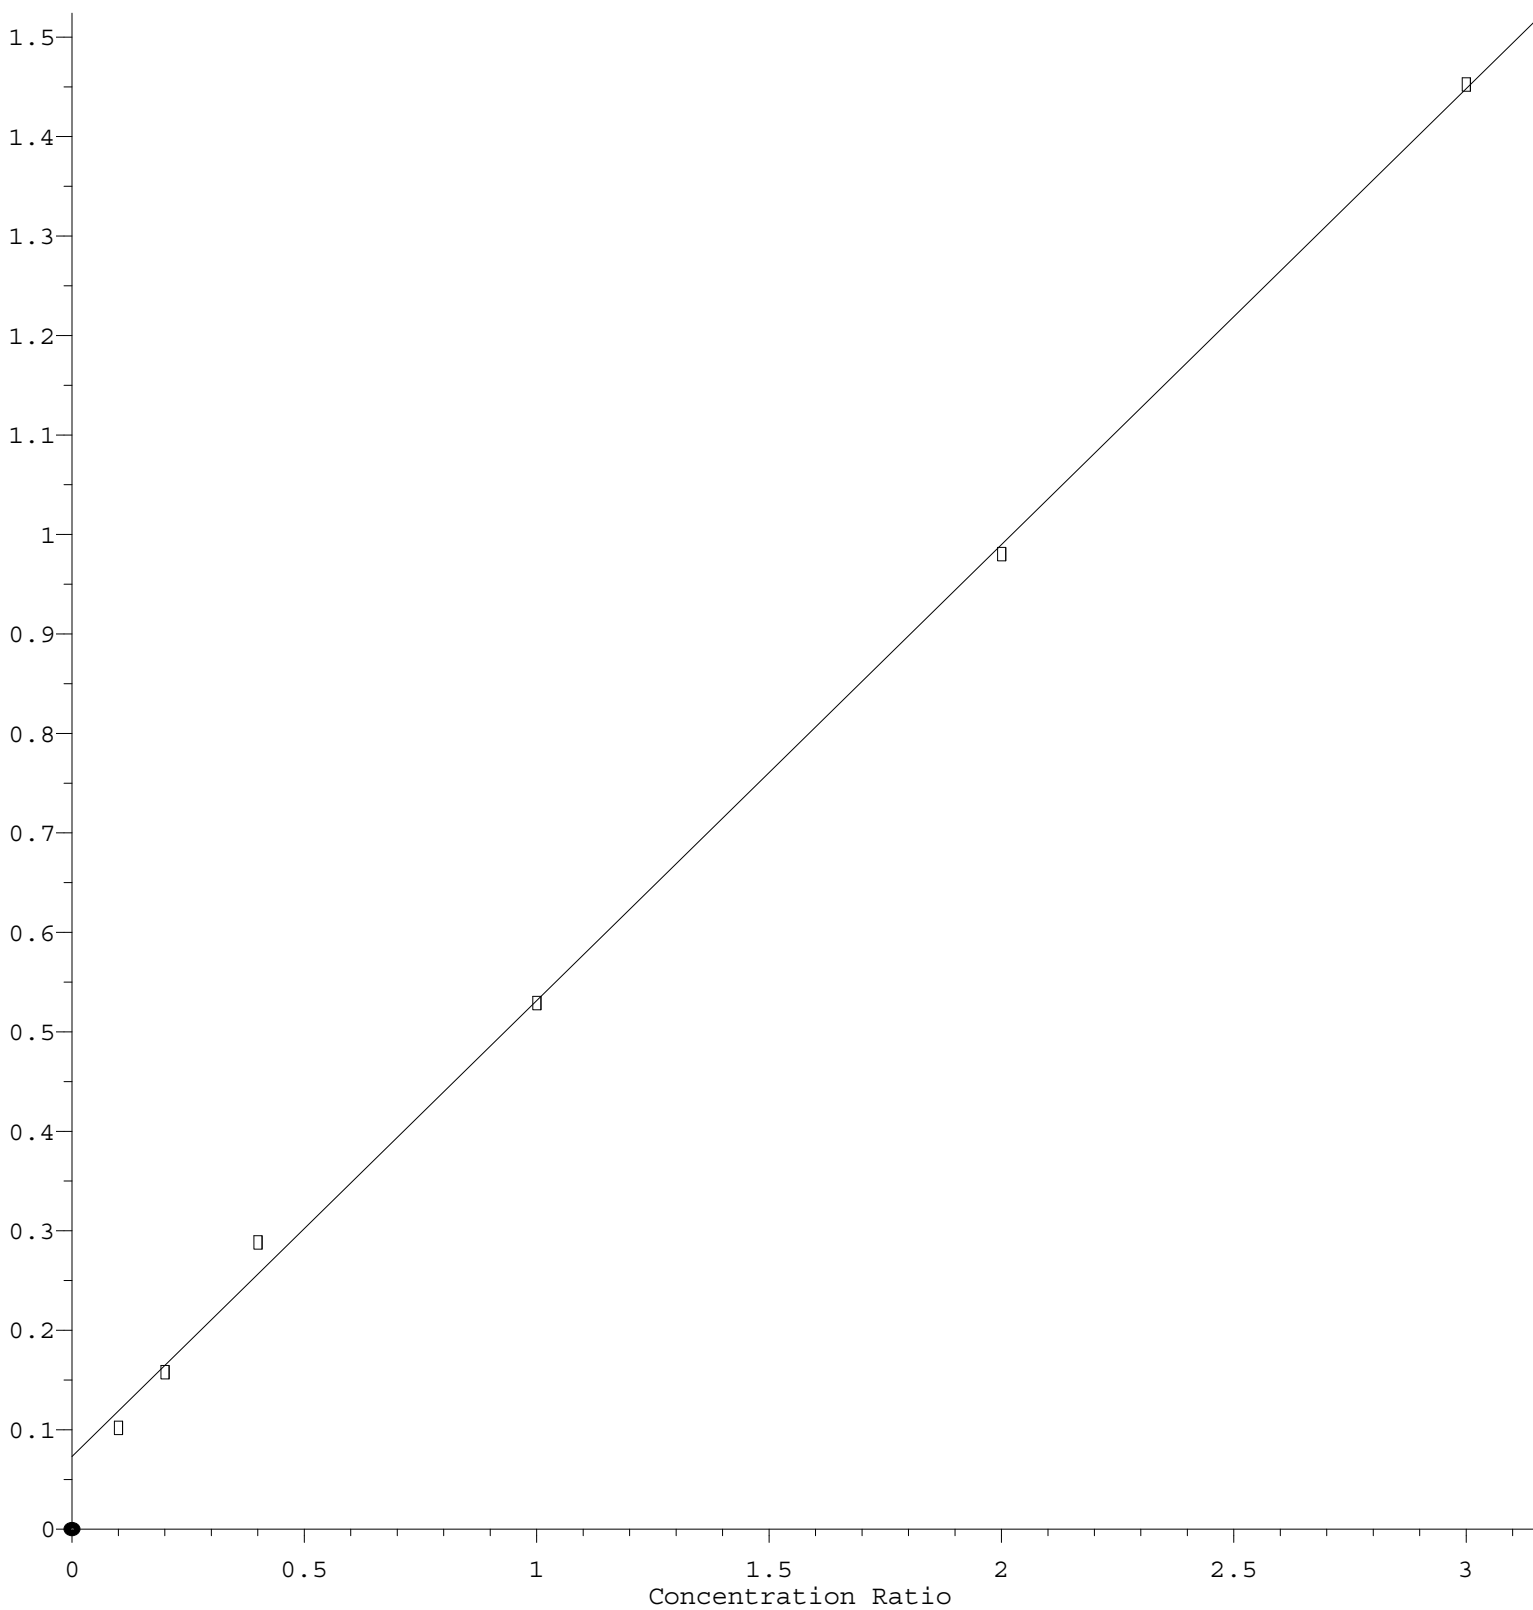

$$\text{Response} = 4.584\text{e-}001 * \text{Amt} + 7.294\text{e-}002$$


Coef of Det (r^2) = 0.998961 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D071122S.M

Calibration Table Last Updated: Tue Jul 12 07:04:44 2022

Methylene Chloride

Response Ratio

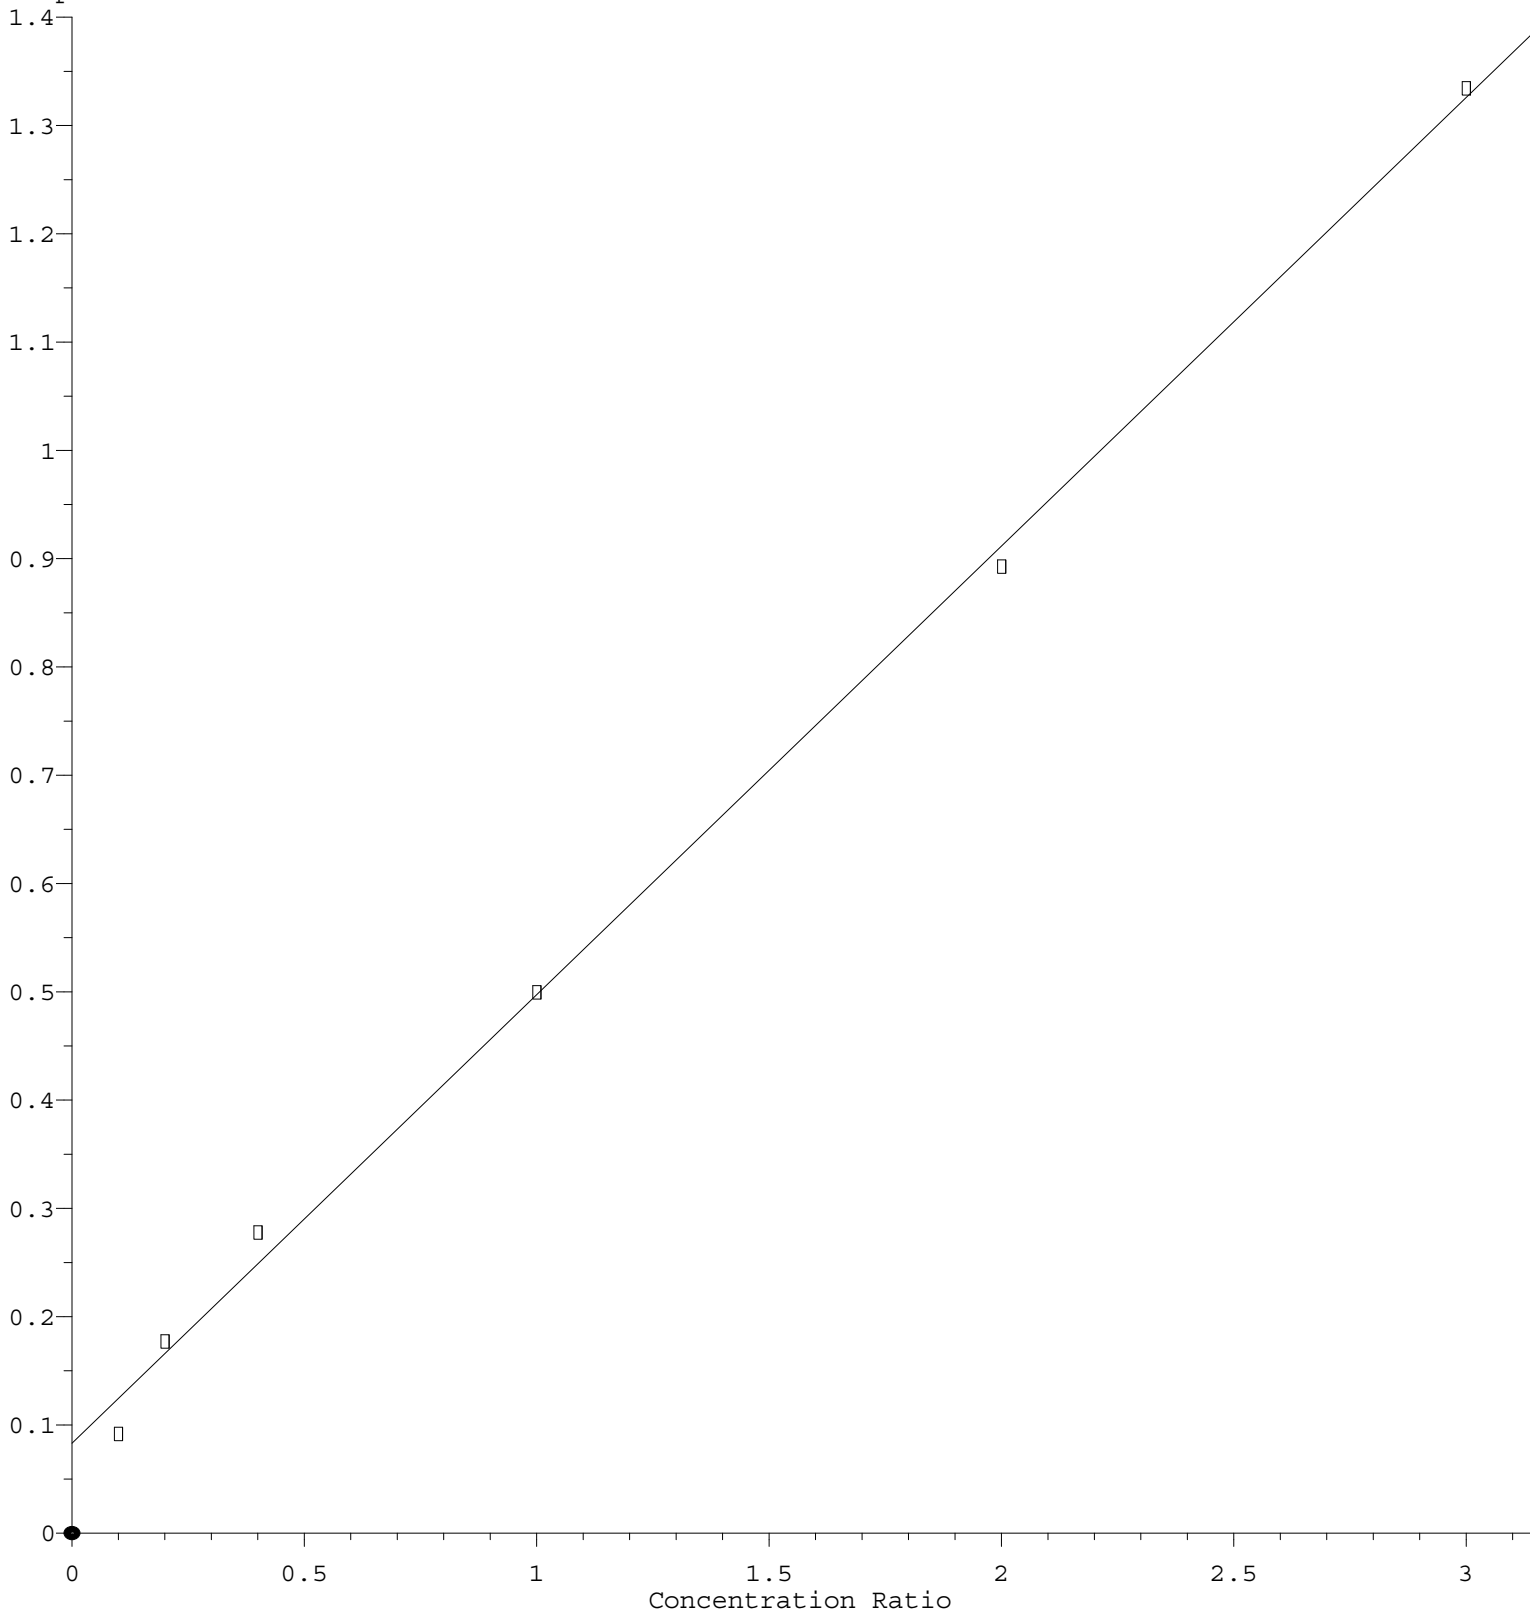


$$\text{Response} = 4.145\text{e-}001 * \text{Amt} + 8.257\text{e-}002$$

Coef of Det (r^2) = 0.997866 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D071122S.M

Calibration Table Last Updated: Tue Jul 12 07:04:44 2022


Methyl Acetate

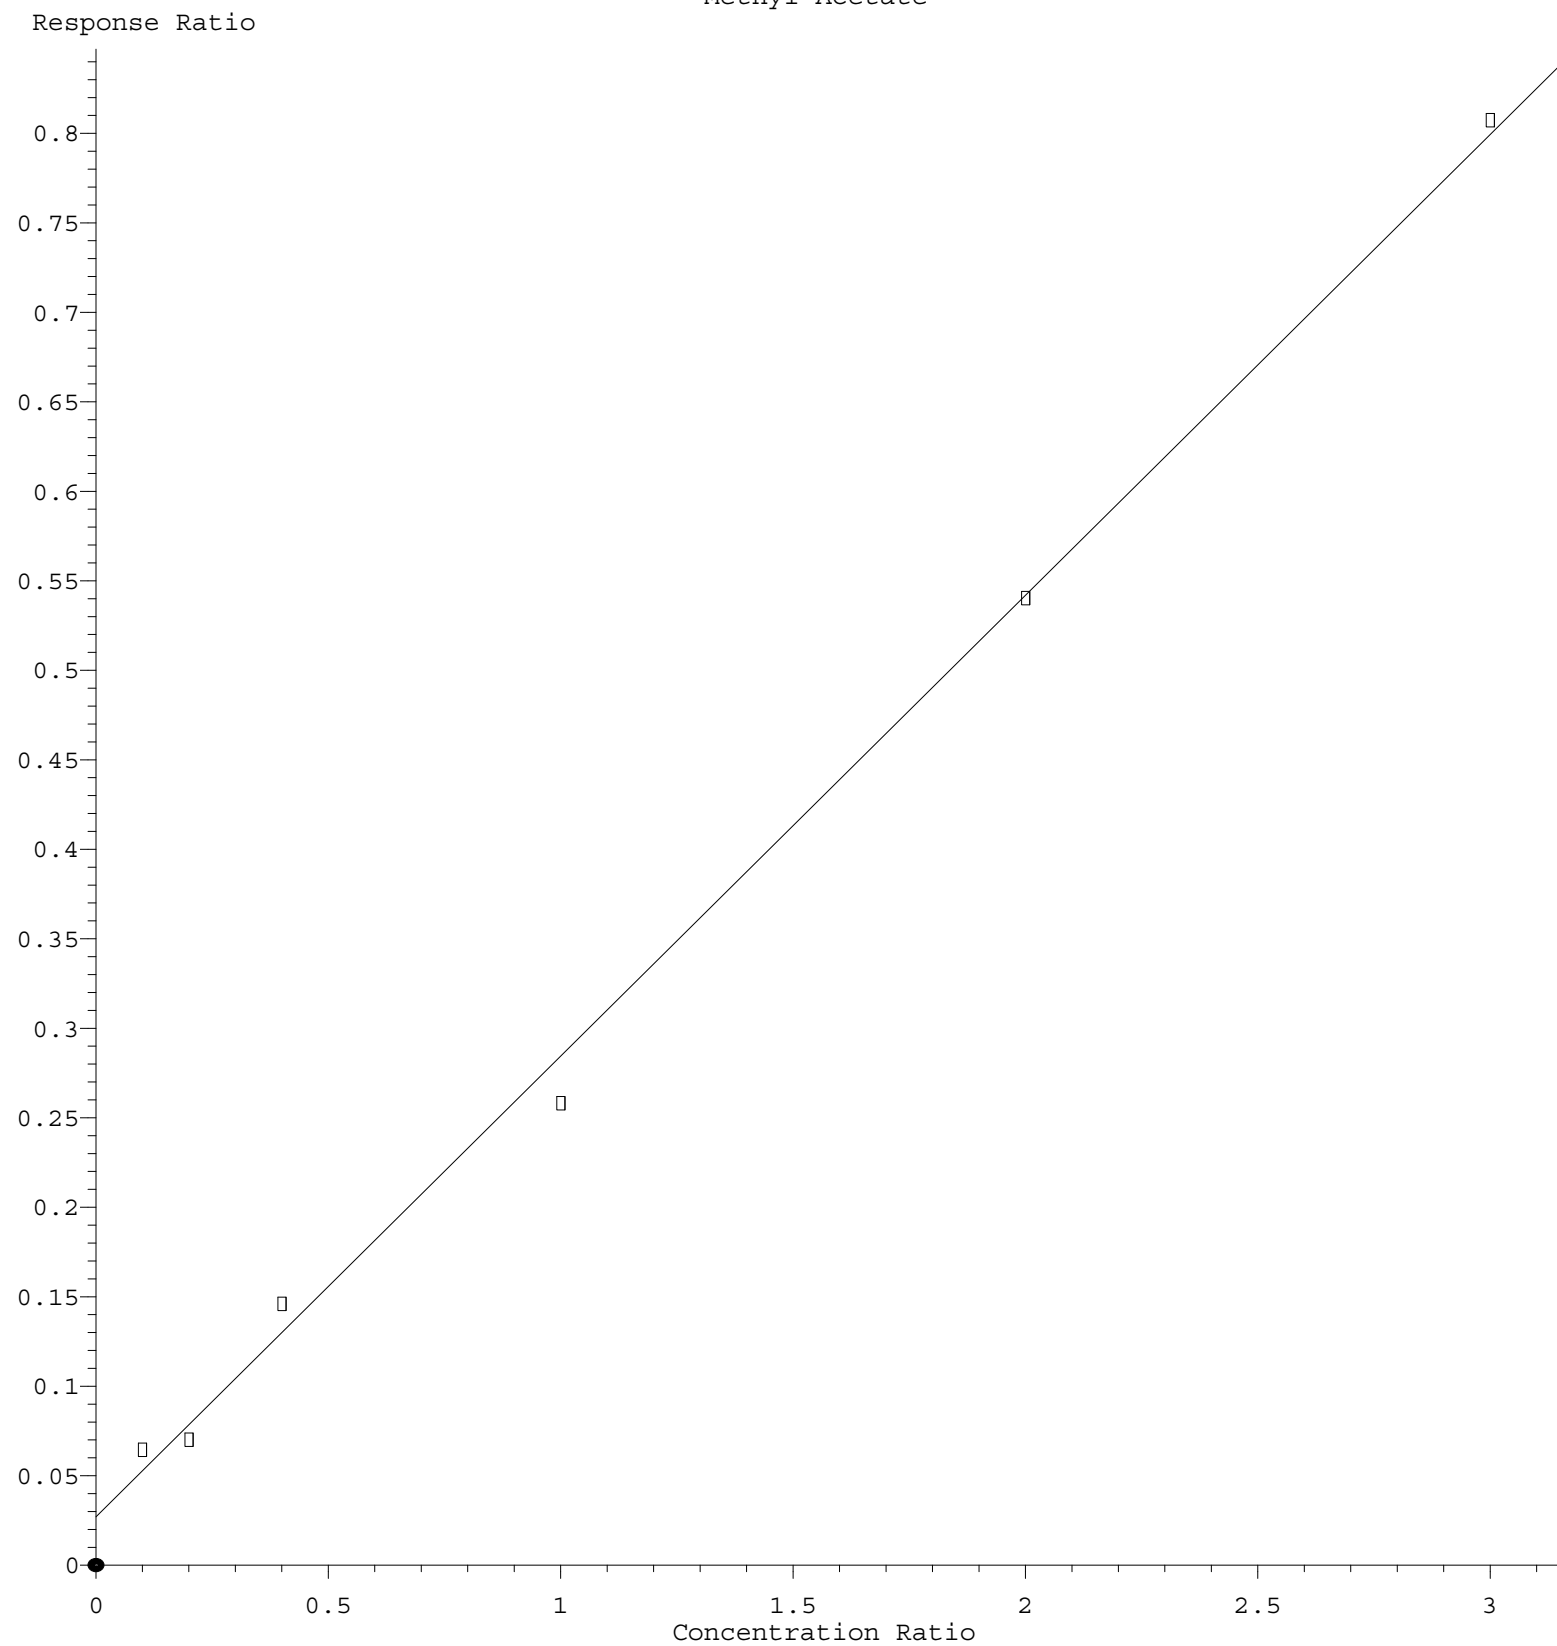

Response = 2.576e-001 * Amt + 2.673e-002
Coef of Det (r^2) = 0.997264 Curve Fit: Linear
Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D071122S.M
Calibration Table Last Updated: Tue Jul 12 07:04:44 2022

Carbon Disulfide

Response Ratio

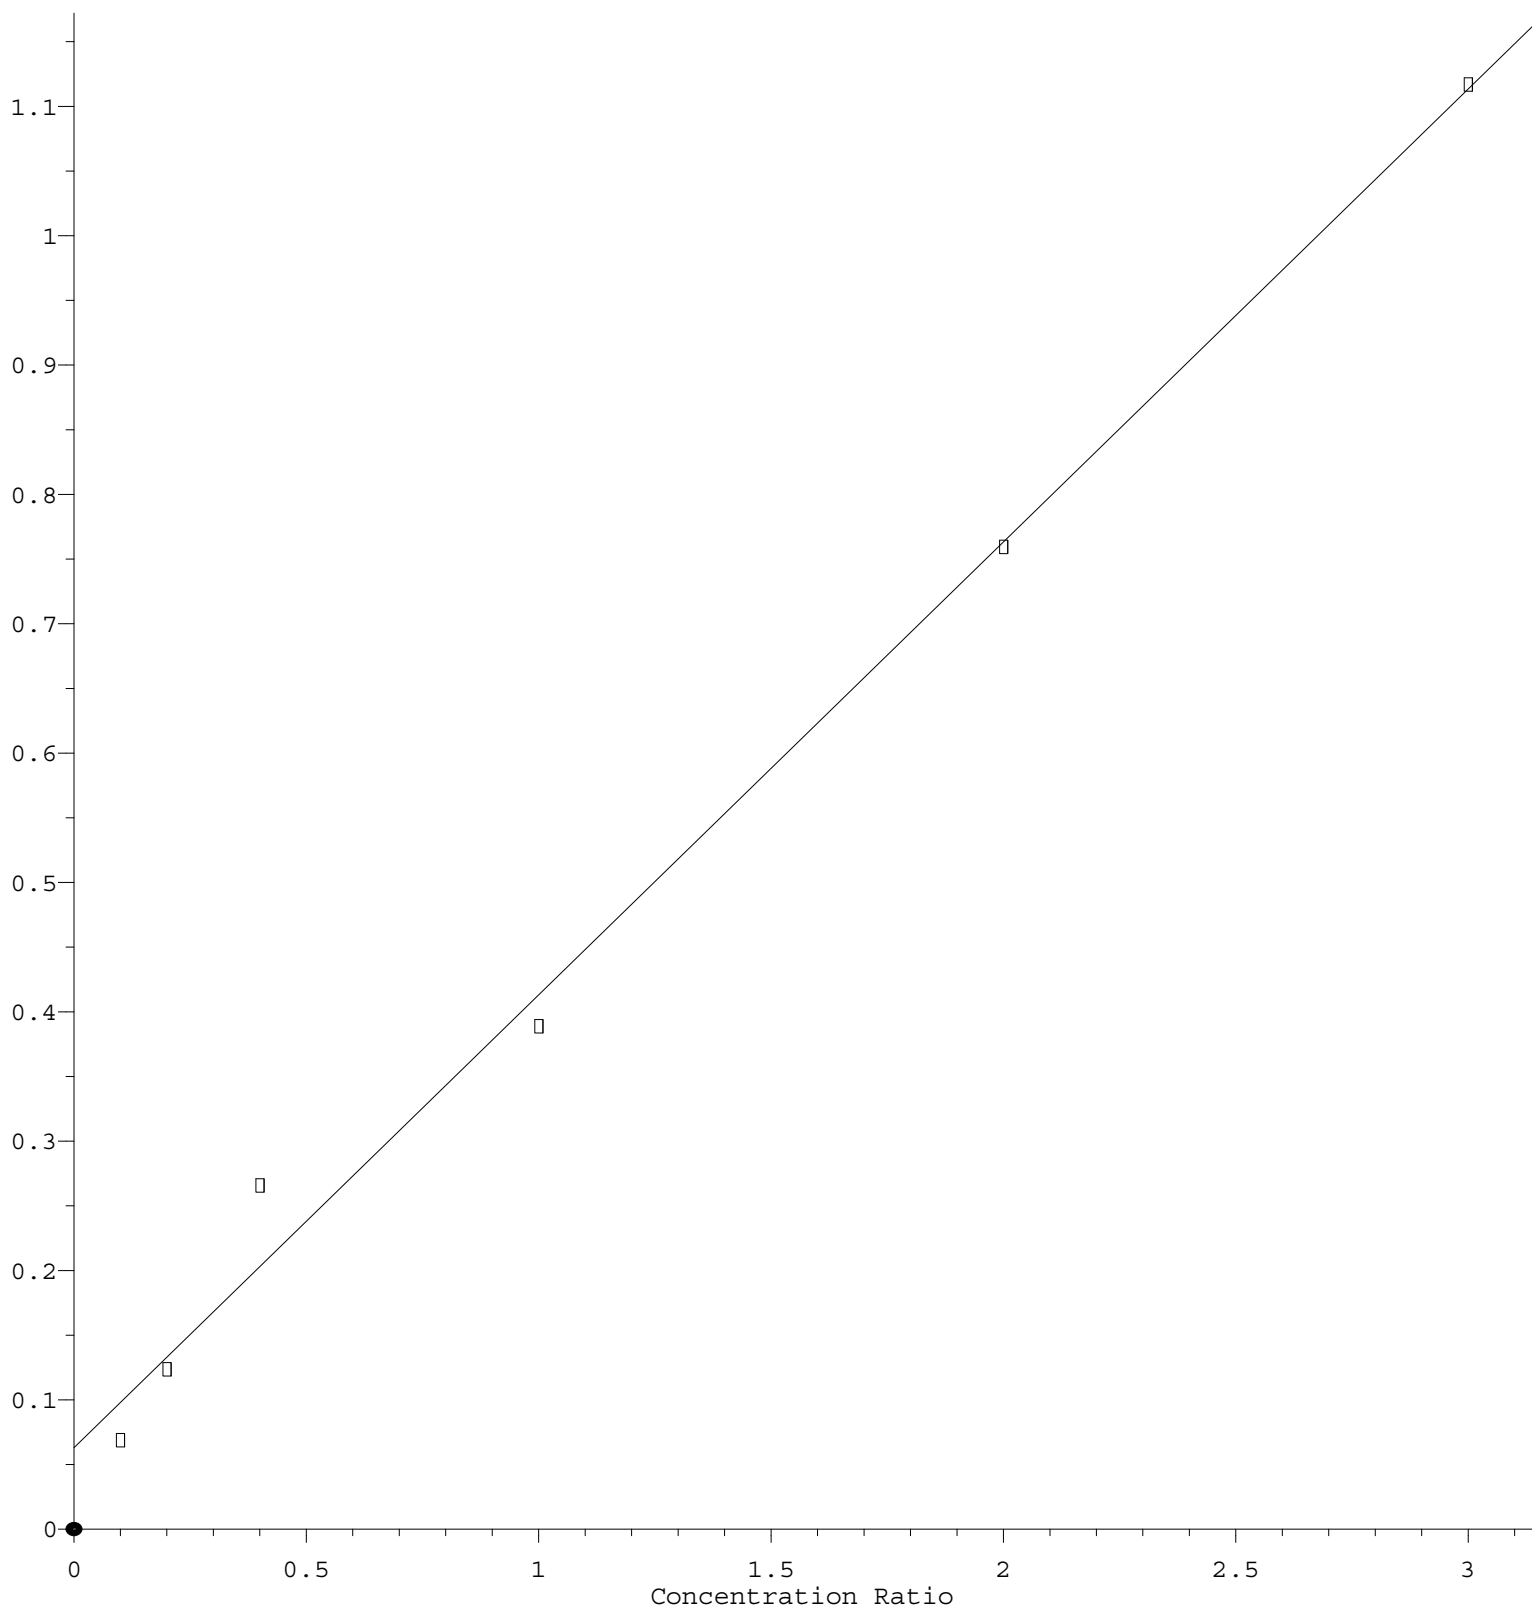


$$\text{Response} = 3.500\text{e-}001 * \text{Amt} + 6.297\text{e-}002$$

Coef of Det (r^2) = 0.993380 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D071122S.M


Calibration Table Last Updated: Tue Jul 12 07:04:44 2022

Acrolein

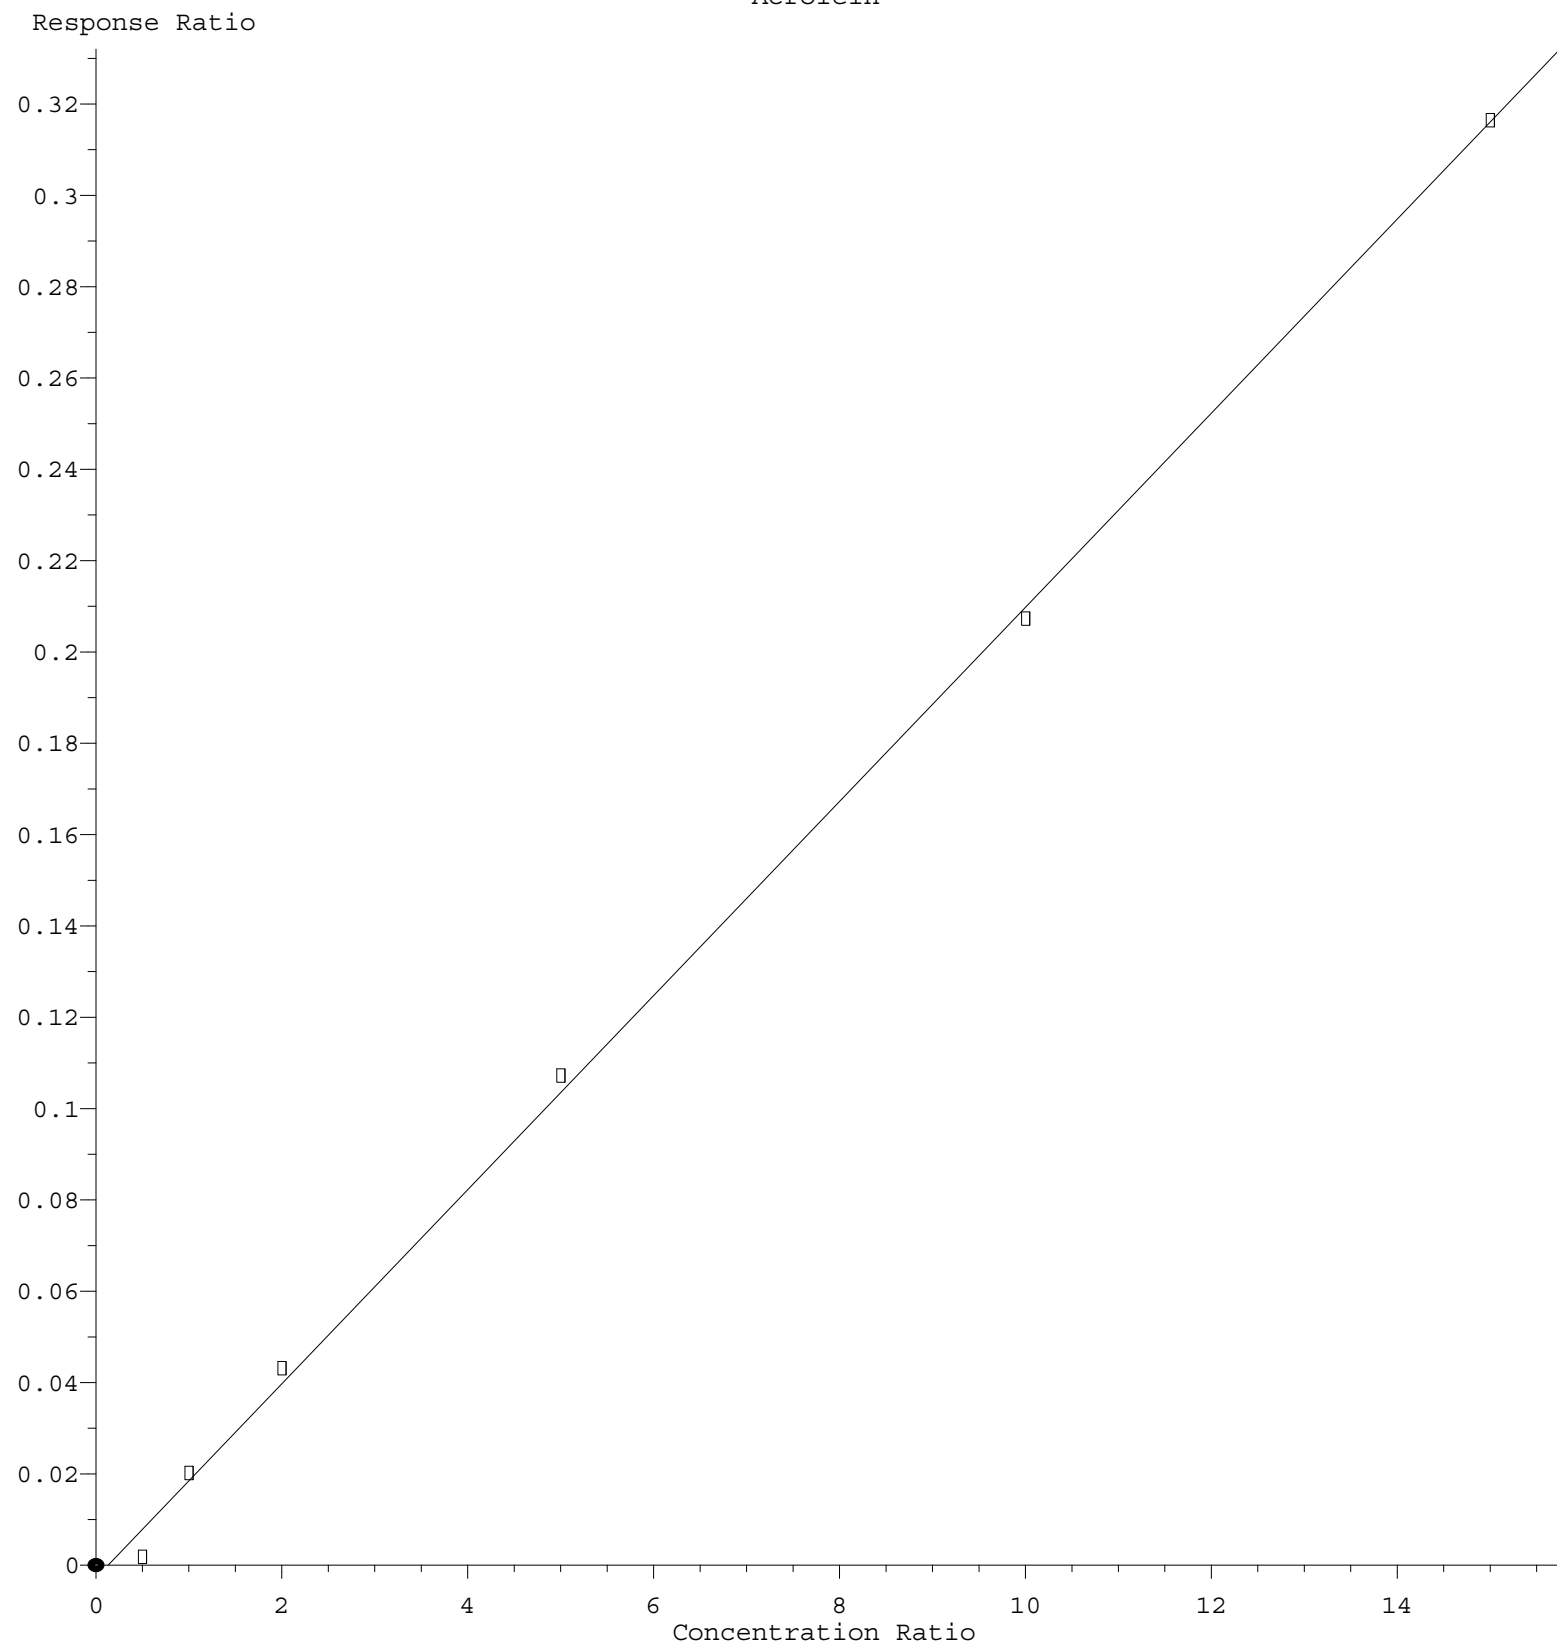

Response = $2.126 \times 10^{-2} \times \text{Amt} - 2.691 \times 10^{-3}$
 Coef of Det (r^2) = 0.999069 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D071122S.M
 Calibration Table Last Updated: Tue Jul 12 07:04:44 2022


Bromomethane

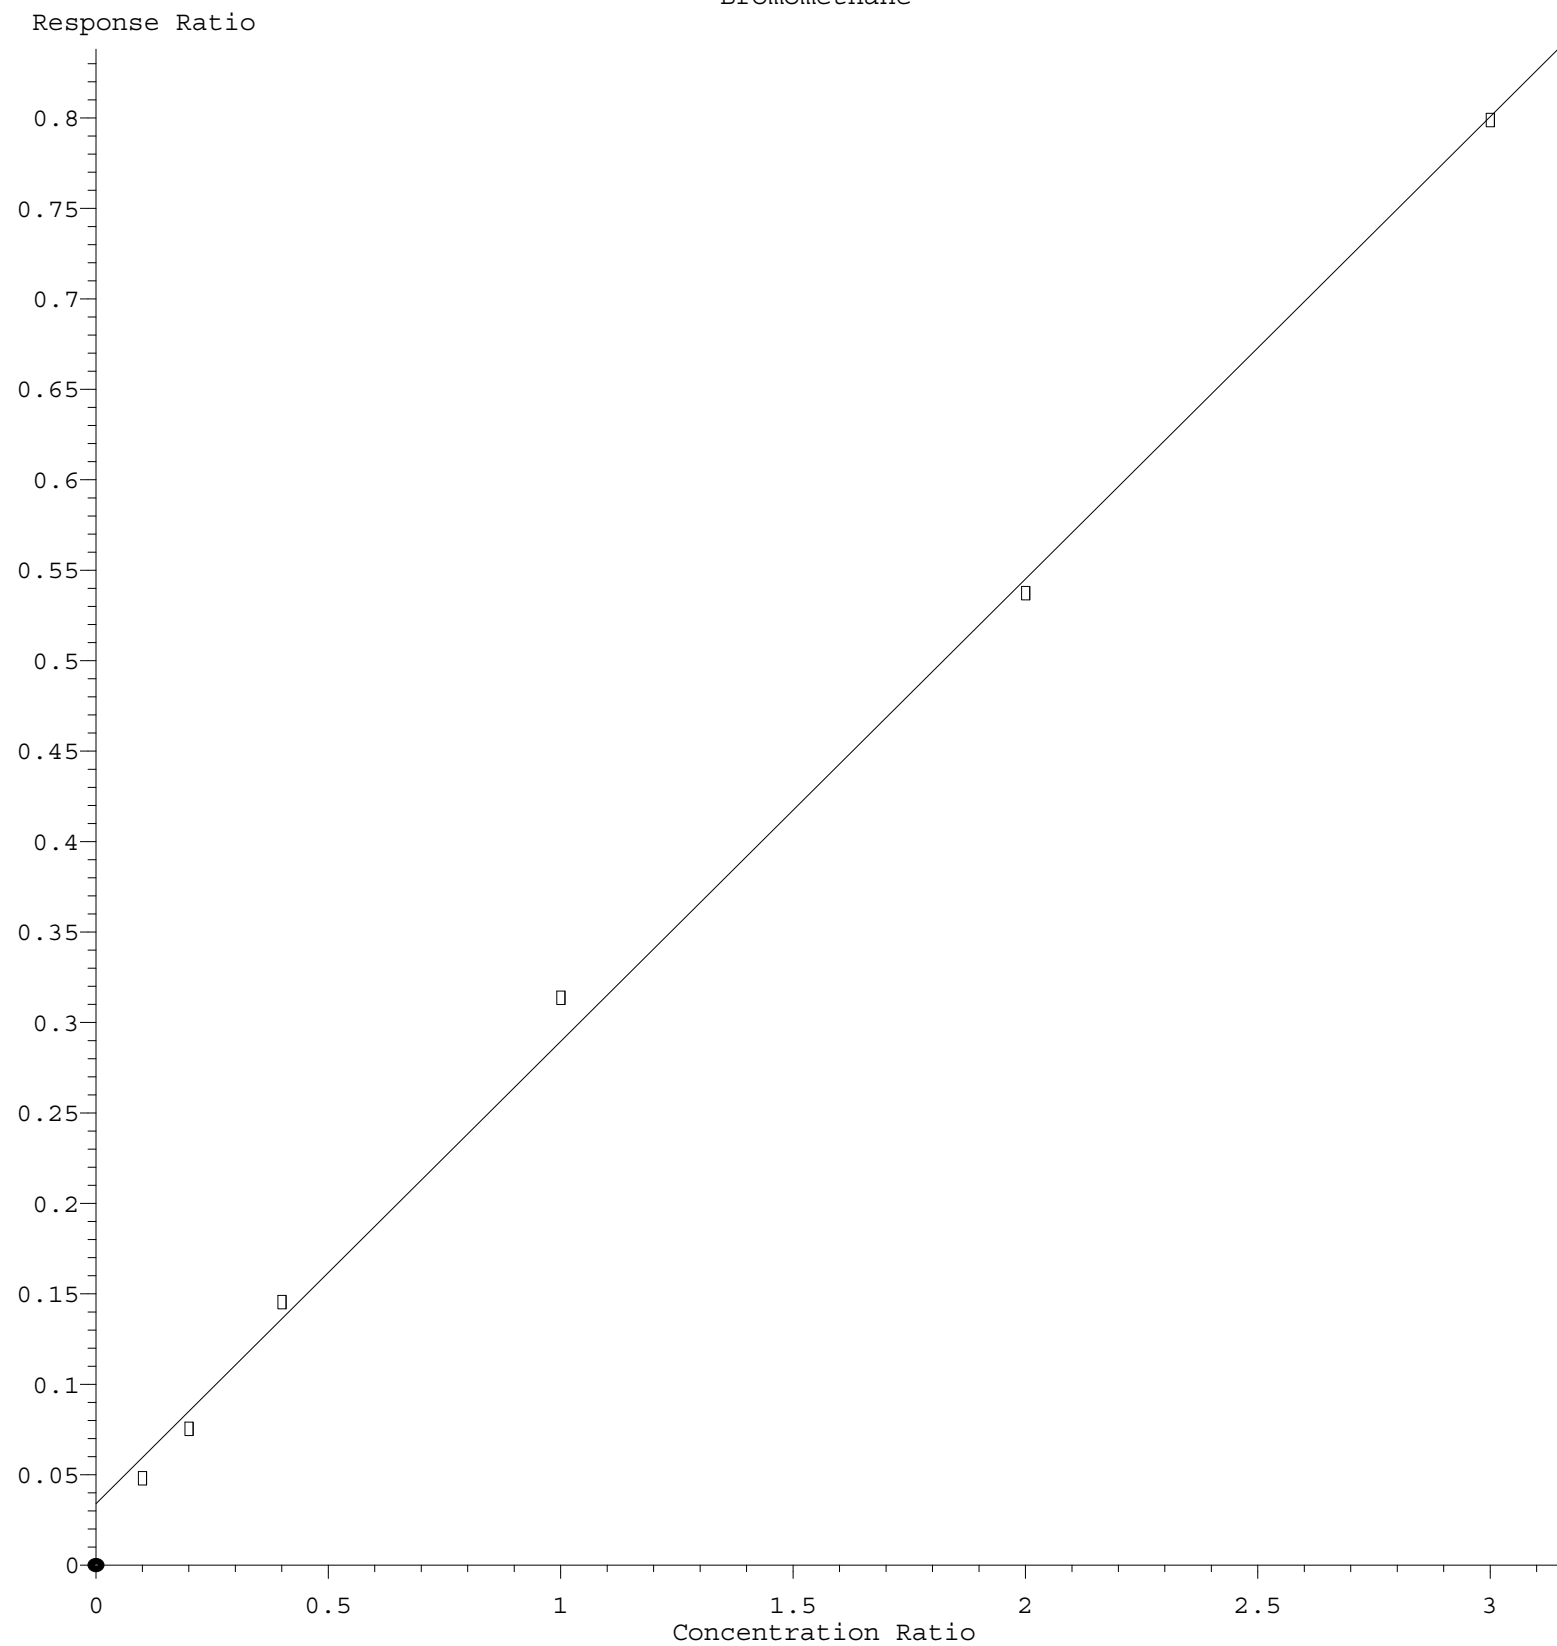

Response = 2.557e-001 * Amt + 3.423e-002
 Coef of Det (r^2) = 0.997830 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D071122S.M
 Calibration Table Last Updated: Tue Jul 12 07:04:44 2022

Vinyl Chloride

Response Ratio

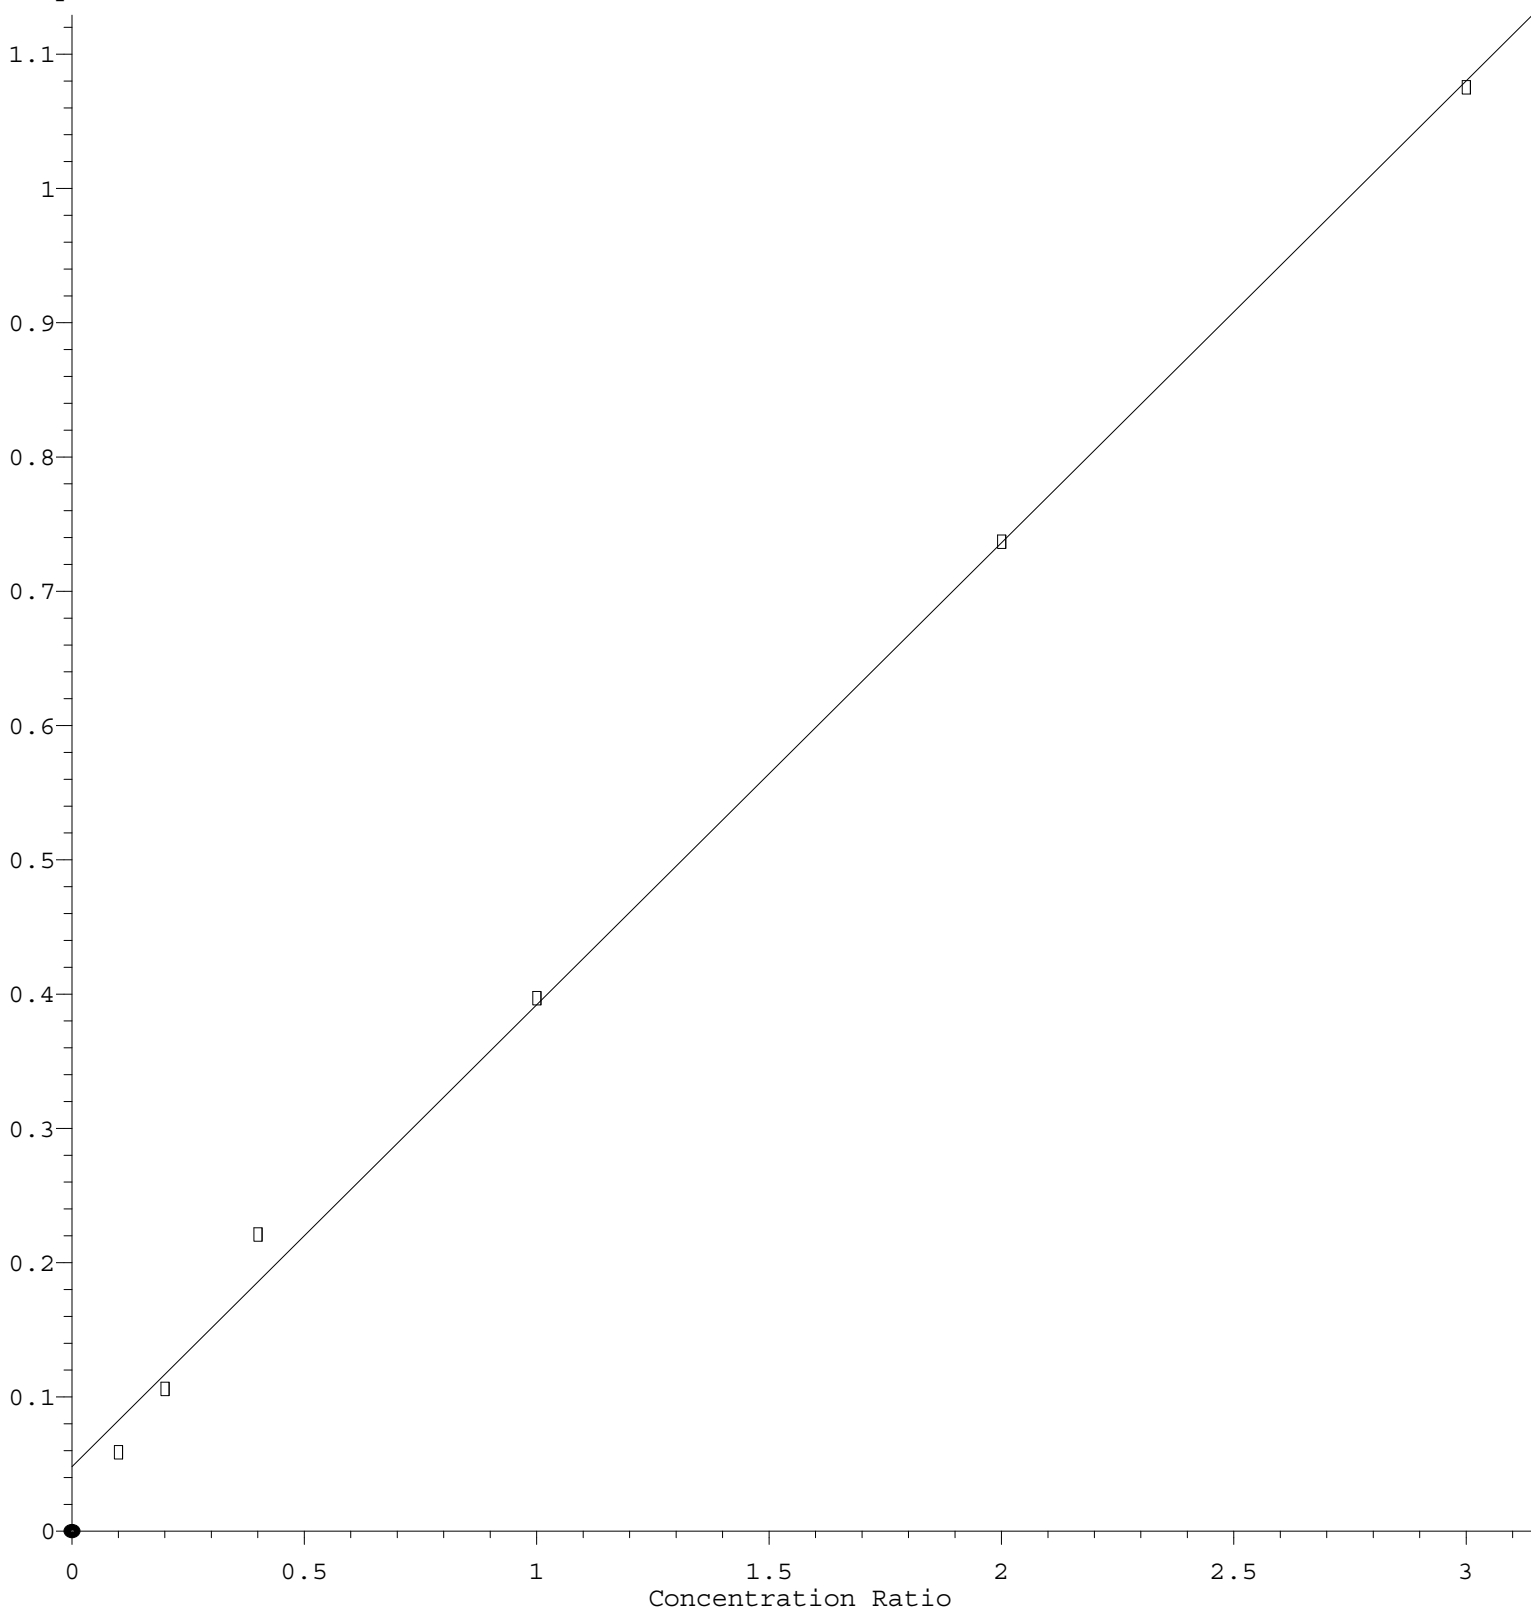

$$\text{Response} = 3.440\text{e-}001 * \text{Amt} + 4.832\text{e-}002$$

Coef of Det (r^2) = 0.997524 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA D\Method\82D071122S.M

Calibration Table Last Updated: Tue Jul 12 07:04:44 2022