


# Vinyl Acetate

Response Ratio

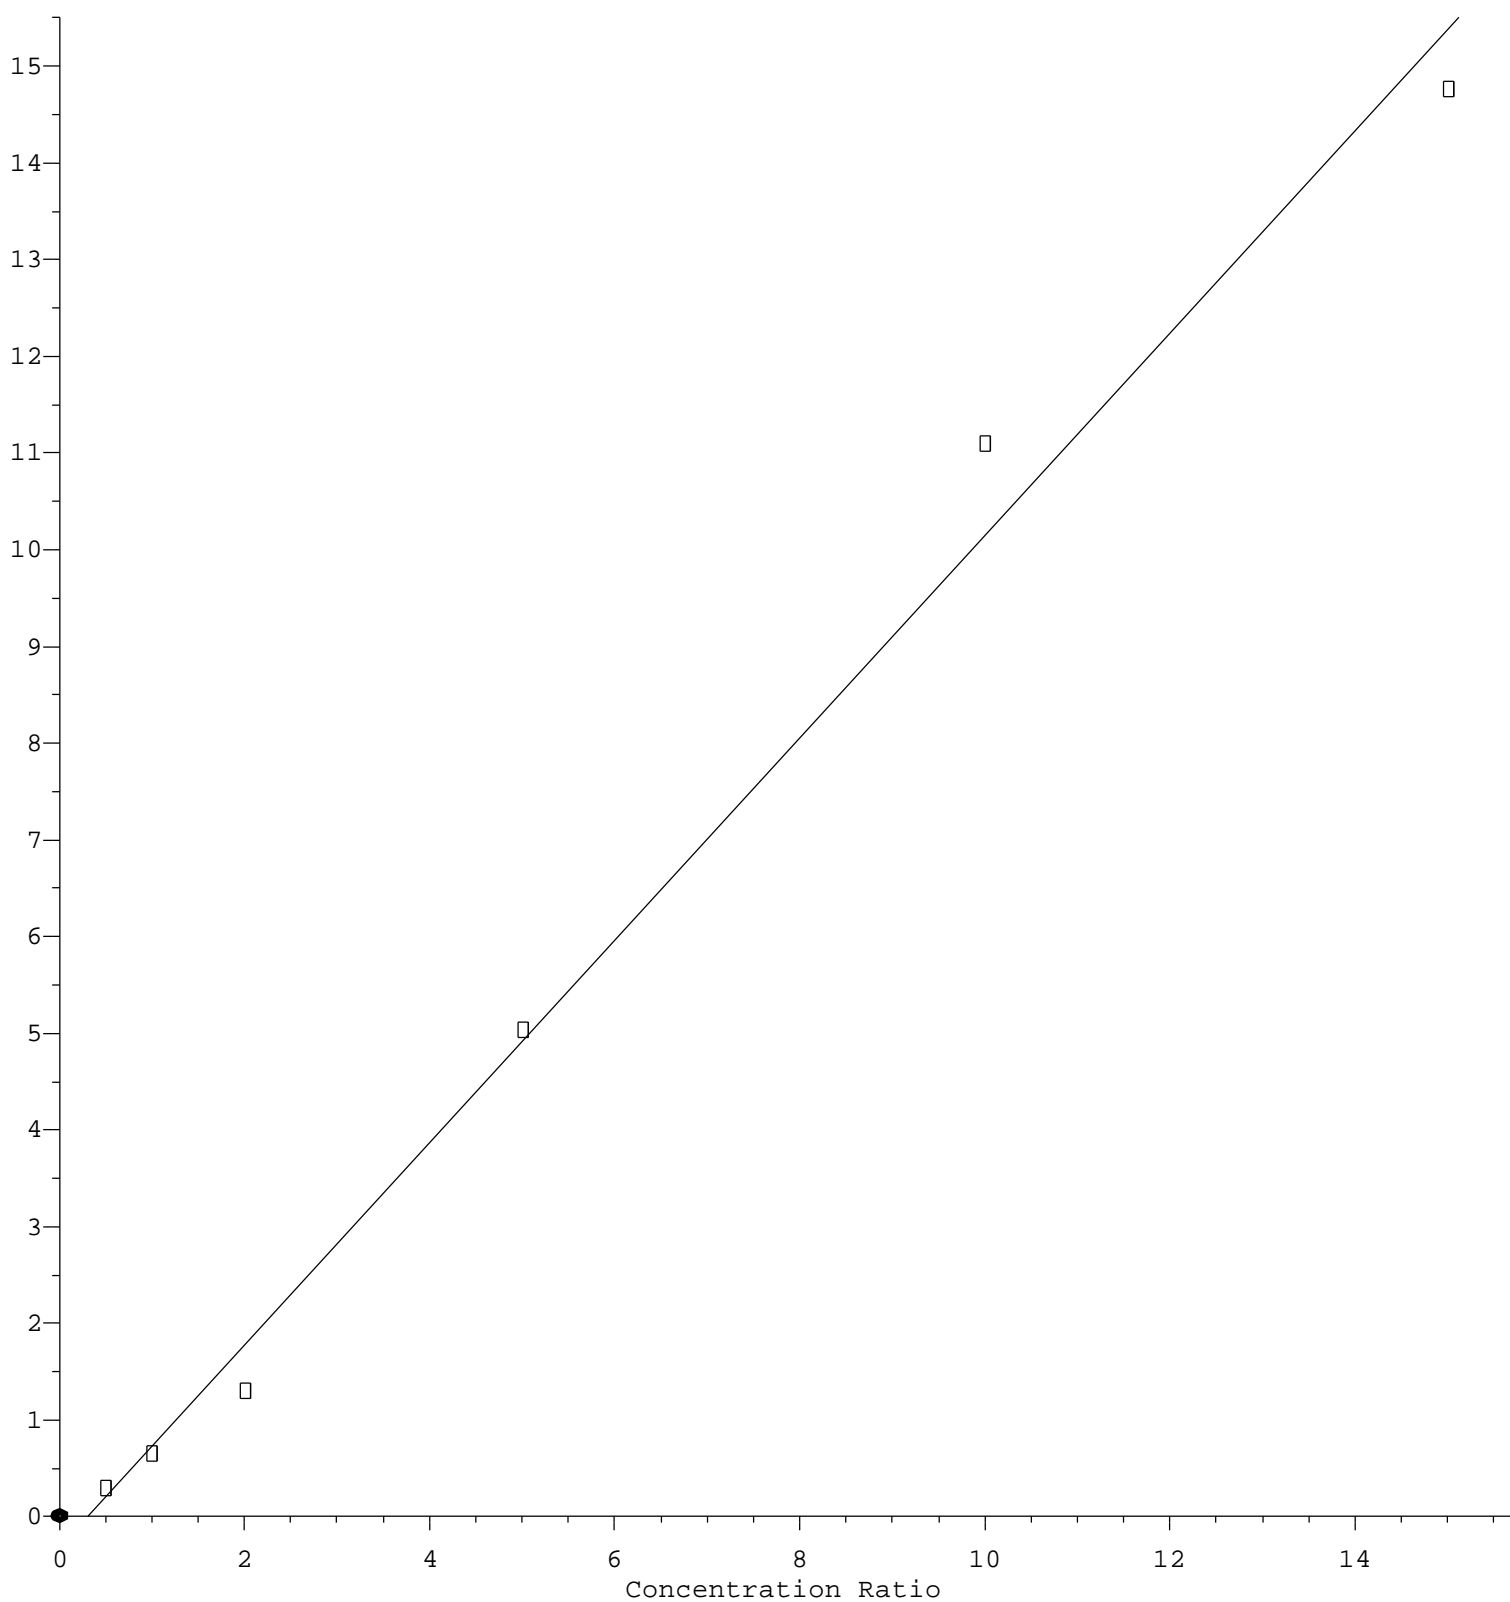

$$\text{Response} = 1.046e+000 * \text{Amt} - 3.228e-001$$


Coef of Det ( $r^2$ ) = 0.991800 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA\_D\Method\82D071321S.M

Calibration Table Last Updated: Wed Jul 14 06:00:31 2021

## Cyclohexane


Response Ratio

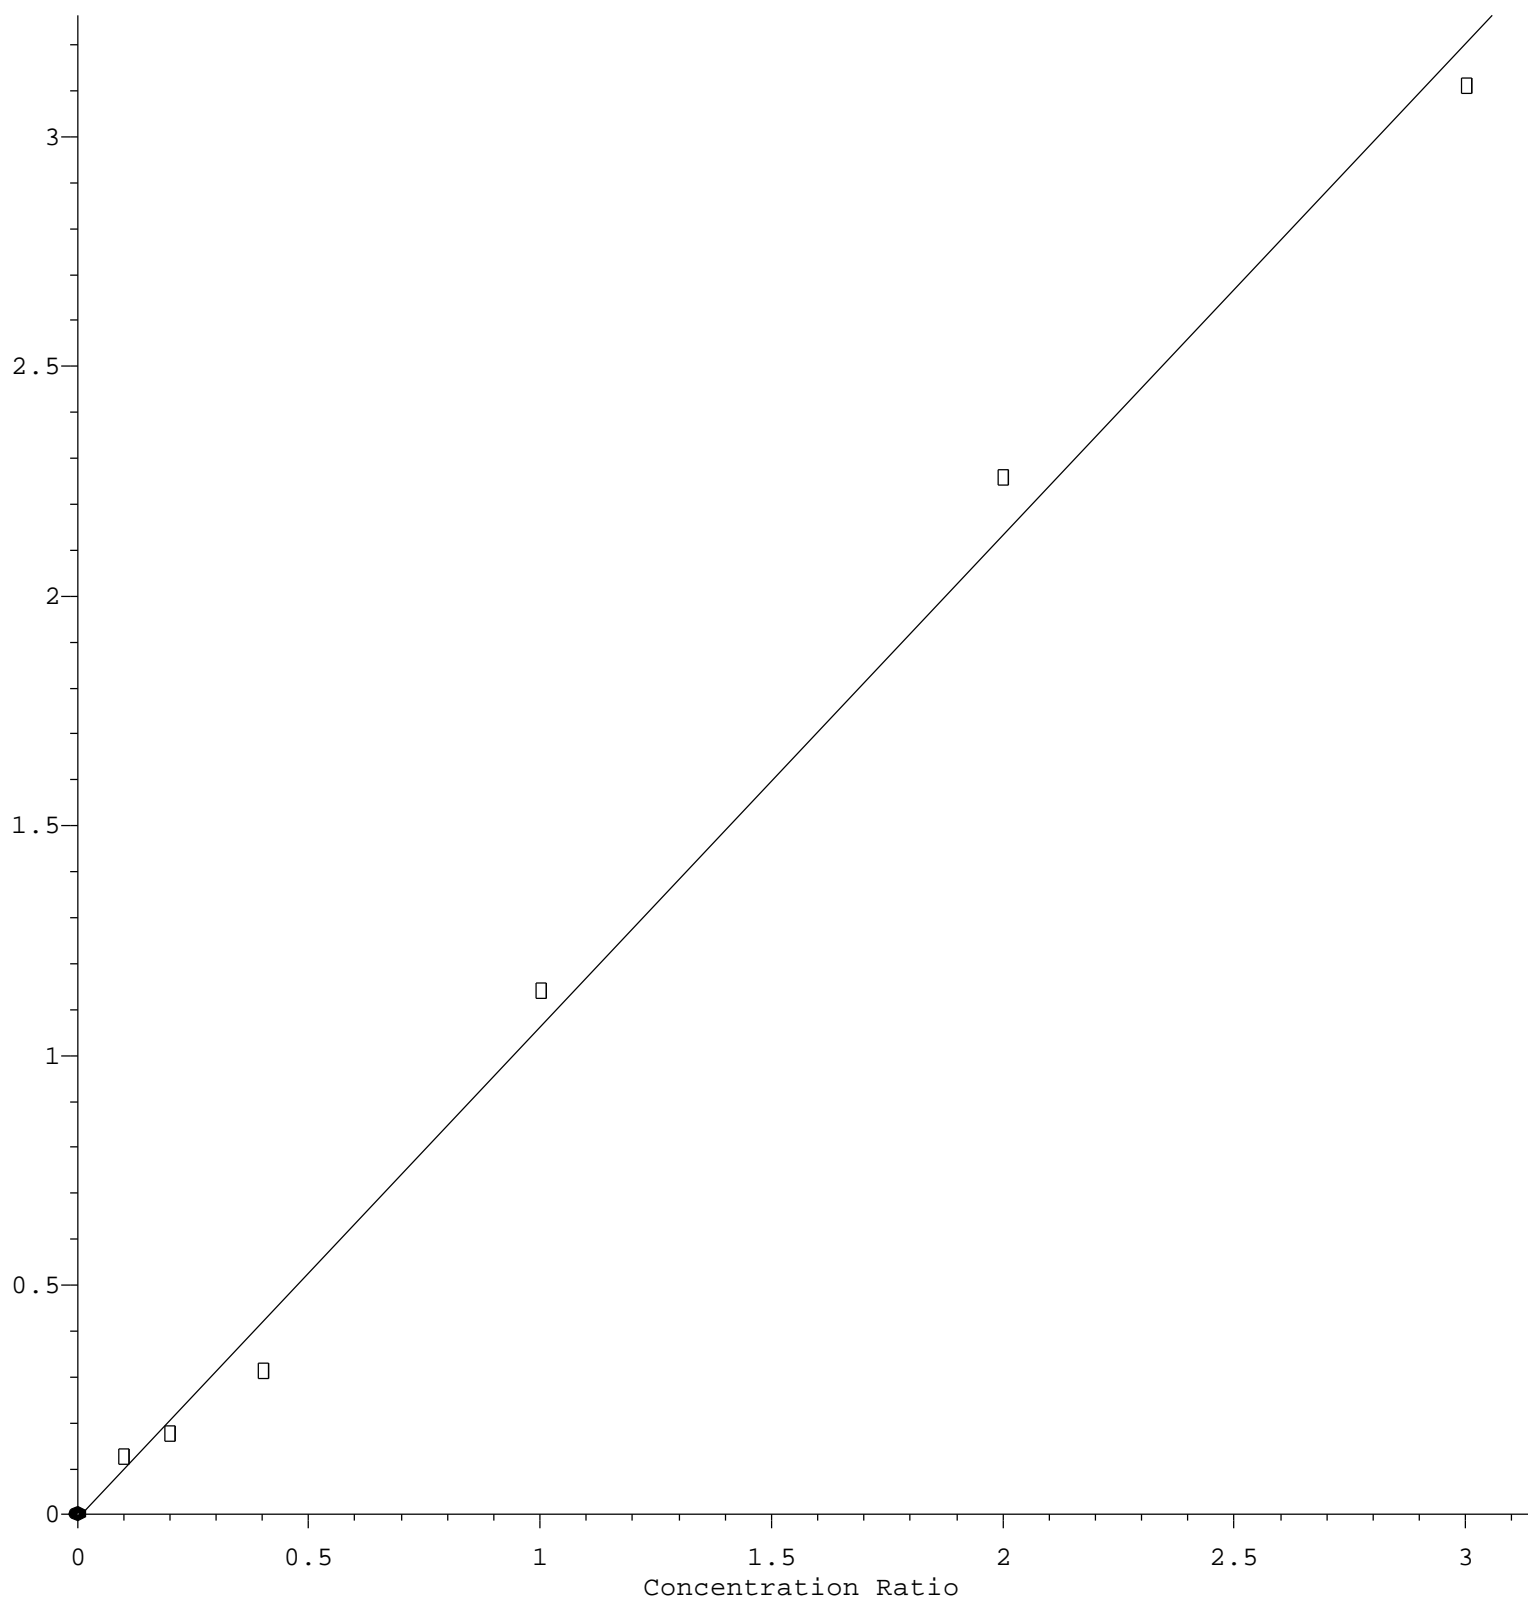

Response = 1.070e+000 \* Amt - 8.646e-003  
Coef of Det (r^2) = 0.994357 Curve Fit: Linear  
Method Name: Z:\voasrv\HPCHEM1\MSVOA\_D\Method\82D071321S.M  
Calibration Table Last Updated: Wed Jul 14 06:00:31 2021

## Methylcyclohexane

Response Ratio

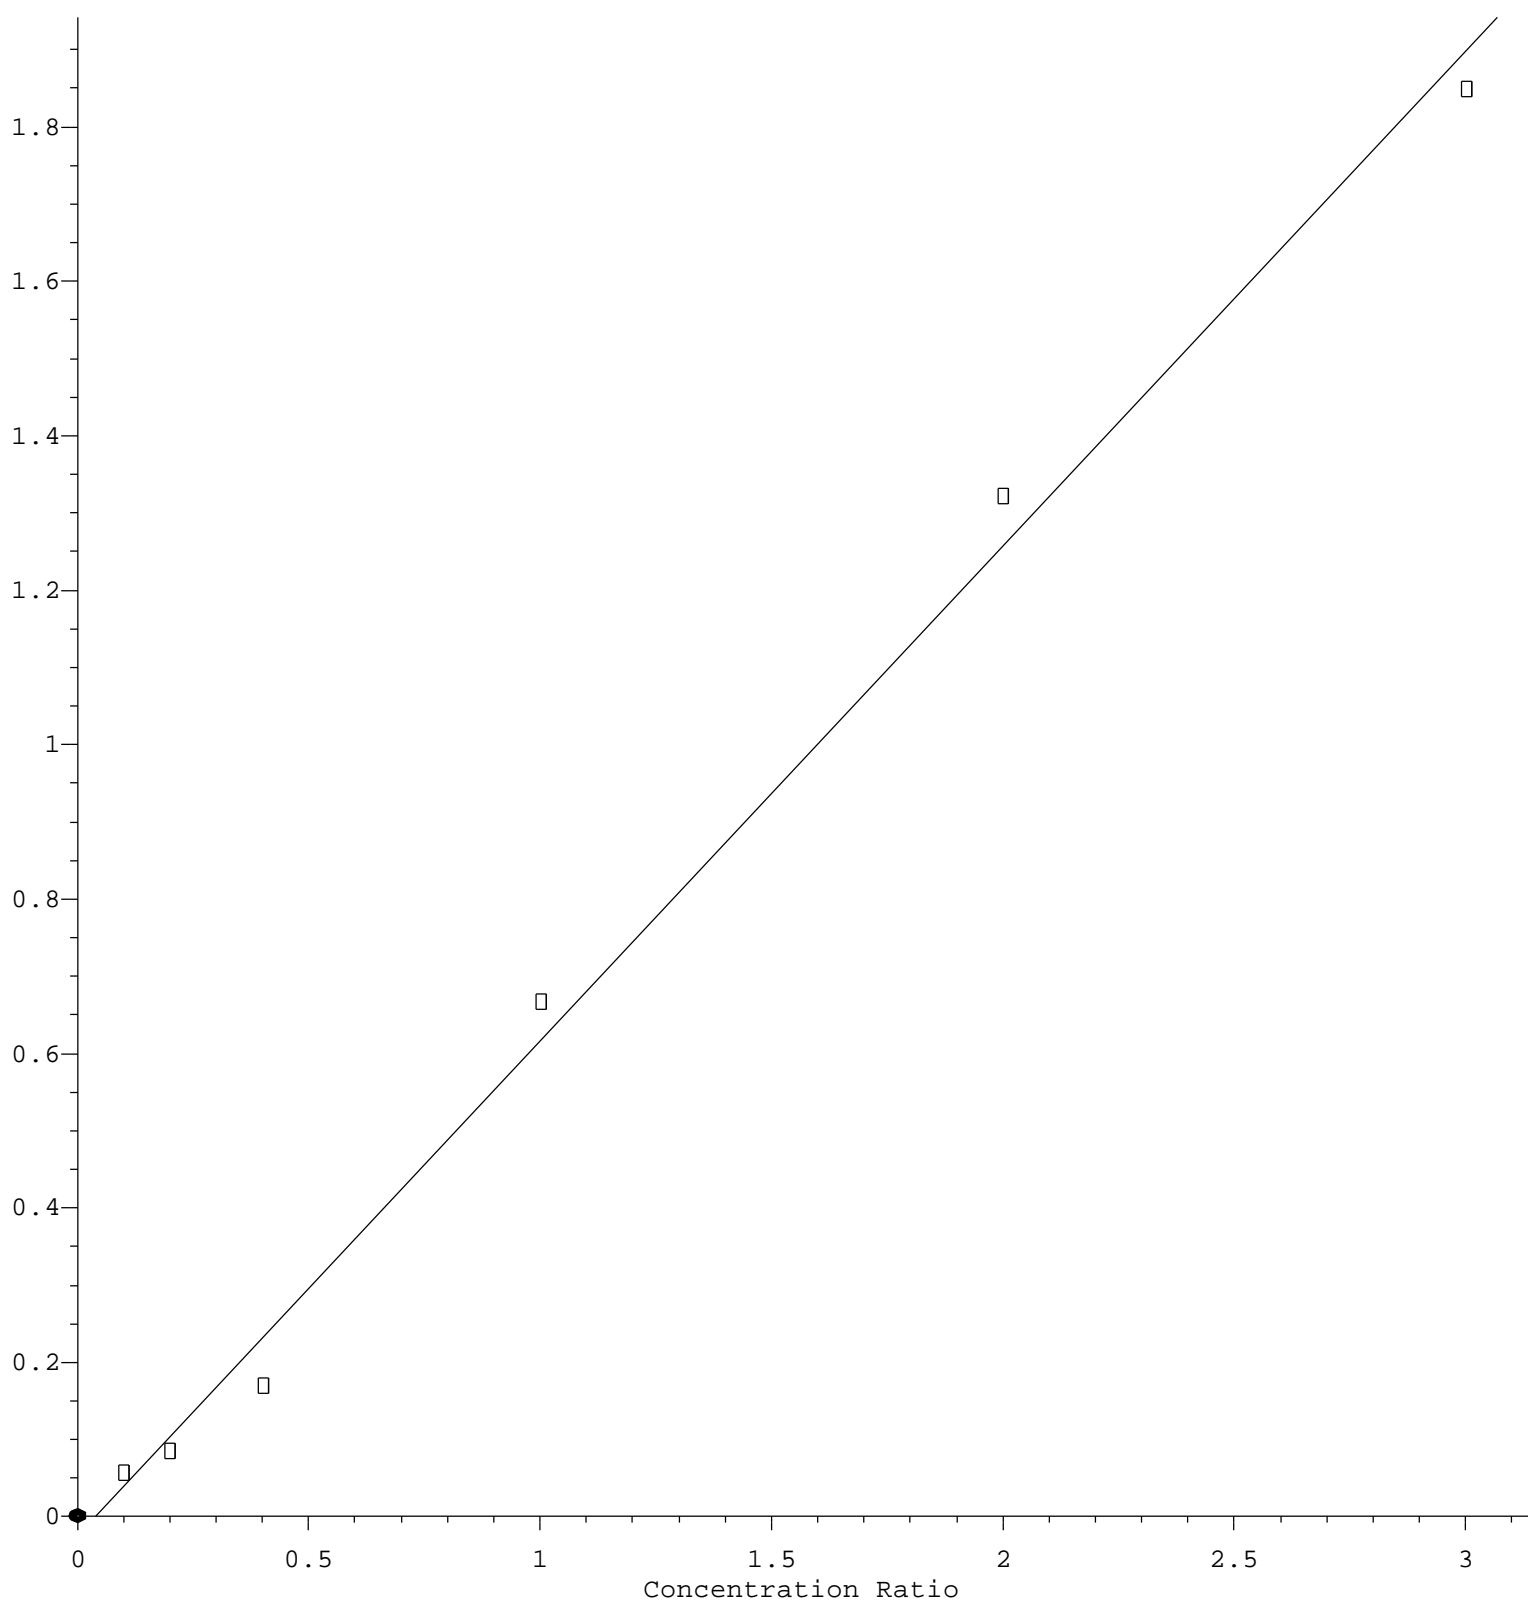


$$\text{Response} = 6.413\text{e-}001 * \text{Amt} - 2.512\text{e-}002$$

Coef of Det ( $r^2$ ) = 0.995162 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA\_D\Method\82D071321S.M


Calibration Table Last Updated: Wed Jul 14 06:00:31 2021

## Methyl methacrylate

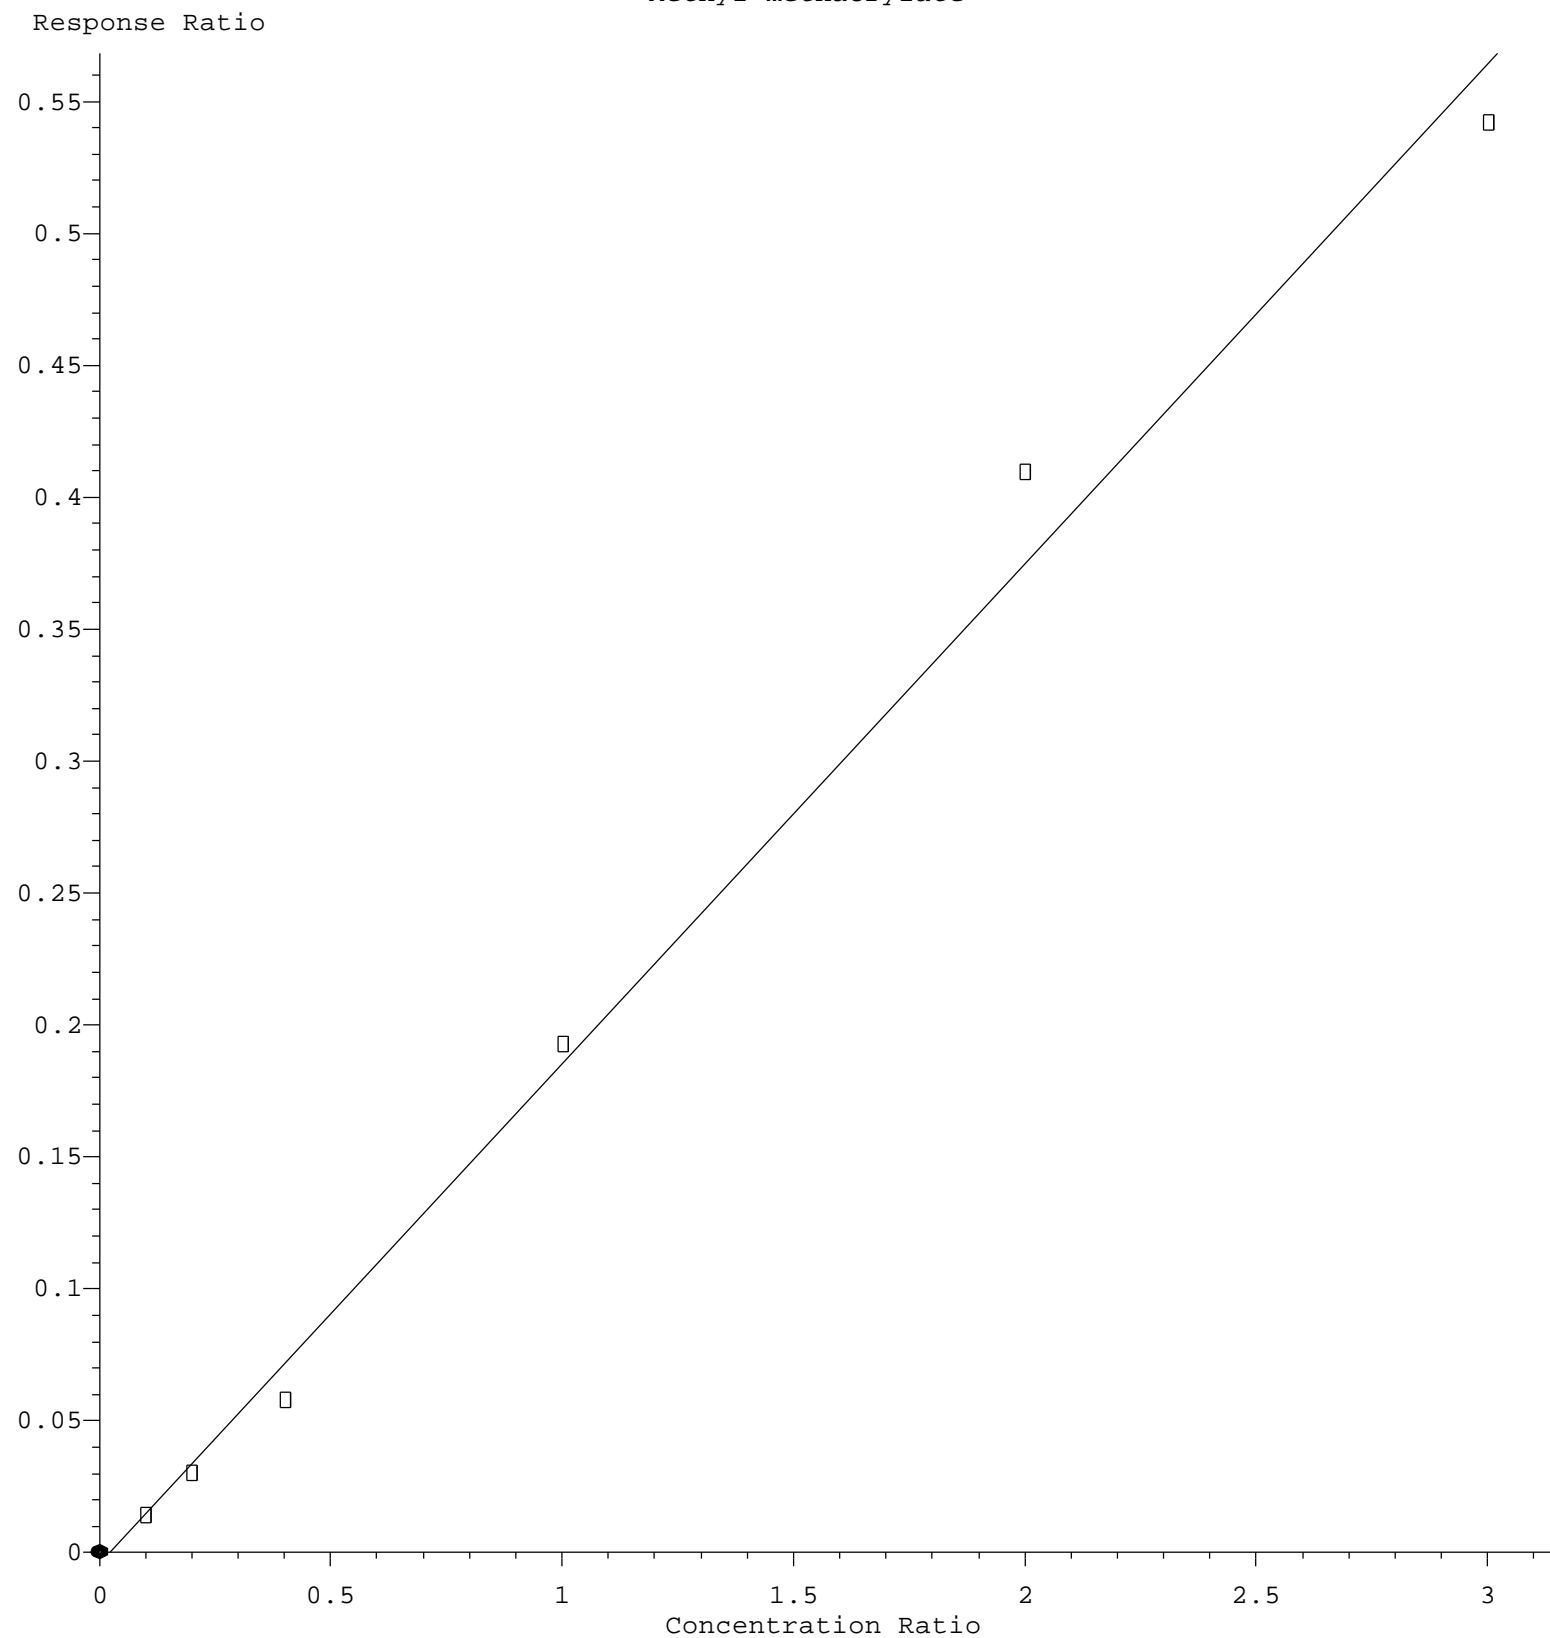

Response = 1.897e-001 \* Amt - 4.182e-003  
Coef of Det (r^2) = 0.991971    Curve Fit: Linear  
Method Name:    Z:\voasrv\HPCHEM1\MSVOA\_D\Method\82D071321S.M  
Calibration Table Last Updated: Wed Jul 14 06:00:31 2021


## 1,4-Dioxane

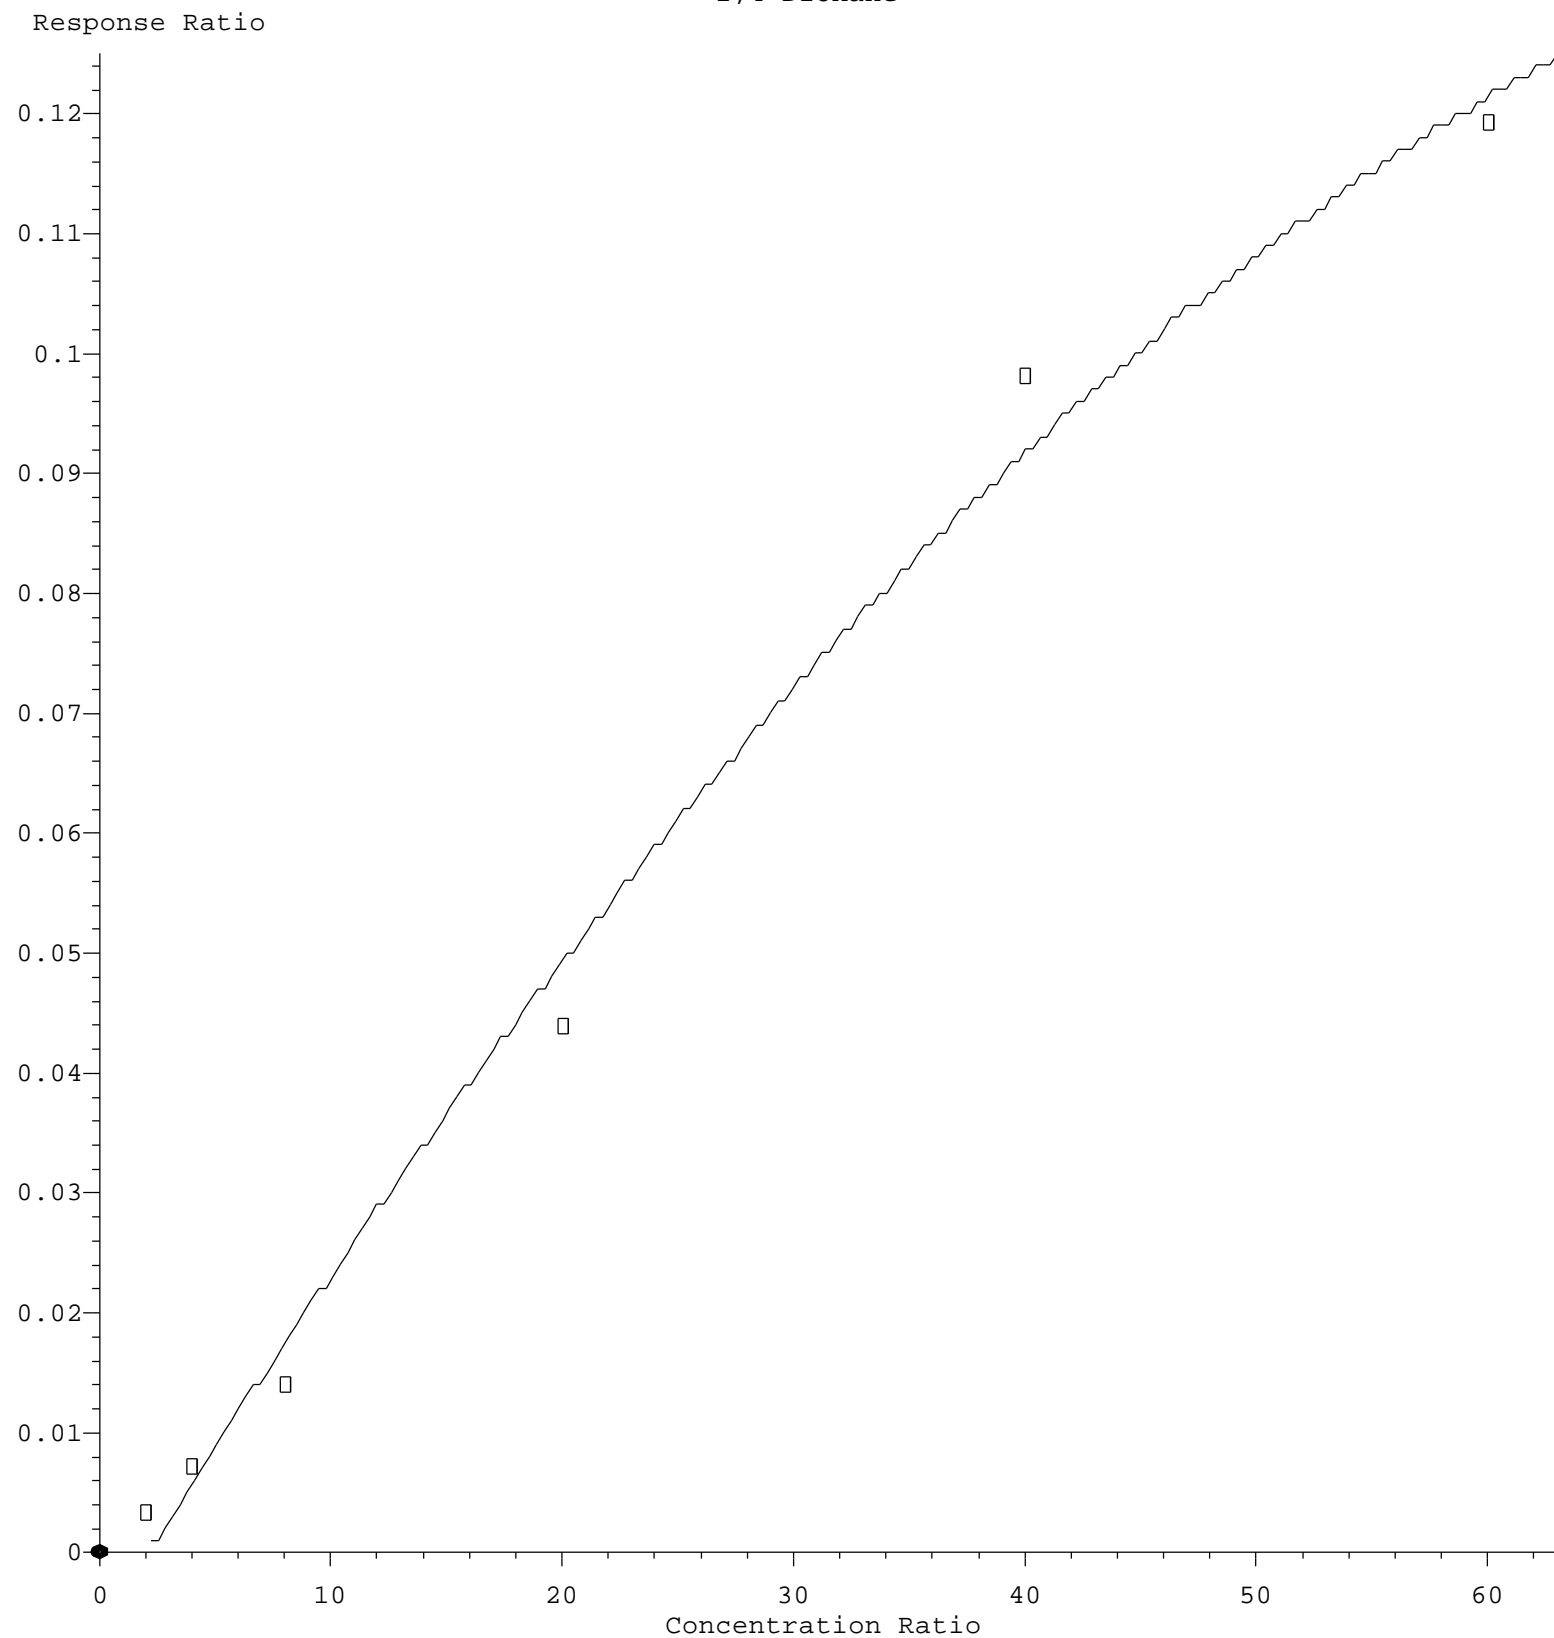

$R = -1.616e-005 A^2 + 3.096e-003 A - 6.216e-003$   
Coef of Det ( $r^2$ ) = 0.992011    Curve Fit: Quadratic  
Method Name:    Z:\voasrv\HPCHEM1\MSVOA\_D\Method\82D071321S.M  
Calibration Table Last Updated: Wed Jul 14 06:00:31 2021

## Ethyl methacrylate

Response Ratio

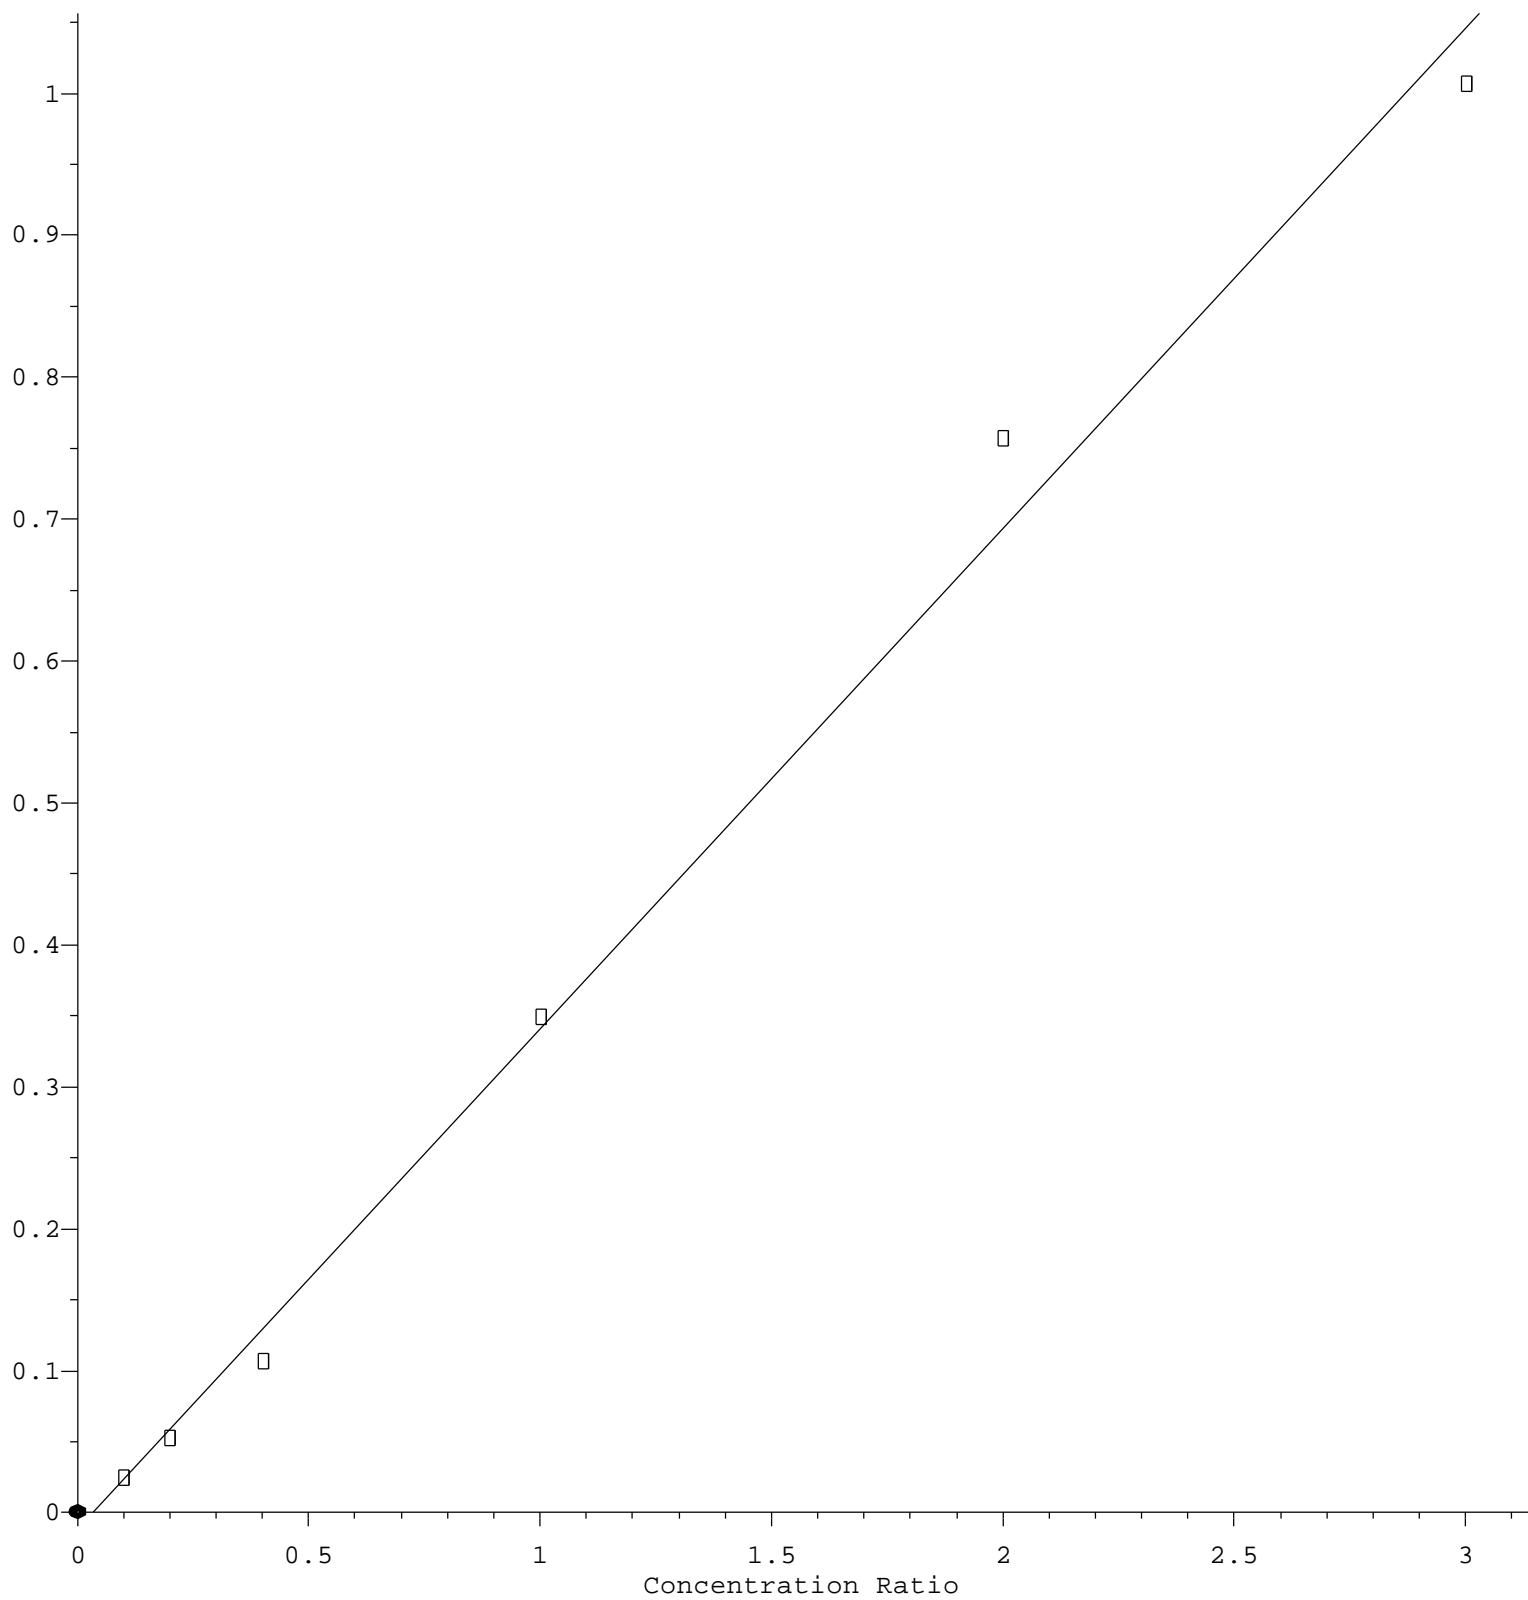

$$\text{Response} = 3.528\text{e-}001 * \text{Amt} - 1.175\text{e-}002$$


Coef of Det ( $r^2$ ) = 0.992642 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA\_D\Method\82D071321S.M

Calibration Table Last Updated: Wed Jul 14 06:00:31 2021

## 2-Chloroethyl Vinyl ether

Response Ratio

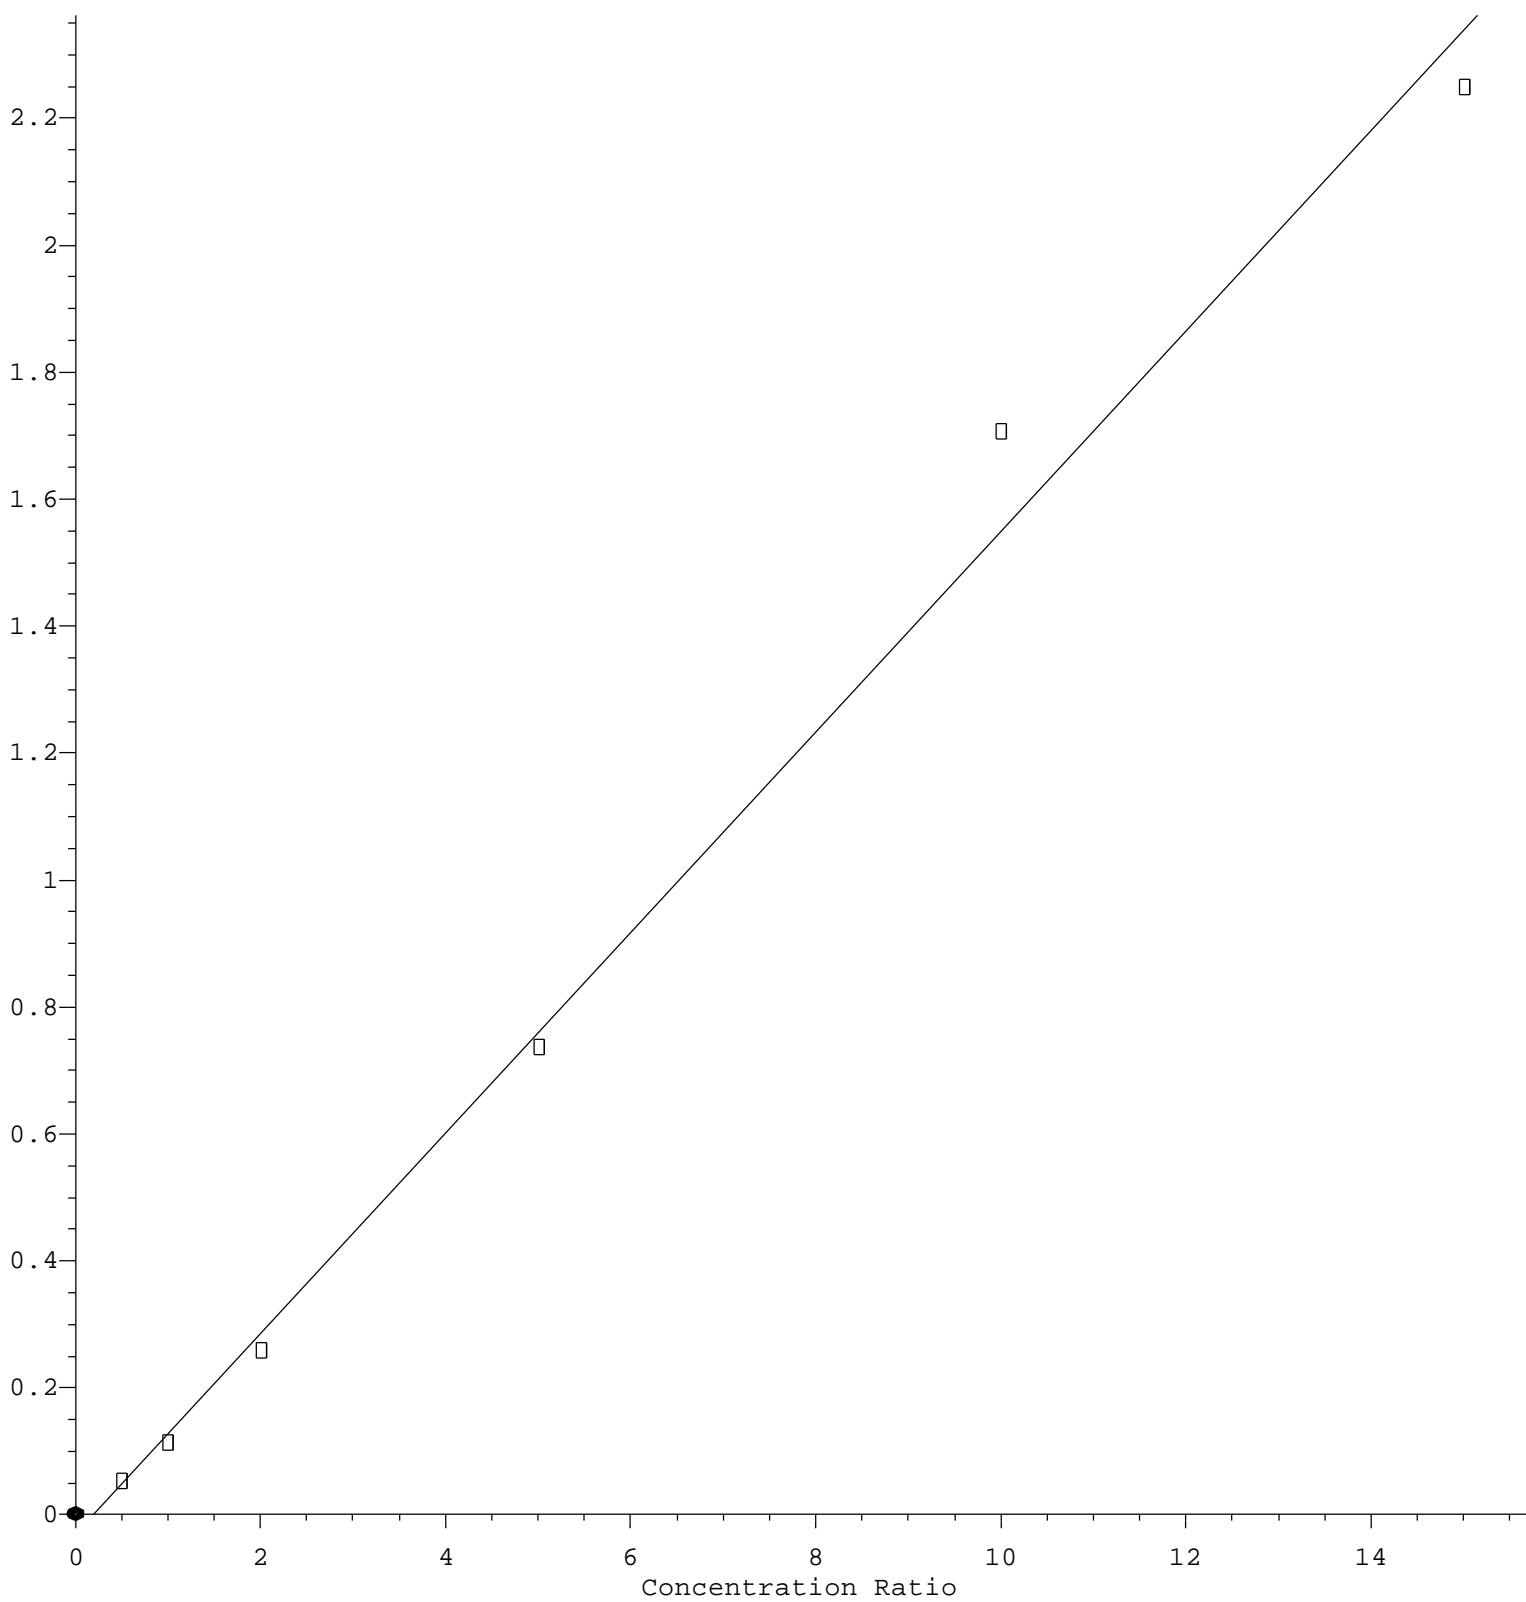

$$\text{Response} = 1.579\text{e-}001 * \text{Amt} - 2.956\text{e-}002$$


Coef of Det ( $r^2$ ) = 0.991959 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA\_D\Method\82D071321S.M

Calibration Table Last Updated: Wed Jul 14 06:00:31 2021

# Naphthalene

Response Ratio

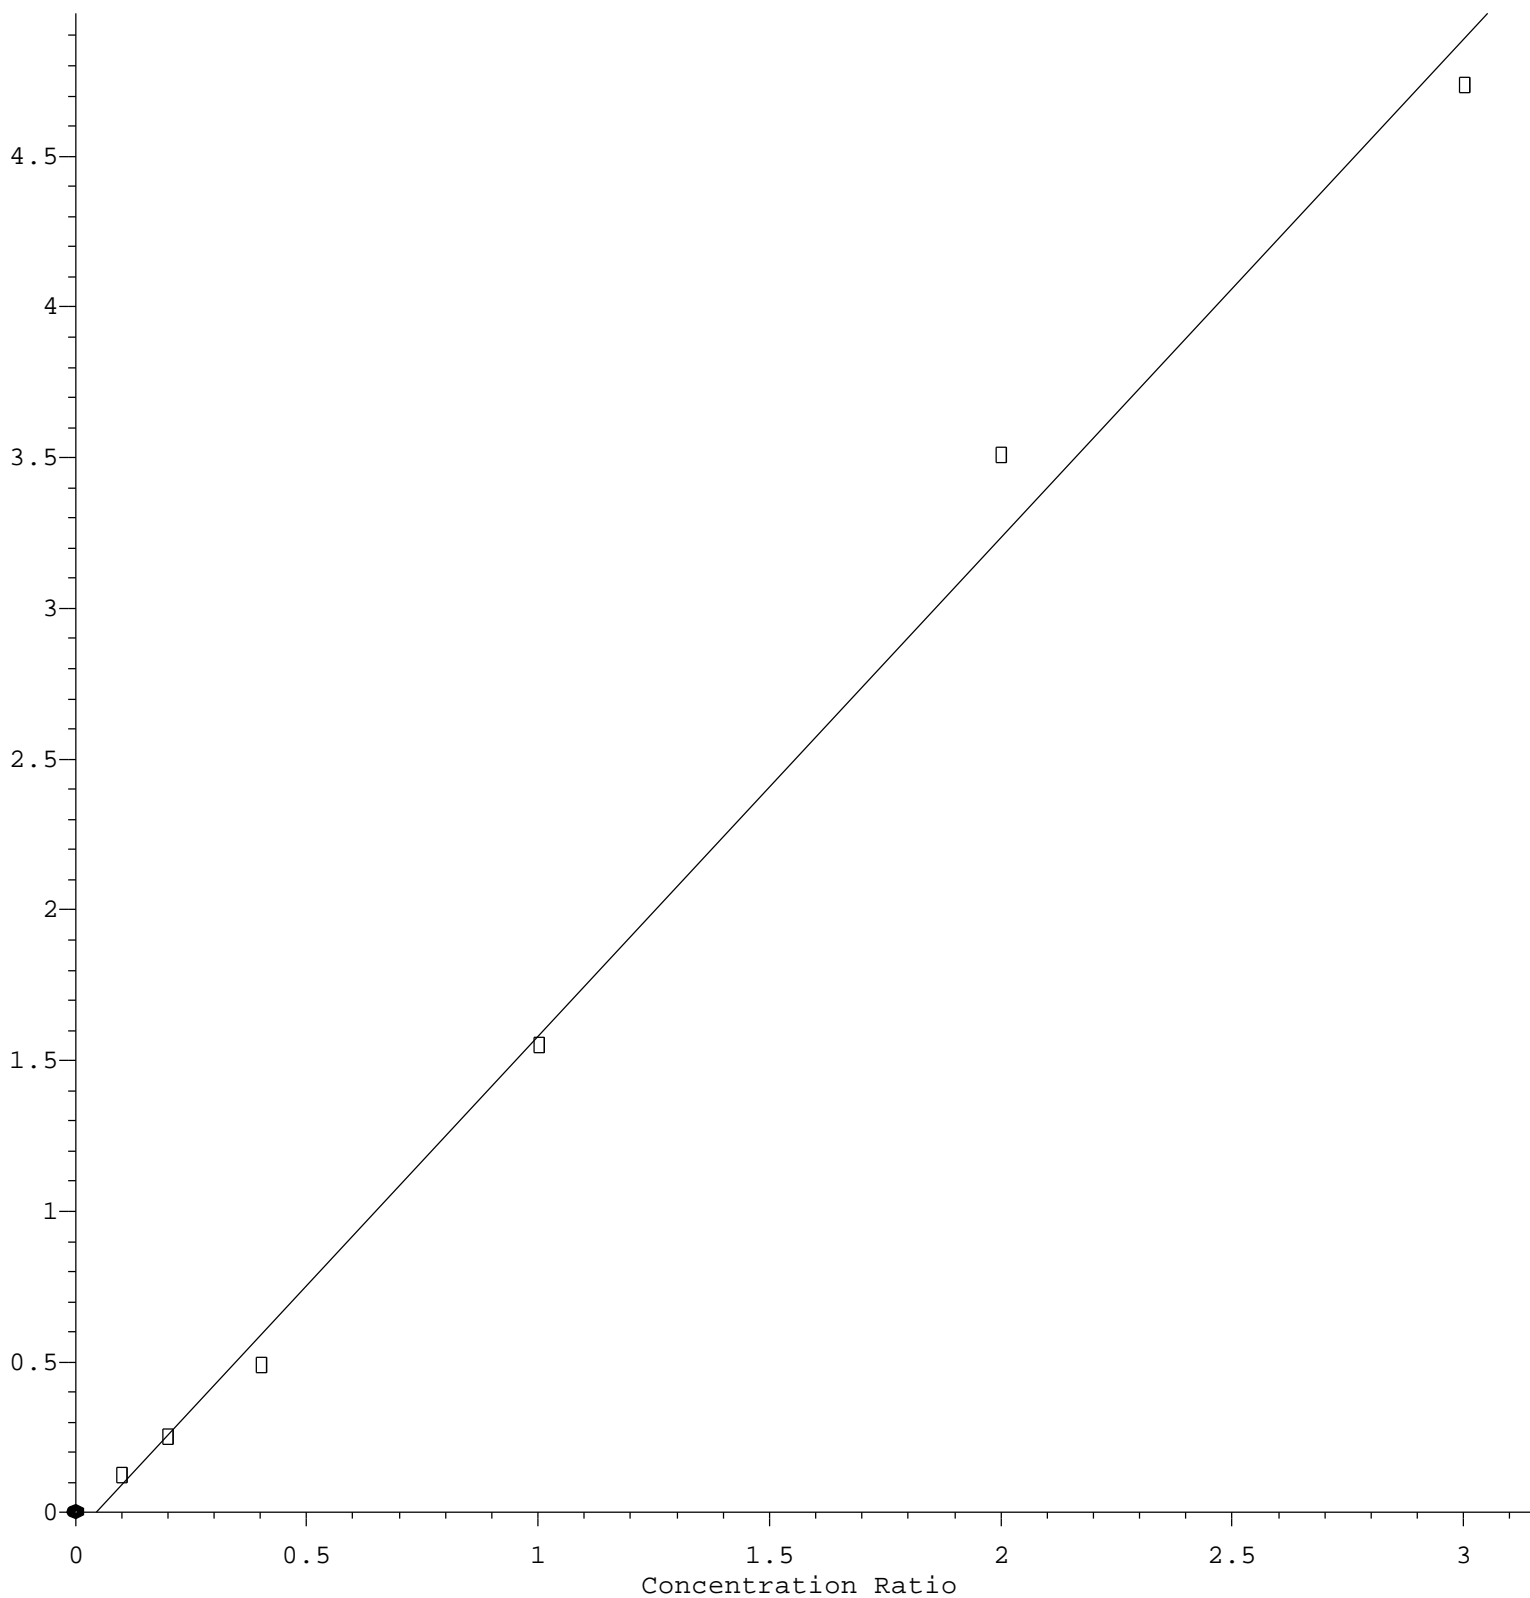

$$\text{Response} = 1.655\text{e}+000 * \text{Amt} - 7.297\text{e}-002$$

Coef of Det (r^2) = 0.994128 Curve Fit: Linear


Method Name: Z:\voasrv\HPCHEM1\MSVOA\_D\Method\82D071321S.M

Calibration Table Last Updated: Wed Jul 14 06:00:31 2021



# Dichlorodifluoromethane

Response Ratio

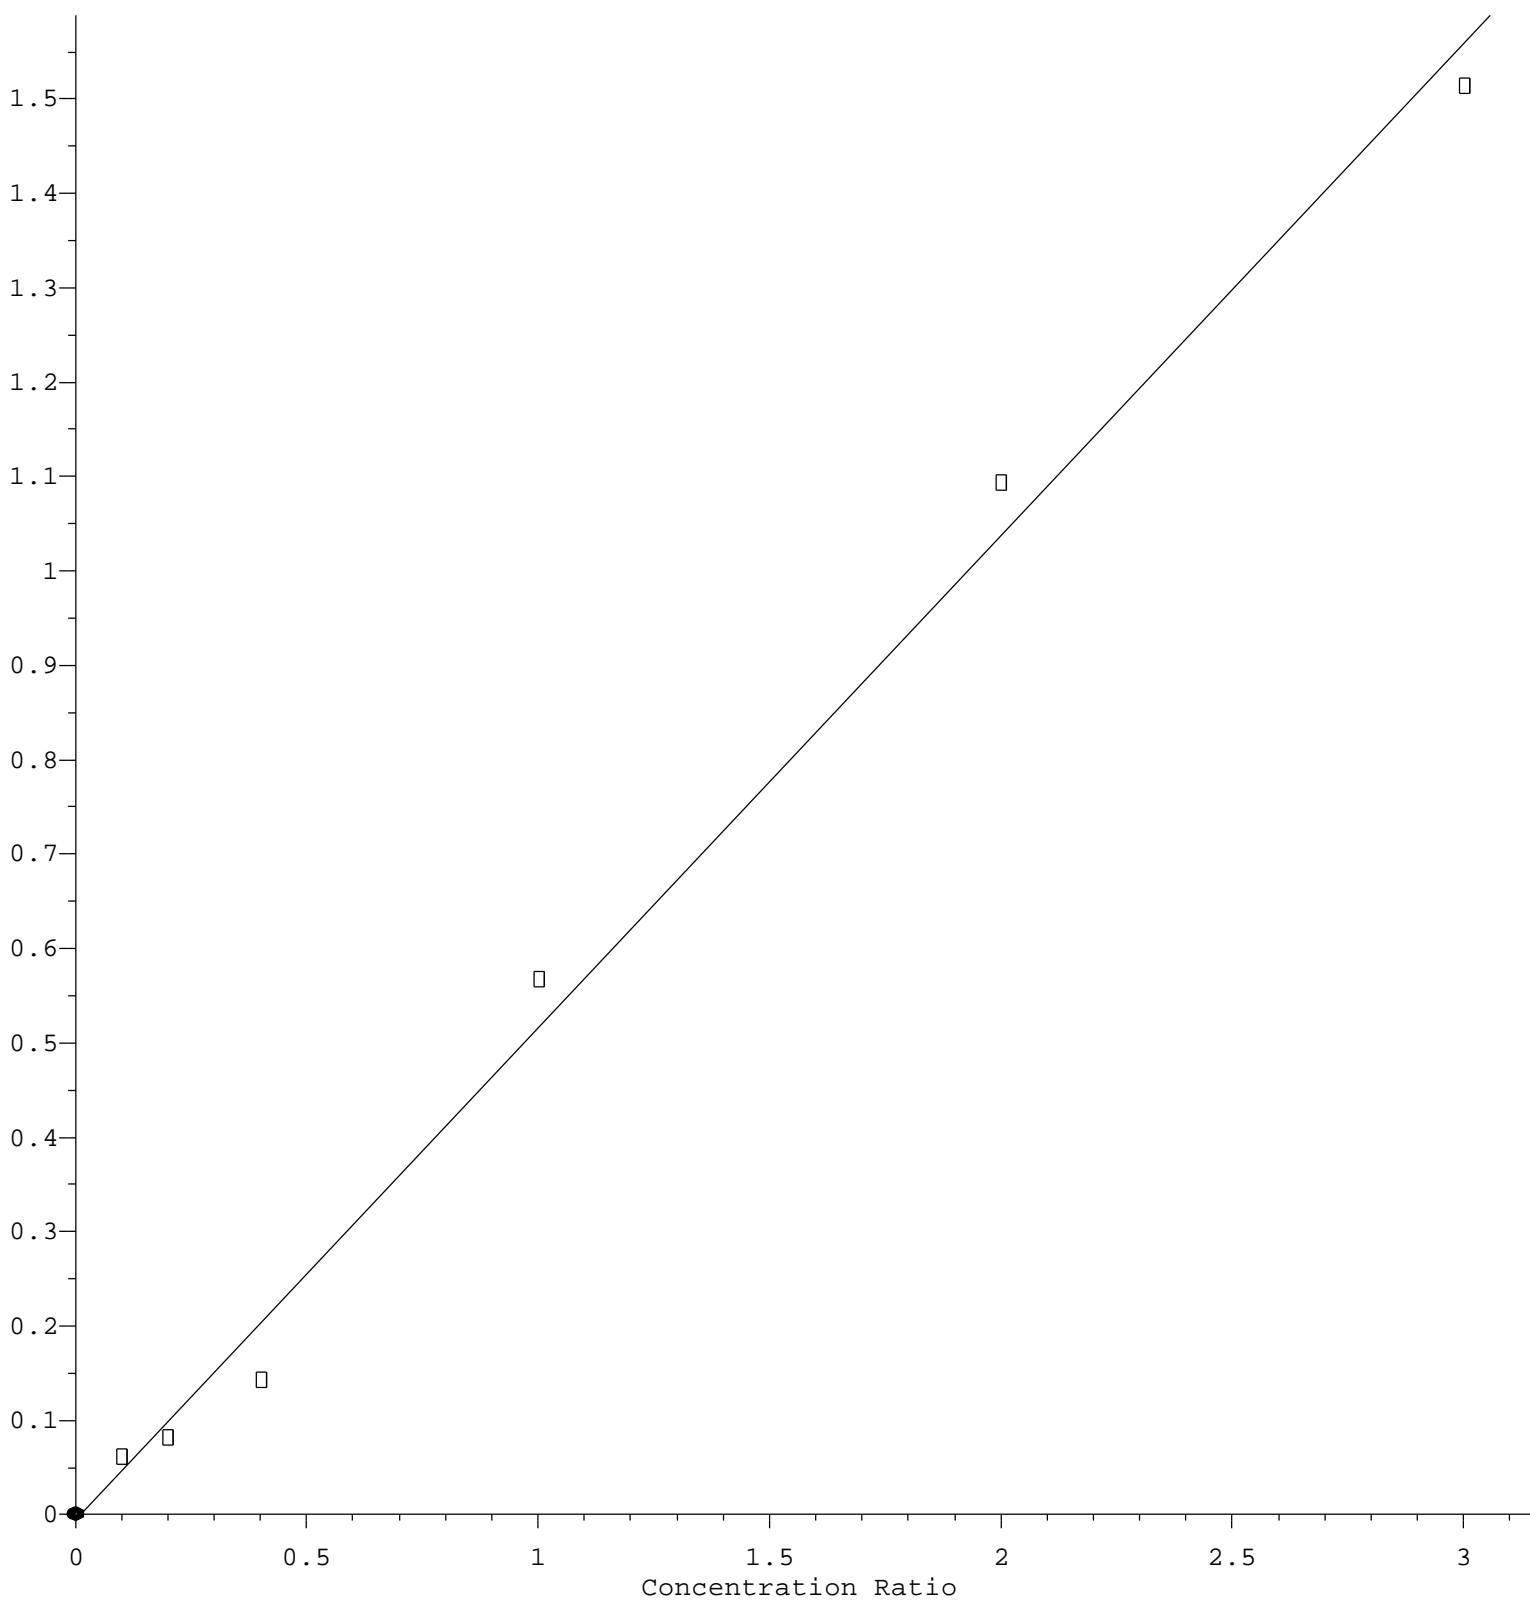

$$\text{Response} = 5.219\text{e-}001 * \text{Amt} - 6.414\text{e-}003$$


Coef of Det ( $r^2$ ) = 0.993482 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA\_D\Method\82D071321S.M

Calibration Table Last Updated: Wed Jul 14 06:00:31 2021

## Chloromethane

Response Ratio

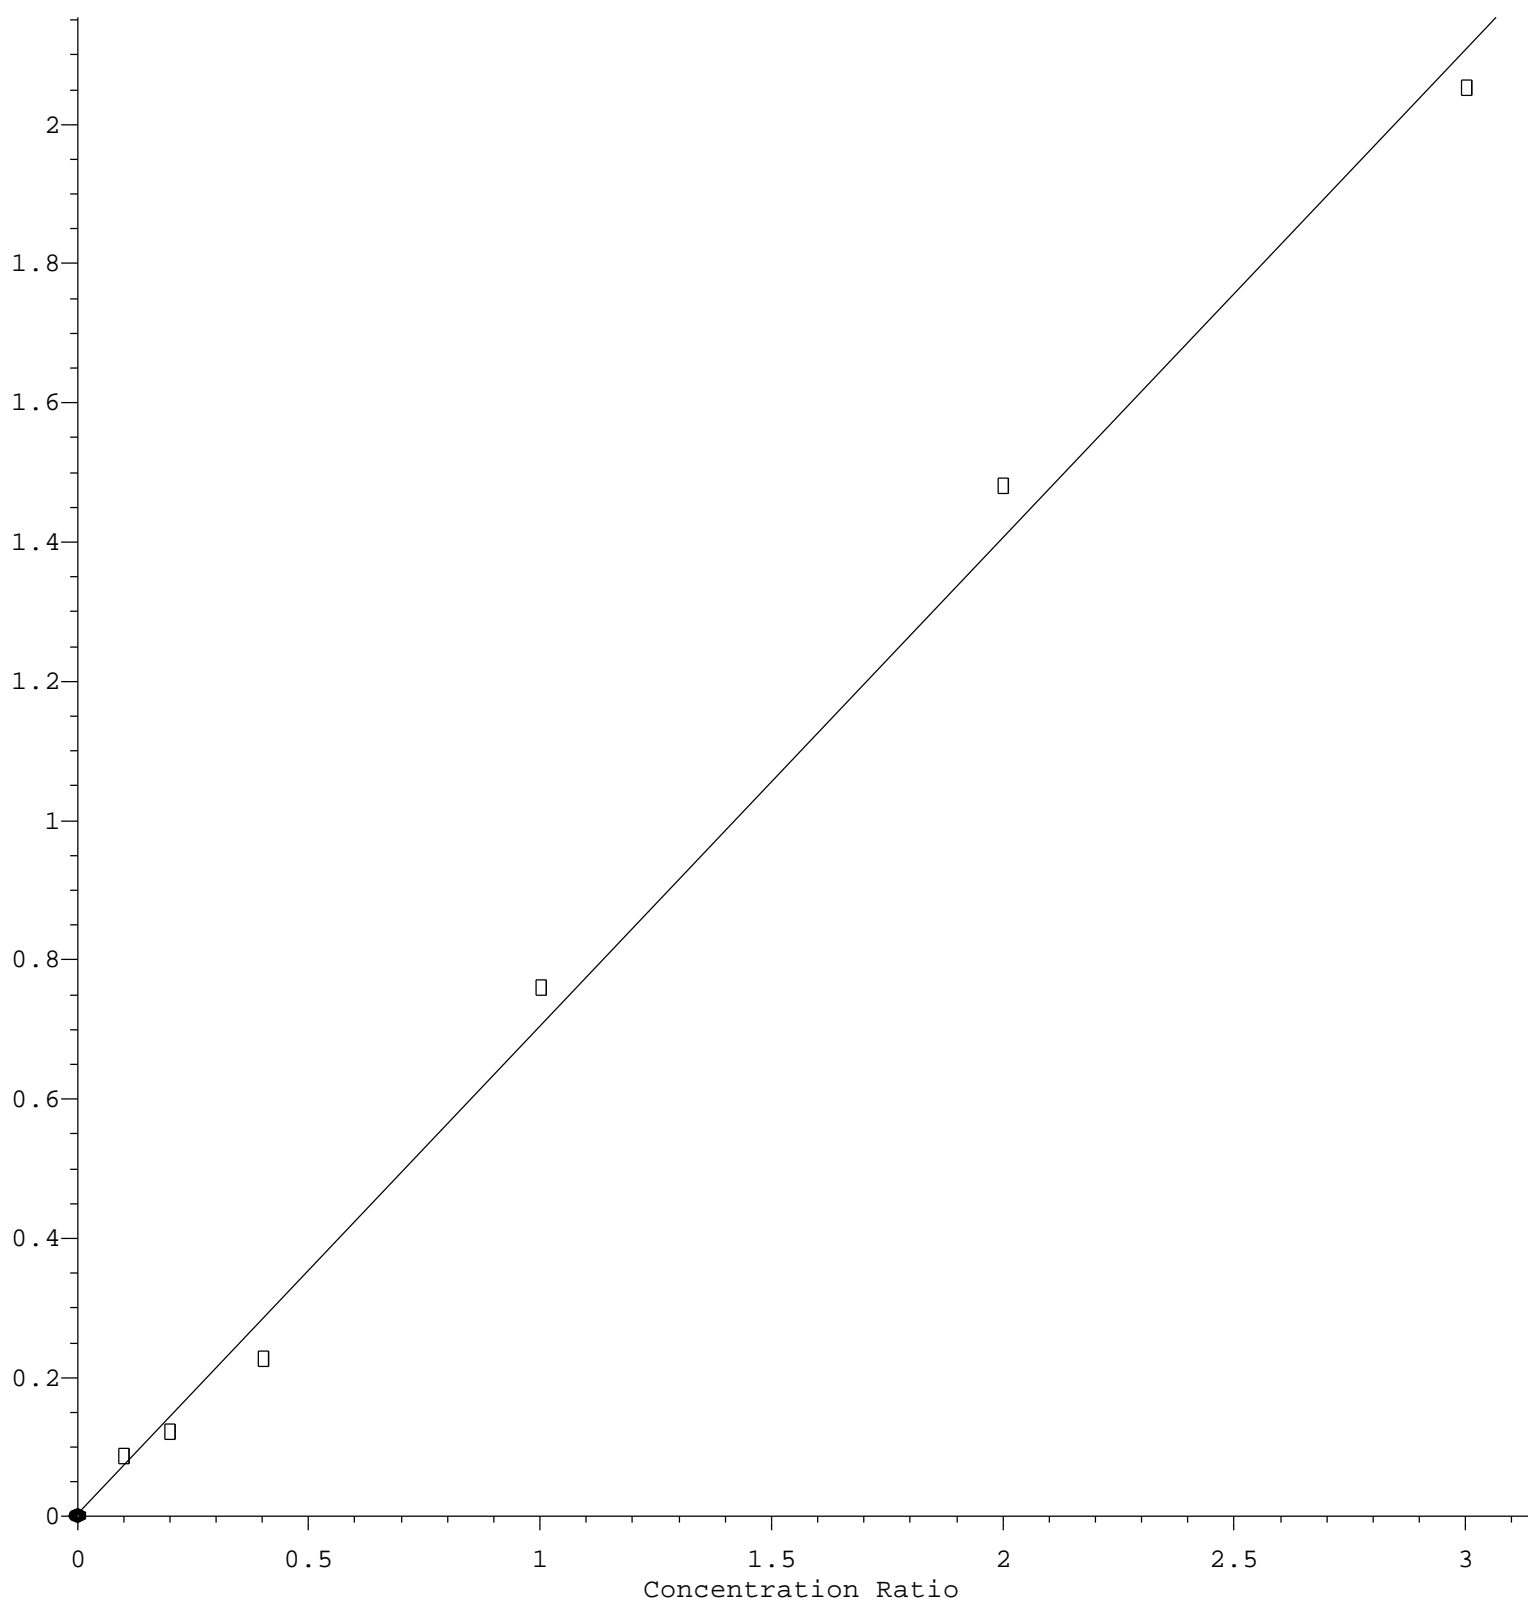

$$\text{Response} = 7.015\text{e-}001 * \text{Amt} + 4.122\text{e-}003$$


Coef of Det ( $r^2$ ) = 0.995272 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA\_D\Method\82D071321S.M

Calibration Table Last Updated: Wed Jul 14 06:00:31 2021

# Bromomethane

Response Ratio

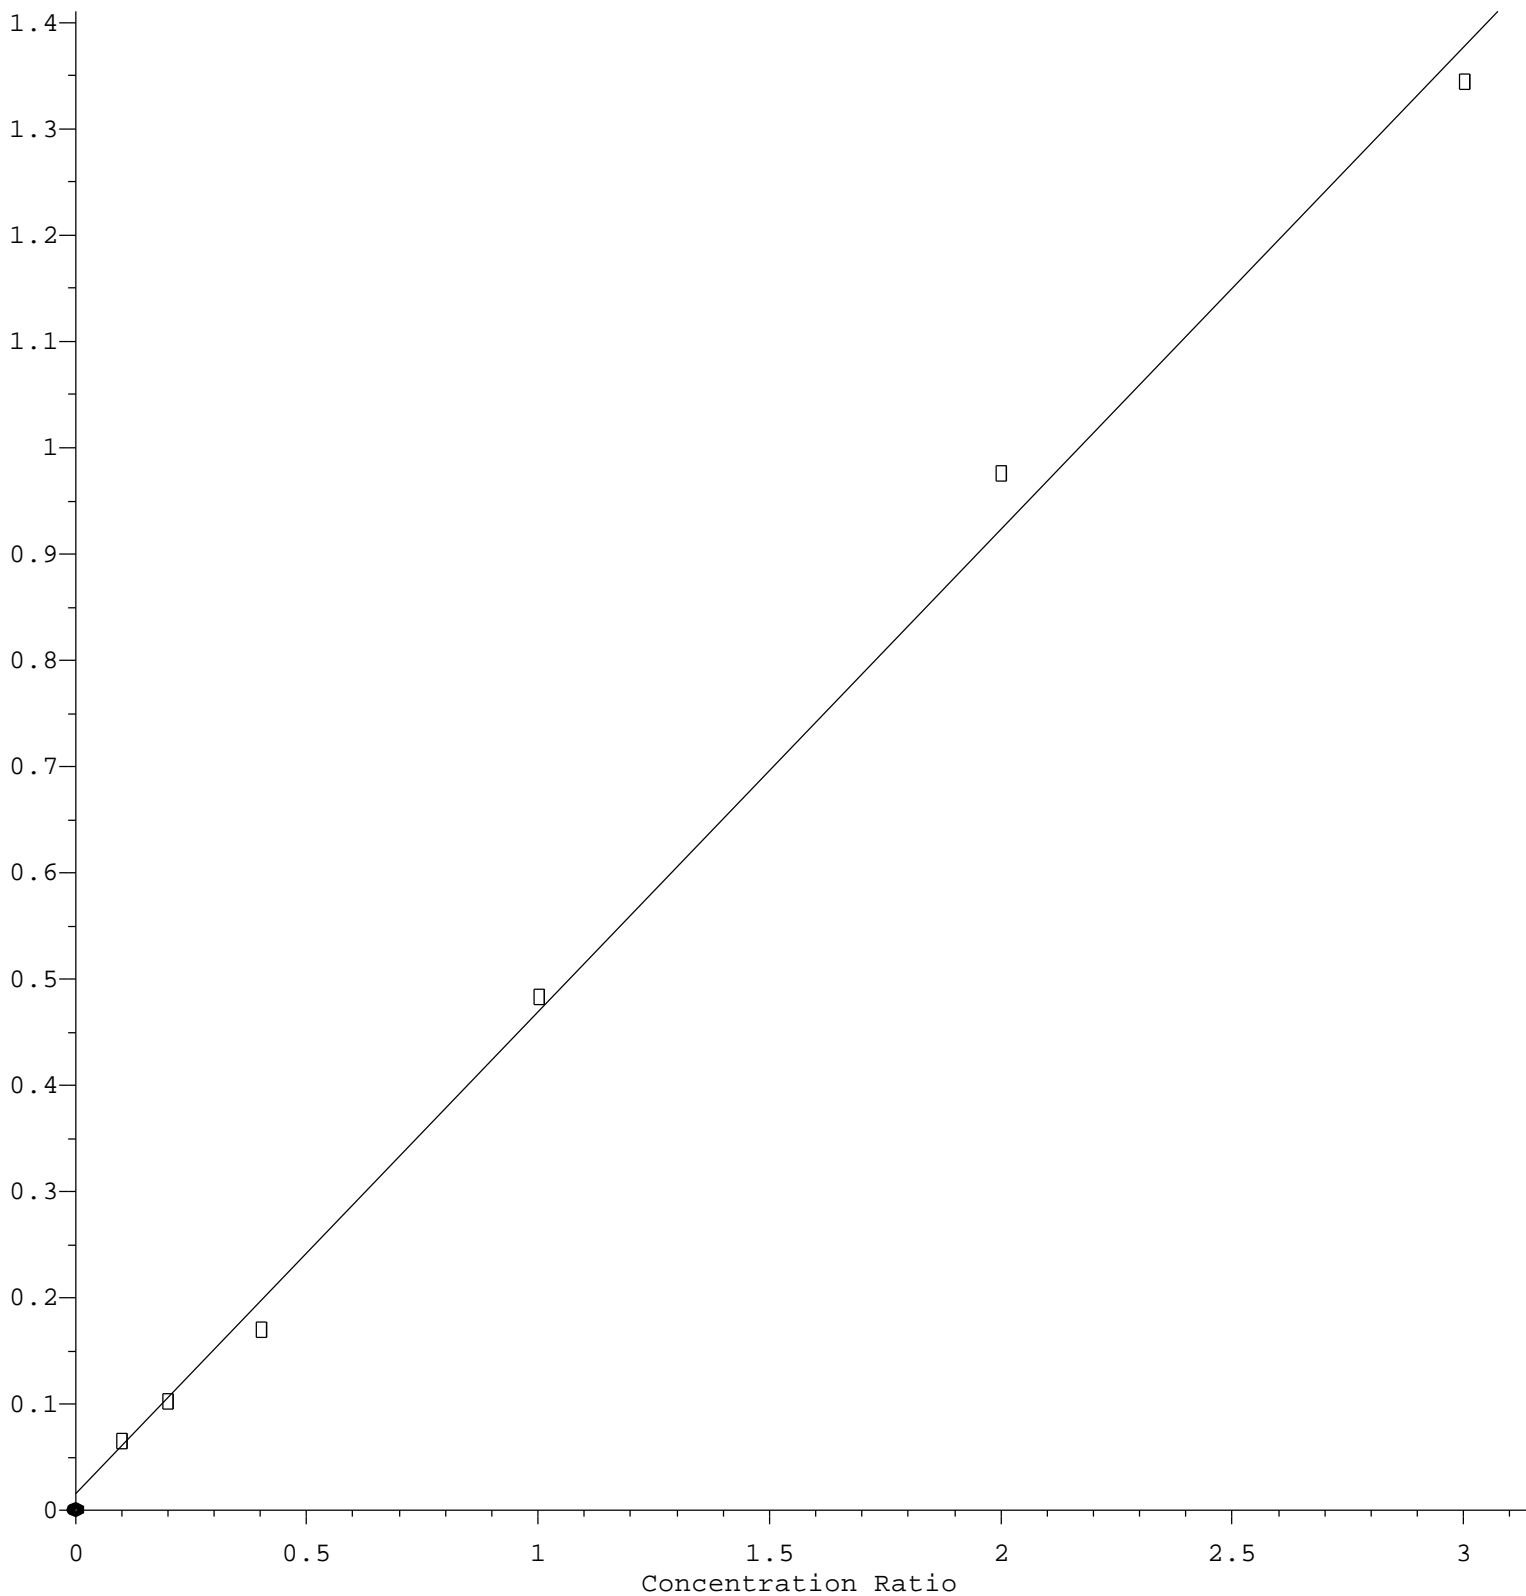

$$\text{Response} = 4.538\text{e-}001 * \text{Amt} + 1.615\text{e-}002$$


Coef of Det (r^2) = 0.996565 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA\_D\Method\82D071321S.M

Calibration Table Last Updated: Wed Jul 14 06:00:31 2021

## Methyl Iodide

Response Ratio

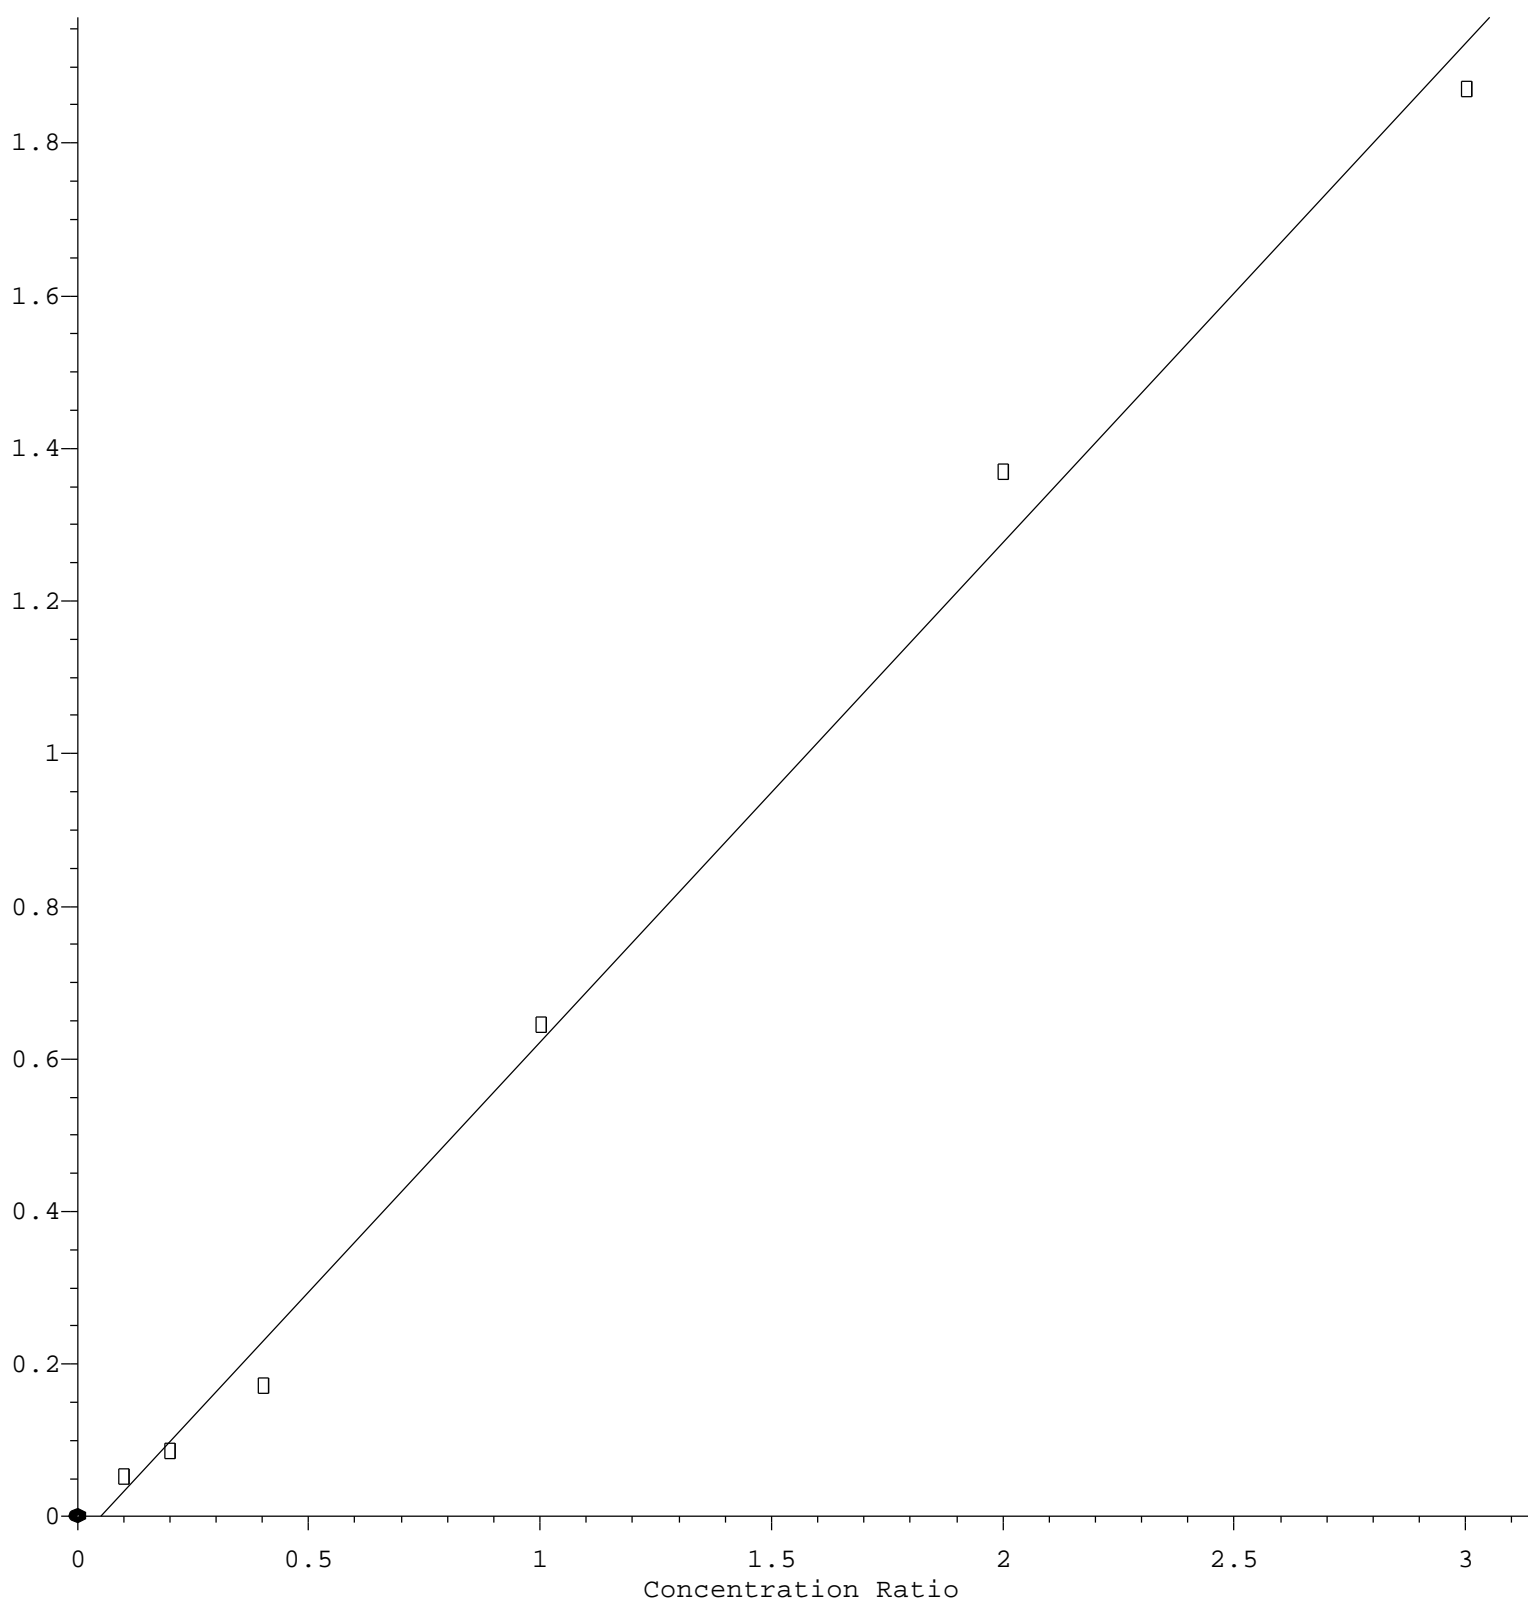

$$\text{Response} = 6.544\text{e-}001 * \text{Amt} - 3.231\text{e-}002$$


Coef of Det ( $r^2$ ) = 0.994293 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA\_D\Method\82D071321S.M

Calibration Table Last Updated: Wed Jul 14 06:00:31 2021

# Acetone


Response Ratio

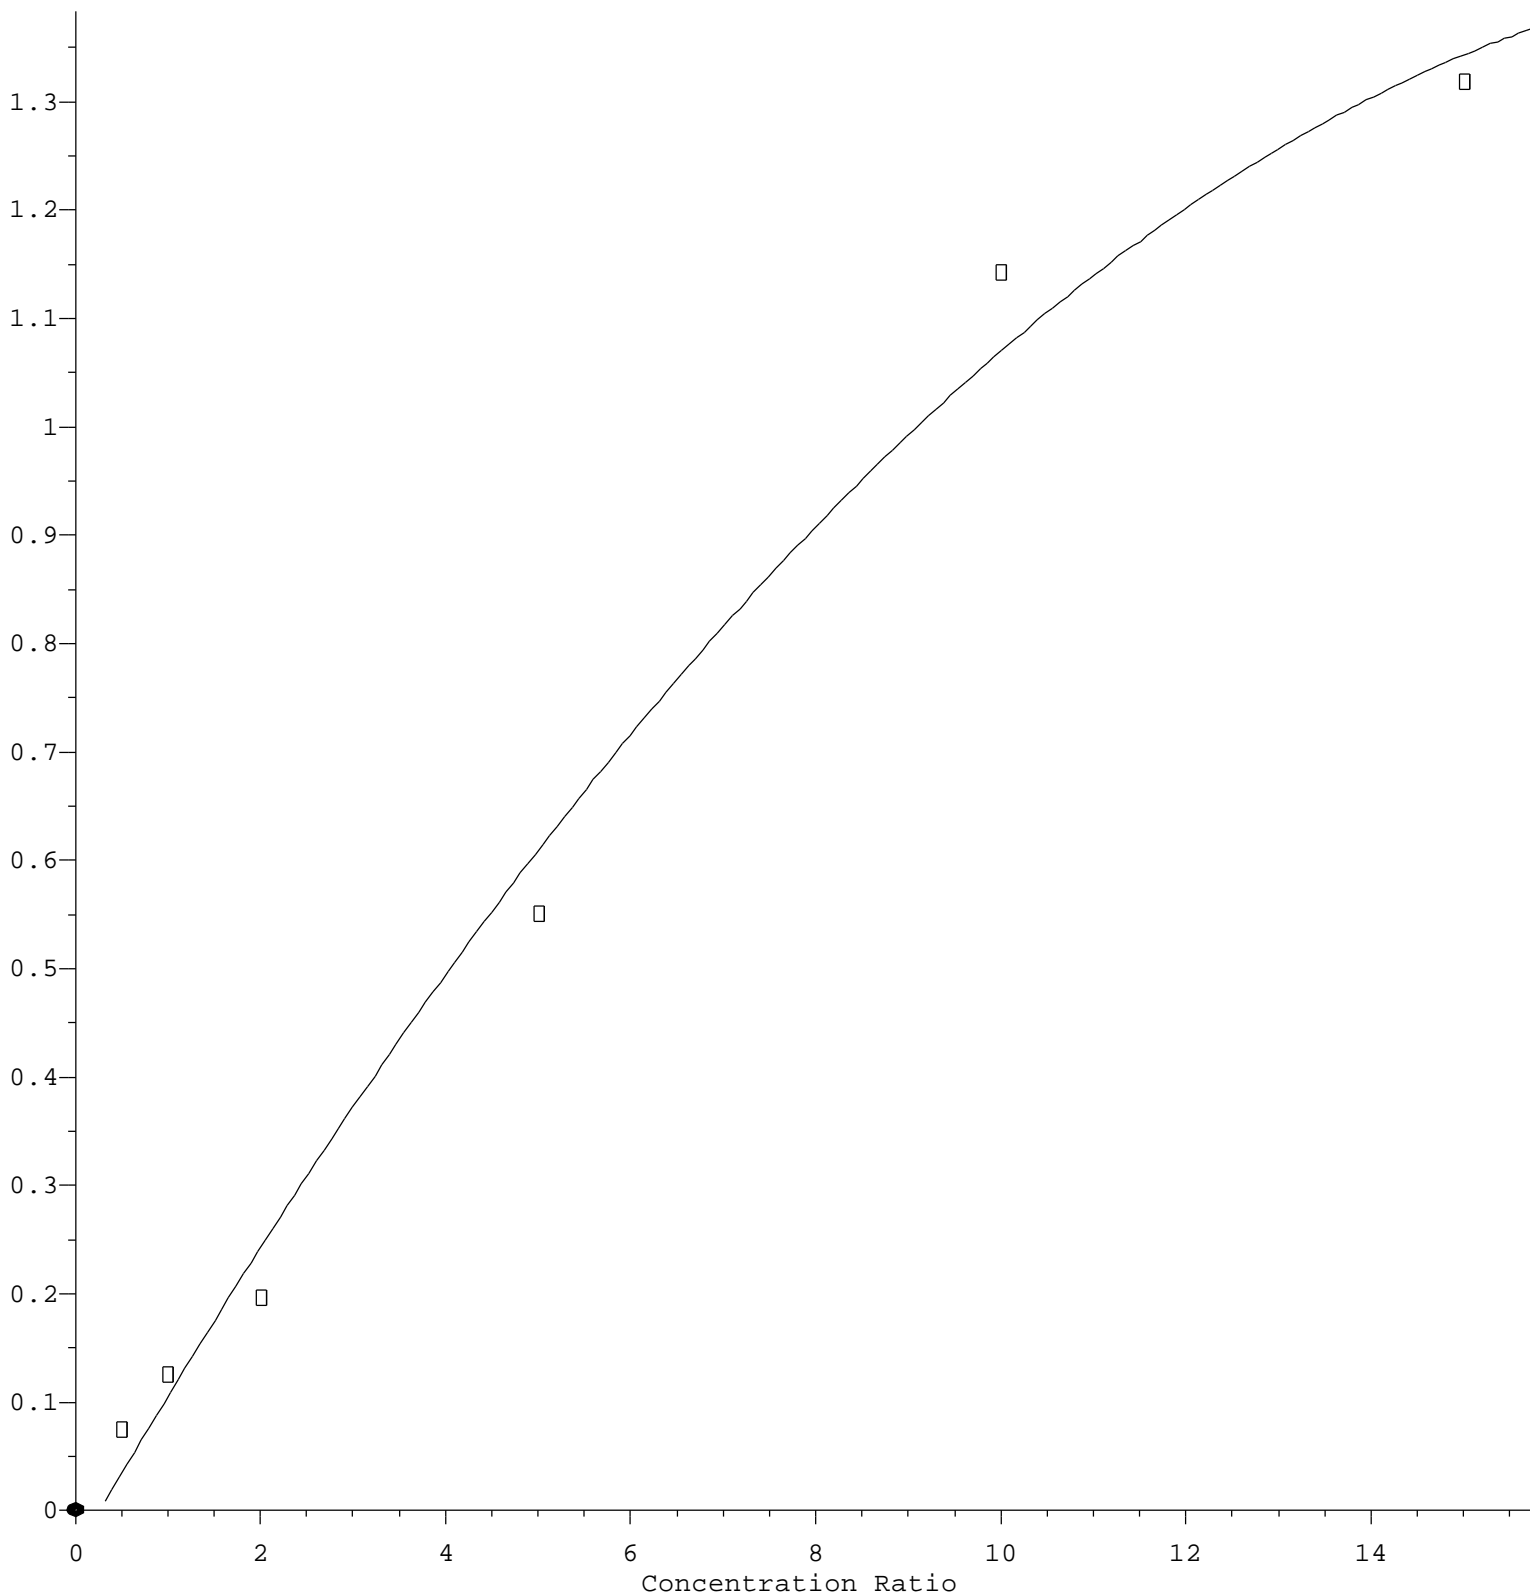

$R = -3.752e-003 A^2 + 1.484e-001 A - 3.877e-002$   
 Coef of Det ( $r^2$ ) = 0.990790    Curve Fit: Quadratic  
 Method Name:    Z:\voasrv\HPCHEM1\MSVOA\_D\Method\82D071321S.M  
 Calibration Table Last Updated: Wed Jul 14 06:00:31 2021

## Carbon Disulfide

Response Ratio

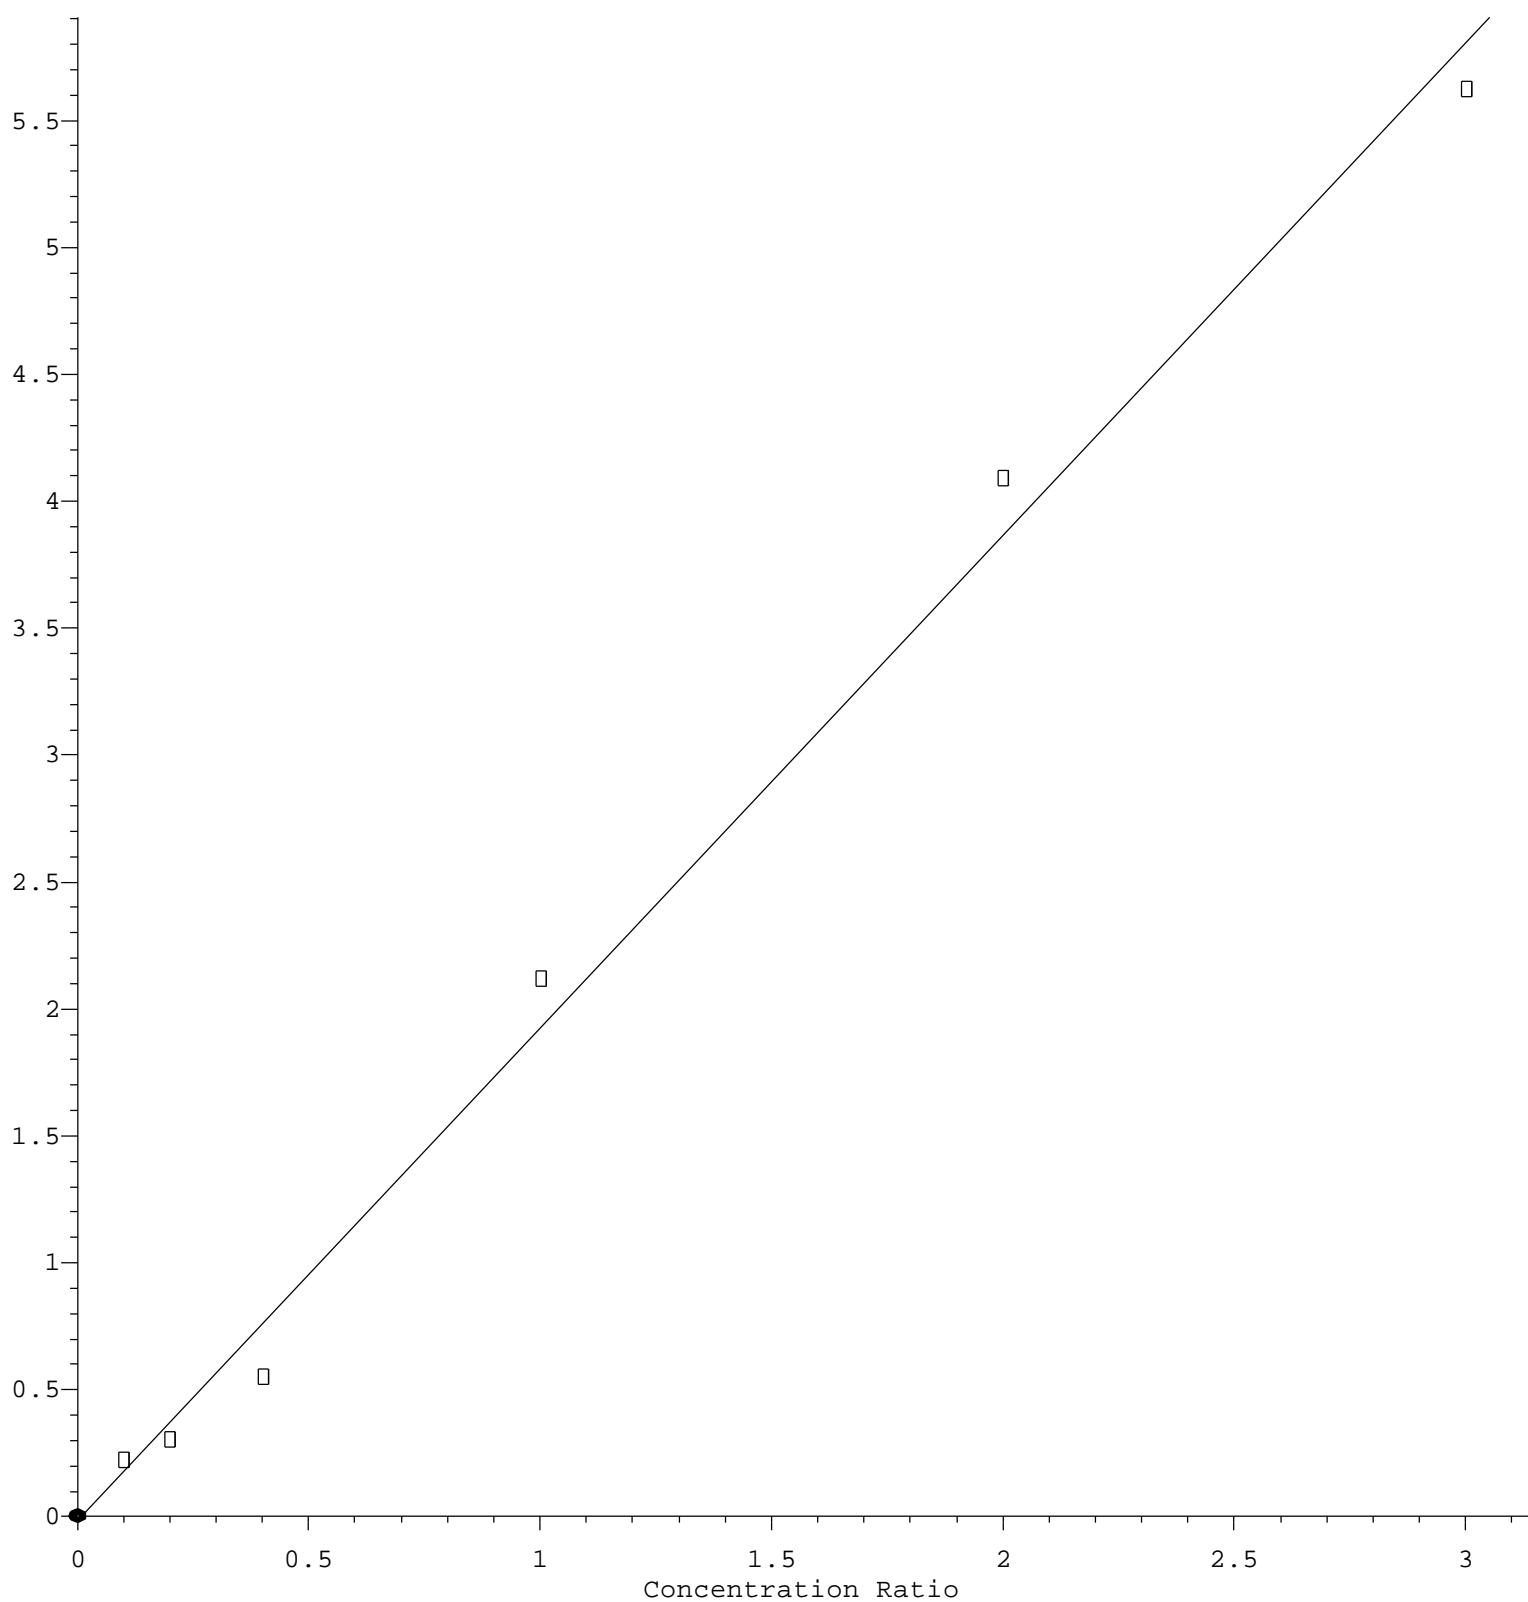

$$\text{Response} = 1.941\text{e}+000 * \text{Amt} - 1.690\text{e}-002$$


Coef of Det ( $r^2$ ) = 0.993193 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA\_D\Method\82D071321S.M

Calibration Table Last Updated: Wed Jul 14 06:00:31 2021

## Methyl Acetate

Response Ratio

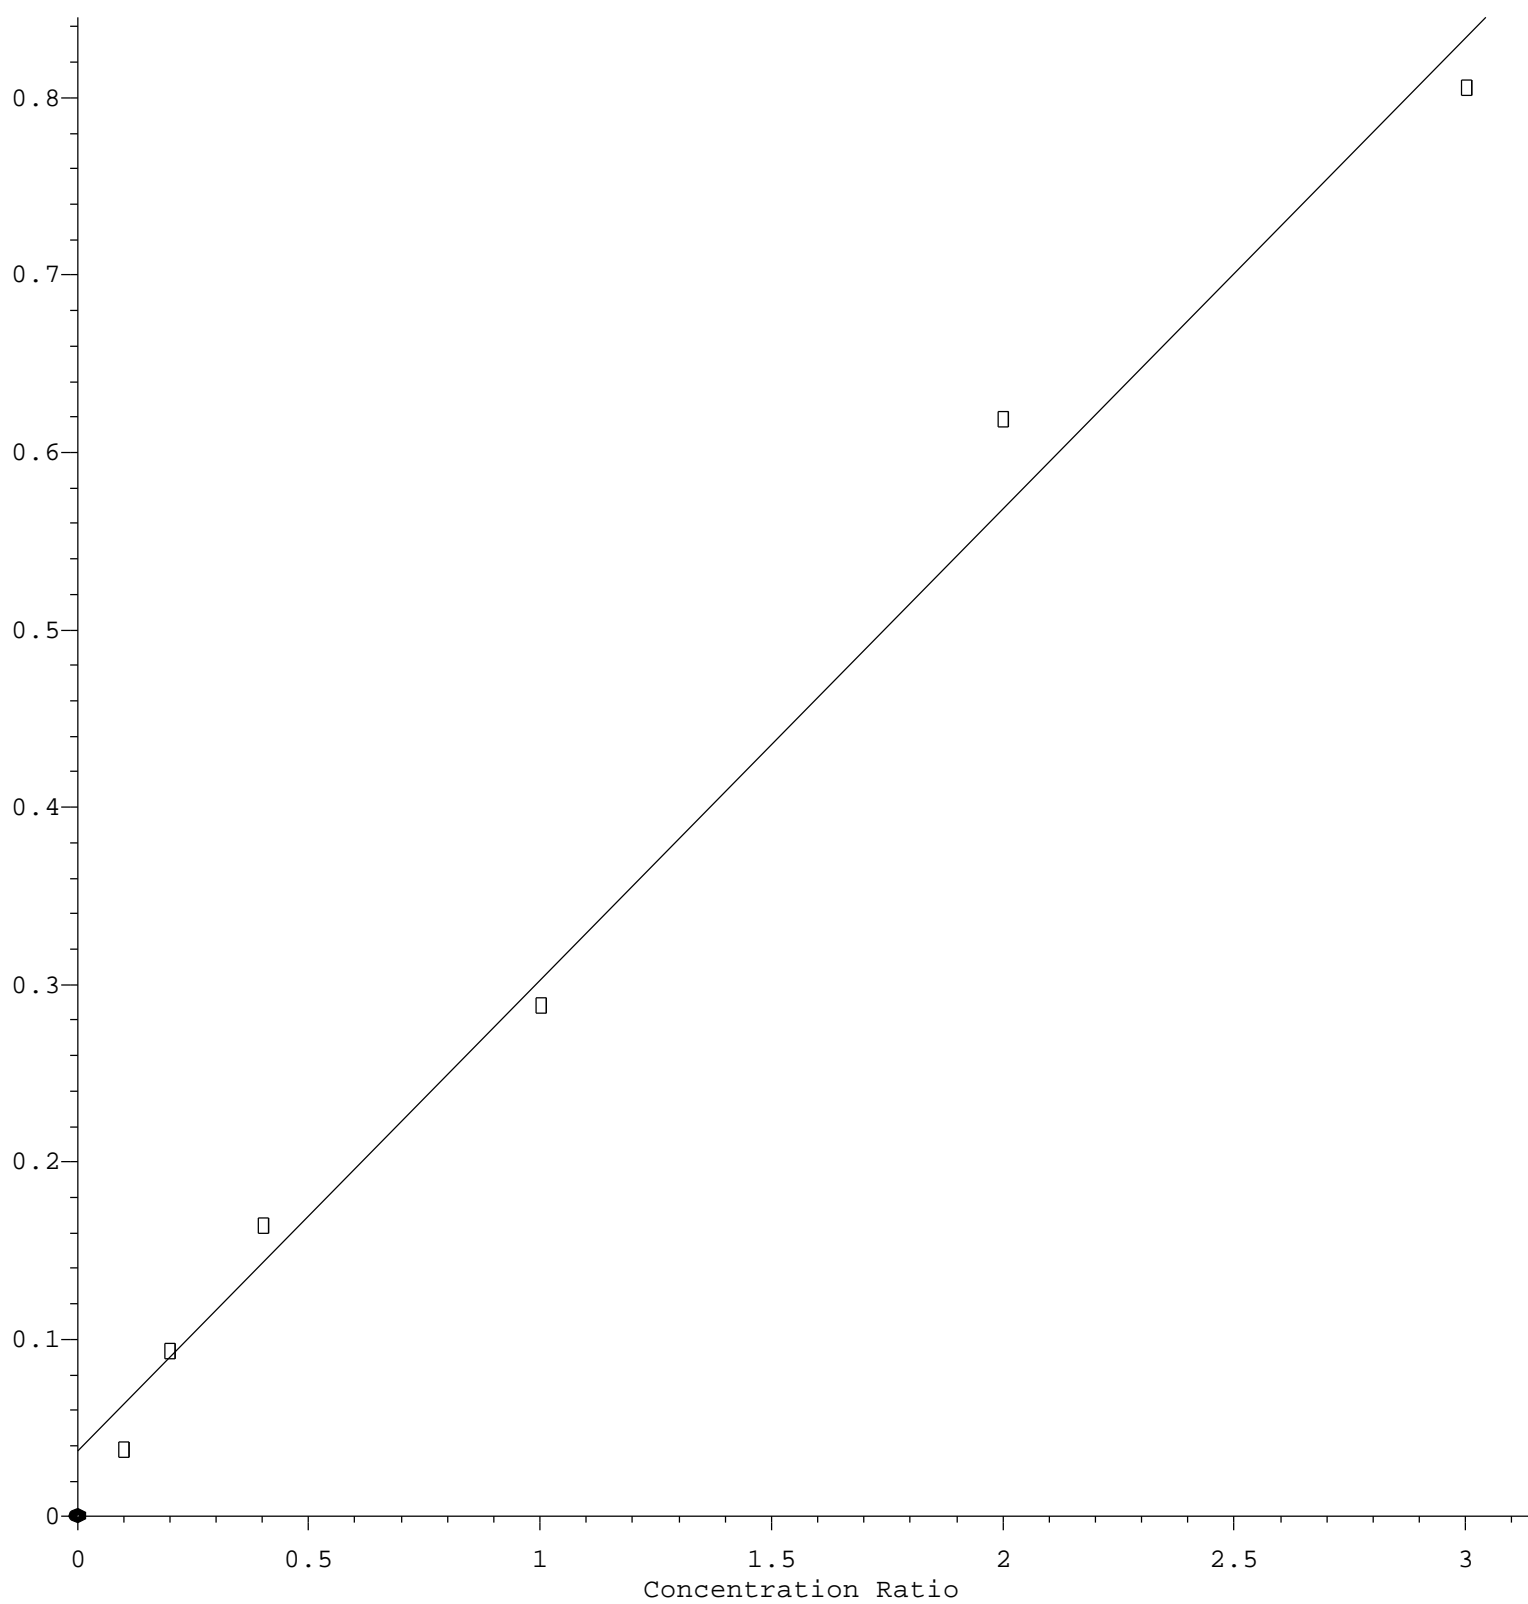

$$\text{Response} = 2.659\text{e-}001 * \text{Amt} + 3.743\text{e-}002$$


Coef of Det ( $r^2$ ) = 0.990384 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA\_D\Method\82D071321S.M

Calibration Table Last Updated: Wed Jul 14 06:00:31 2021

## Methylene Chloride

Response Ratio

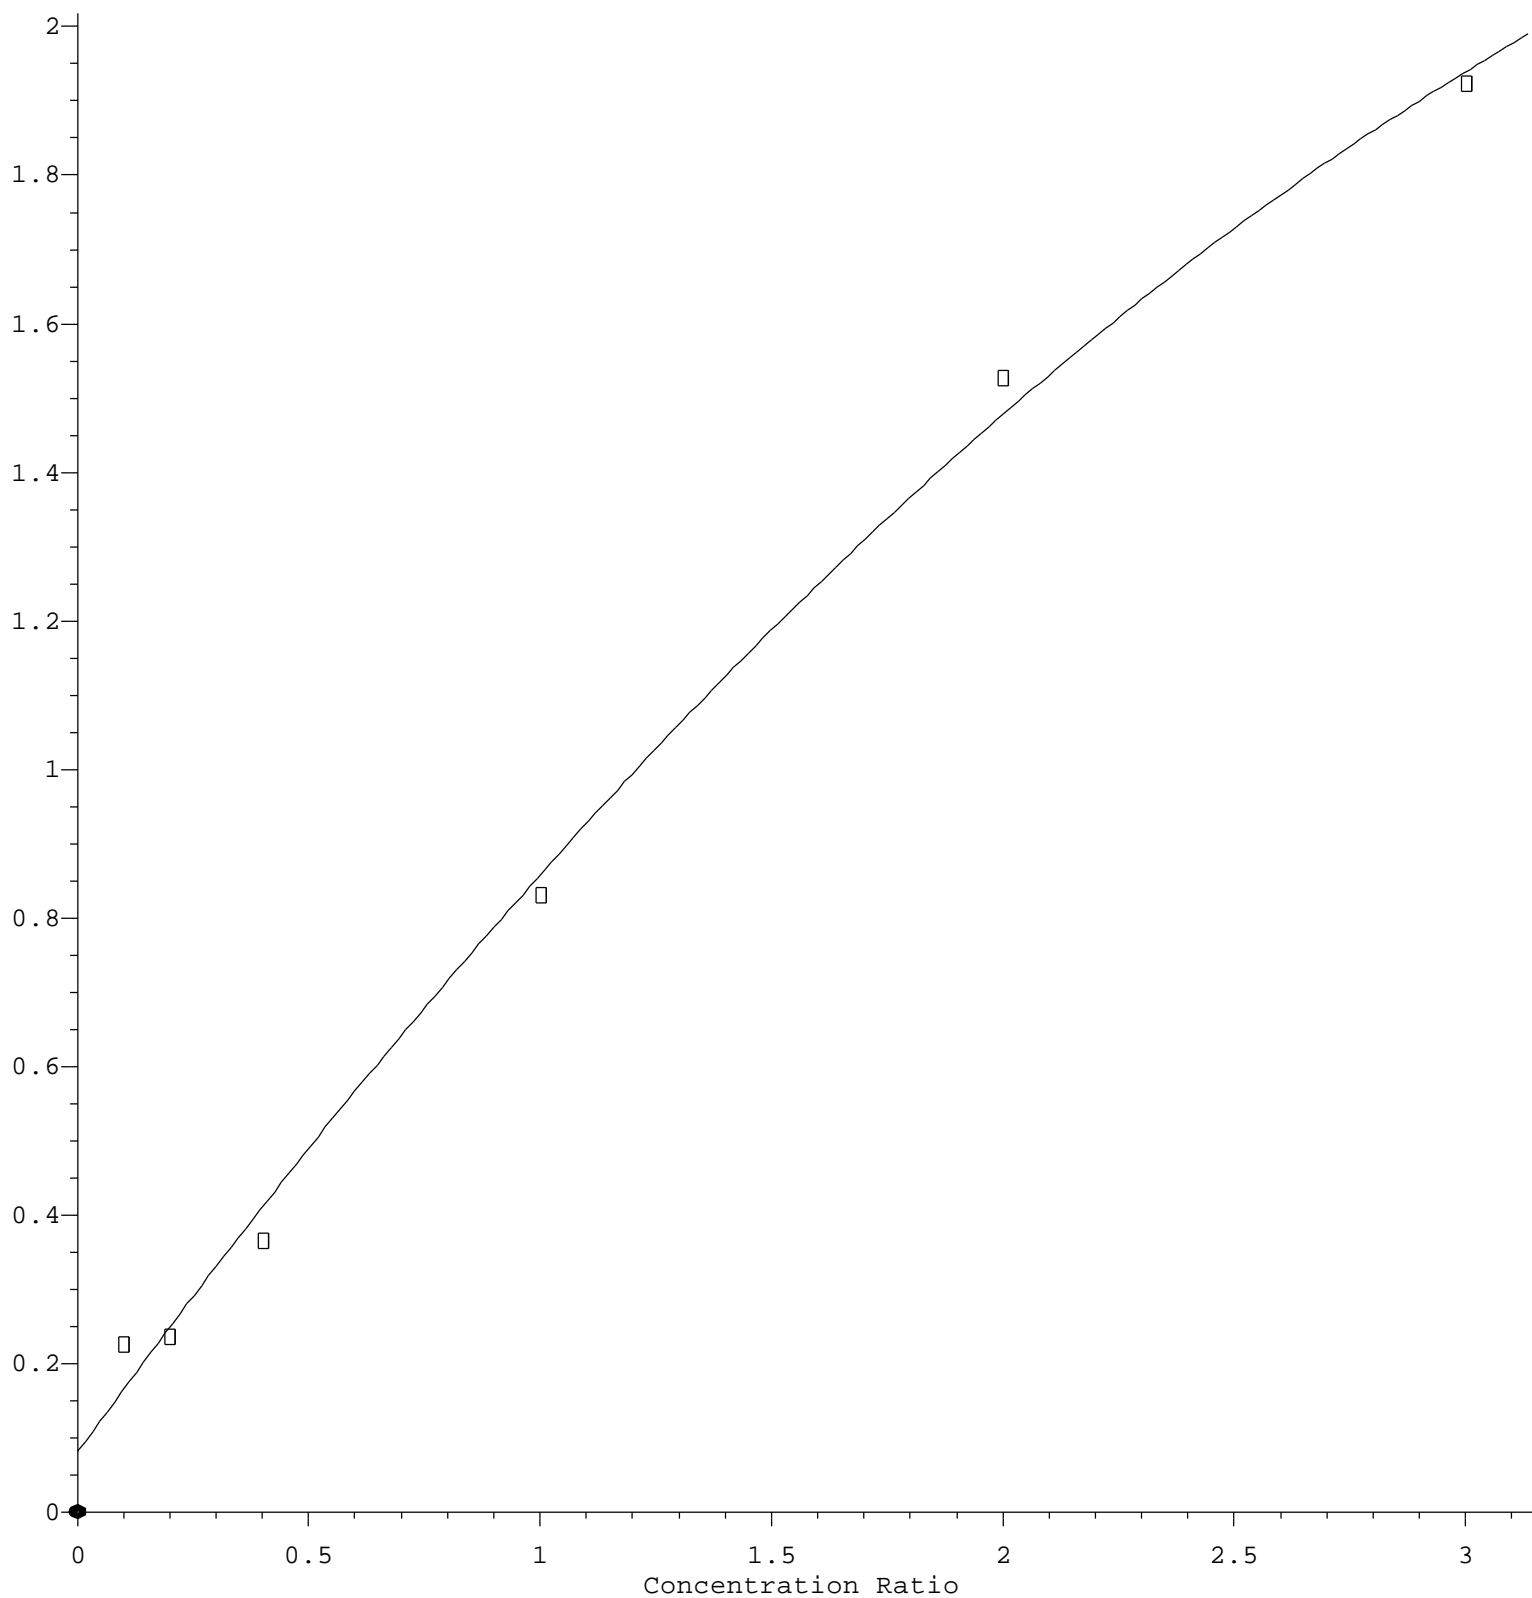

$R = -7.894e-002 A^2 + 8.560e-001 A + 8.176e-002$   
Coef of Det ( $r^2$ ) = 0.996439    Curve Fit: Quadratic  
Method Name:    Z:\voasrv\HPCHEM1\MSVOA\_D\Method\82D071321S.M  
Calibration Table Last Updated: Wed Jul 14 06:00:31 2021