



Dichlorodifluoromethane

Response Ratio

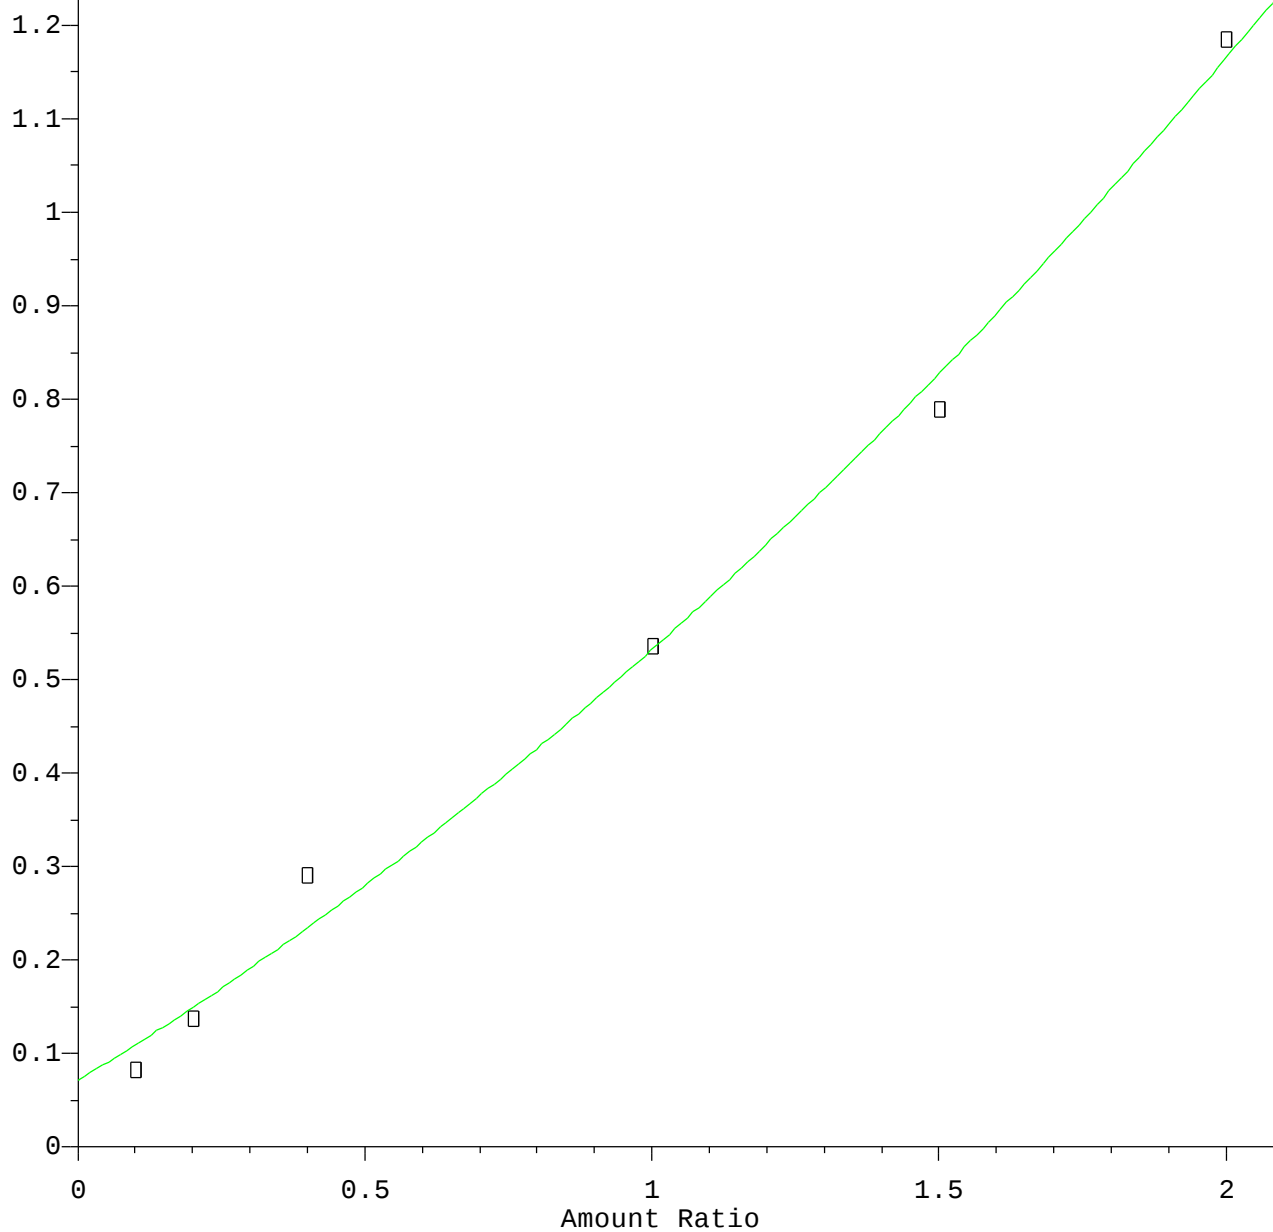


$R = 8.56e-002 A^2 + 3.76e-001 A + 7.06e-002$
Coef of Det (r^2) = 0.994 Curve Fit: Quadratic


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D071519S.M
Calibration Table Last Updated: Tue Jul 16 08:11:56 2019

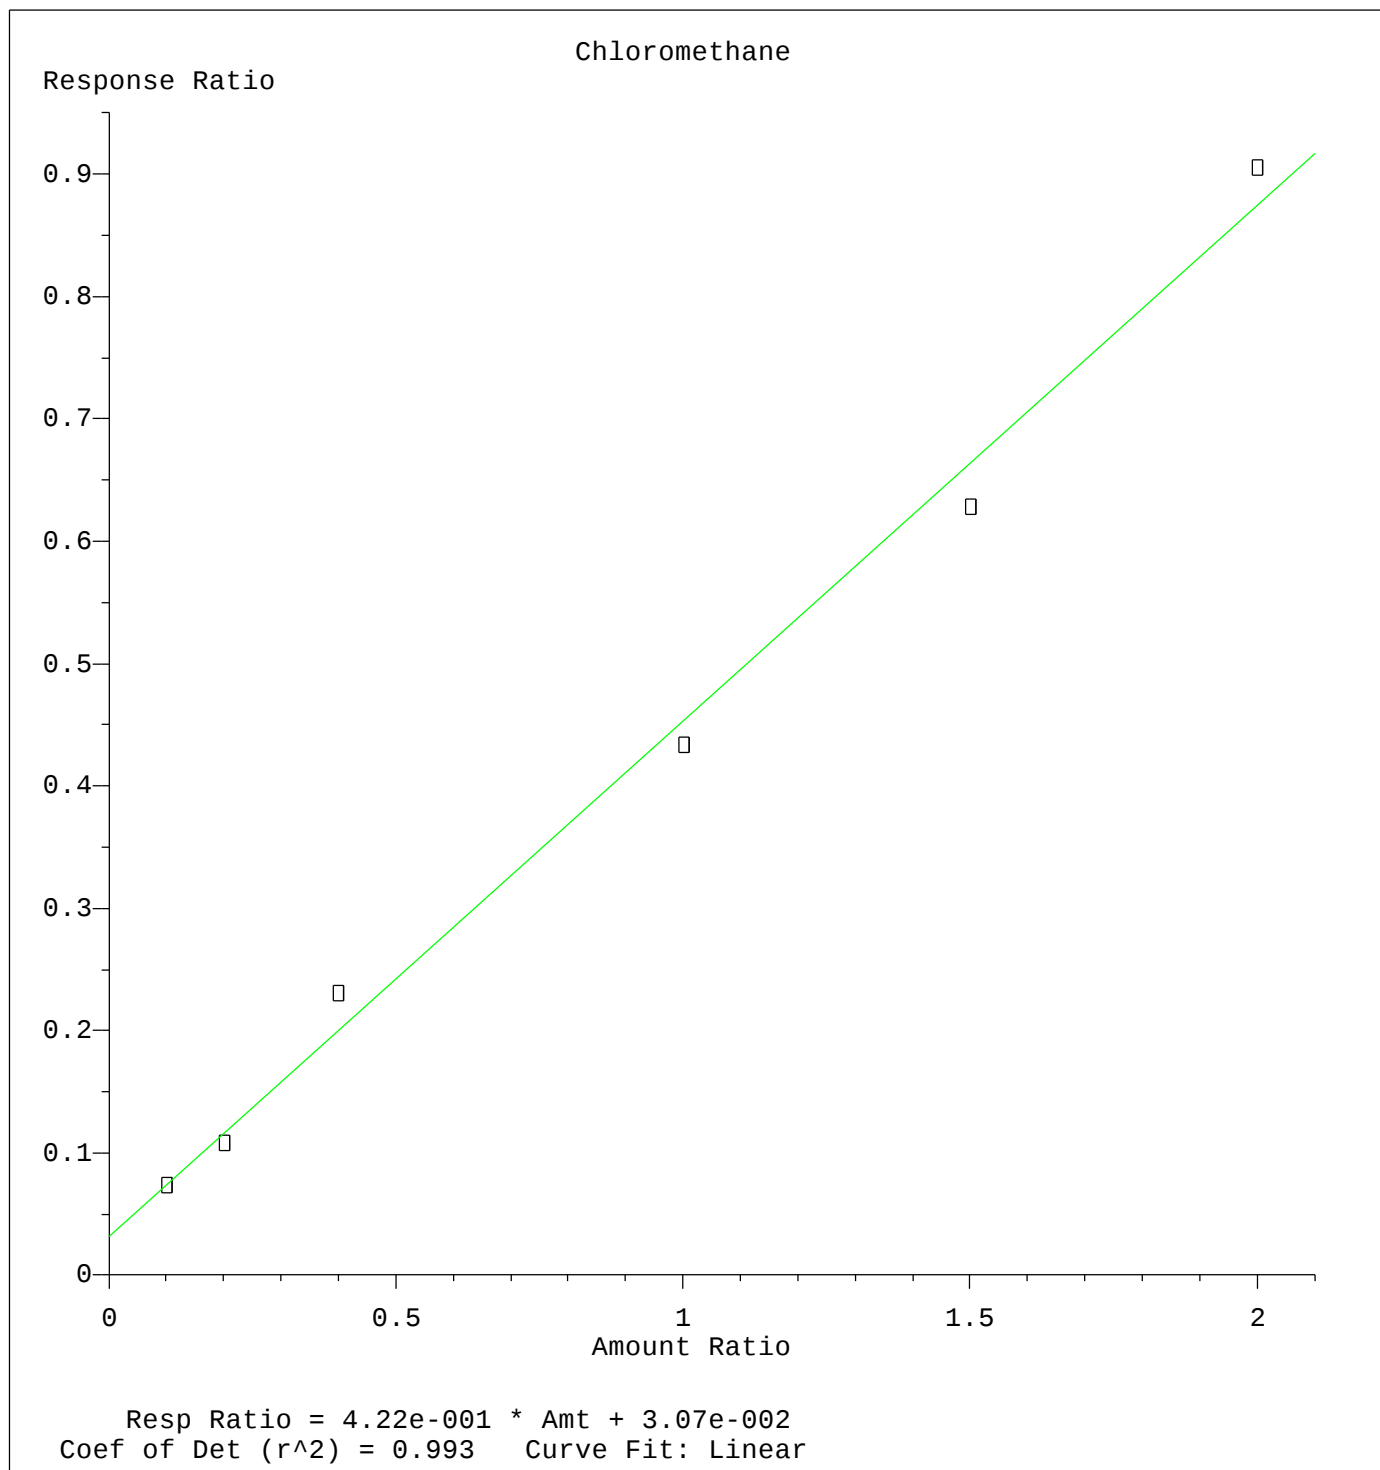

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D071519S.M
Calibration Table Last Updated: Tue Jul 16 08:11:56 2019

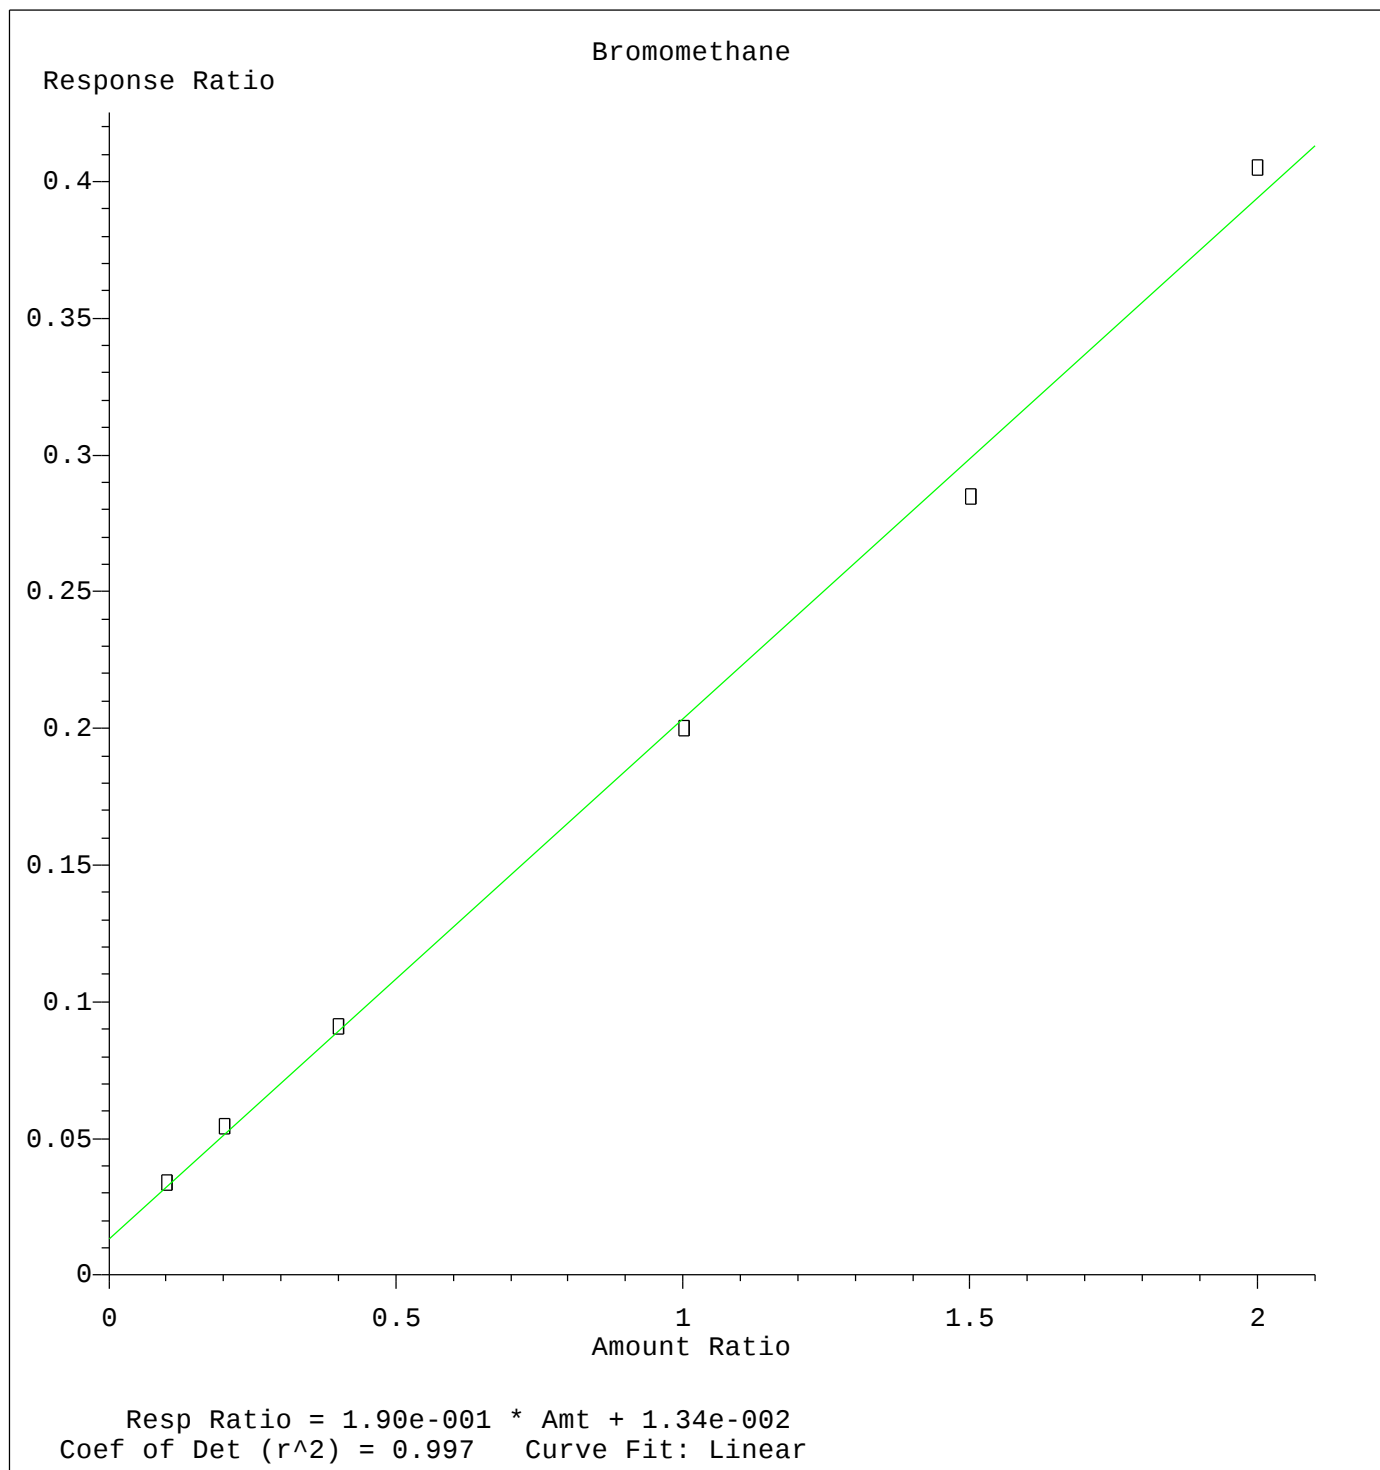

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D071519S.M
Calibration Table Last Updated: Tue Jul 16 08:11:56 2019

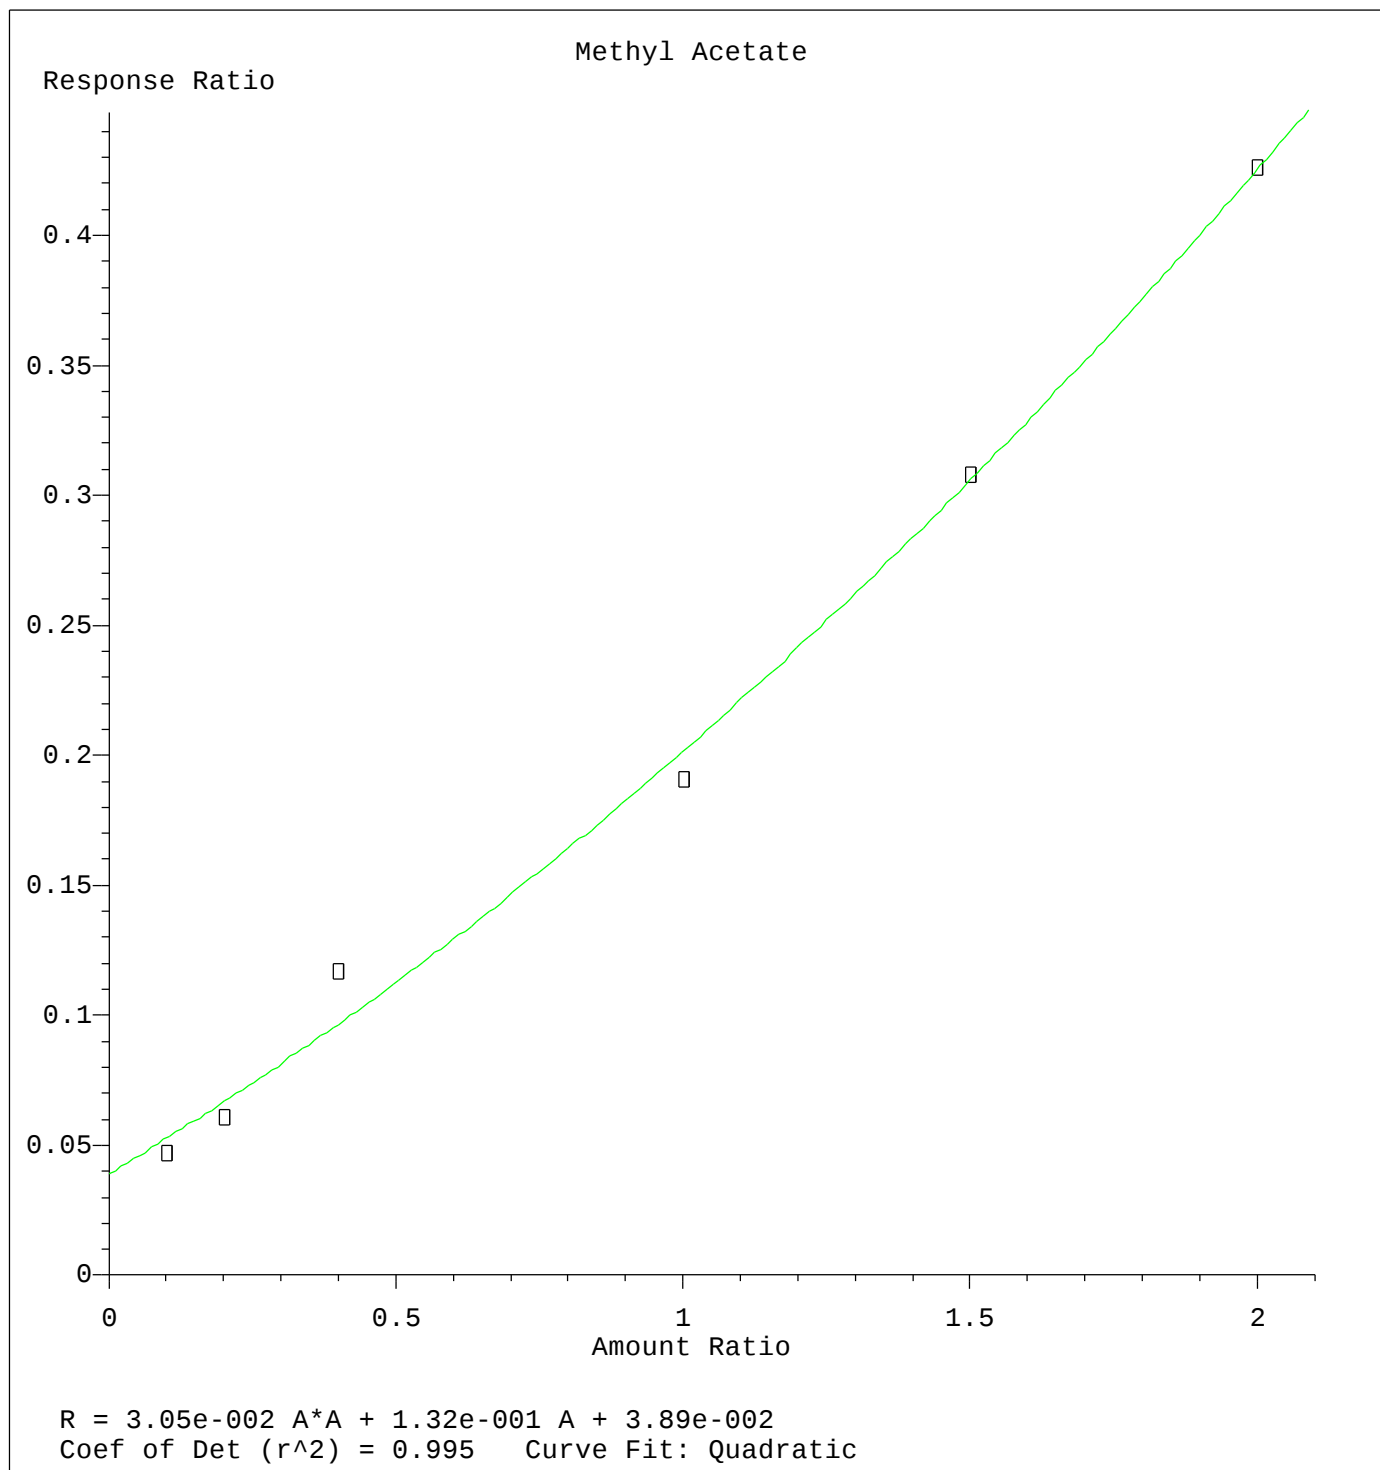

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D071519S.M
Calibration Table Last Updated: Tue Jul 16 08:11:56 2019