


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD071719\
Data File : VD063120.D
Acq On : 17 Jul 2019 9:10
Operator : VA/AP
Sample : BFB
Misc : 5.00µl/5ml/MSVOA D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D071519S.M
Title : SW846 8260
Last Update : Tue Jul 16 08:11:56 2019

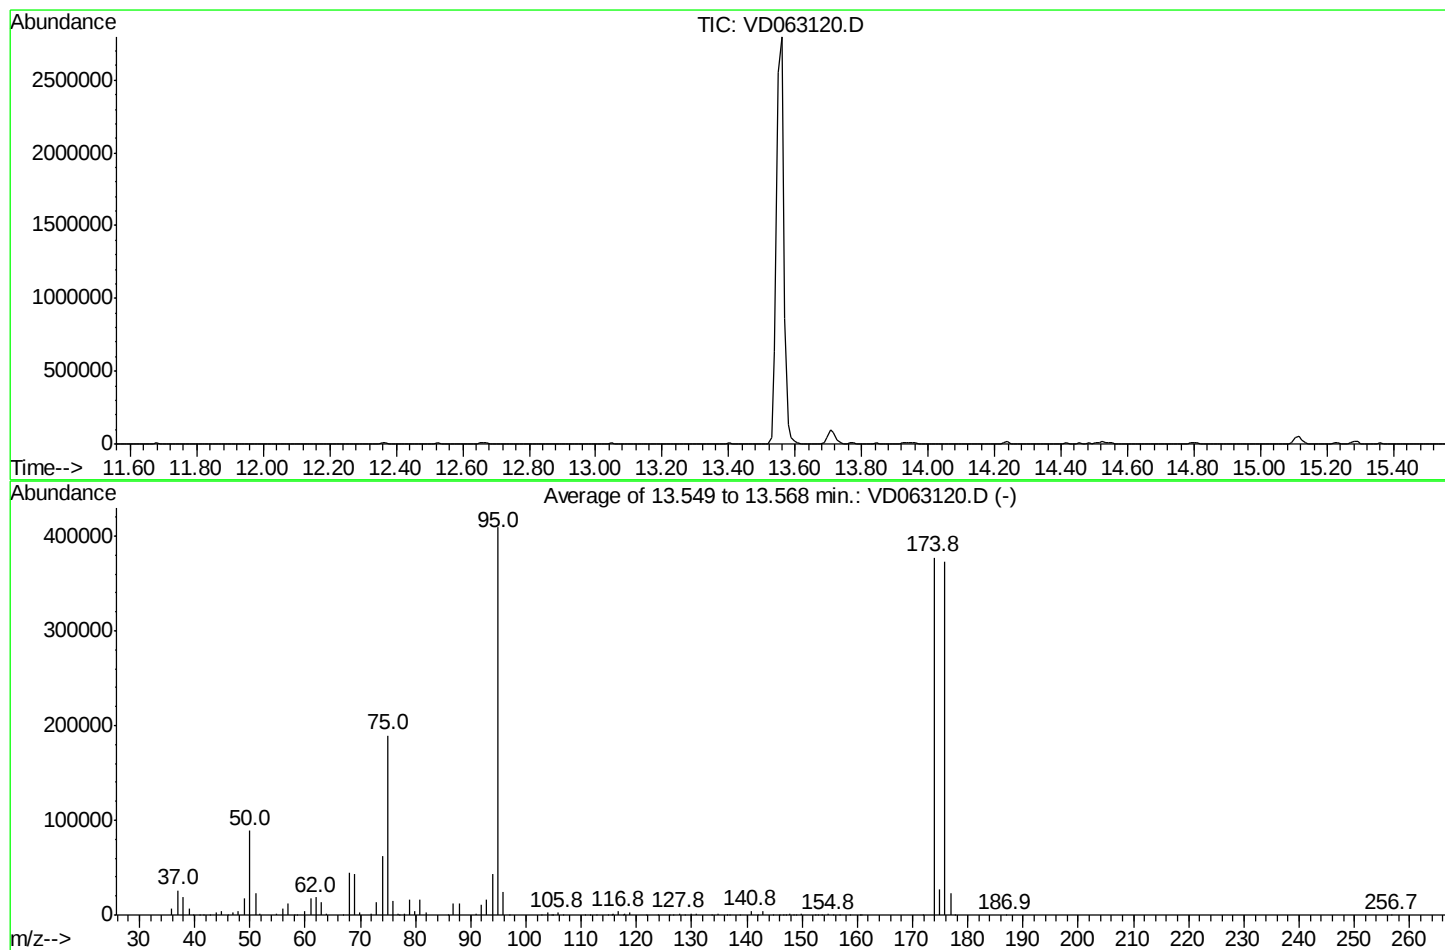

AutoFind: Scans 1231, 1232, 1233; Background Corrected with Scan 1226

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.7	88944	PASS
75	95	30	60	46.4	189858	PASS
95	95	100	100	100.0	409280	PASS
96	95	5	9	6.0	24618	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	92.2	377472	PASS
175	174	5	9	7.1	26762	PASS
176	174	95	101	98.7	372693	PASS
177	176	5	9	6.0	22545	PASS